

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091919\
 Data File : PL052623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2019 13:47
 Operator : SG\AJ
 Sample : K4847-04 (Sig #1); K4947-02 (Sig #2)
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-28-COMP

Manual Integrations
 APPROVED

Ankita
 9/20/2019 3:51:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 00:56:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	4.046	156.6E6	45419339	20.087m	20.845
28)	SA Decachlor...	8.350	9.120	104.5E6	35684843	11.955	14.902

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091919\
Data File : PL052623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2019 13:47
Operator : SG\AJ
Sample : K4847-04 (Sig #1); K4947-02 (Sig #2)
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-28-COMP


Manual Integrations
APPROVED

Ankita
9/20/2019 3:51:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 00:56:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

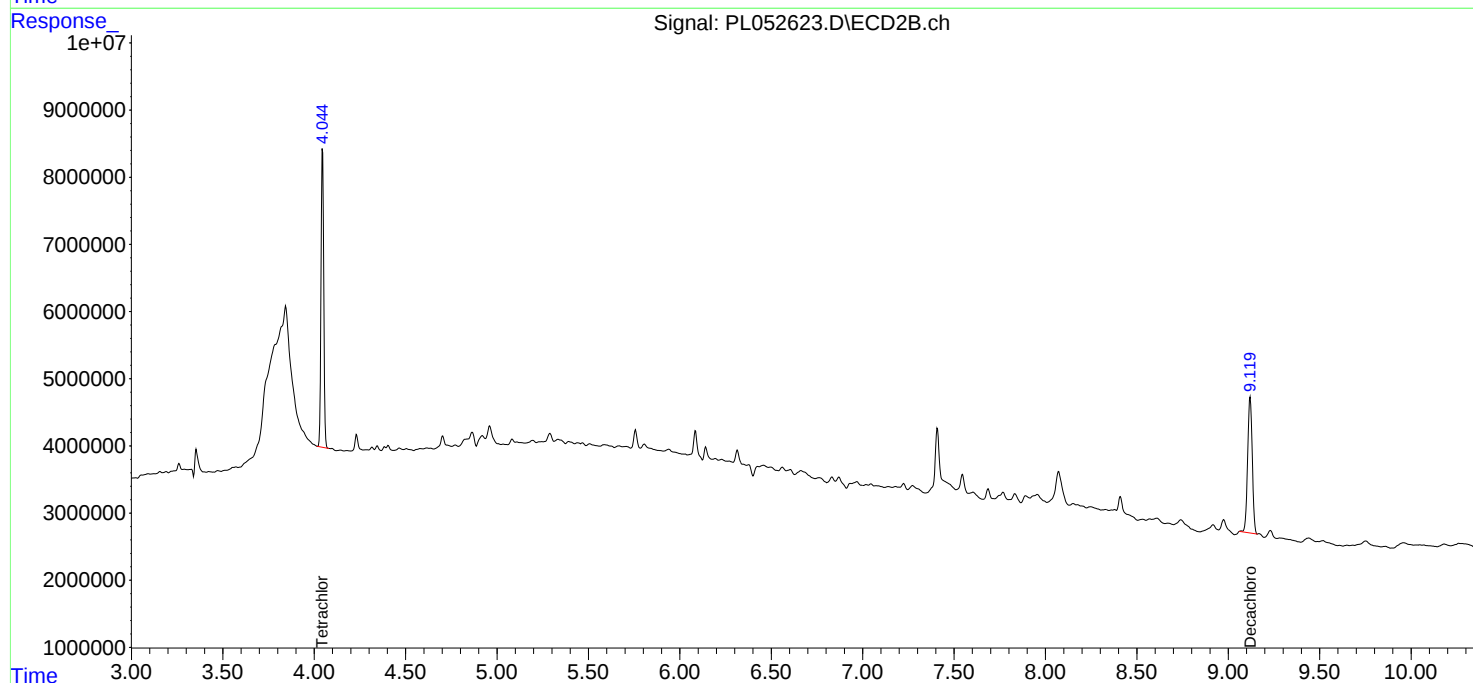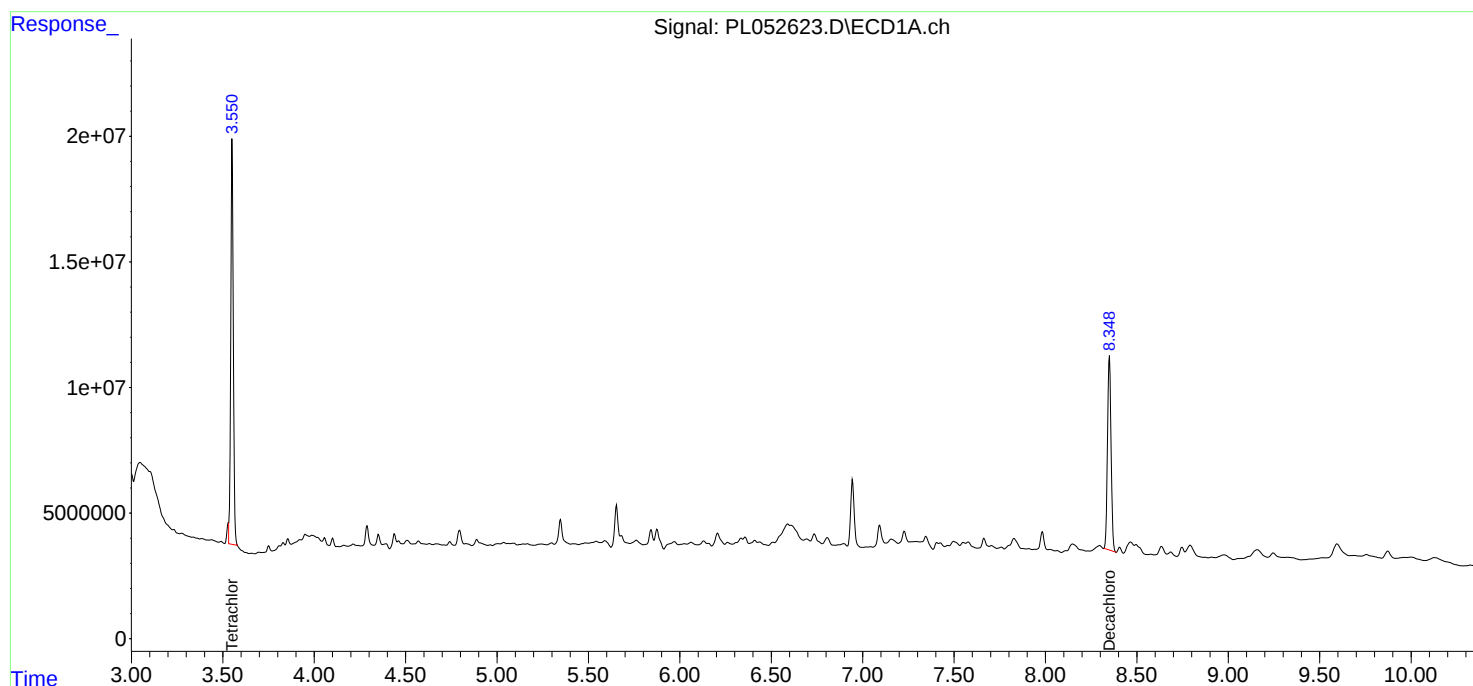

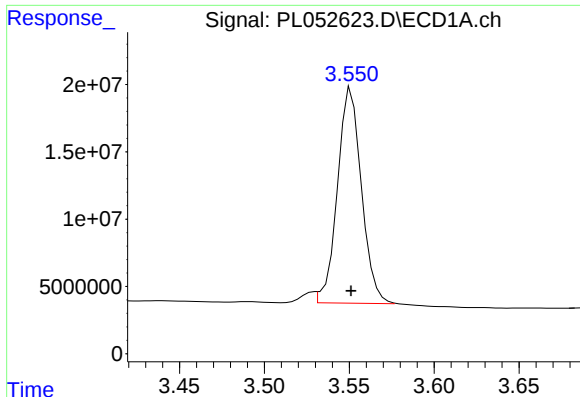


#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: -0.001 min
Response: 156630432
Conc: 20.09 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-28-COMP


Manual Integrations
APPROVED

Ankita
9/20/2019 3:51:40 PM

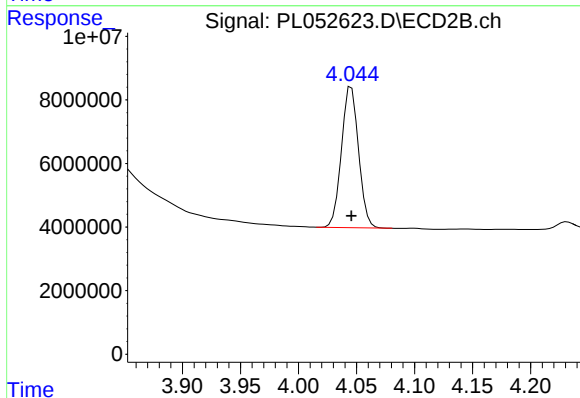


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 45419339
Conc: 20.84 ng/ml

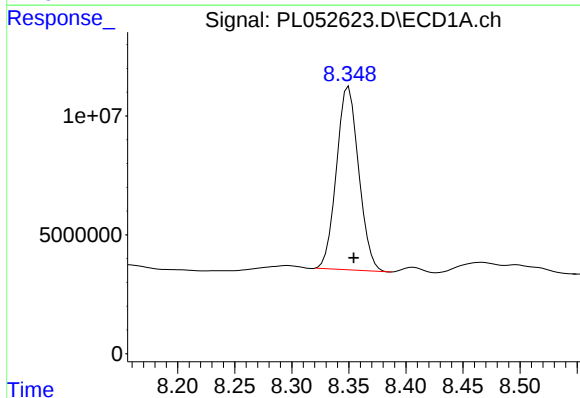

#28 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: -0.005 min
Response: 104537321
Conc: 11.95 ng/ml

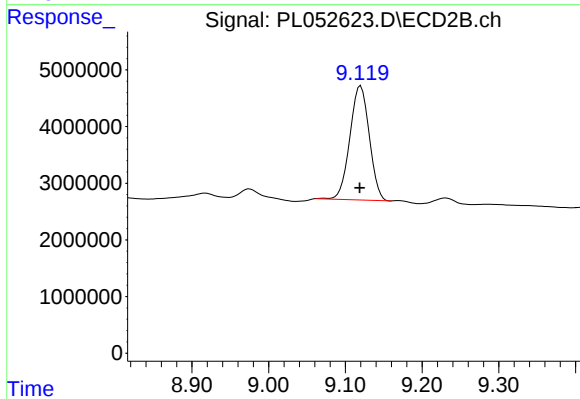

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.001 min
Response: 35684843
Conc: 14.90 ng/ml