

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091919\
 Data File : PL052625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2019 14:17
 Operator : SG\AJ
 Sample : K4960-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ROLL-OFF-COMP

Manual Integrations
 APPROVED

Ankita
 9/20/2019 3:51:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 00:56:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	4.044	93966524	25034613	12.051	11.489m
28) SA Decachlor...	8.350	9.120	105.4E6	35200273	12.057	14.700
Target Compounds						
12) B 4,4'-DDE	5.744	6.381	24292512	5972723	2.603	2.450m
17) MA 4,4'-DDT	6.506	7.172	17413897	5798074	2.244	3.170 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091919\
Data File : PL052625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2019 14:17
Operator : SG\AJ
Sample : K4960-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP


Manual Integrations
APPROVED

Ankita
9/20/2019 3:51:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 00:56:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

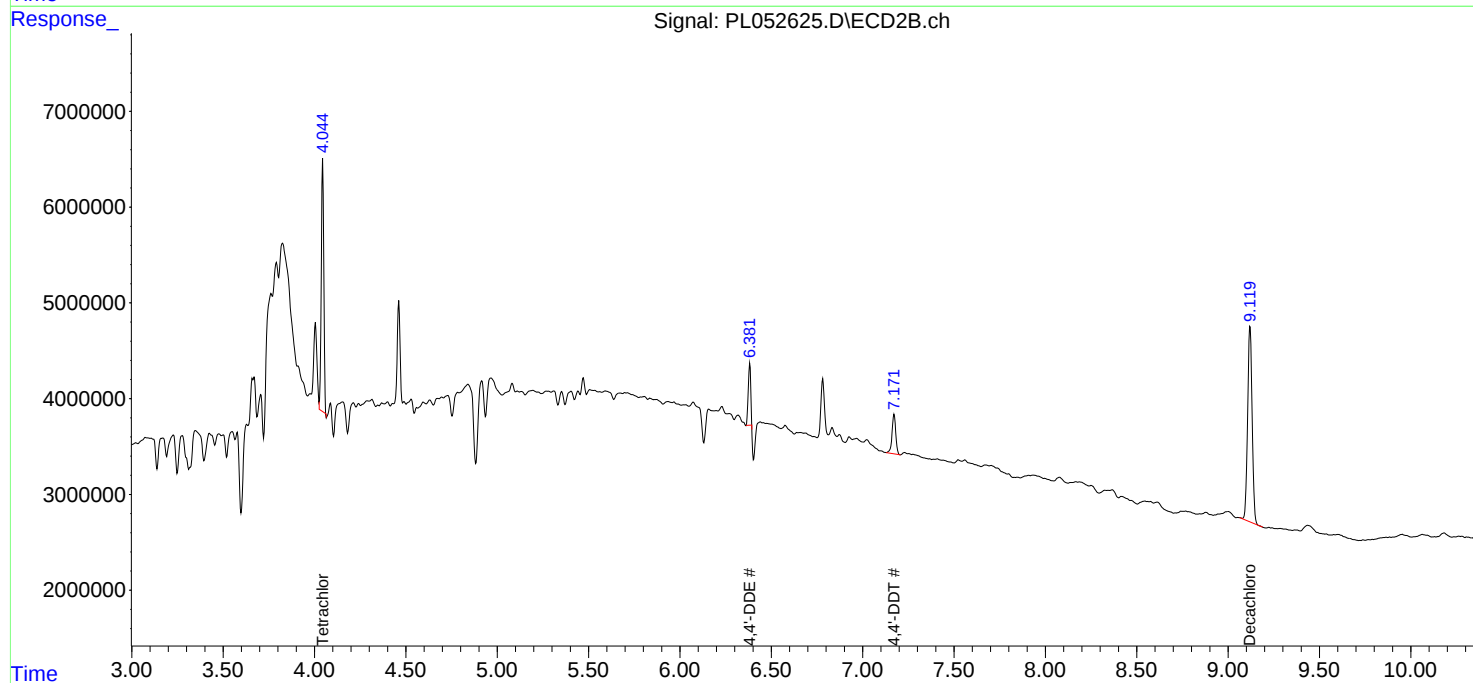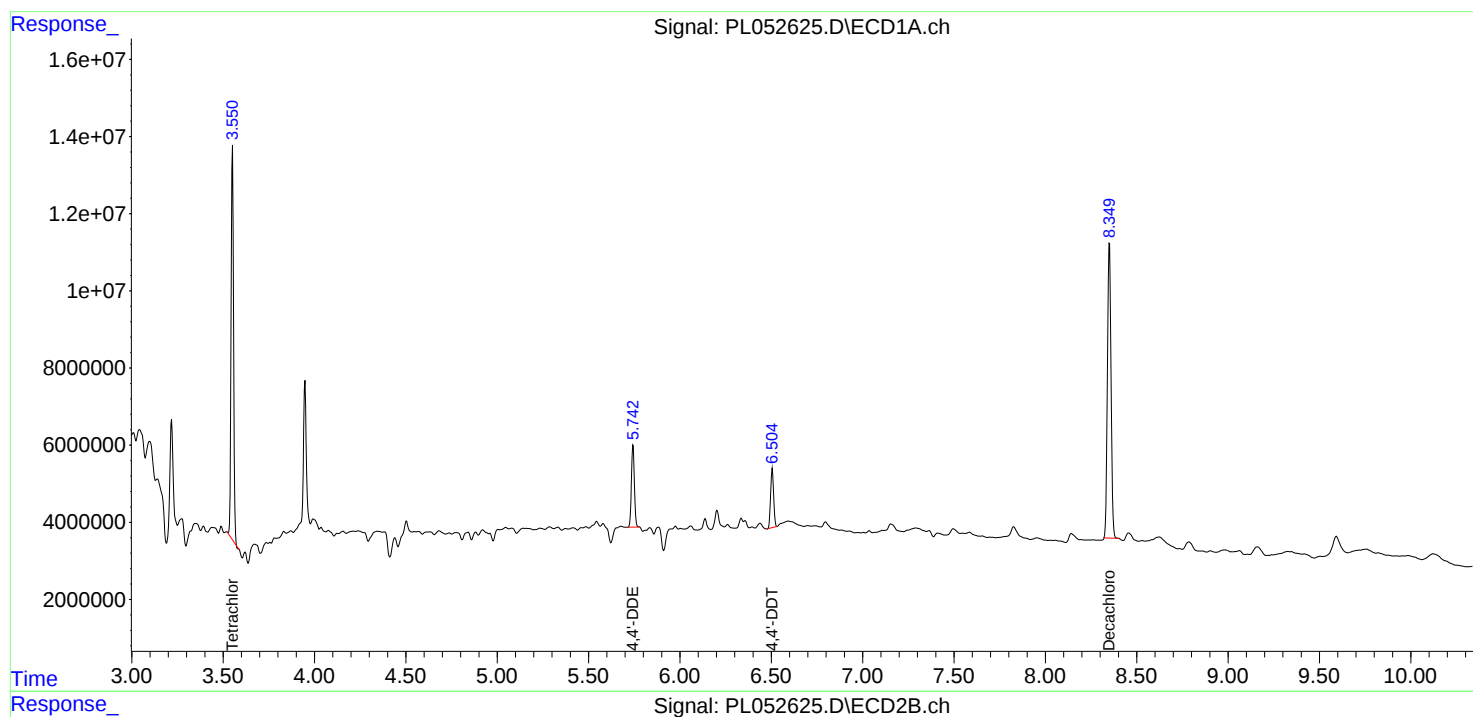

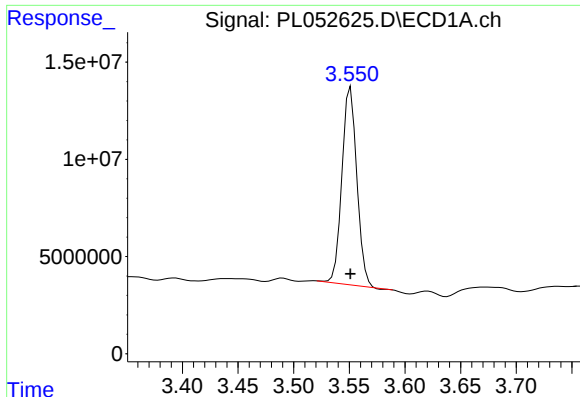


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 93966524
Conc: 12.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP


Manual Integrations
APPROVED

Ankita
9/20/2019 3:51:41 PM

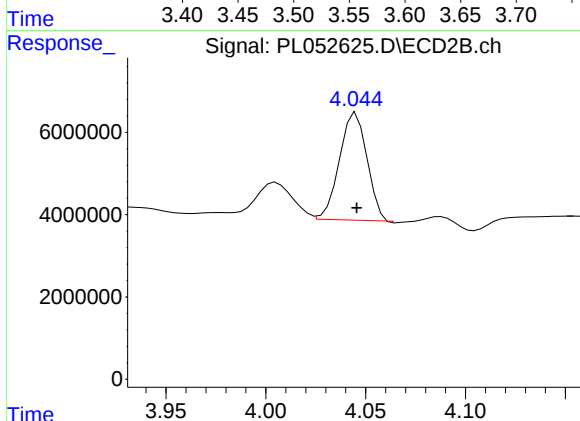


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 25034613
Conc: 11.49 ng/ml m

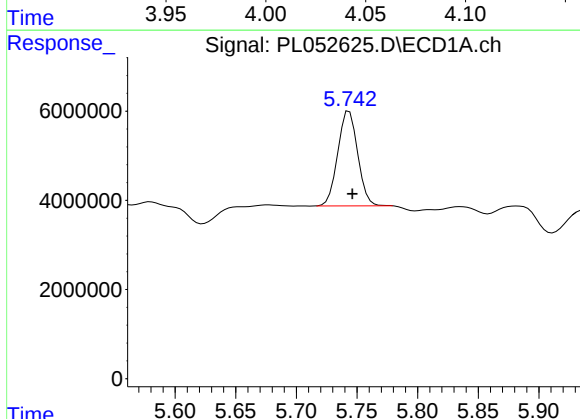


#12 4,4'-DDE

R.T.: 5.744 min
Delta R.T.: -0.002 min
Response: 24292512
Conc: 2.60 ng/ml

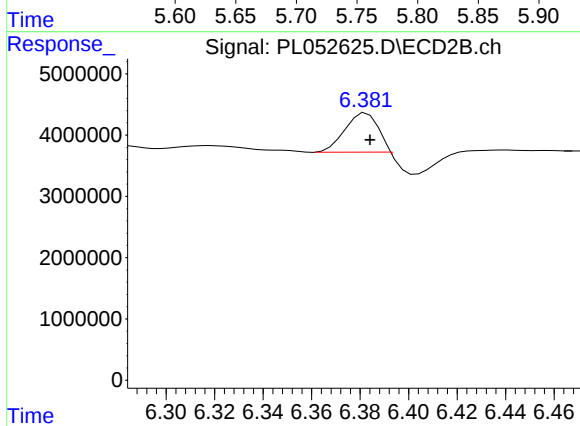

#12 4,4'-DDE

R.T.: 6.381 min
Delta R.T.: -0.003 min
Response: 5972723
Conc: 2.45 ng/ml m

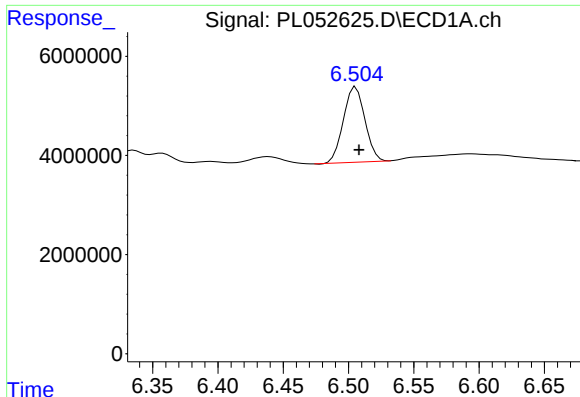


#17 4,4'-DDT

R.T.: 6.506 min
Delta R.T.: -0.003 min
Response: 17413897
Conc: 2.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP


Manual Integrations
APPROVED

Ankita
9/20/2019 3:51:41 PM

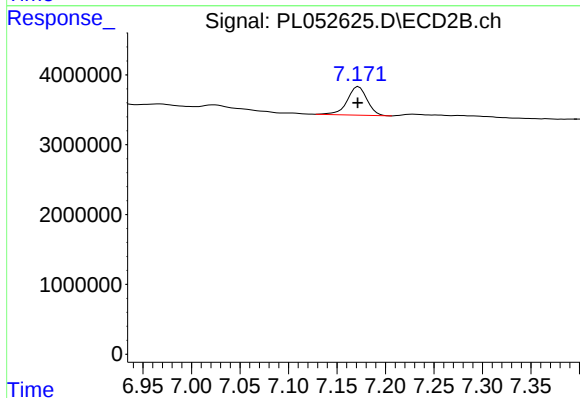


#17 4,4'-DDT

R.T.: 7.172 min
Delta R.T.: 0.000 min
Response: 5798074
Conc: 3.17 ng/ml

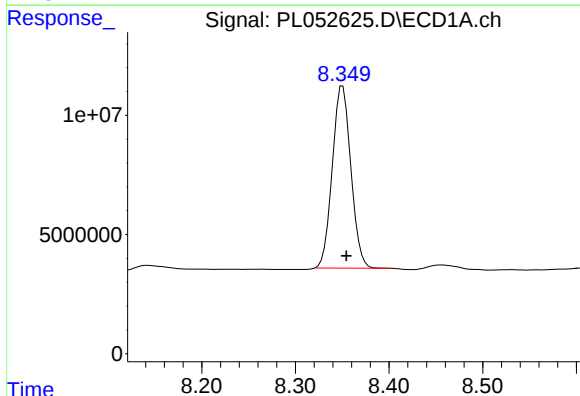

#28 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: -0.004 min
Response: 105430467
Conc: 12.06 ng/ml

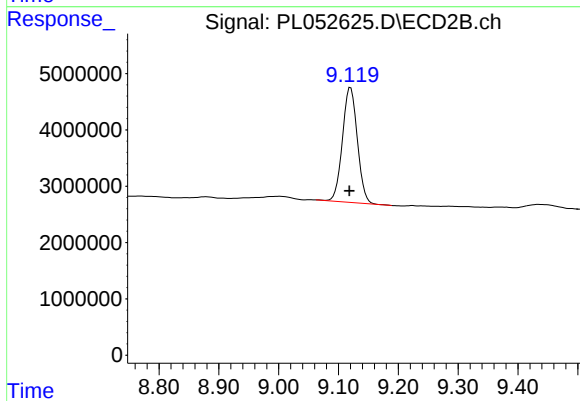

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.002 min
Response: 35200273
Conc: 14.70 ng/ml