

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091922\
 Data File : PL077839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 13:17
 Operator : AR\AJ
 Sample : PB147731BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 17:57:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.624	30096505	56791198	18.775	19.130
28)	SA Decachlor...	8.913	7.725	26449886	48152793	20.465	19.183
Target Compounds							
2)	A alpha-BHC	3.889	0.000	156311	0	0.066	N.D. #
7)	B delta-BHC	4.650f	0.000	469283	0	0.229	N.D. #
10)	B gamma-Chl...	0.000	4.803	0	1526017	N.D.	0.448 #
14)	MA Endrin	0.000	5.473f	0	1854345	N.D.	0.650 #
15)	B Endosulfa...	6.689	0.000	1868633	0	1.353	N.D. #
21)	B Endrin ke...	7.558	6.660	1534135	494841	1.110	0.163 #
25)	Chlordane-3	0.000	4.803	0	1526017	N.D.	4.436 #
27)	Chlordane-5	0.000	5.535	0	2985602	N.D.	31.731 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091922\
Data File : PL077839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 13:17
Operator : AR\AJ
Sample : PB147731BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 17:57:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

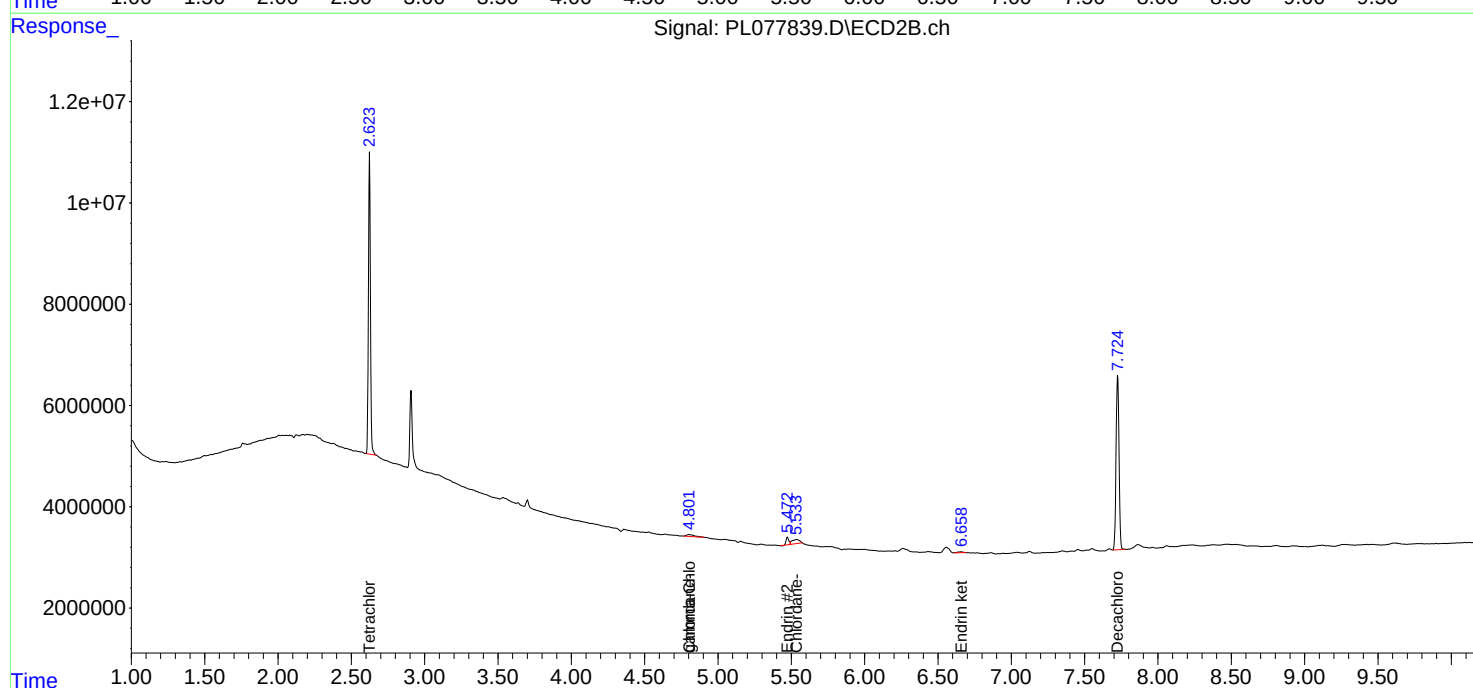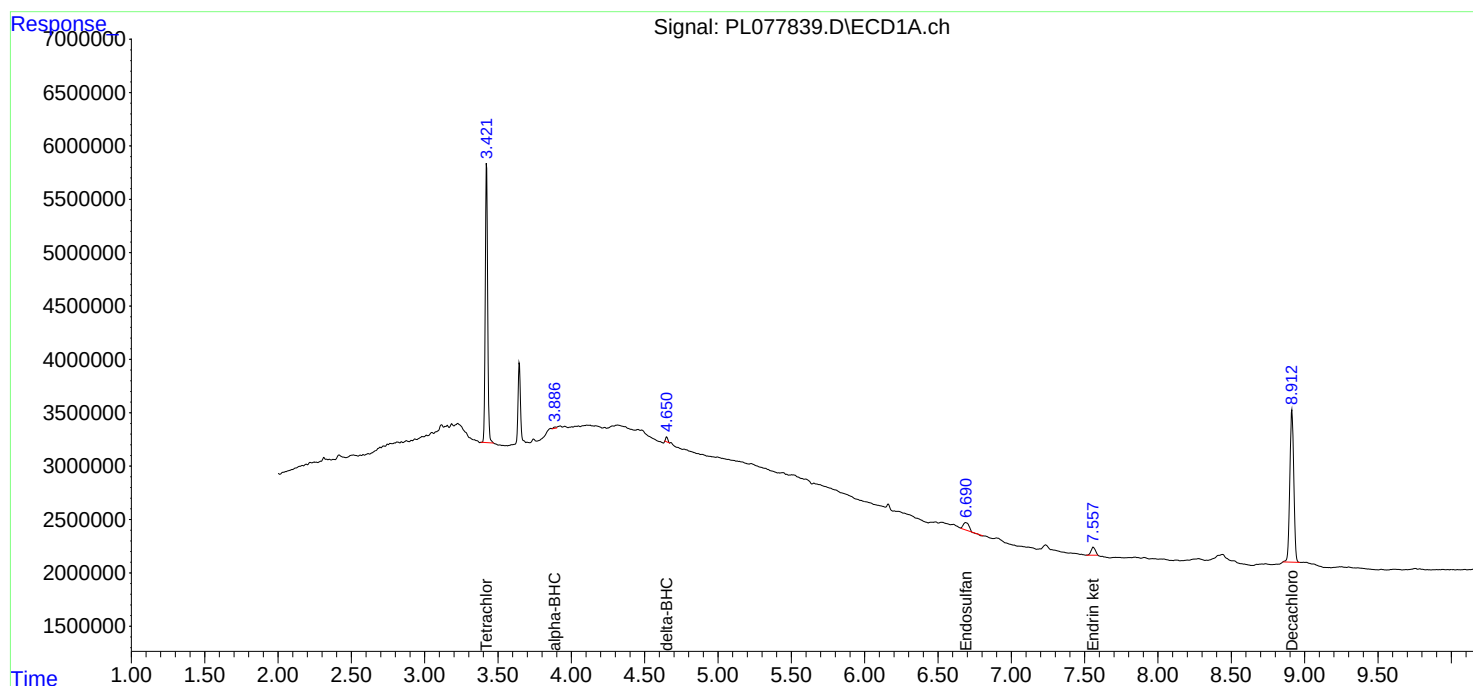


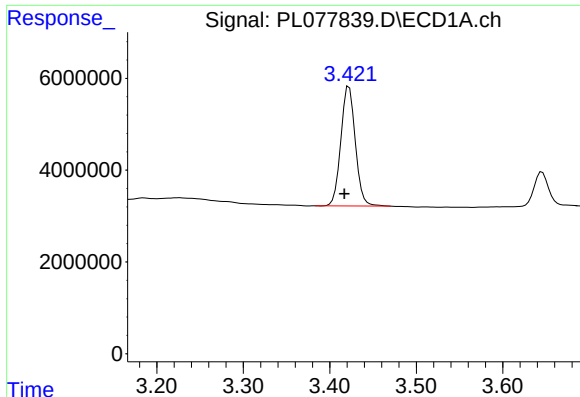

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.005 min
Response: 30096505
Conc: 18.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

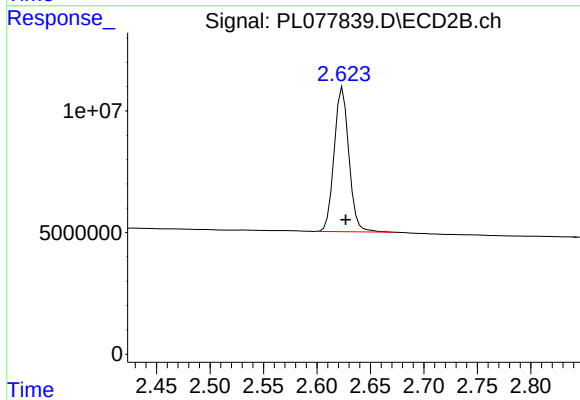


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: -0.003 min
Response: 56791198
Conc: 19.13 ng/ml

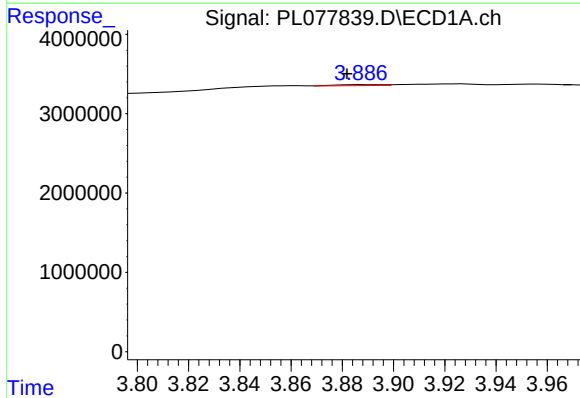


#2 alpha-BHC

R.T.: 3.889 min
Delta R.T.: 0.007 min
Response: 156311
Conc: 0.07 ng/ml

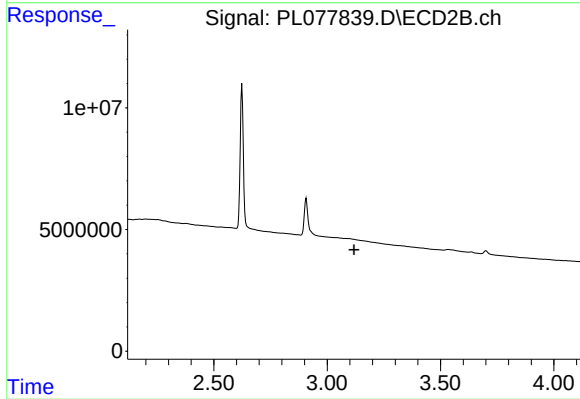

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.119 min
Response: 0
Conc: N.D.

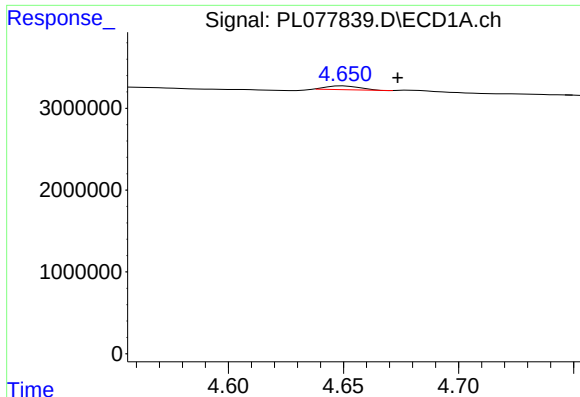

#7 delta-BHC


R.T.: 4.650 min
Delta R.T.: -0.024 min
Response: 469283
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

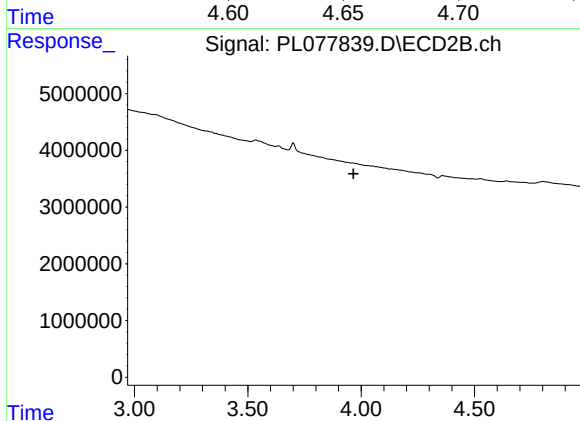


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

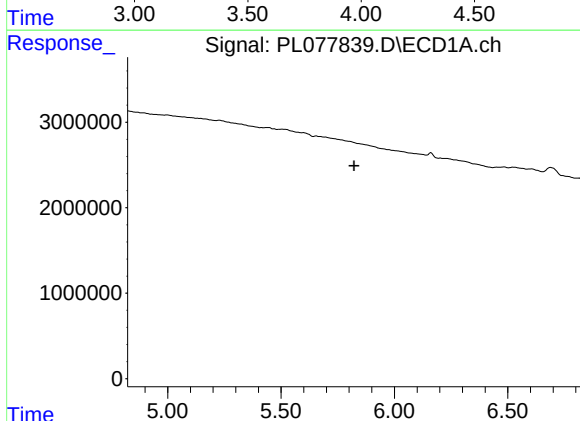


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.823 min
Response: 0
Conc: N.D.

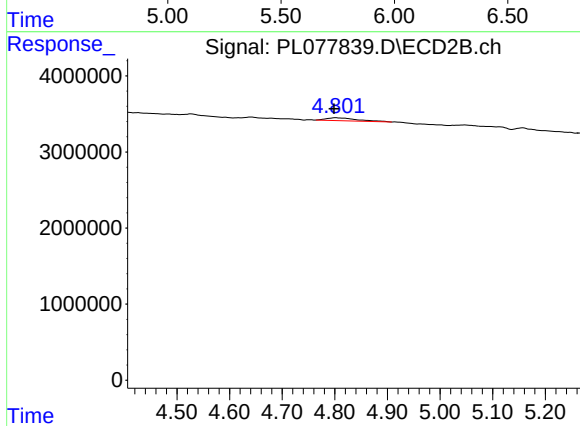

#10 gamma-Chlordane


R.T.: 4.803 min
Delta R.T.: 0.004 min
Response: 1526017
Conc: 0.45 ng/ml

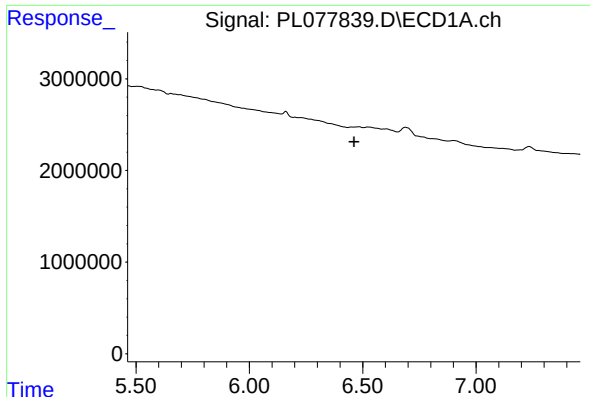

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

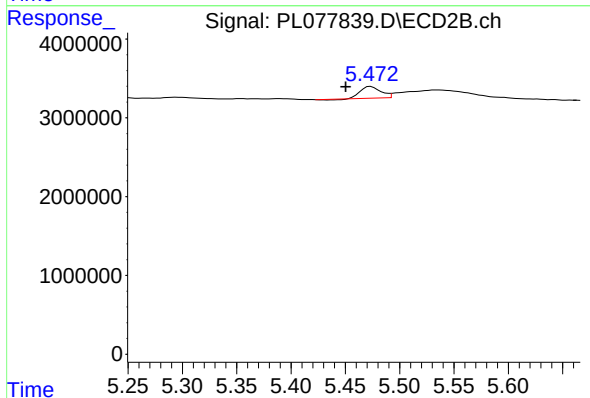


#14 Endrin

R.T.: 5.473 min
Delta R.T.: 0.023 min
Response: 1854345
Conc: 0.65 ng/ml

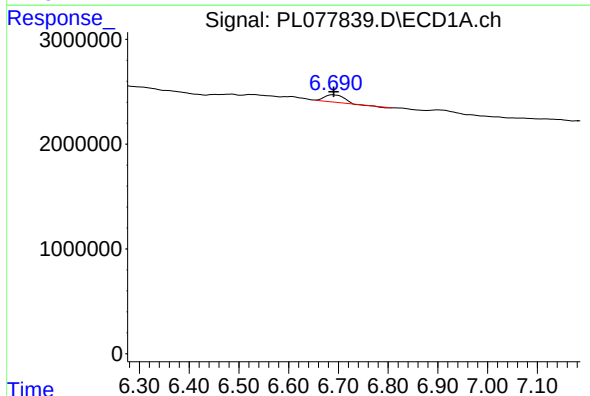


#15 Endosulfan II

R.T.: 6.689 min
Delta R.T.: -0.002 min
Response: 1868633
Conc: 1.35 ng/ml

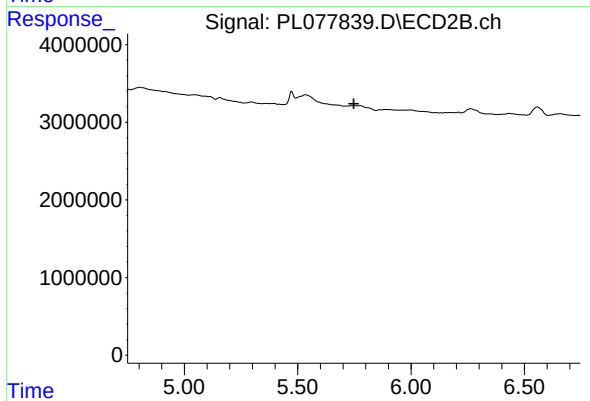

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.747 min
Response: 0
Conc: N.D.

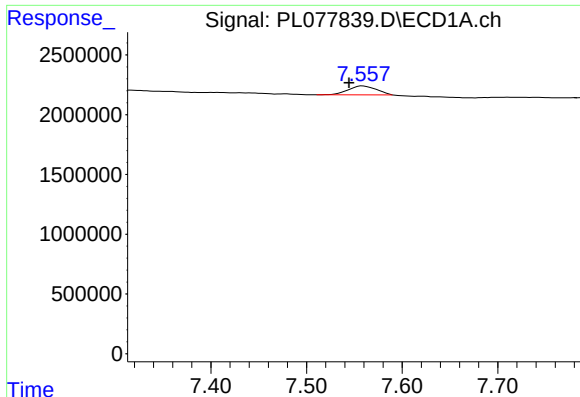

#21 Endrin ketone


R.T.: 7.558 min
Delta R.T.: 0.014 min
Response: 1534135
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

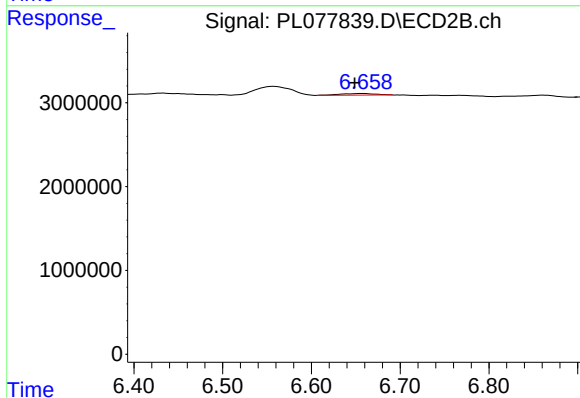


#21 Endrin ketone

R.T.: 6.660 min
Delta R.T.: 0.011 min
Response: 494841
Conc: 0.16 ng/ml

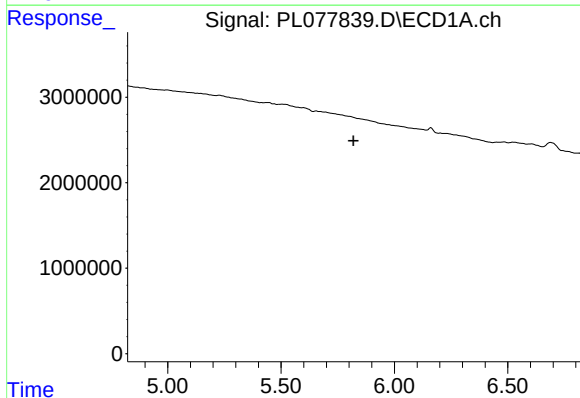


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.820 min
Response: 0
Conc: N.D.

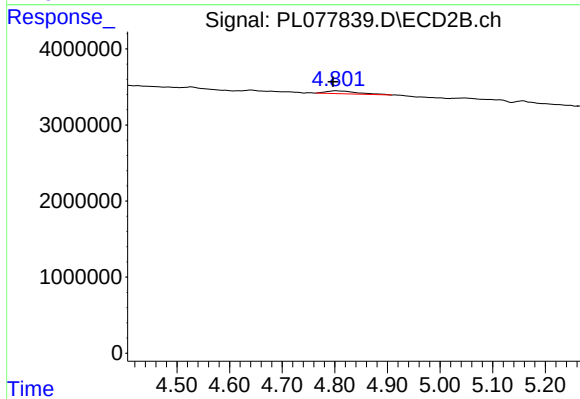

#25 Chlordane-3


R.T.: 4.803 min
Delta R.T.: 0.006 min
Response: 1526017
Conc: 4.44 ng/ml

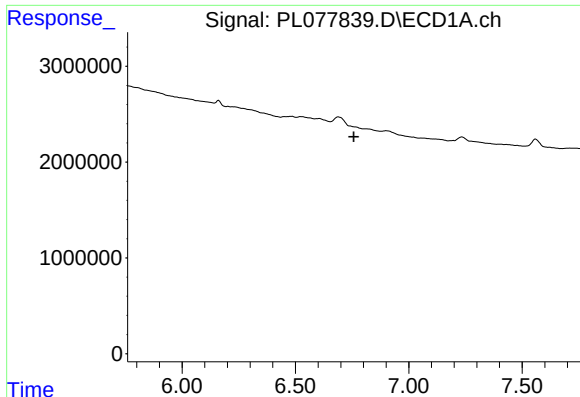

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

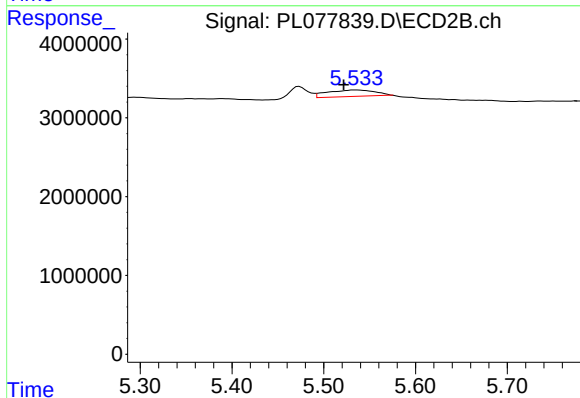


#27 Chlordane-5

R.T.: 5.535 min
Delta R.T.: 0.013 min
Response: 2985602
Conc: 31.73 ng/ml

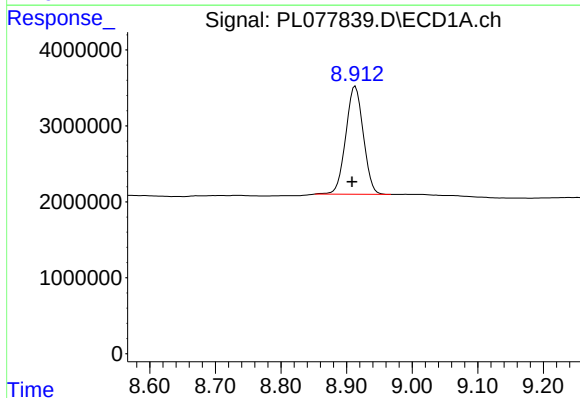

#28 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.005 min
Response: 26449886
Conc: 20.47 ng/ml

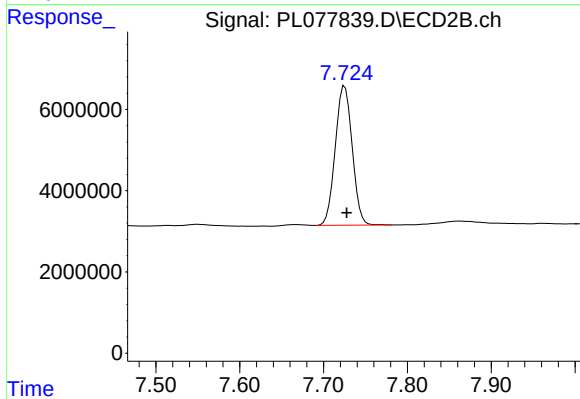

#28 Decachlorobiphenyl

R.T.: 7.725 min
Delta R.T.: -0.002 min
Response: 48152793
Conc: 19.18 ng/ml