

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091922\
 Data File : PL077845.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 14:44
 Operator : AR\AJ
 Sample : IBLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 17:58:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.623	32870061	64956707	20.505	21.880
28)	SA Decachlor...	8.903	7.720	28231809	52317138	21.844	20.842
Target Compounds							
3)	MA gamma-BHC...	4.235f	0.000	18612	0	0.008	N.D. #
5)	MB Aldrin	0.000	4.061	0	1077707	N.D.	0.284 #
6)	B beta-BHC	0.000	3.741	0	171851	N.D.	0.103 #
12)	B 4,4'-DDE	0.000	5.051	0	165394	N.D.	0.051 #
14)	MA Endrin	0.000	5.468f	0	1173658	N.D.	0.412 #
15)	B Endosulfa...	6.707f	0.000	910165	0	0.659	N.D. #
18)	B Endrin al...	0.000	5.934	0	352947	N.D.	0.171 #
21)	B Endrin ke...	7.569f	0.000	399672	0	0.289	N.D. #
23)	Chlordane-1	0.000	3.602	0	720639	N.D.	6.632 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091922\
Data File : PL077845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 14:44
Operator : AR\AJ
Sample : IBLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 17:58:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

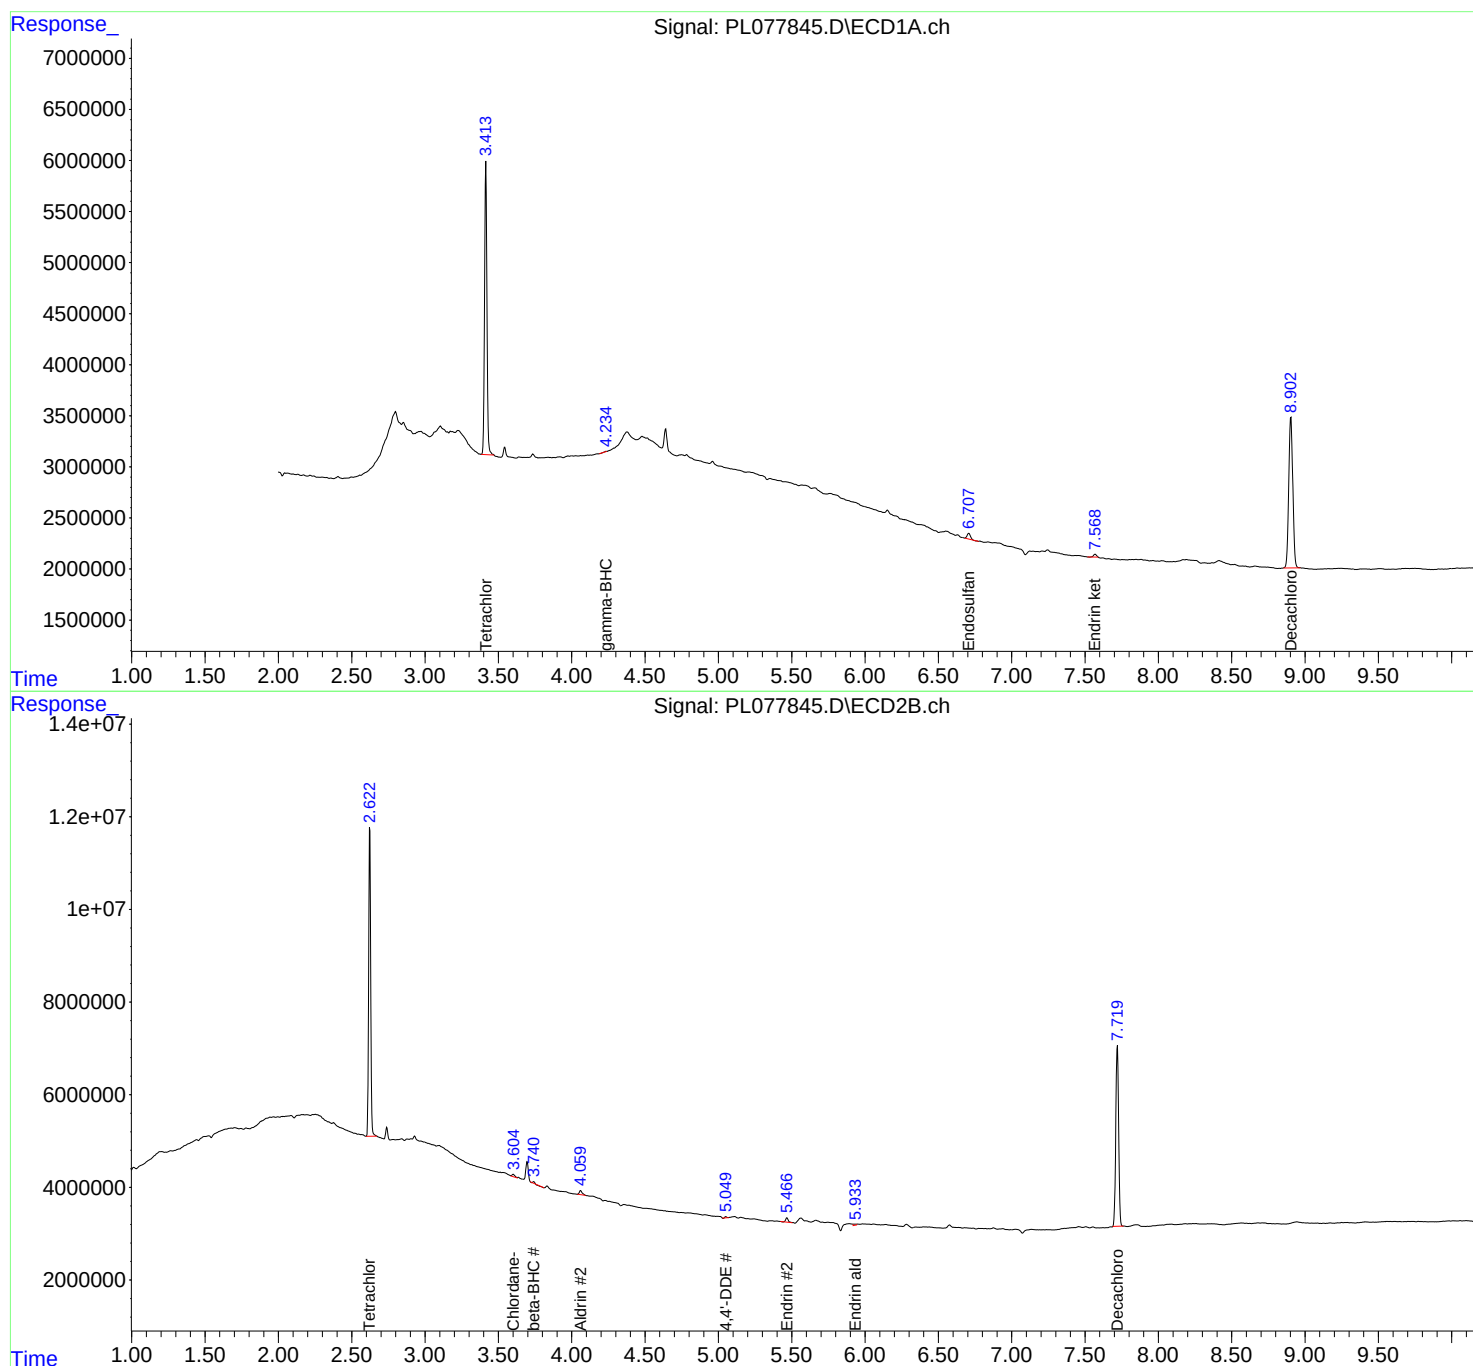


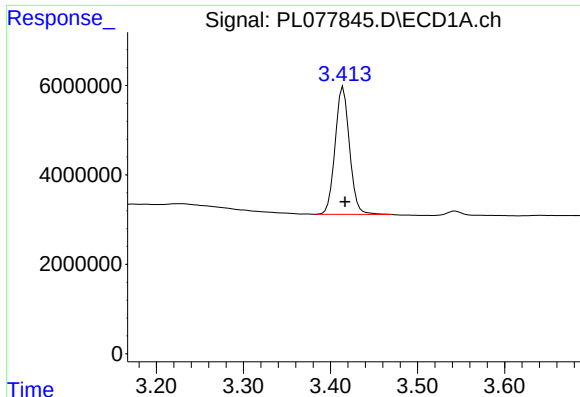

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: -0.002 min
Response: 32870061
Conc: 20.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

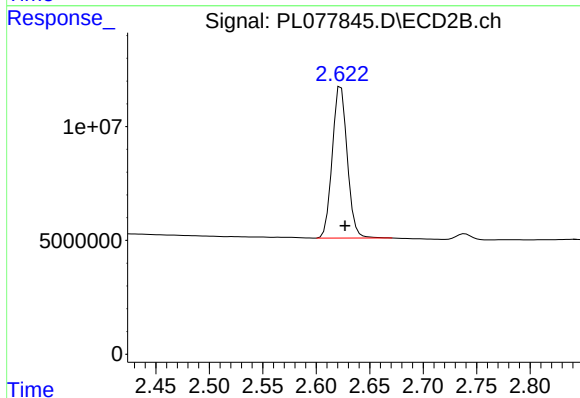


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: -0.004 min
Response: 64956707
Conc: 21.88 ng/ml

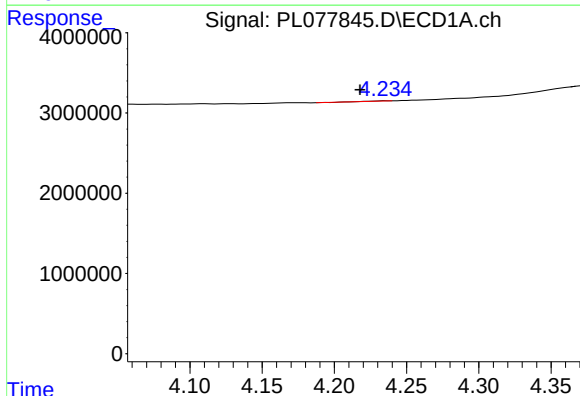


#3 gamma-BHC (Lindane)

R.T.: 4.235 min
Delta R.T.: 0.017 min
Response: 18612
Conc: 0.01 ng/ml

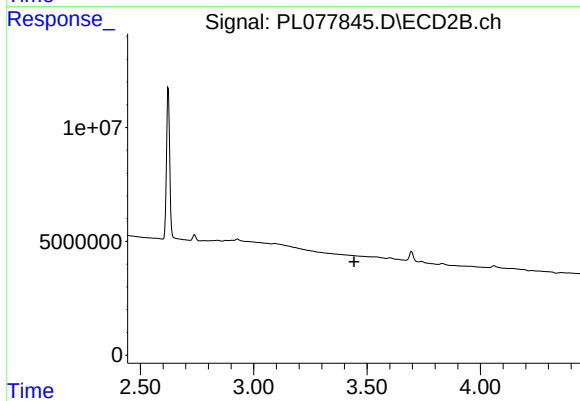

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.443 min
Response: 0
Conc: N.D.

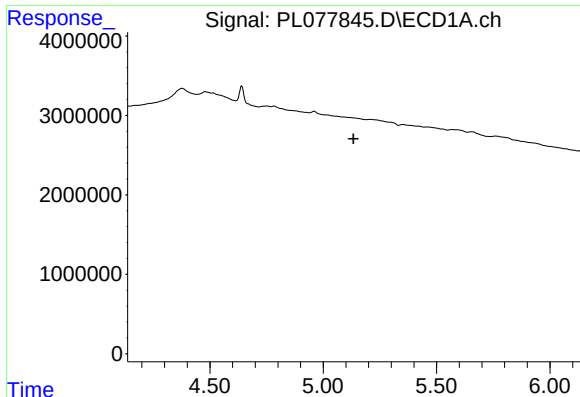

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.134 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

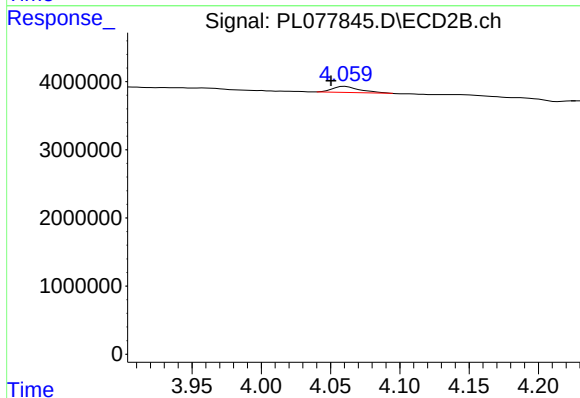


#5 Aldrin

R.T.: 4.061 min
Delta R.T.: 0.010 min
Response: 1077707
Conc: 0.28 ng/ml

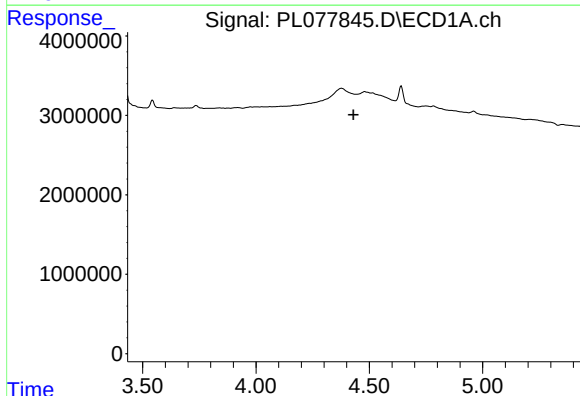


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.430 min
Response: 0
Conc: N.D.

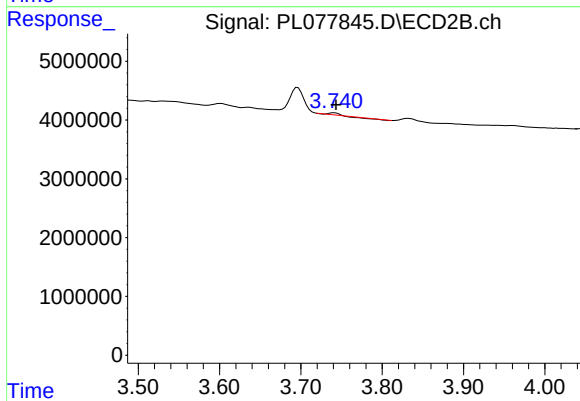

#6 beta-BHC


R.T.: 3.741 min
Delta R.T.: -0.002 min
Response: 171851
Conc: 0.10 ng/ml

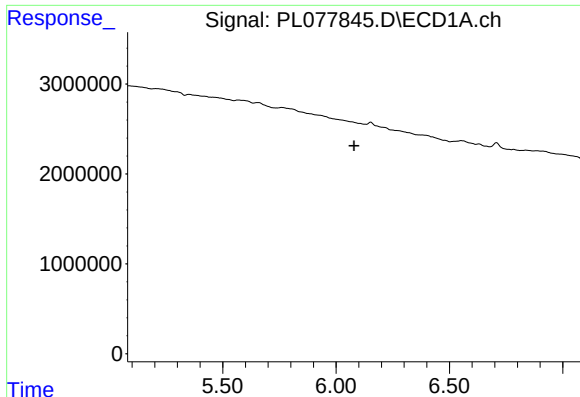

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.080 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

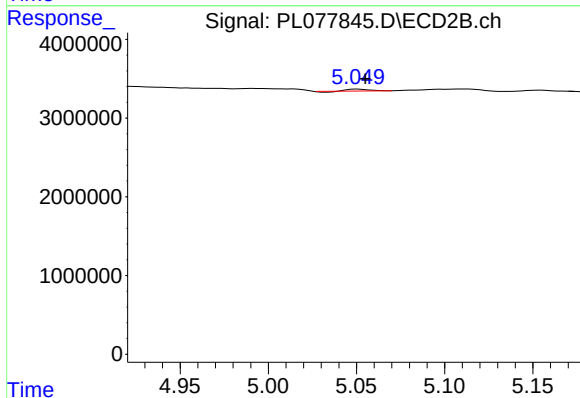


#12 4,4'-DDE

R.T.: 5.051 min
Delta R.T.: -0.004 min
Response: 165394
Conc: 0.05 ng/ml

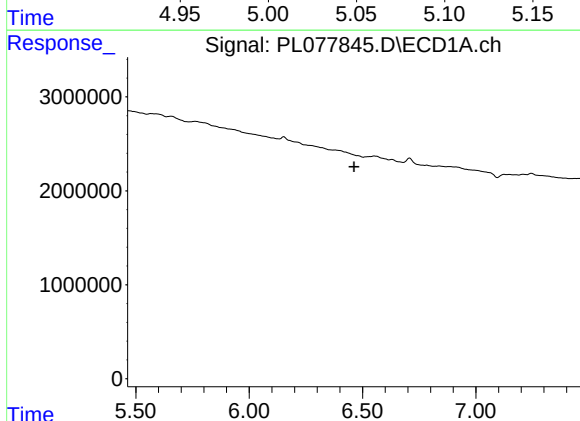


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

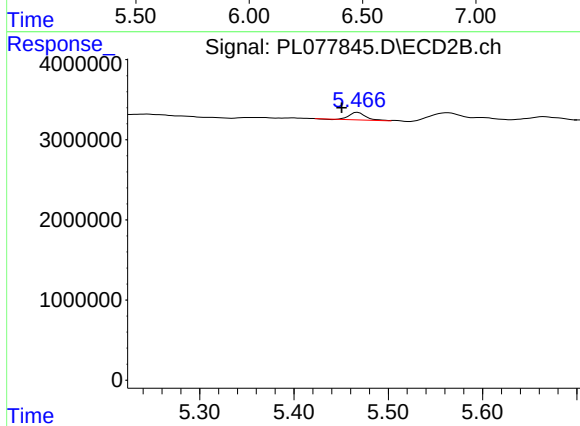

#14 Endrin


R.T.: 5.468 min
Delta R.T.: 0.017 min
Response: 1173658
Conc: 0.41 ng/ml

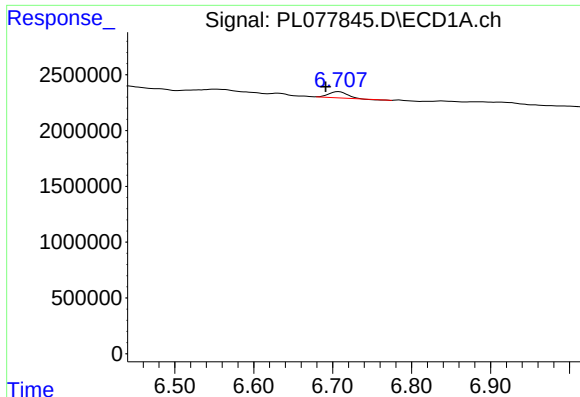

#15 Endosulfan II


R.T.: 6.707 min
Delta R.T.: 0.016 min
Response: 910165
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

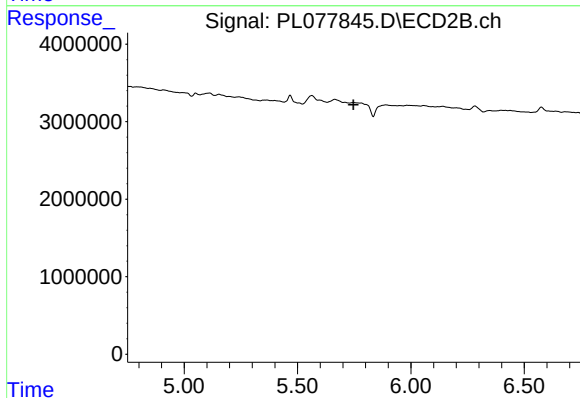


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.747 min
Response: 0
Conc: N.D.

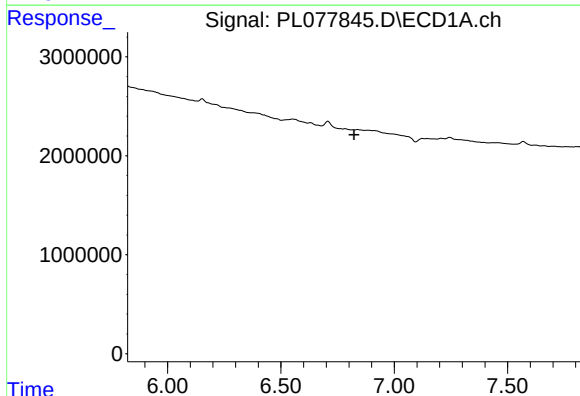


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.823 min
Response: 0
Conc: N.D.

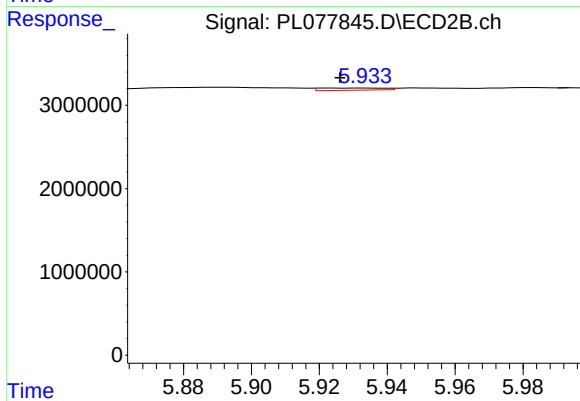

#18 Endrin aldehyde


R.T.: 5.934 min
Delta R.T.: 0.008 min
Response: 352947
Conc: 0.17 ng/ml

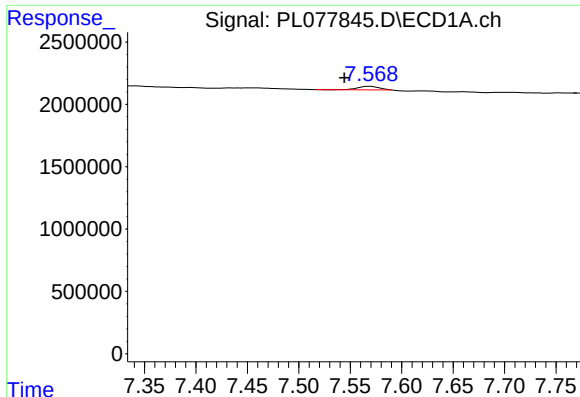

#21 Endrin ketone


R.T.: 7.569 min
Delta R.T.: 0.025 min
Response: 399672
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

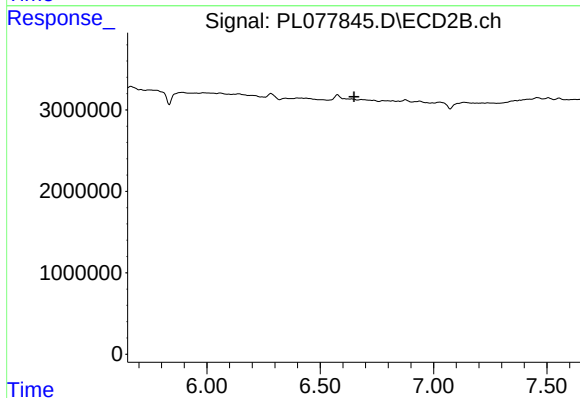


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

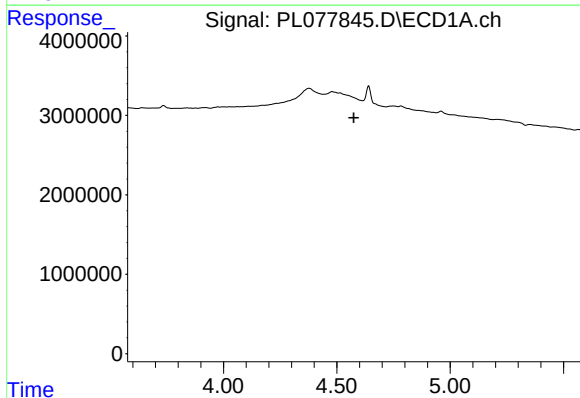


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.575 min
Response: 0
Conc: N.D.

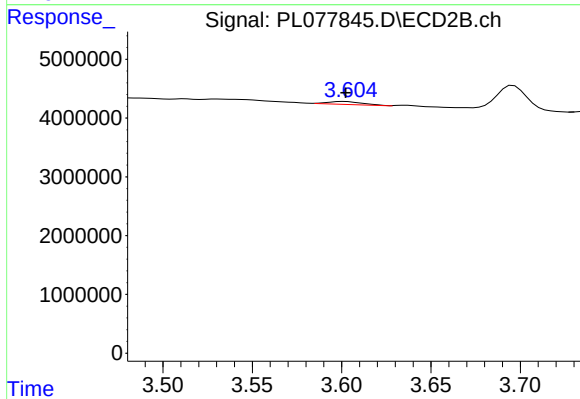

#23 Chlordane-1


R.T.: 3.602 min
Delta R.T.: 0.000 min
Response: 720639
Conc: 6.63 ng/ml

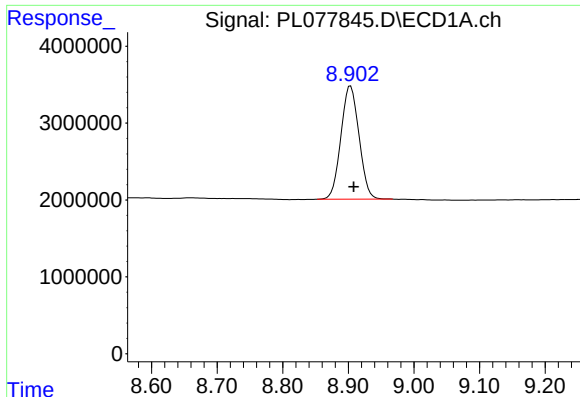

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: -0.005 min
Response: 28231809
Conc: 21.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

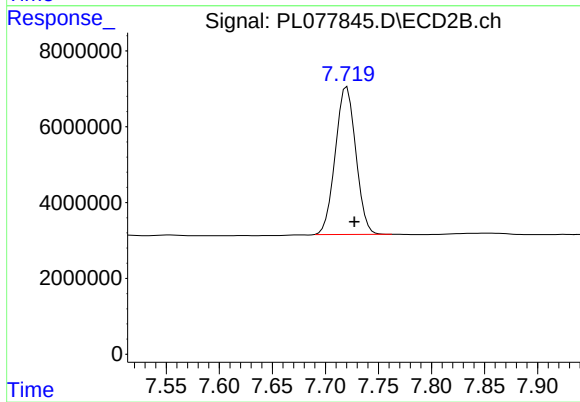

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: -0.007 min
Response: 52317138
Conc: 20.84 ng/ml