

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
 Data File : PL085413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 23:43
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 10:04:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 10:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	2.649	241.5E6	135.0E6	75.124	76.341
28)	SA Decachlor...	8.941	7.825	228.7E6	139.6E6	70.341	71.961
Target Compounds							
23)	Chlordane-1	4.576	3.647	109.2E6	40829315	759.272	766.635
24)	Chlordane-2	5.109	4.228	114.4E6	52298577	731.074	696.843
25)	Chlordane-3	5.822	4.859	472.3E6	161.7E6	760.757	788.856
26)	Chlordane-4	5.905	4.922	569.4E6	175.6E6	751.673	781.051
27)	Chlordane-5	6.755	5.595	97098785	46866459	754.138	748.075


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
Data File : PL085413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 23:43
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 10:04:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 10:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

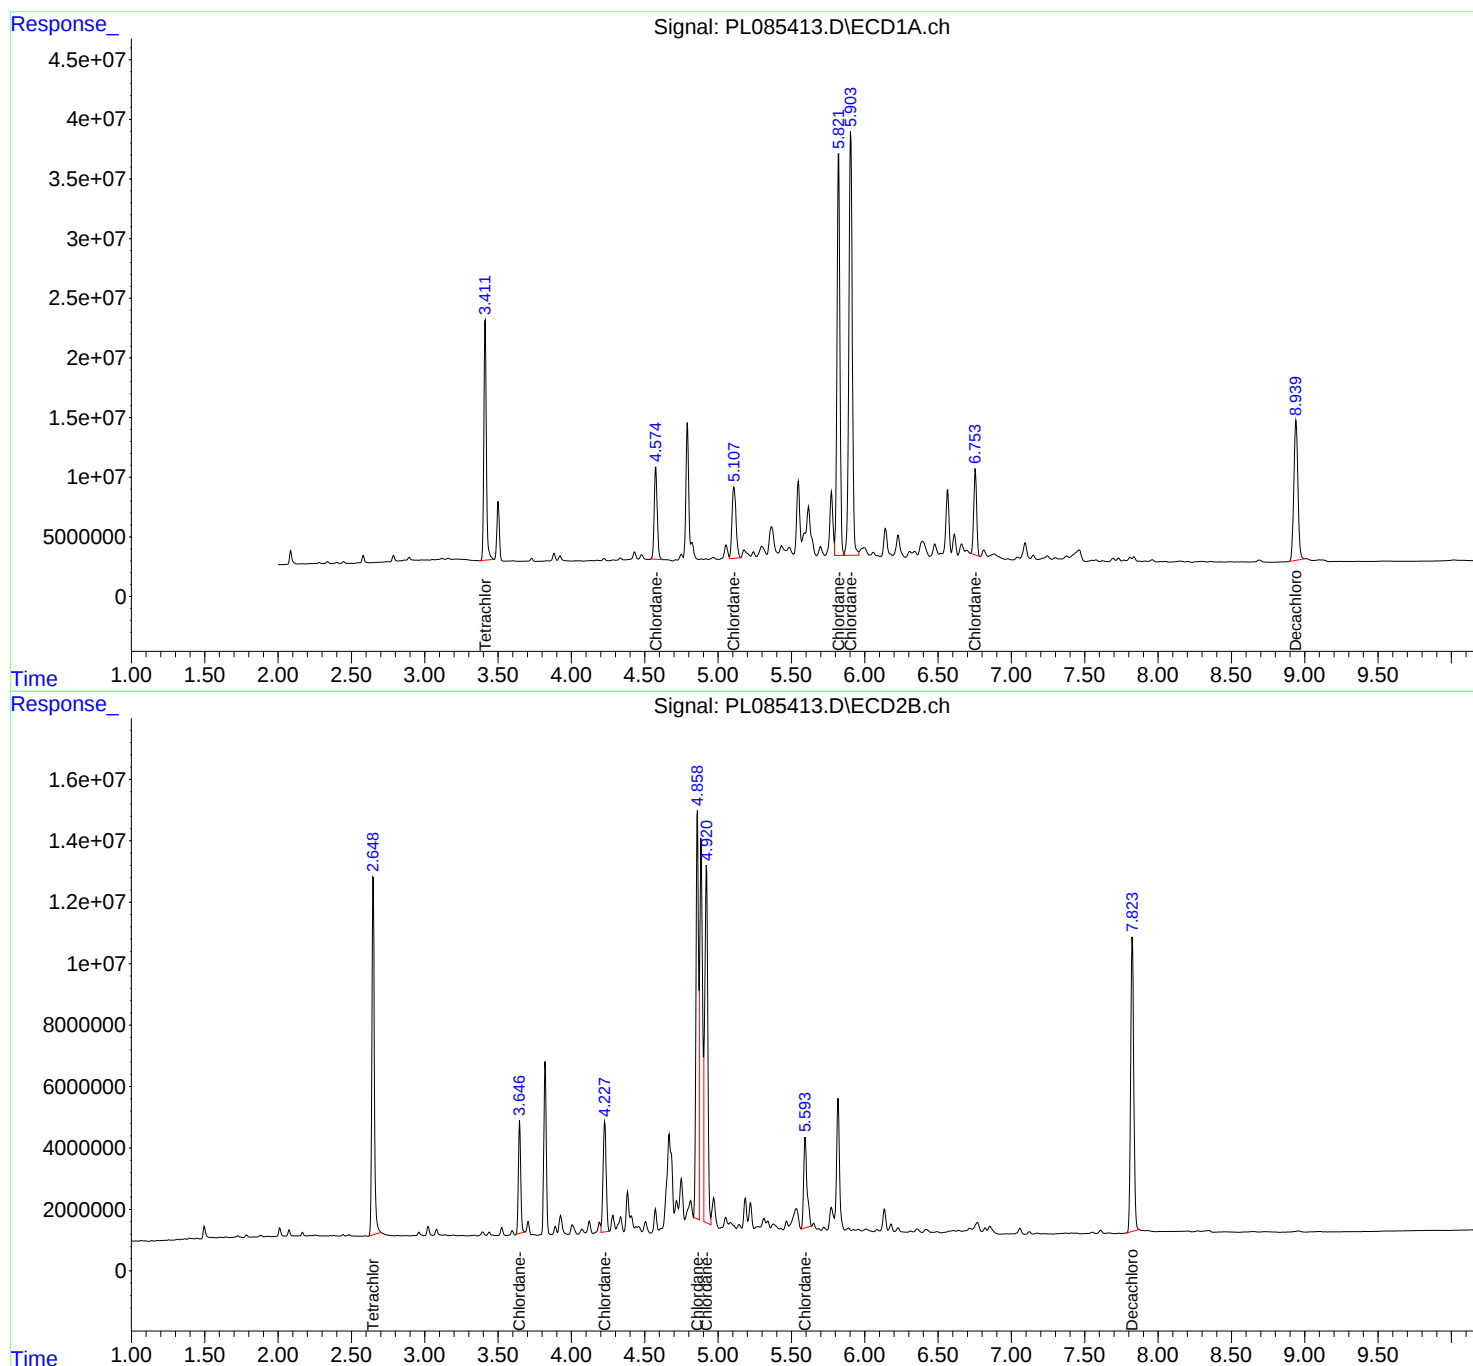


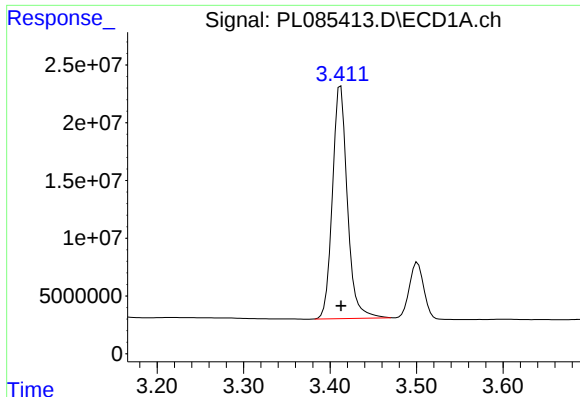

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 241490438
Conc: 75.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

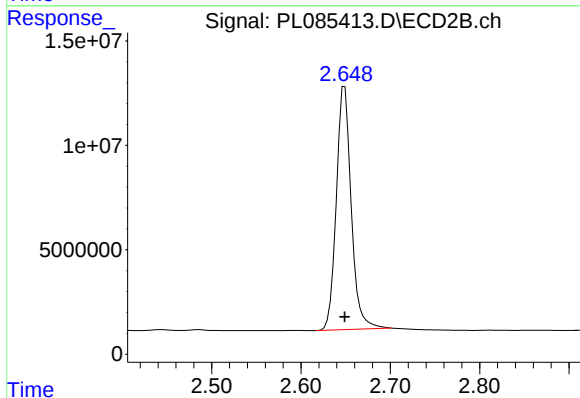


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 135028910
Conc: 76.34 ng/ml

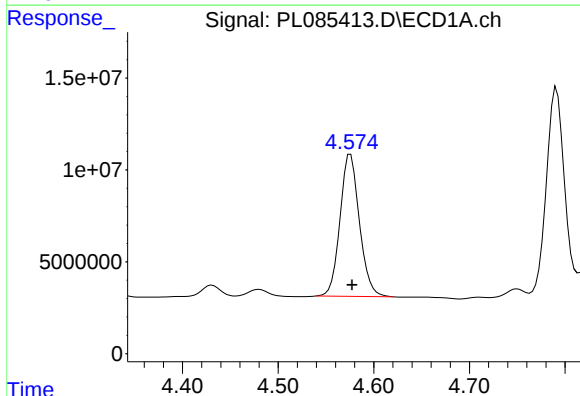


#23 Chlordane-1

R.T.: 4.576 min
Delta R.T.: -0.002 min
Response: 109158864
Conc: 759.27 ng/ml

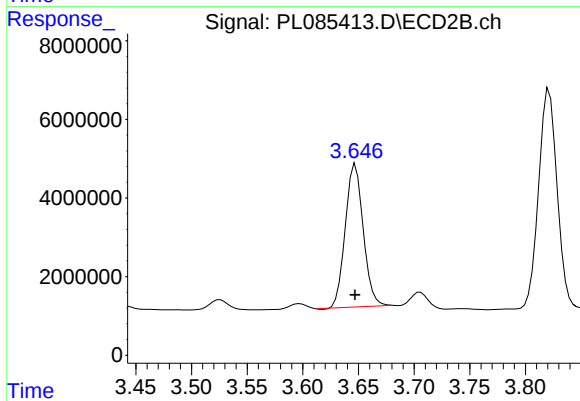

#23 Chlordane-1


R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 40829315
Conc: 766.63 ng/ml

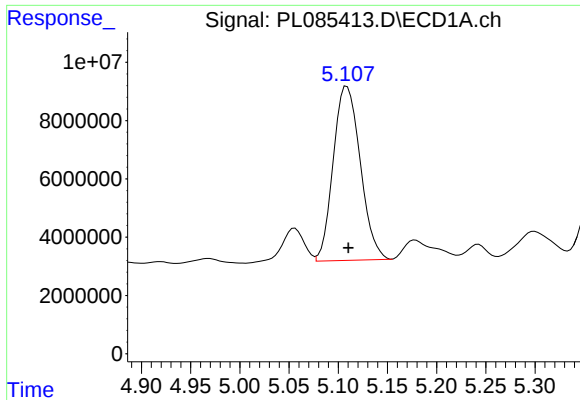

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: -0.002 min
Response: 114354166
Conc: 731.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

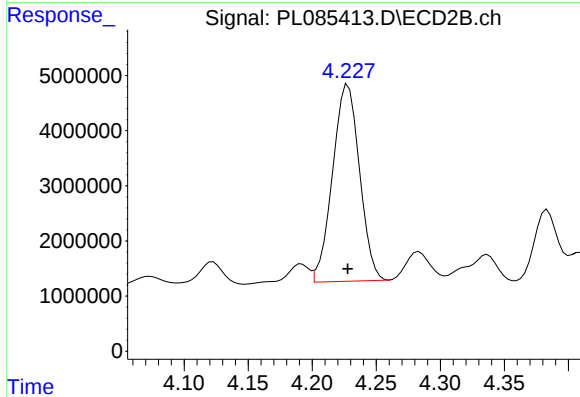


#24 Chlordane-2

R.T.: 4.228 min
Delta R.T.: 0.000 min
Response: 52298577
Conc: 696.84 ng/ml

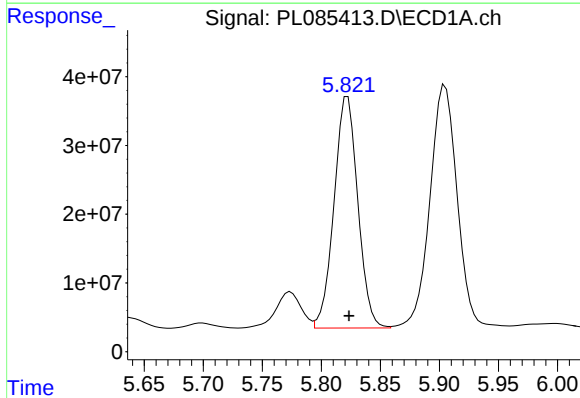


#25 Chlordane-3

R.T.: 5.822 min
Delta R.T.: -0.001 min
Response: 472331977
Conc: 760.76 ng/ml

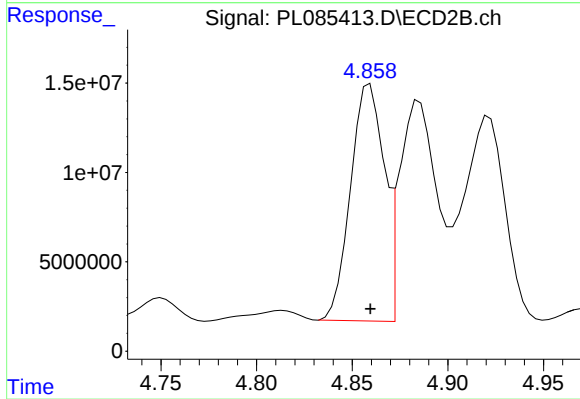

#25 Chlordane-3


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 161697842
Conc: 788.86 ng/ml

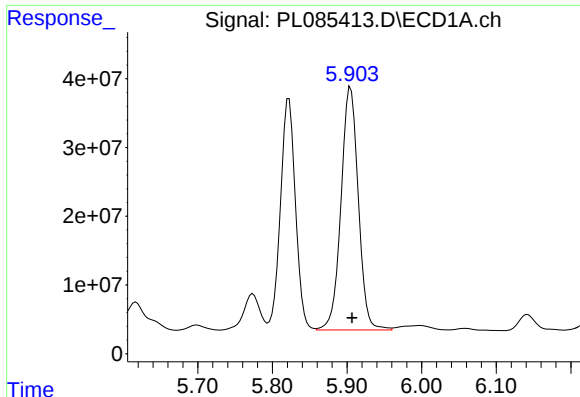

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: -0.002 min
Response: 569409843
Conc: 751.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

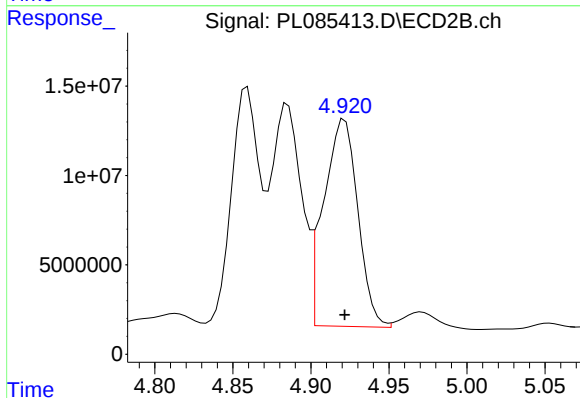


#26 Chlordane-4

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 175584780
Conc: 781.05 ng/ml

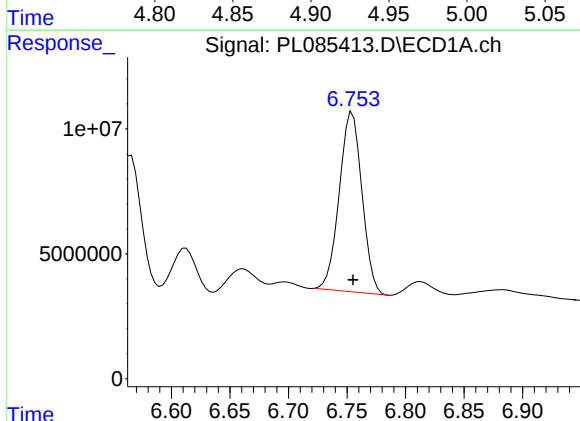


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 97098785
Conc: 754.14 ng/ml

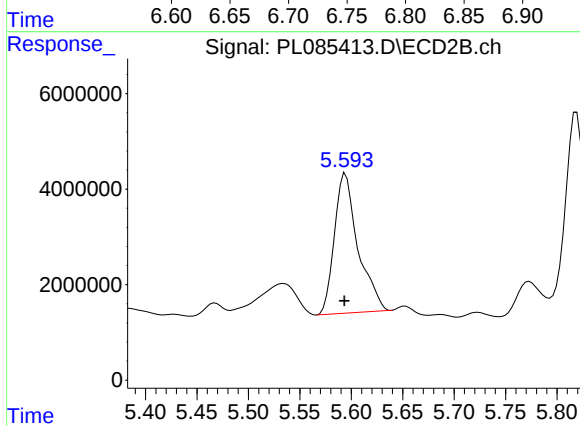

#27 Chlordane-5


R.T.: 5.595 min
Delta R.T.: 0.001 min
Response: 46866459
Conc: 748.07 ng/ml

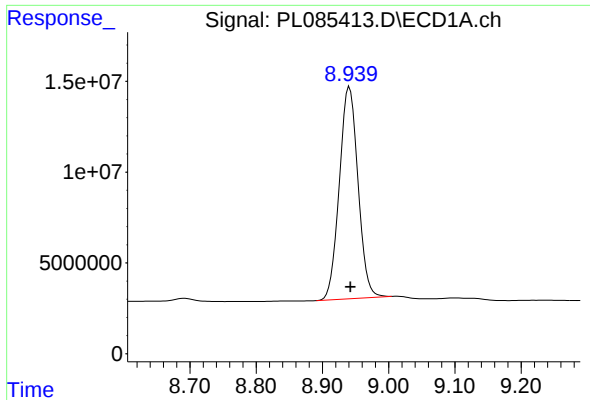

#28 Decachlorobiphenyl

R.T.: 8.941 min
Delta R.T.: -0.002 min
Response: 228659432
Conc: 70.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

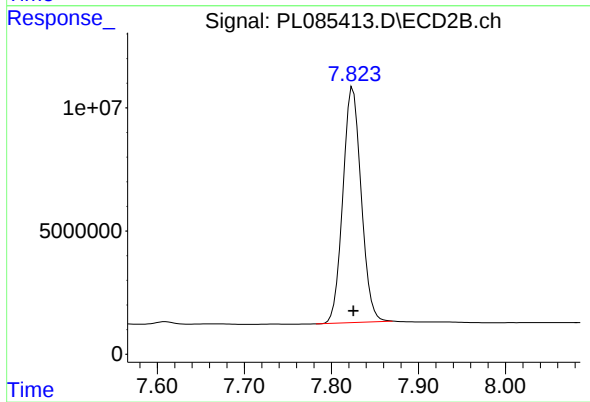

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 139562809
Conc: 71.96 ng/ml