

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
 Data File : PL085406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 22:05
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 06:52:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 06:49:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.415	2.650	61924908	28231695	18.593	18.558
28) SA Decachlor...	8.942	7.825	67593000	38442278	19.858	19.636
Target Compounds						
9) A Endosulfan I	5.950	4.975	39477703	18952110	9.577	10.393
10) B gamma-Chl...	5.822	4.859	43391860	19517536	9.894	9.203
12) B 4,4'-DDE	6.083	5.122	75509763	37429462	18.927	18.492
13) MA Dieldrin	6.227	5.242	80739354	39690140	18.613	18.147
19) B Endosulfa...	7.045	6.222	71004838	35301400	19.420	18.771
20) A Methoxychlor	7.402	6.518	189.6E6	100.5E6	86.508	94.715
21) B Endrin ke...	7.528	6.726	75207352	45660639	18.527	18.286



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
Data File : PL085406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 22:05
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 06:52:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 06:49:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

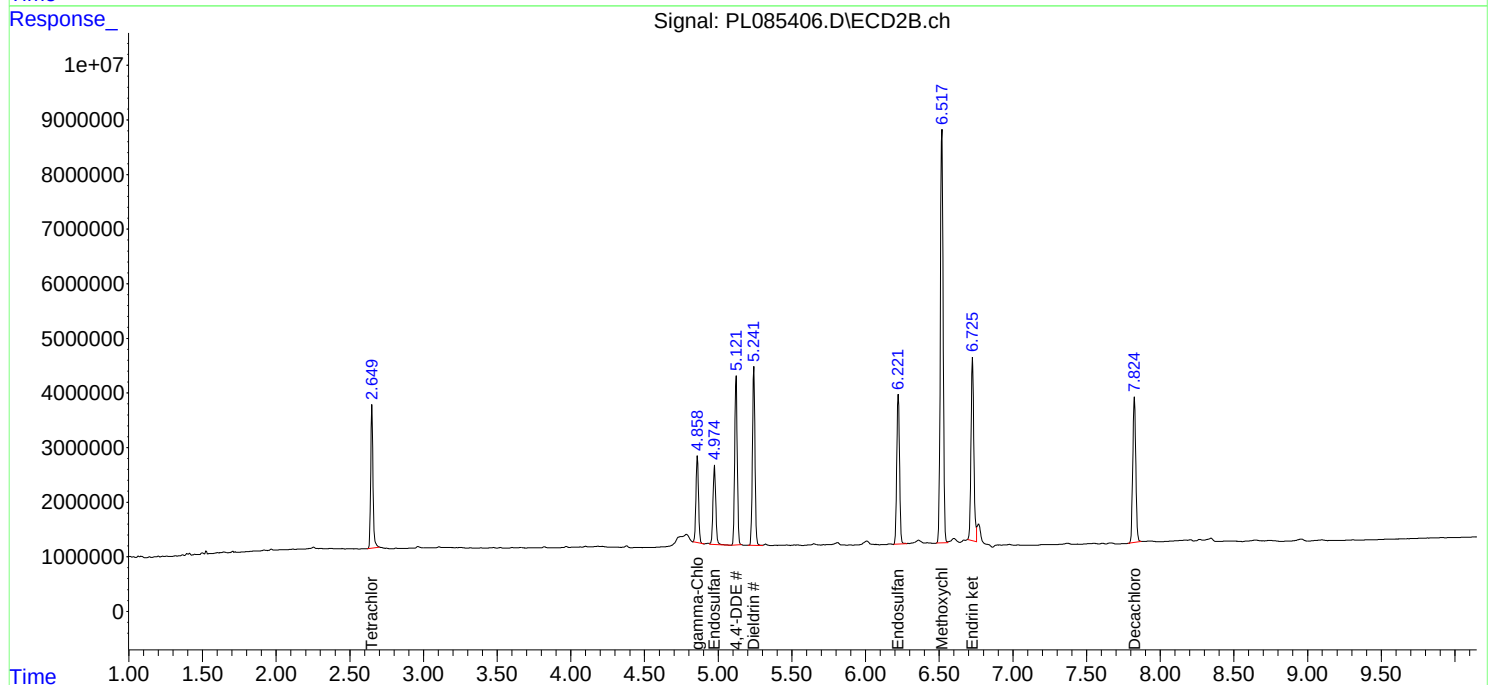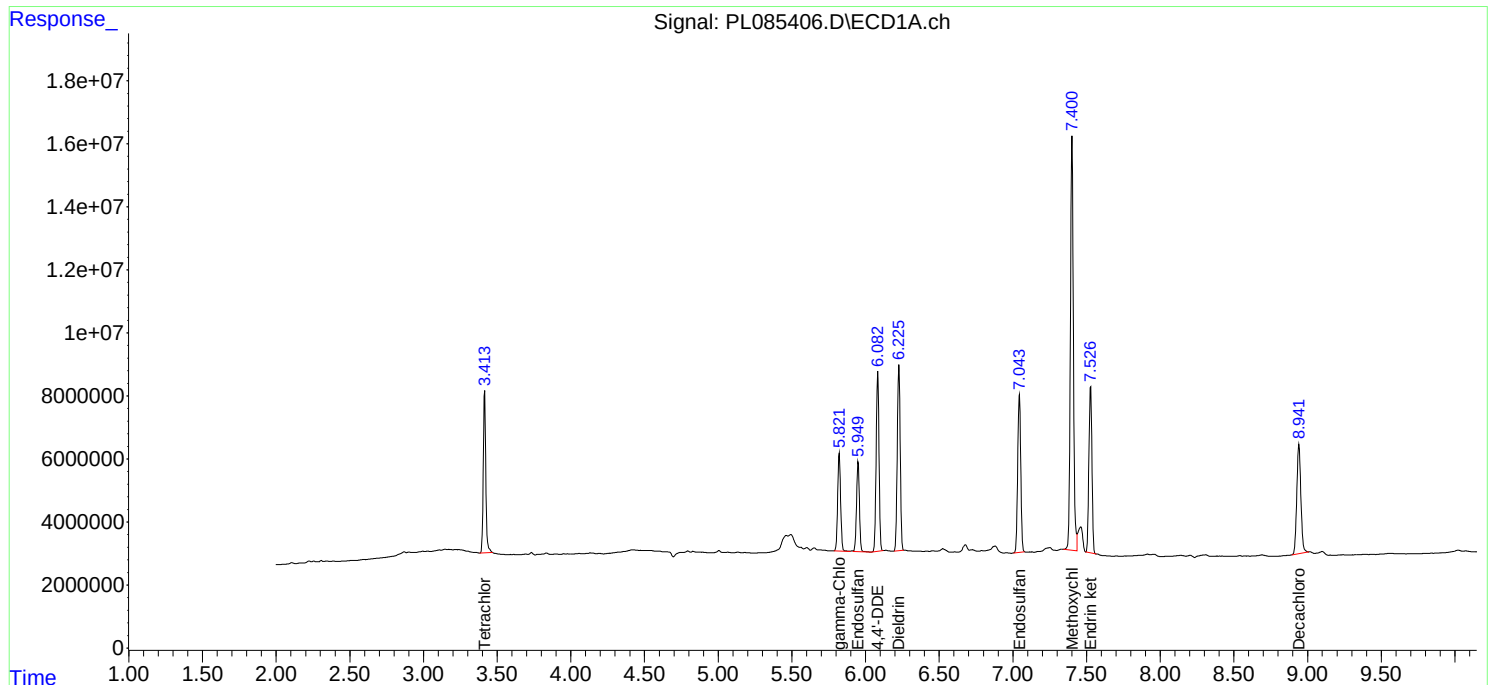


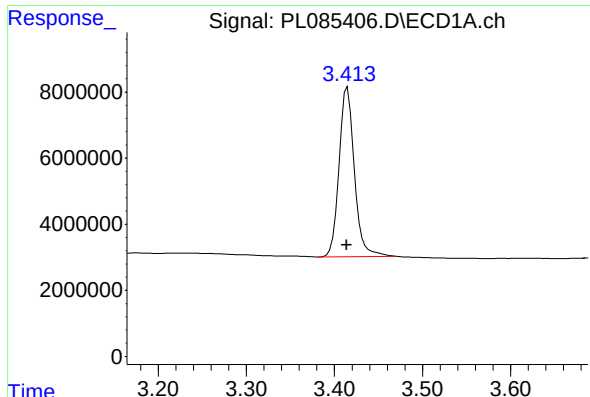

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 61924908
Conc: 18.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

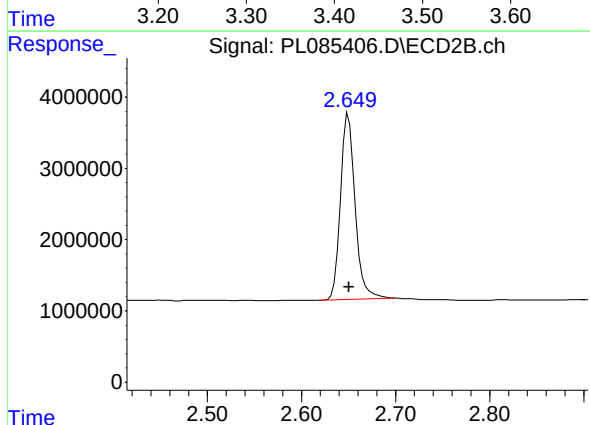


#1 Tetrachloro-m-xylene

R.T.: 2.650 min
Delta R.T.: 0.000 min
Response: 28231695
Conc: 18.56 ng/ml

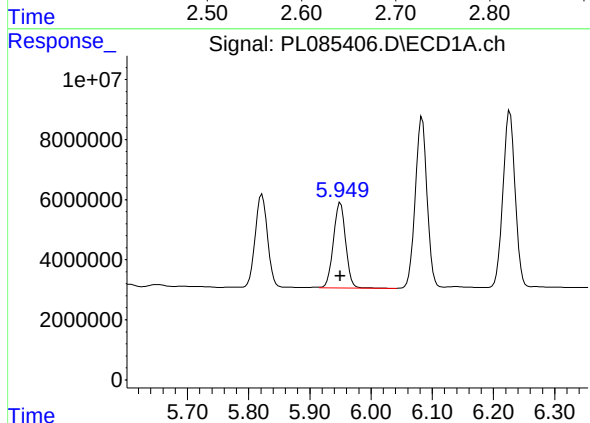


#9 Endosulfan I

R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 39477703
Conc: 9.58 ng/ml

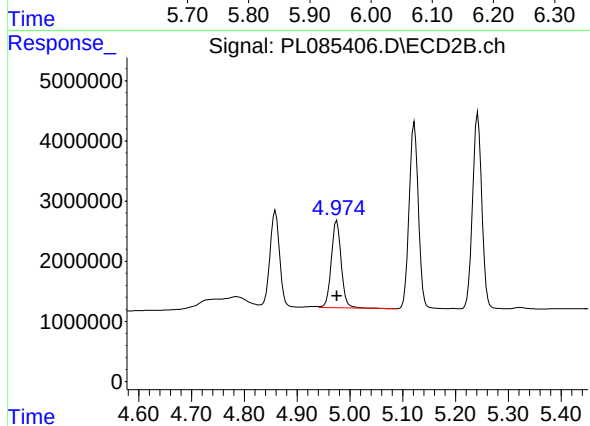

#9 Endosulfan I


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 18952110
Conc: 10.39 ng/ml

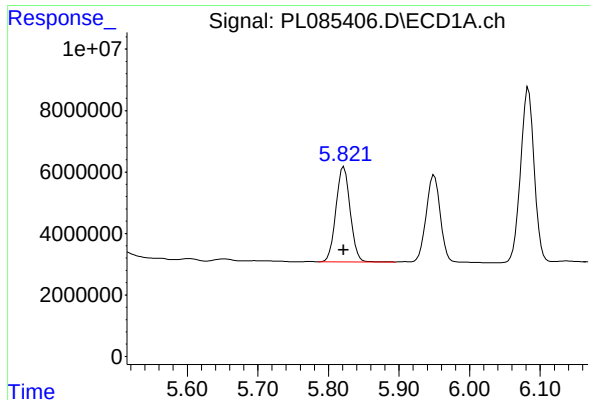

#10 gamma-Chlordane


R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 43391860
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

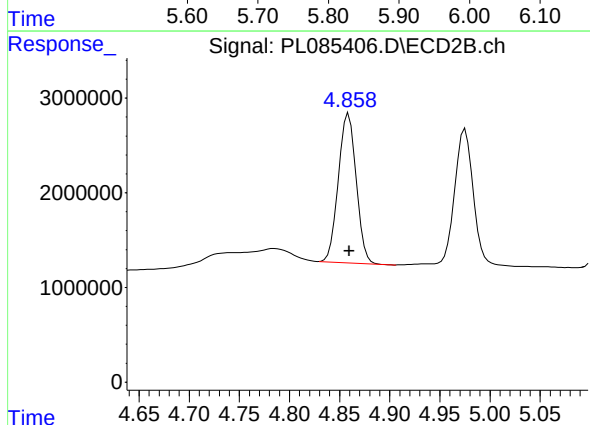


#10 gamma-Chlordane

R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 19517536
Conc: 9.20 ng/ml

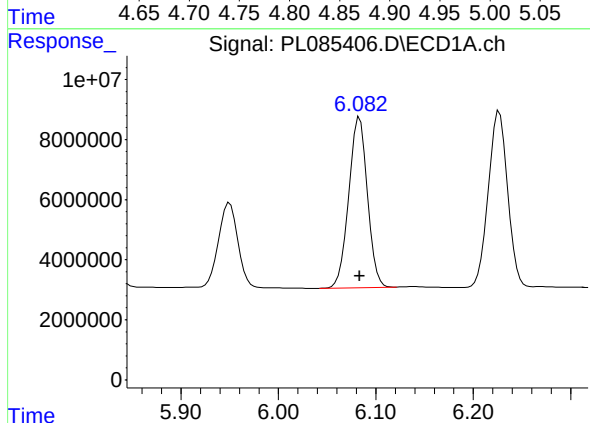


#12 4,4'-DDE

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 75509763
Conc: 18.93 ng/ml

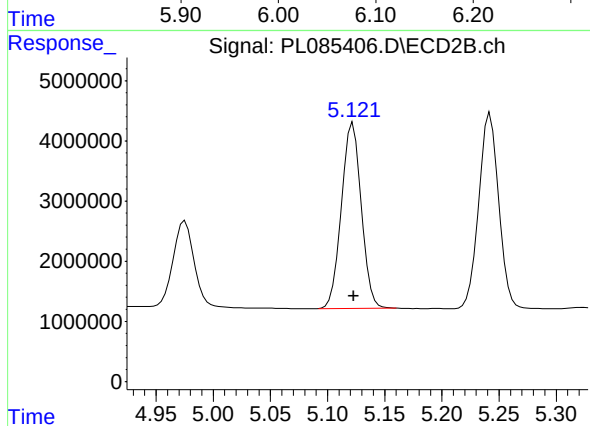

#12 4,4'-DDE


R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 37429462
Conc: 18.49 ng/ml

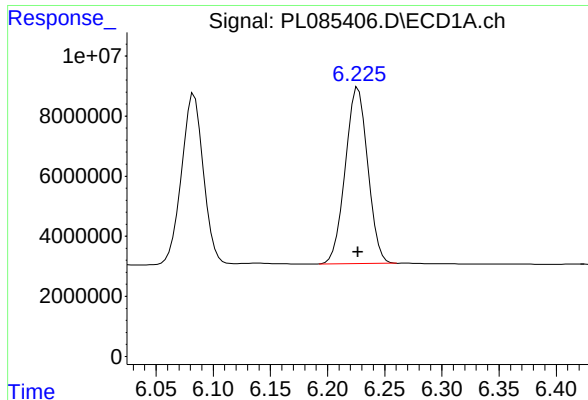

#13 Dieldrin


R.T.: 6.227 min
Delta R.T.: 0.000 min
Response: 80739354
Conc: 18.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

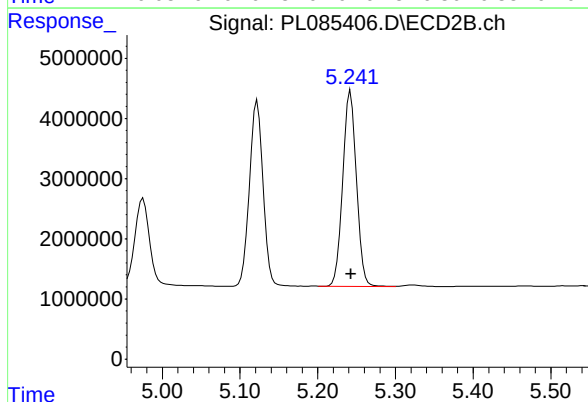


#13 Dieldrin

R.T.: 5.242 min
Delta R.T.: 0.000 min
Response: 39690140
Conc: 18.15 ng/ml

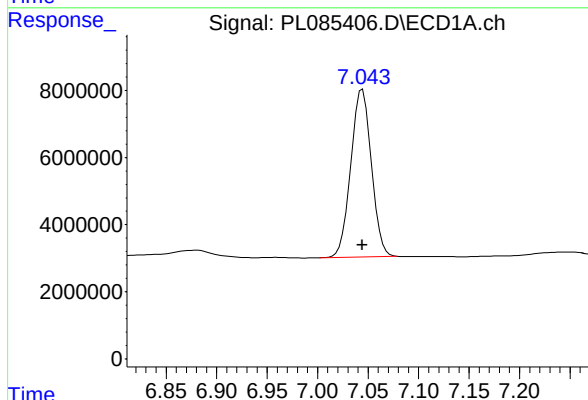


#19 Endosulfan Sulfate

R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 71004838
Conc: 19.42 ng/ml

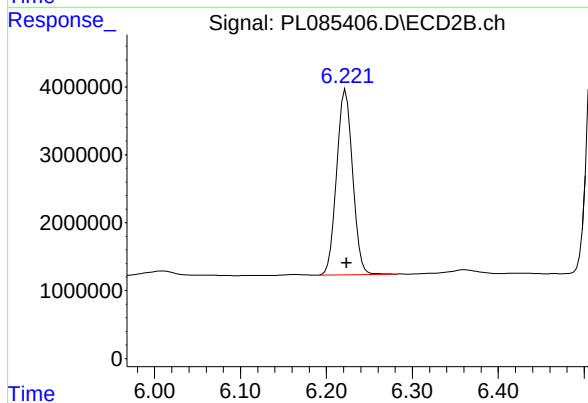

#19 Endosulfan Sulfate


R.T.: 6.222 min
Delta R.T.: 0.000 min
Response: 35301400
Conc: 18.77 ng/ml

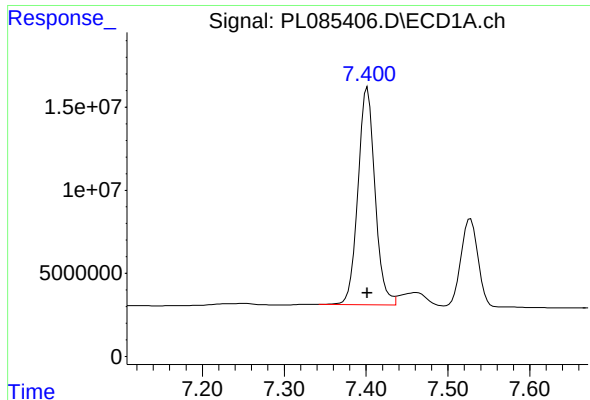

#20 Methoxychlor


R.T.: 7.402 min
Delta R.T.: 0.000 min
Response: 189587213
Conc: 86.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

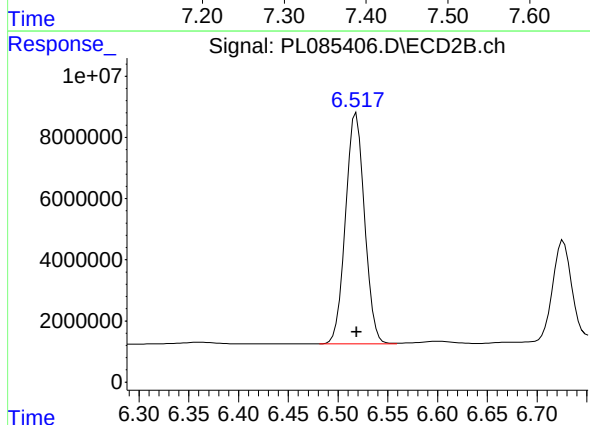


#20 Methoxychlor

R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 100471565
Conc: 94.71 ng/ml

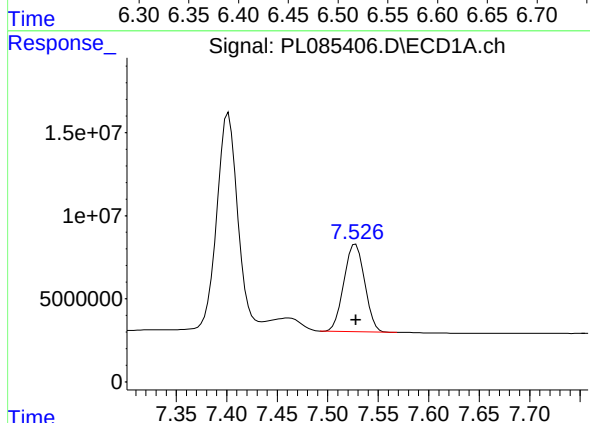


#21 Endrin ketone

R.T.: 7.528 min
Delta R.T.: 0.000 min
Response: 75207352
Conc: 18.53 ng/ml

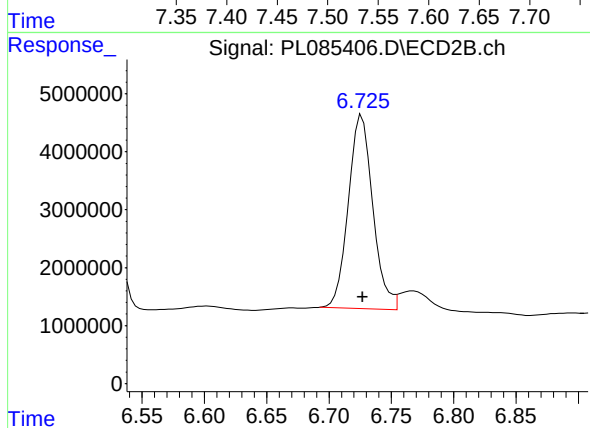

#21 Endrin ketone


R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 45660639
Conc: 18.29 ng/ml

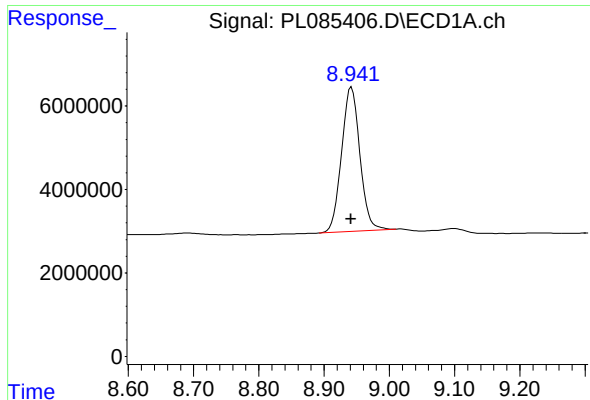

#28 Decachlorobiphenyl

R.T.: 8.942 min
Delta R.T.: 0.000 min
Response: 67593000
Conc: 19.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

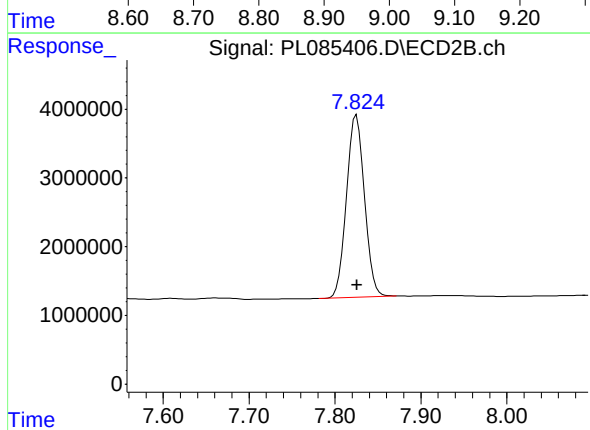

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 38442278
Conc: 19.64 ng/ml