

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
 Data File : PL085413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 23:43
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 10:18:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 10:17:57 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.412	2.649	241.5E6	135.0E6	75.331	75.570
28) SA Decachlor...	8.941	7.825	228.7E6	139.6E6	73.876	74.257
Target Compounds						
23) Chlordane-1	4.576	3.647	109.2E6	40829315	757.264	755.053
24) Chlordane-2	5.109	4.228	114.4E6	52298577	750.563	734.518
25) Chlordane-3	5.822	4.859	472.3E6	161.7E6	752.662	762.467
26) Chlordane-4	5.905	4.922	569.4E6	175.6E6	750.784	759.726
27) Chlordane-5	6.755	5.595	97098785	46866459	754.533	751.973



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
Data File : PL085413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 23:43
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 10:18:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 10:17:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

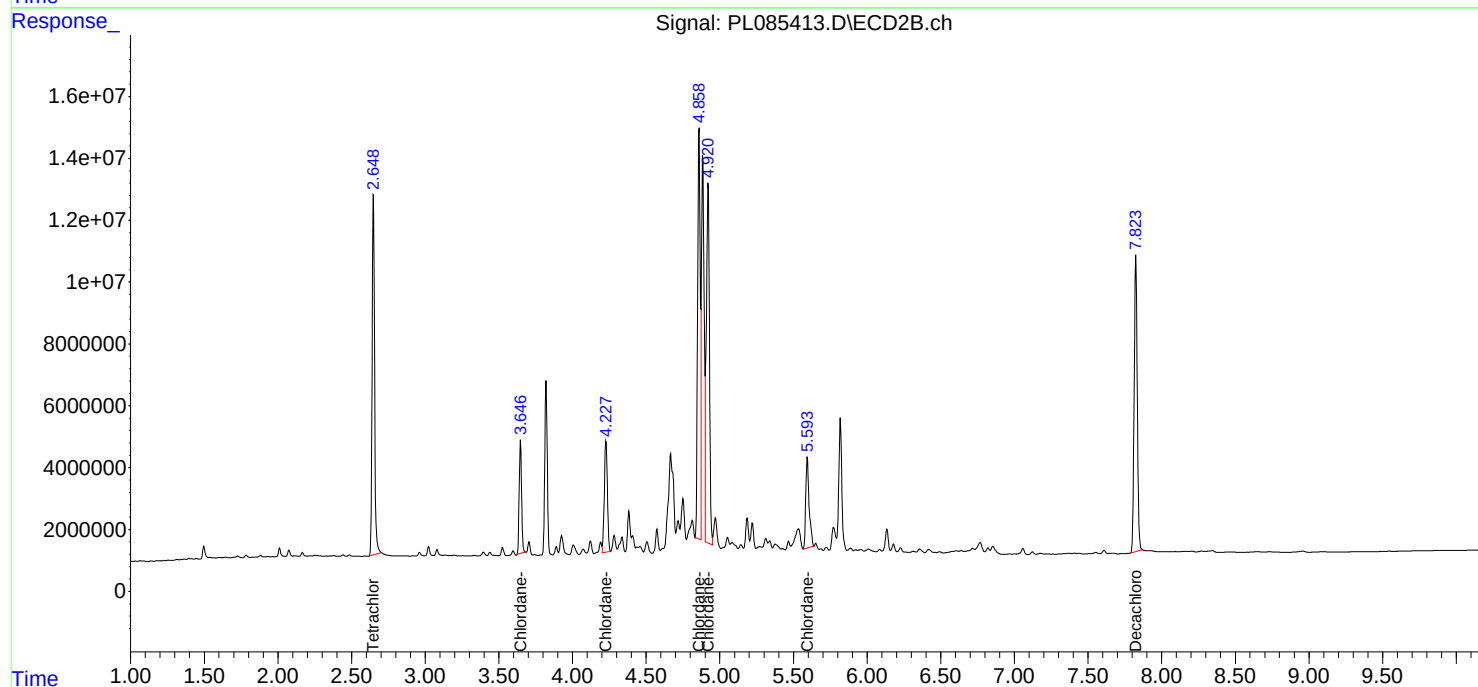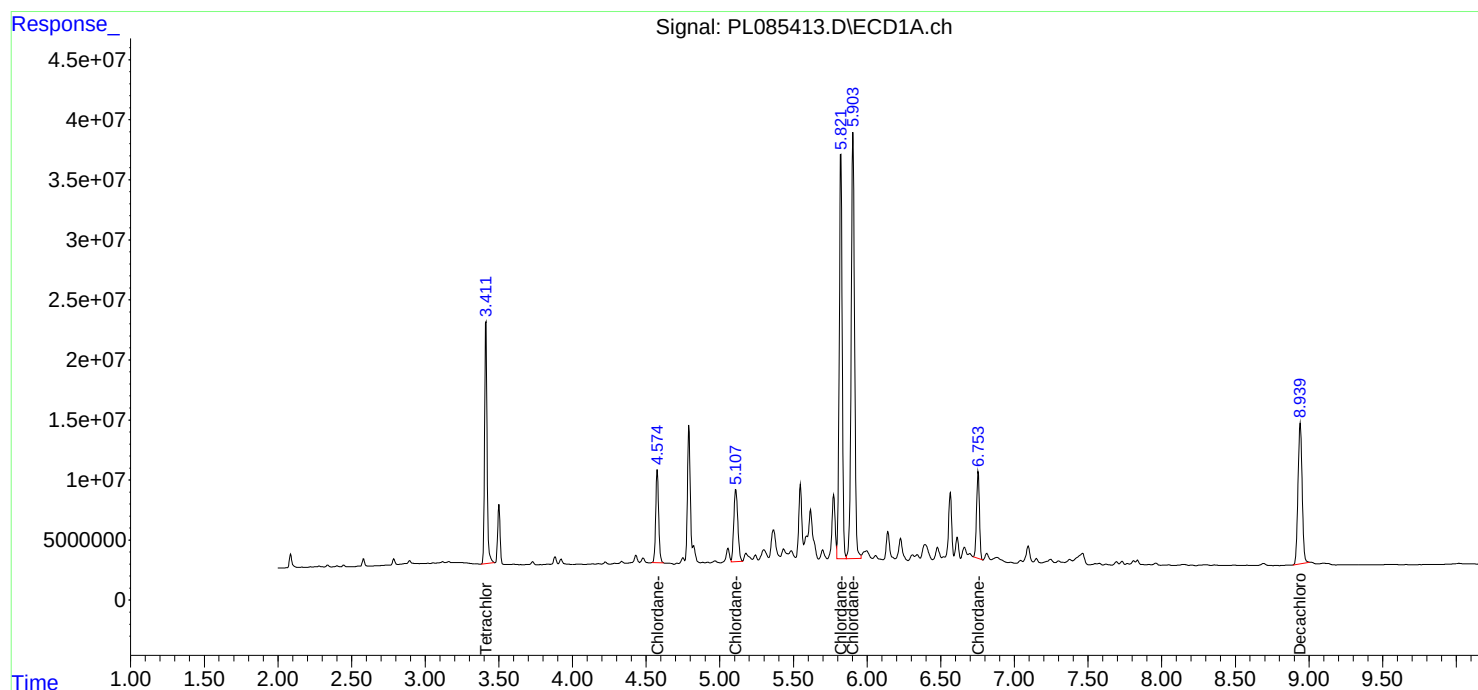


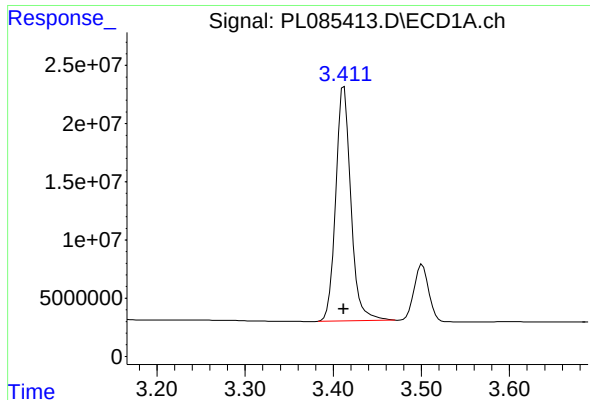

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 241490438
Conc: 75.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

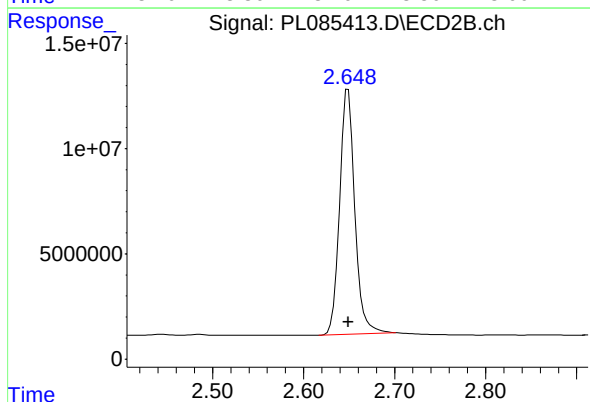


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 135028910
Conc: 75.57 ng/ml

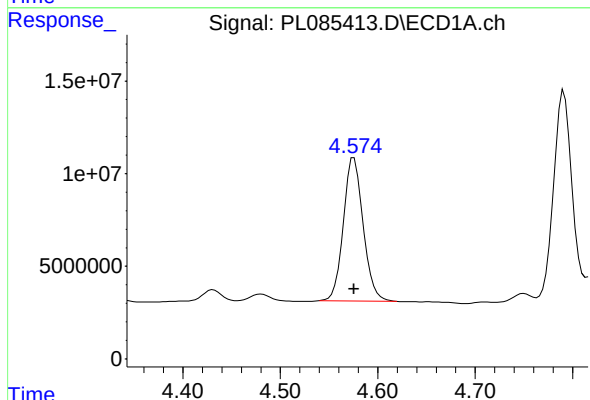


#23 Chlordane-1

R.T.: 4.576 min
Delta R.T.: 0.000 min
Response: 109158864
Conc: 757.26 ng/ml

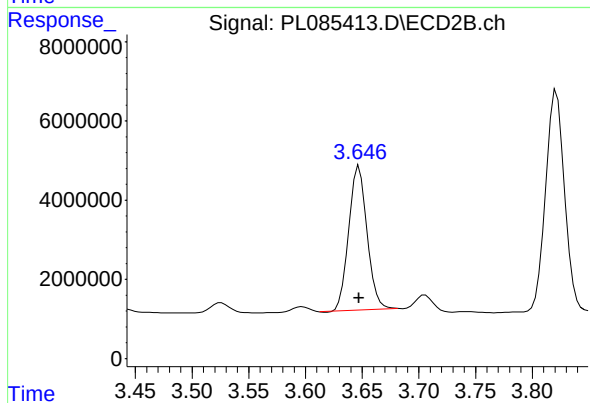

#23 Chlordane-1


R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 40829315
Conc: 755.05 ng/ml

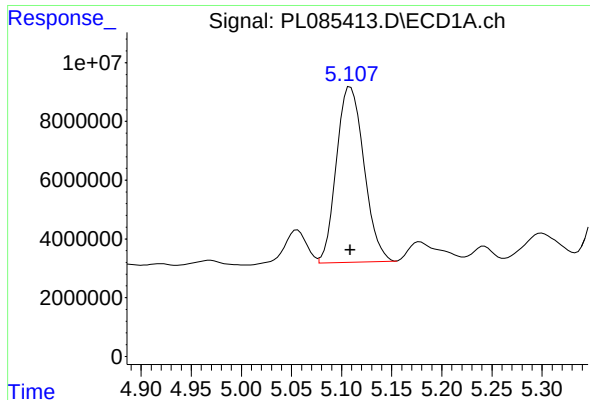

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 114354166
Conc: 750.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

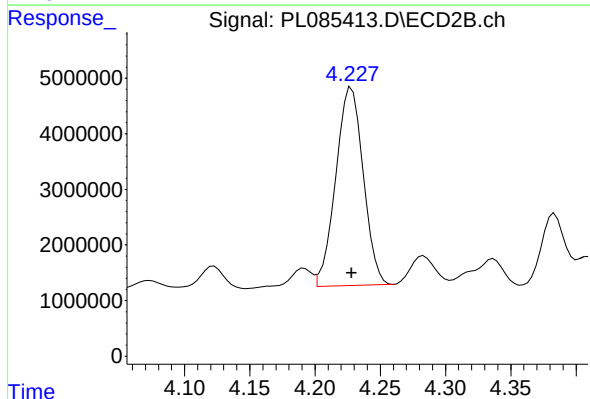


#24 Chlordane-2

R.T.: 4.228 min
Delta R.T.: 0.000 min
Response: 52298577
Conc: 734.52 ng/ml

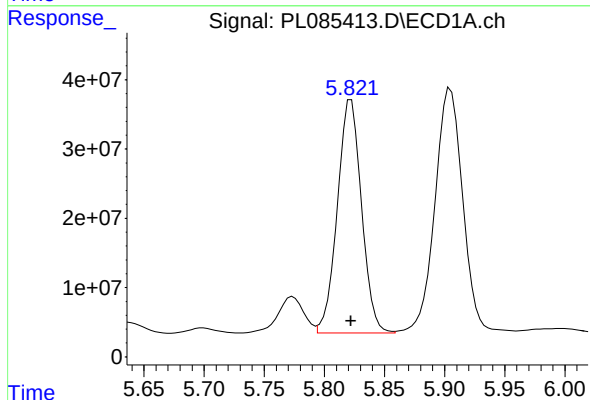


#25 Chlordane-3

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 472331977
Conc: 752.66 ng/ml

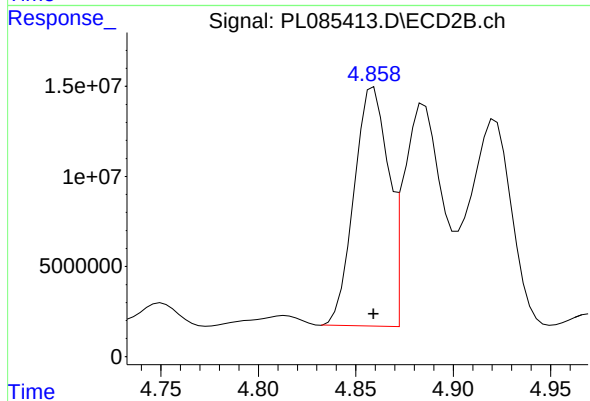

#25 Chlordane-3


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 161697842
Conc: 762.47 ng/ml

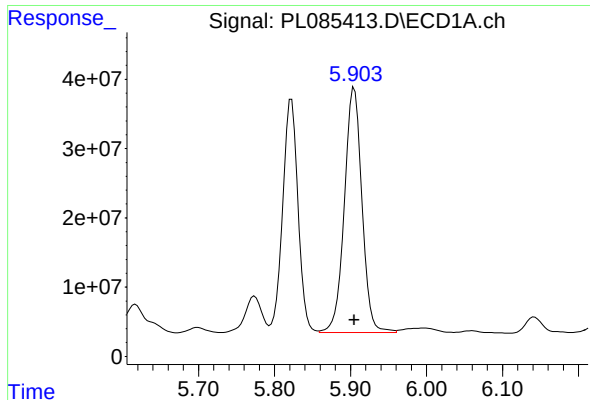

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 569409843
Conc: 750.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

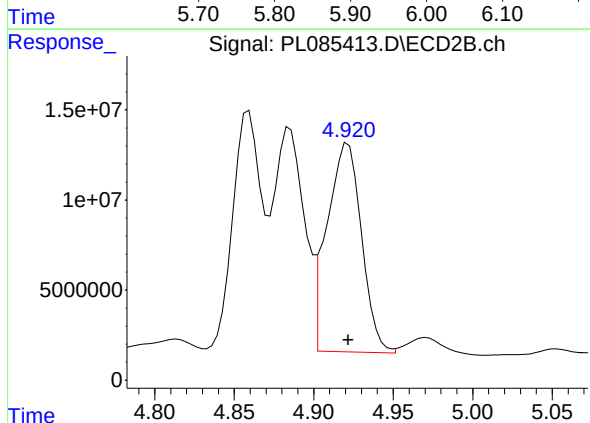


#26 Chlordane-4

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 175584780
Conc: 759.73 ng/ml

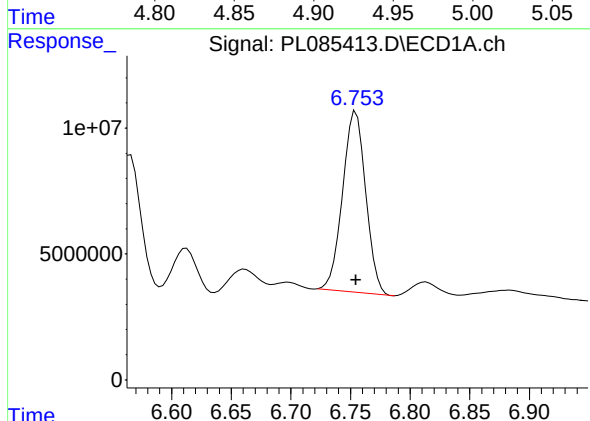


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 97098785
Conc: 754.53 ng/ml

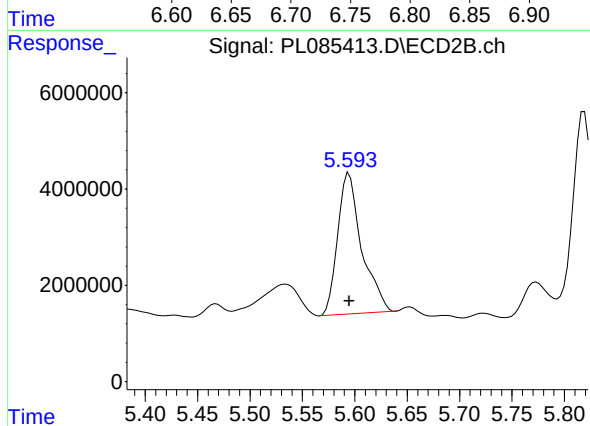

#27 Chlordane-5


R.T.: 5.595 min
Delta R.T.: 0.000 min
Response: 46866459
Conc: 751.97 ng/ml

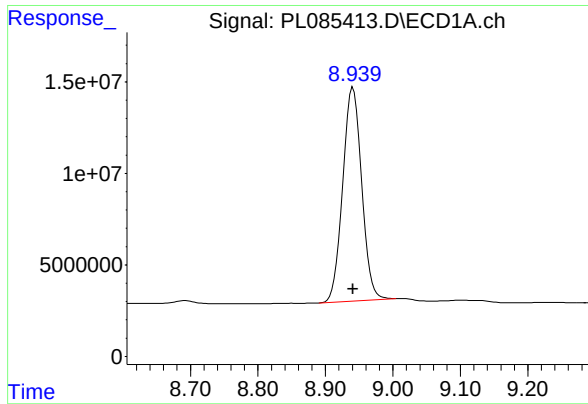

#28 Decachlorobiphenyl

R.T.: 8.941 min
Delta R.T.: 0.000 min
Response: 228659432
Conc: 73.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

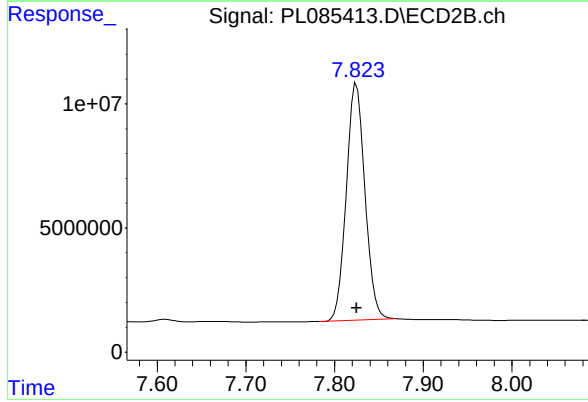

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 139562809
Conc: 74.26 ng/ml