

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
 Data File : PL085414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 23:57
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 10:12:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 10:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.413	2.649	160.7E6	88438287	50.000	50.000
28) SA Decachlor...	8.942	7.825	162.5E6	96970709	50.000	50.000
Target Compounds						
23) Chlordane-1	4.577	3.647	71883933	26628915	500.000	500.000
24) Chlordane-2	5.110	4.228	78209707	37525392	500.000	500.000
25) Chlordane-3	5.824	4.860	310.4E6	102.5E6	500.000	500.000
26) Chlordane-4	5.907	4.922	378.8E6	112.4E6	500.000	500.000
27) Chlordane-5	6.756	5.595	64908067	30925243	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
Data File : PL085414.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 23:57
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 10:12:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 10:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

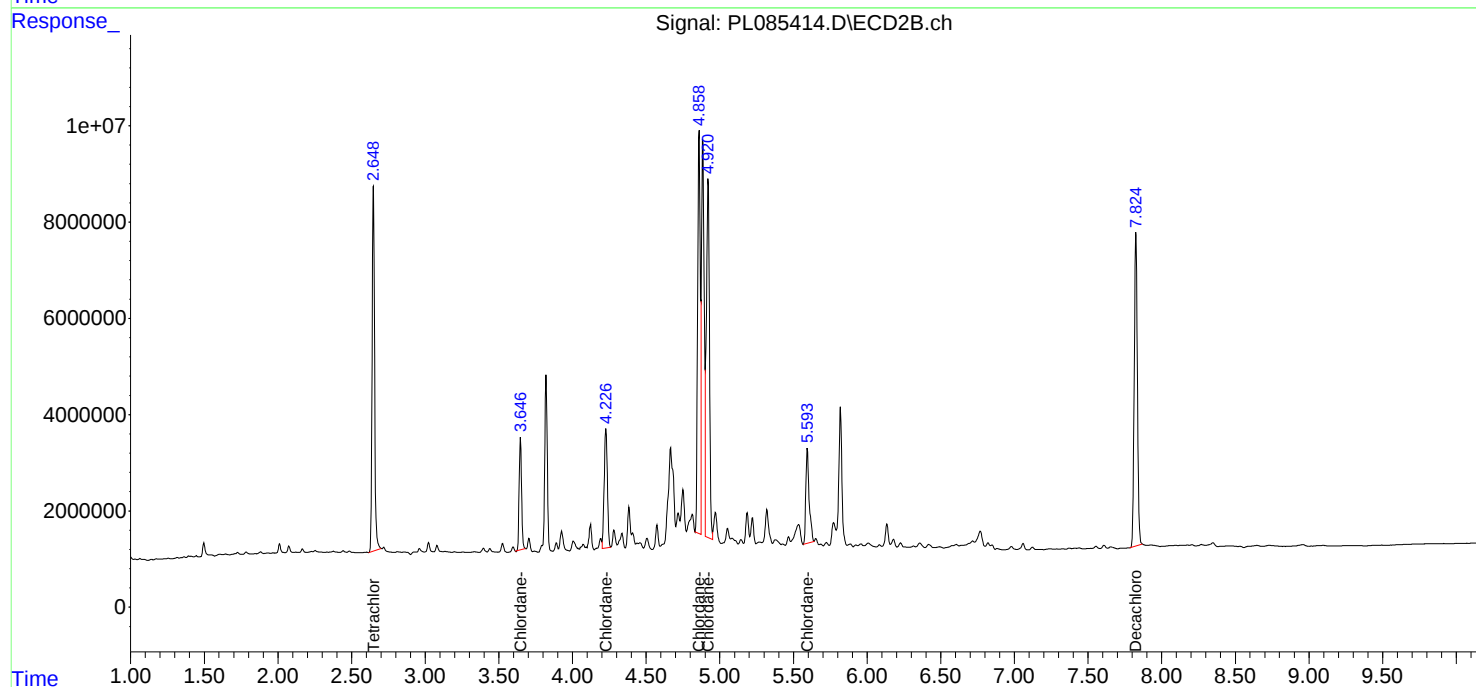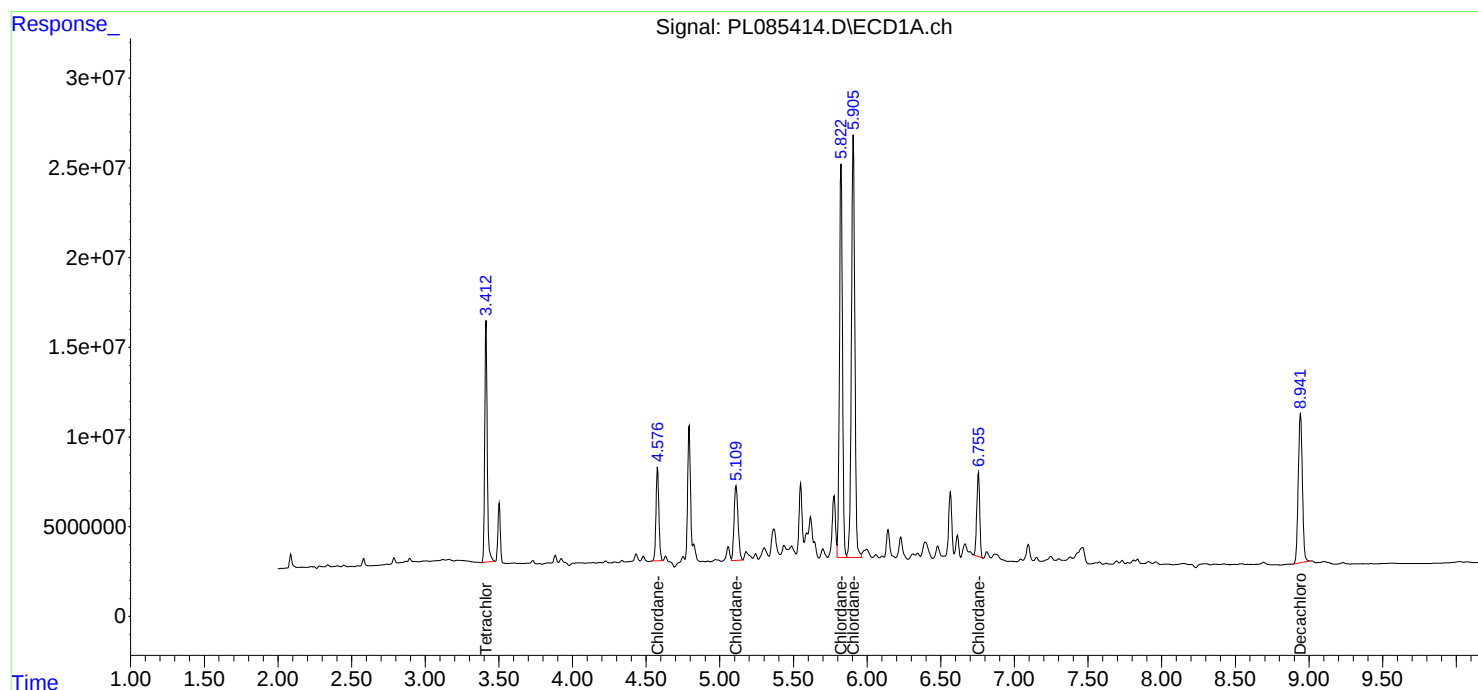


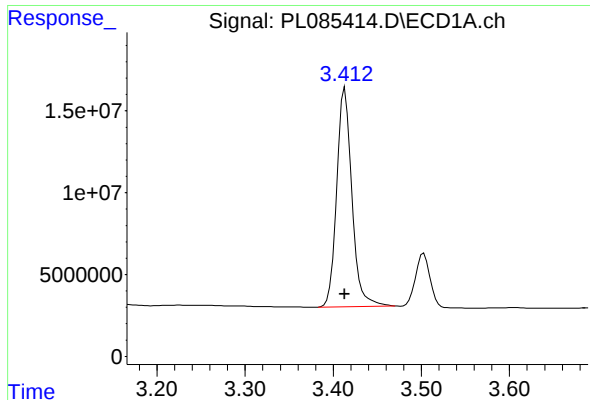

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 160728928
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

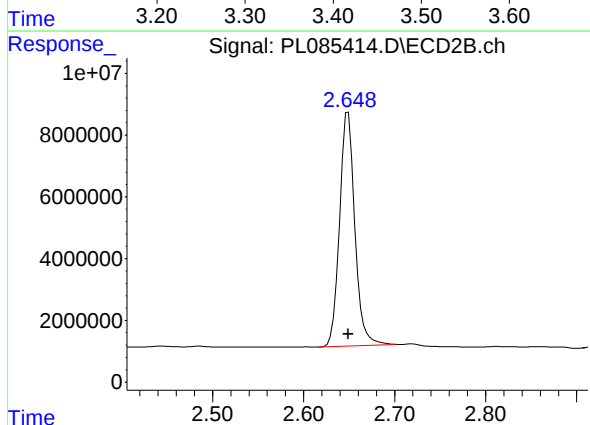


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 88438287
Conc: 50.00 ng/ml

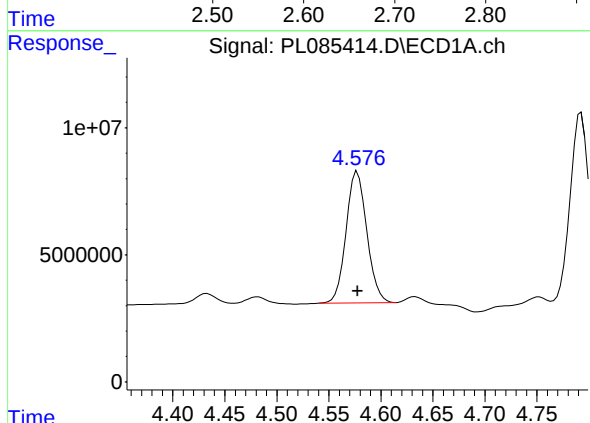


#23 Chlordane-1

R.T.: 4.577 min
Delta R.T.: 0.000 min
Response: 71883933
Conc: 500.00 ng/ml

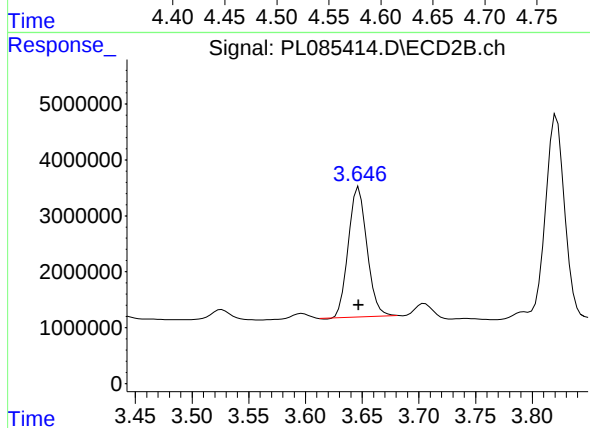

#23 Chlordane-1


R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 26628915
Conc: 500.00 ng/ml

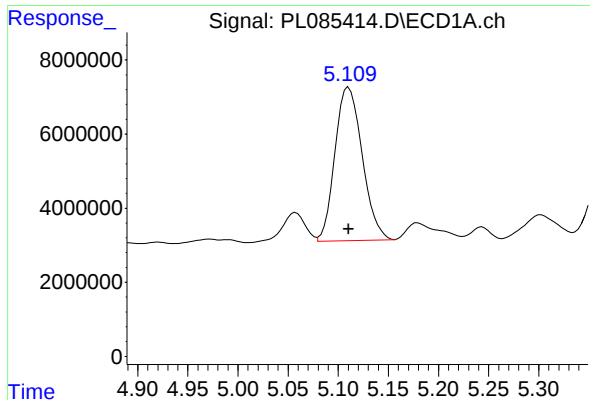

#24 Chlordane-2


R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 78209707
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

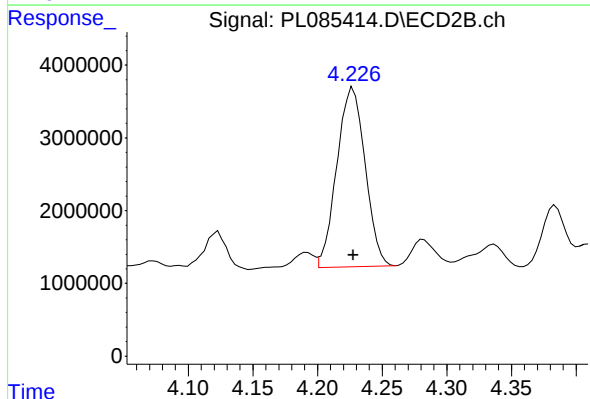


#24 Chlordane-2

R.T.: 4.228 min
Delta R.T.: 0.000 min
Response: 37525392
Conc: 500.00 ng/ml

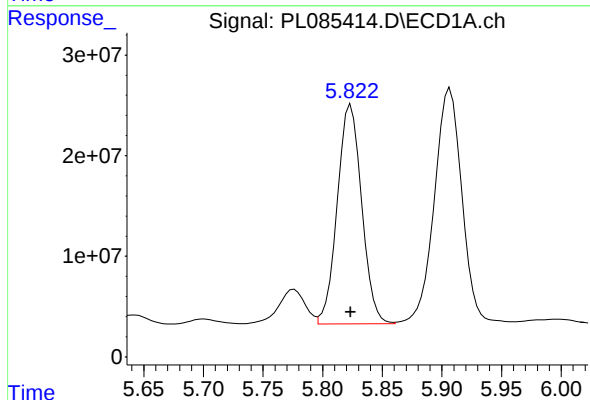


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 310435614
Conc: 500.00 ng/ml

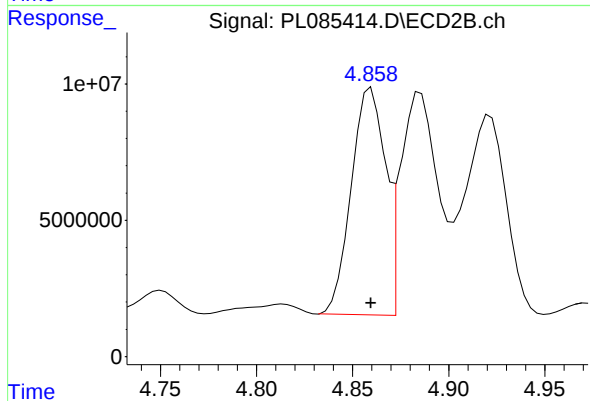

#25 Chlordane-3


R.T.: 4.860 min
Delta R.T.: 0.000 min
Response: 102488846
Conc: 500.00 ng/ml

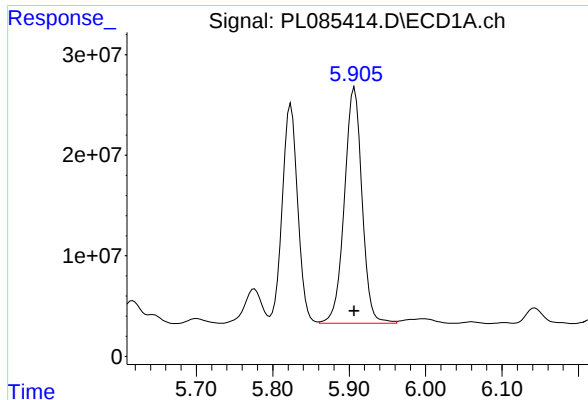

#26 Chlordane-4


R.T.: 5.907 min
Delta R.T.: 0.000 min
Response: 378761768
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

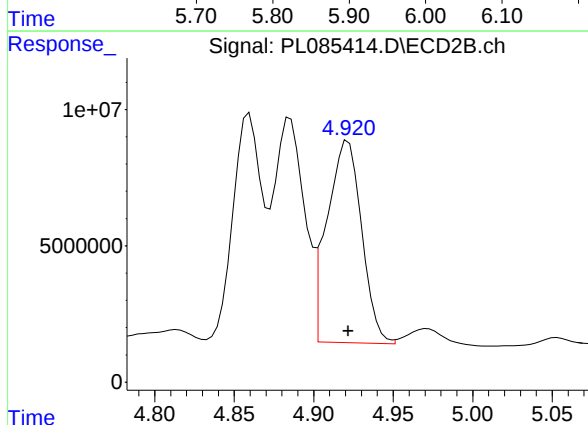


#26 Chlordane-4

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 112402870
Conc: 500.00 ng/ml

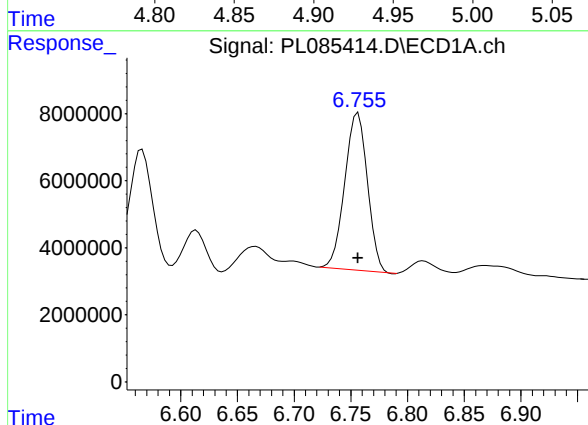


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 64908067
Conc: 500.00 ng/ml

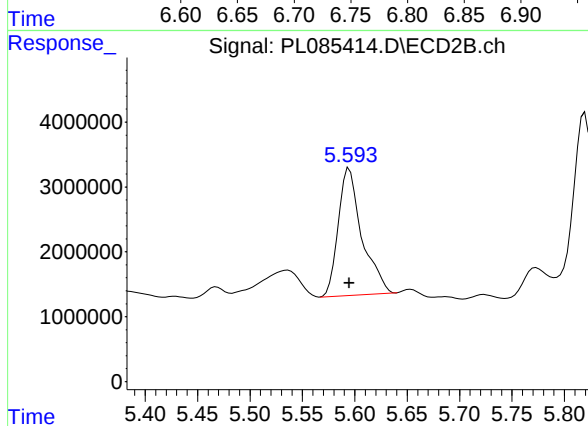

#27 Chlordane-5


R.T.: 5.595 min
Delta R.T.: 0.000 min
Response: 30925243
Conc: 500.00 ng/ml

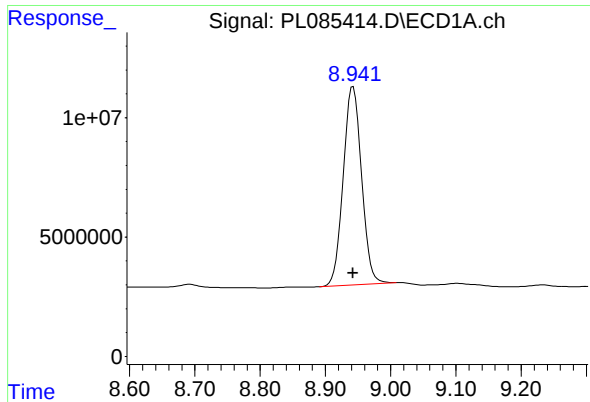

#28 Decachlorobiphenyl

R.T.: 8.942 min
Delta R.T.: 0.000 min
Response: 162536751
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

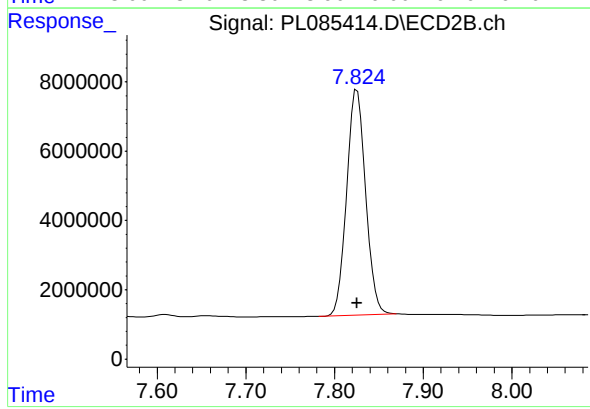

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 96970709
Conc: 50.00 ng/ml