

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
 Data File : PL085415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 00:11
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 10:19:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 10:19:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.413	2.649	81356969	44847916	25.283	25.075
28) SA Decachlor...	8.942	7.824	82851684	47933409	26.303	25.376
Target Compounds						
23) Chlordane-1	4.576	3.647	37687533	13686313	258.489	252.318
24) Chlordane-2	5.109	4.227	41714061	18651438	267.428	258.860
25) Chlordane-3	5.822	4.858	155.6E6	51043467	248.491	242.951
26) Chlordane-4	5.905	4.921	191.9E6	55940352	252.241	243.986
27) Chlordane-5	6.755	5.593	33400423	15445288	257.093	248.361



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
Data File : PL085415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 00:11
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 10:19:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 10:19:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

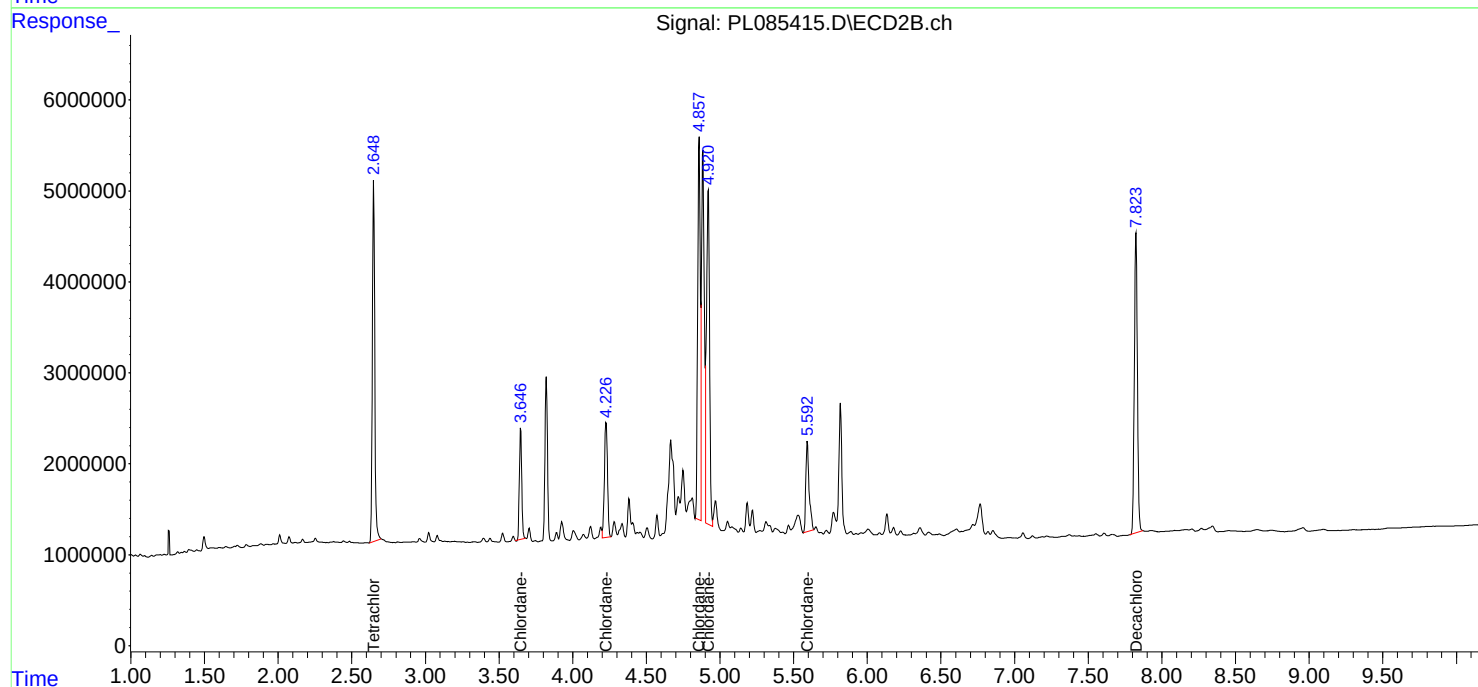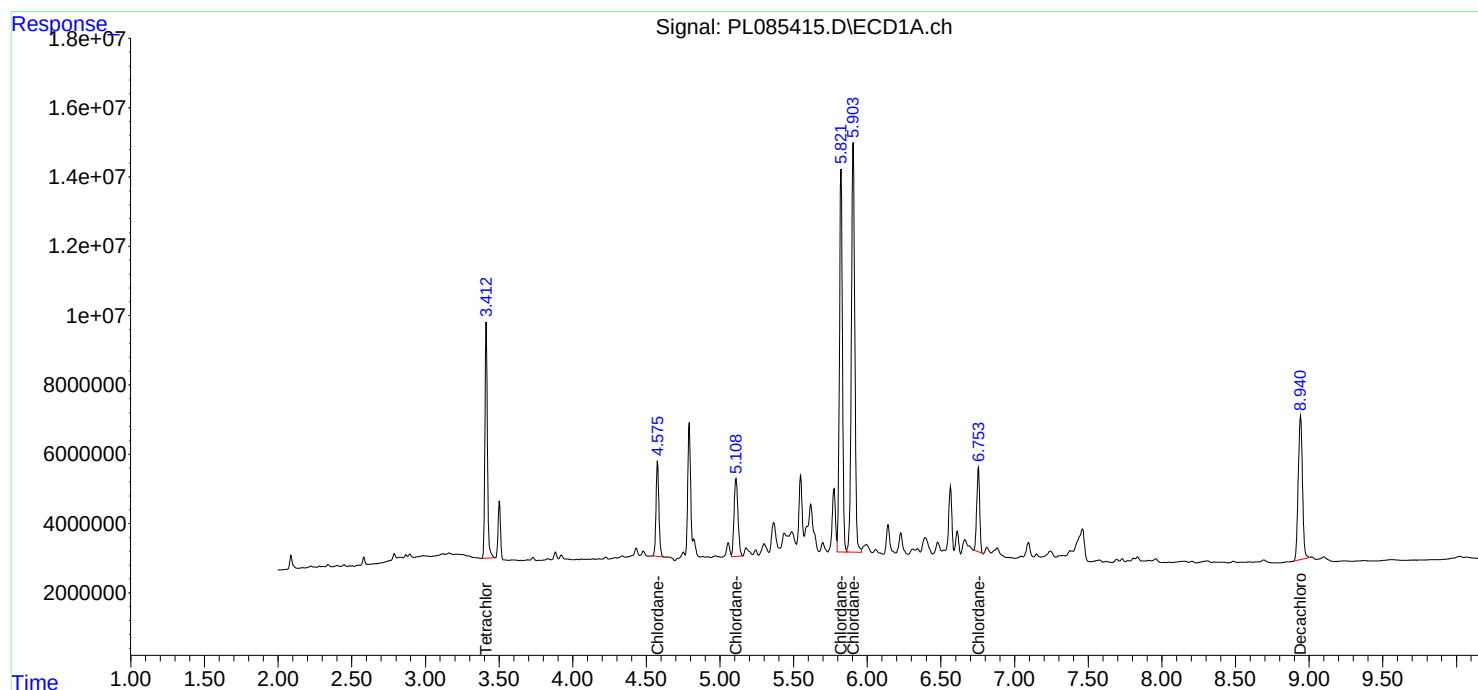


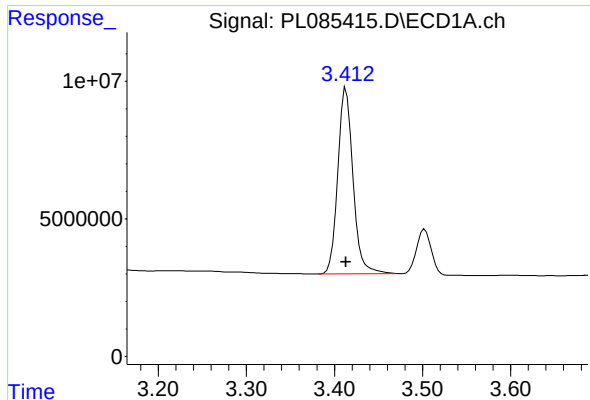

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 81356969
Conc: 25.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

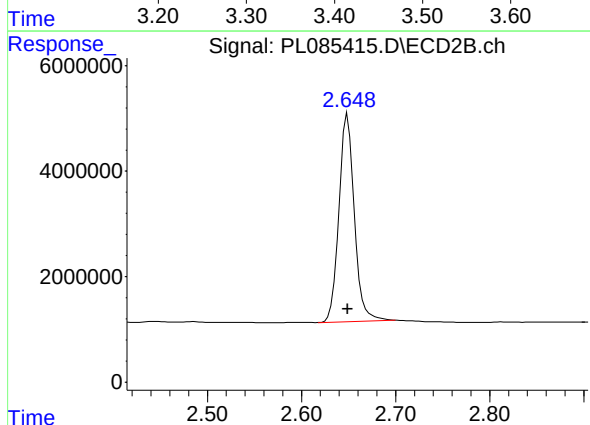


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 44847916
Conc: 25.07 ng/ml

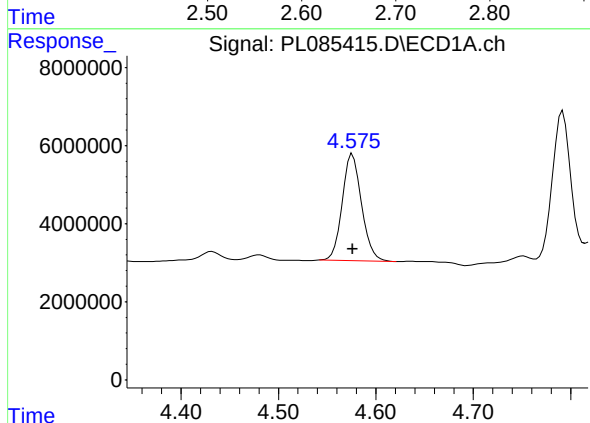


#23 Chlordane-1

R.T.: 4.576 min
Delta R.T.: 0.000 min
Response: 37687533
Conc: 258.49 ng/ml

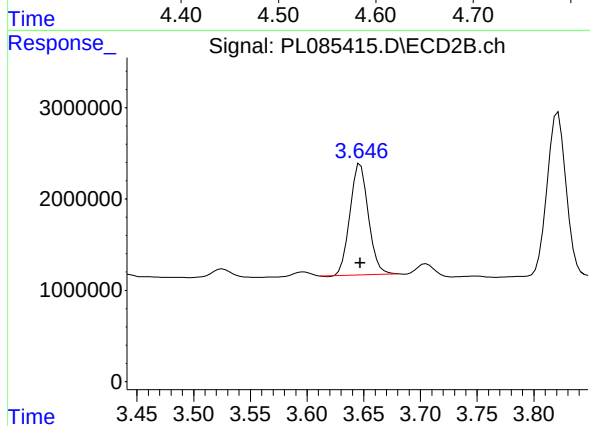

#23 Chlordane-1


R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 13686313
Conc: 252.32 ng/ml

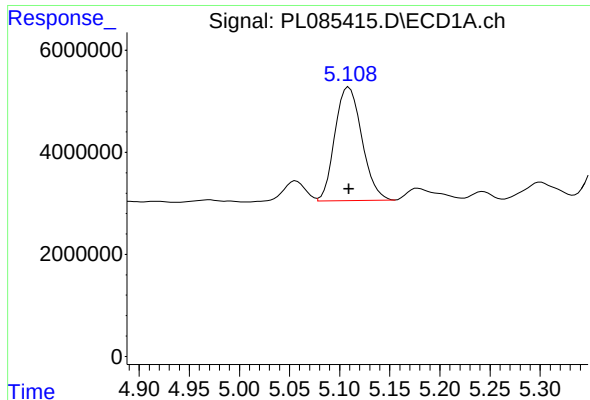

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 41714061
Conc: 267.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

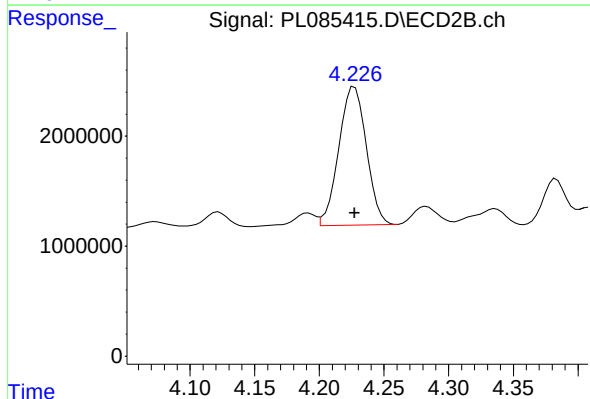


#24 Chlordane-2

R.T.: 4.227 min
Delta R.T.: 0.000 min
Response: 18651438
Conc: 258.86 ng/ml

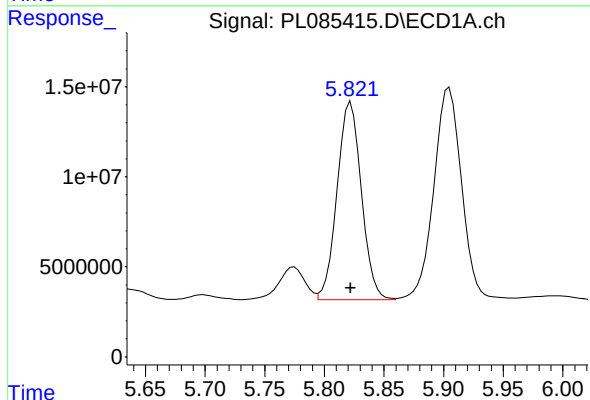


#25 Chlordane-3

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 155626969
Conc: 248.49 ng/ml

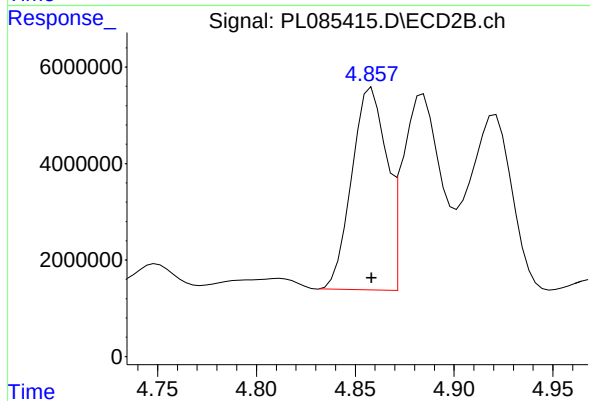

#25 Chlordane-3


R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 51043467
Conc: 242.95 ng/ml

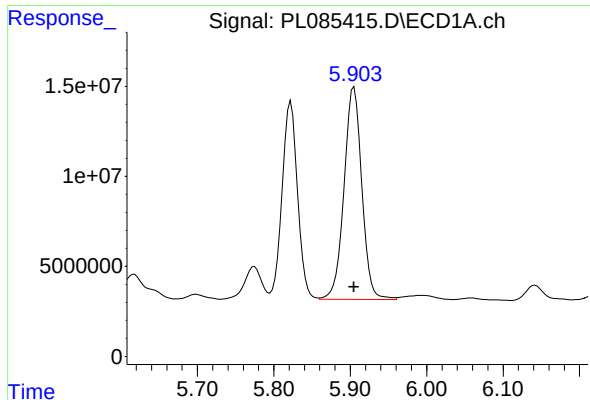

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 191878237
Conc: 252.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

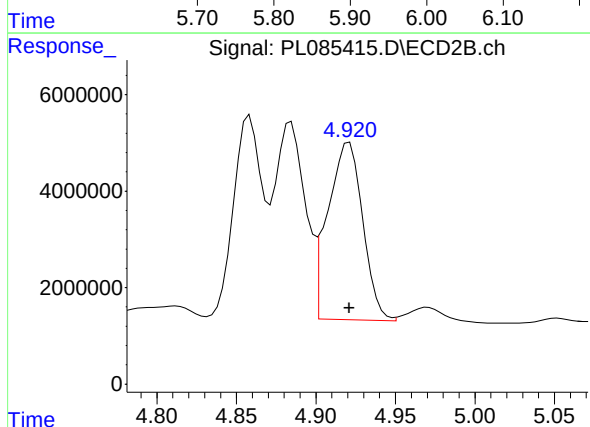


#26 Chlordane-4

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 55940352
Conc: 243.99 ng/ml

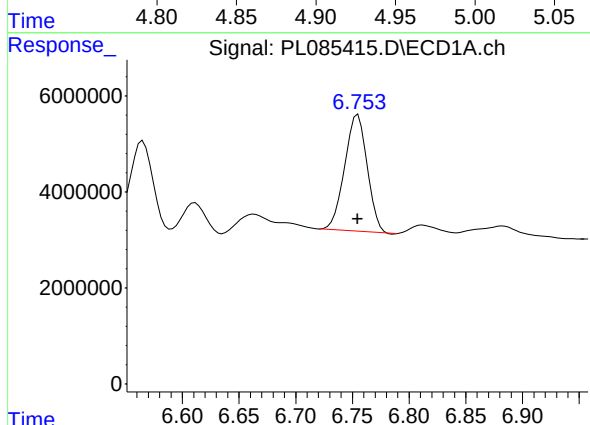


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 33400423
Conc: 257.09 ng/ml

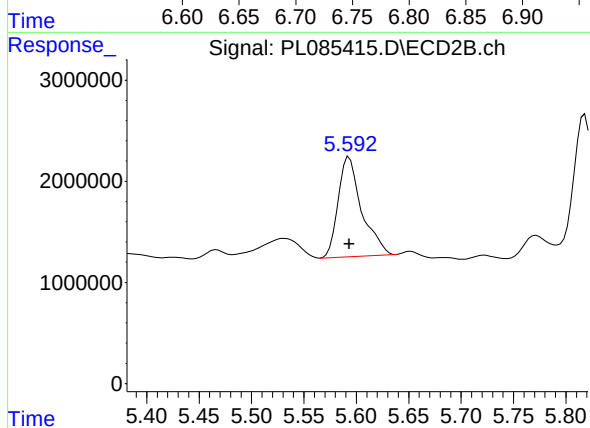

#27 Chlordane-5


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 15445288
Conc: 248.36 ng/ml

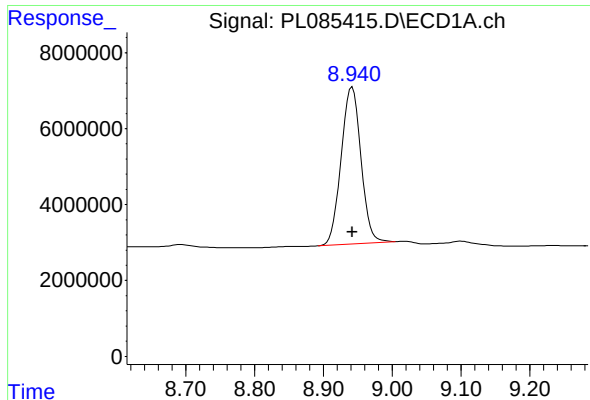

#28 Decachlorobiphenyl

R.T.: 8.942 min
Delta R.T.: 0.000 min
Response: 82851684
Conc: 26.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

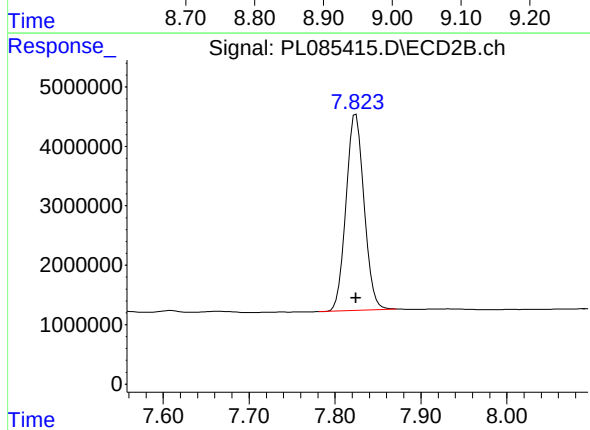

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: 0.000 min
Response: 47933409
Conc: 25.38 ng/ml