

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
 Data File : PL085423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 02:17
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL091923

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 10:13:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 10:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.412	2.649	179.2E6	97364001	55.737	55.046
28) SA Decachlor...	8.943	7.825	169.9E6	100.3E6	52.254	51.716
Target Compounds						
23) Chlordane-1	4.575	3.647	79518516	28987429	553.104	544.285
24) Chlordane-2	5.108	4.227	86549090	38387406	553.314	511.486
25) Chlordane-3	5.822	4.859	344.5E6	111.8E6	554.892	545.219
26) Chlordane-4	5.905	4.922	418.6E6	120.4E6	552.568	535.751
27) Chlordane-5	6.755	5.594	71341071	33050909	549.555	534.368



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091923\
Data File : PL085423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 02:17
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL091923

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 10:13:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 10:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

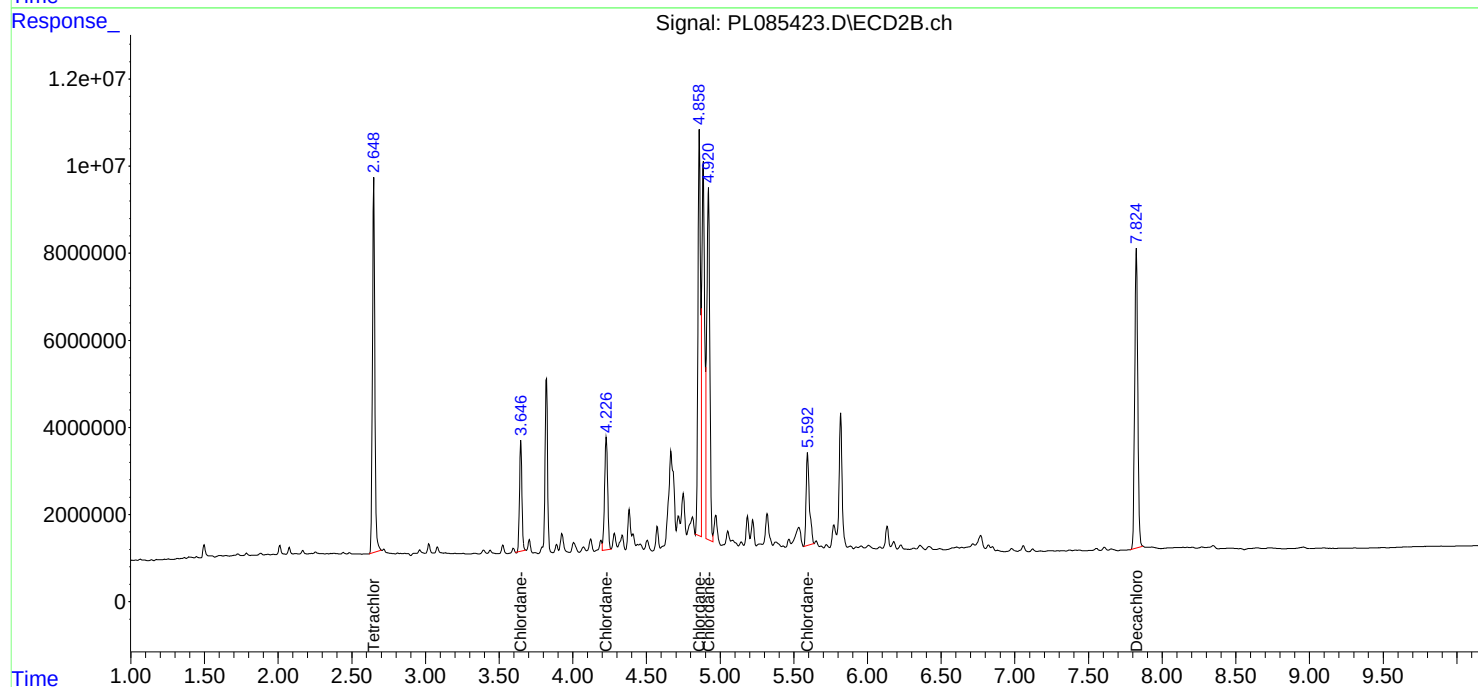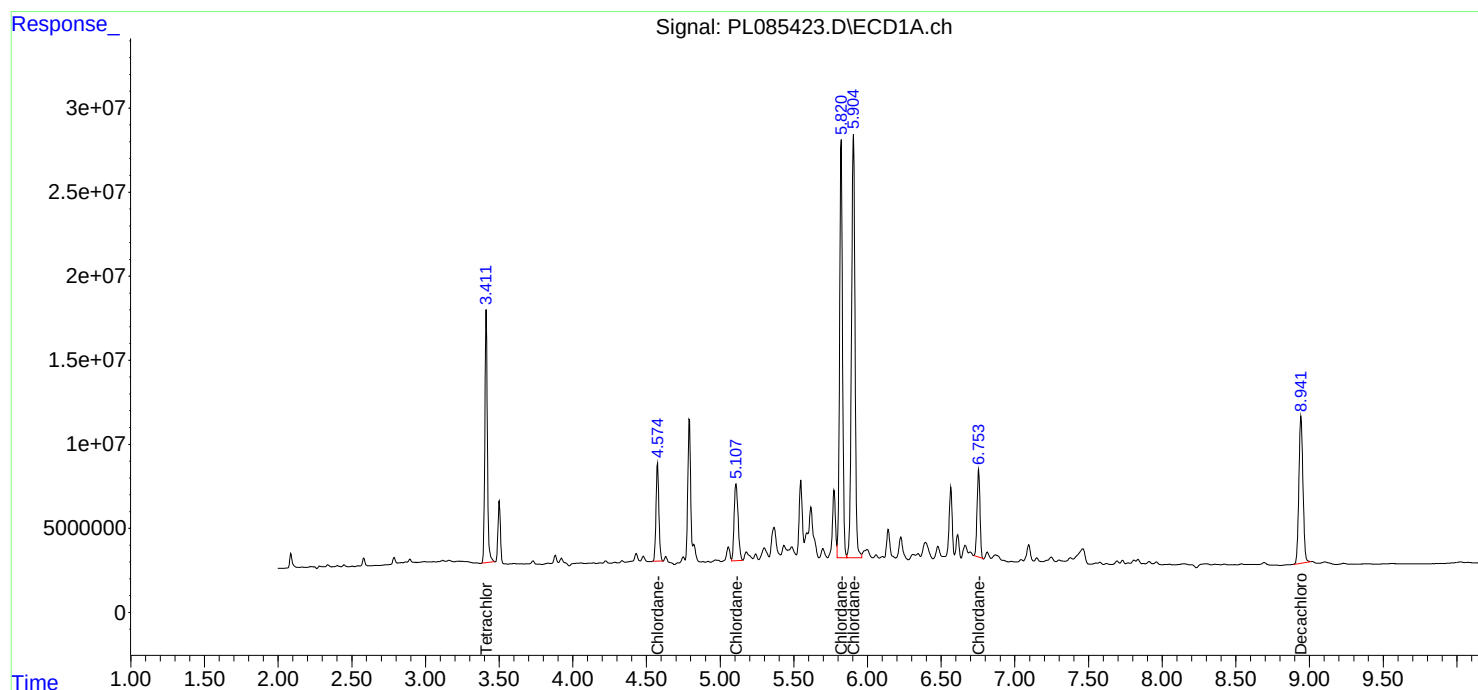


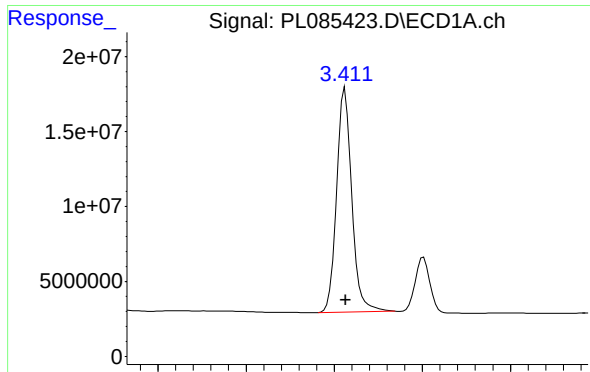

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 179171161
Conc: 55.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091923

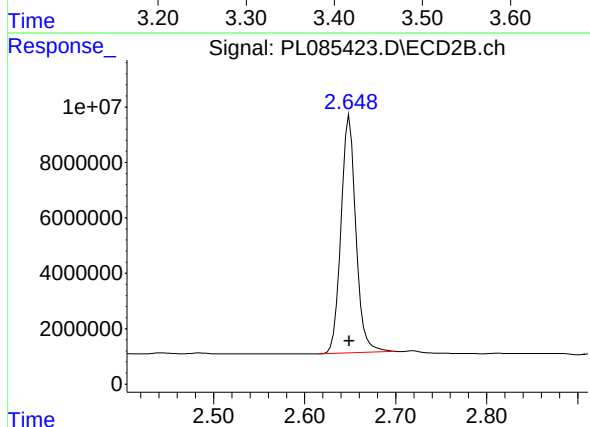


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 97364001
Conc: 55.05 ng/ml

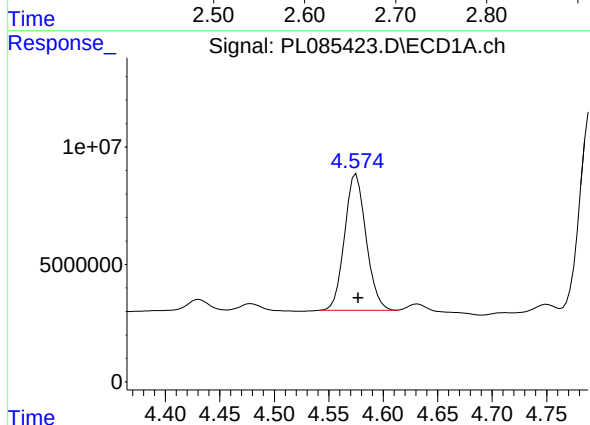


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: -0.002 min
Response: 79518516
Conc: 553.10 ng/ml

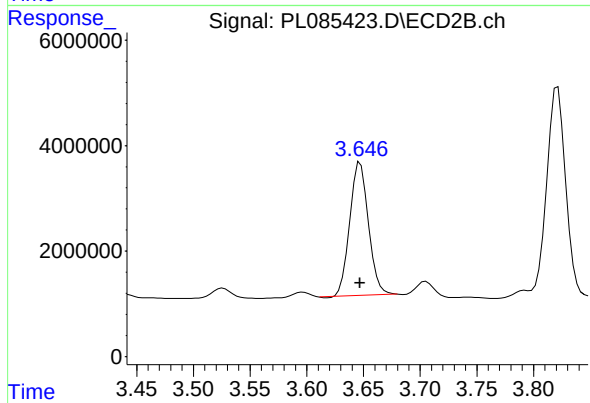

#23 Chlordane-1


R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 28987429
Conc: 544.28 ng/ml

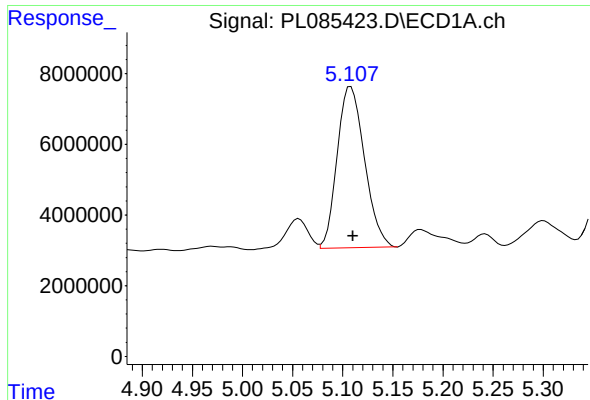

#24 Chlordane-2


R.T.: 5.108 min
Delta R.T.: -0.002 min
Response: 86549090
Conc: 553.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091923

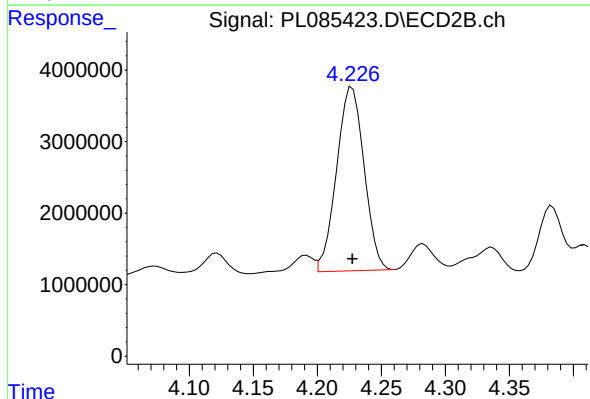


#24 Chlordane-2

R.T.: 4.227 min
Delta R.T.: 0.000 min
Response: 38387406
Conc: 511.49 ng/ml

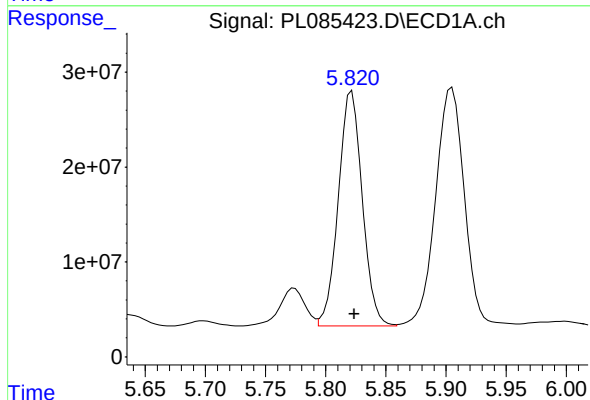


#25 Chlordane-3

R.T.: 5.822 min
Delta R.T.: -0.002 min
Response: 344516353
Conc: 554.89 ng/ml

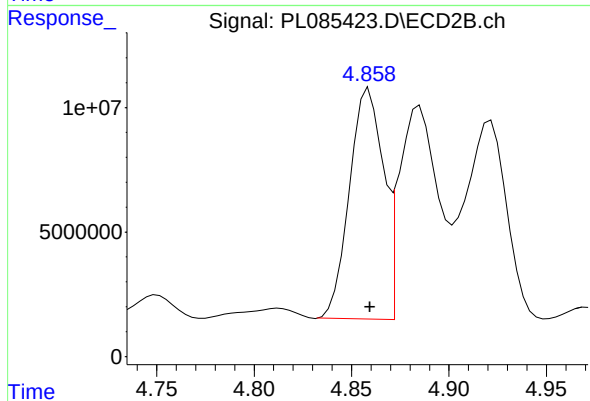

#25 Chlordane-3


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 111757774
Conc: 545.22 ng/ml

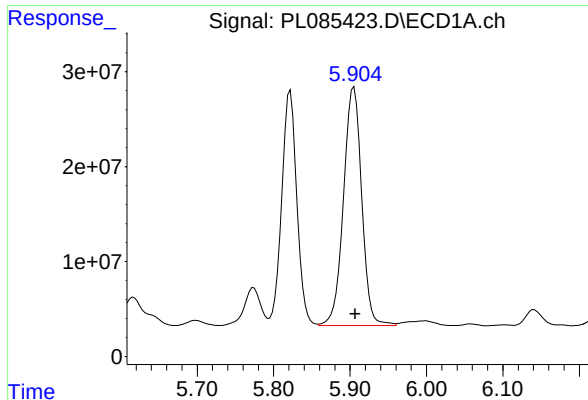

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: -0.002 min
Response: 418583220
Conc: 552.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091923

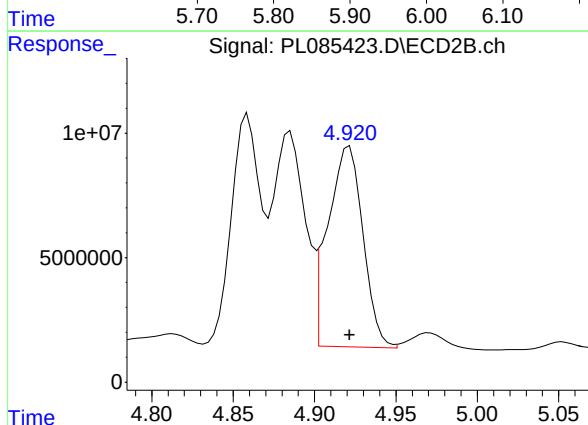


#26 Chlordane-4

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 120439964
Conc: 535.75 ng/ml

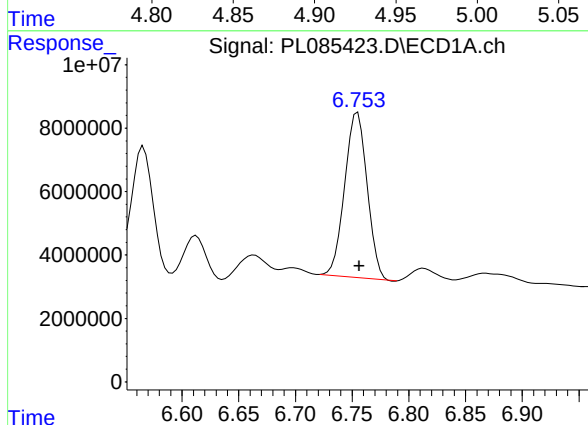


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: -0.002 min
Response: 71341071
Conc: 549.55 ng/ml

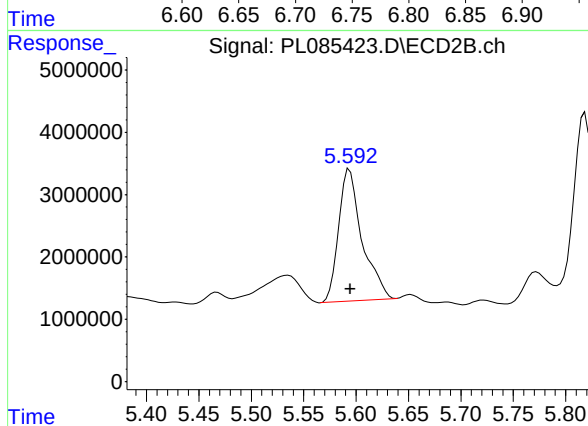

#27 Chlordane-5


R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 33050909
Conc: 534.37 ng/ml

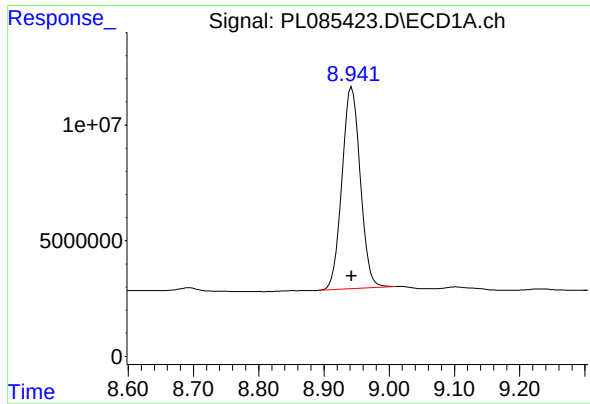

#28 Decachlorobiphenyl

R.T.: 8.943 min
Delta R.T.: 0.000 min
Response: 169863376
Conc: 52.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL091923

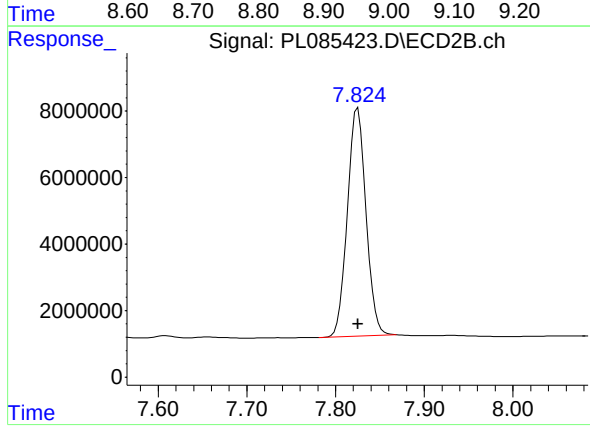

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 100298554
Conc: 51.72 ng/ml