

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092021\
 Data File : PL069910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 15:49
 Operator : AR\AJ
 Sample : M3797-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 02:33:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.630	5.566	5265476	13485666	12.924	11.079
28)	SA Decachlor...	10.397	11.489	3992345	6418271	5.421	5.617
Target Compounds							
3)	MA gamma-BHC...	0.000	6.525f	0	592050	N.D.	0.367 #
4)	MA Heptachlor	6.191f	0.000	588474	0	0.868	N.D. #
9)	A Endosulfan I	0.000	8.463f	0	1061689	N.D.	0.821 #
10)	B gamma-Chl...	0.000	8.295	0	985835	N.D.	0.738 #
11)	B alpha-Chl...	0.000	8.380	0	860052	N.D.	0.632 #
15)	B Endosulfa...	0.000	9.213	0	410096	N.D.	0.364 #
25)	Chlordane-3	0.000	8.295	0	985835	N.D.	5.197 #
26)	Chlordane-4	0.000	8.380	0	860052	N.D.	3.693 #
27)	Chlordane-5	0.000	9.272	0	164325	N.D.	3.908 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092021\
Data File : PL069910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 15:49
Operator : AR\AJ
Sample : M3797-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 02:33:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

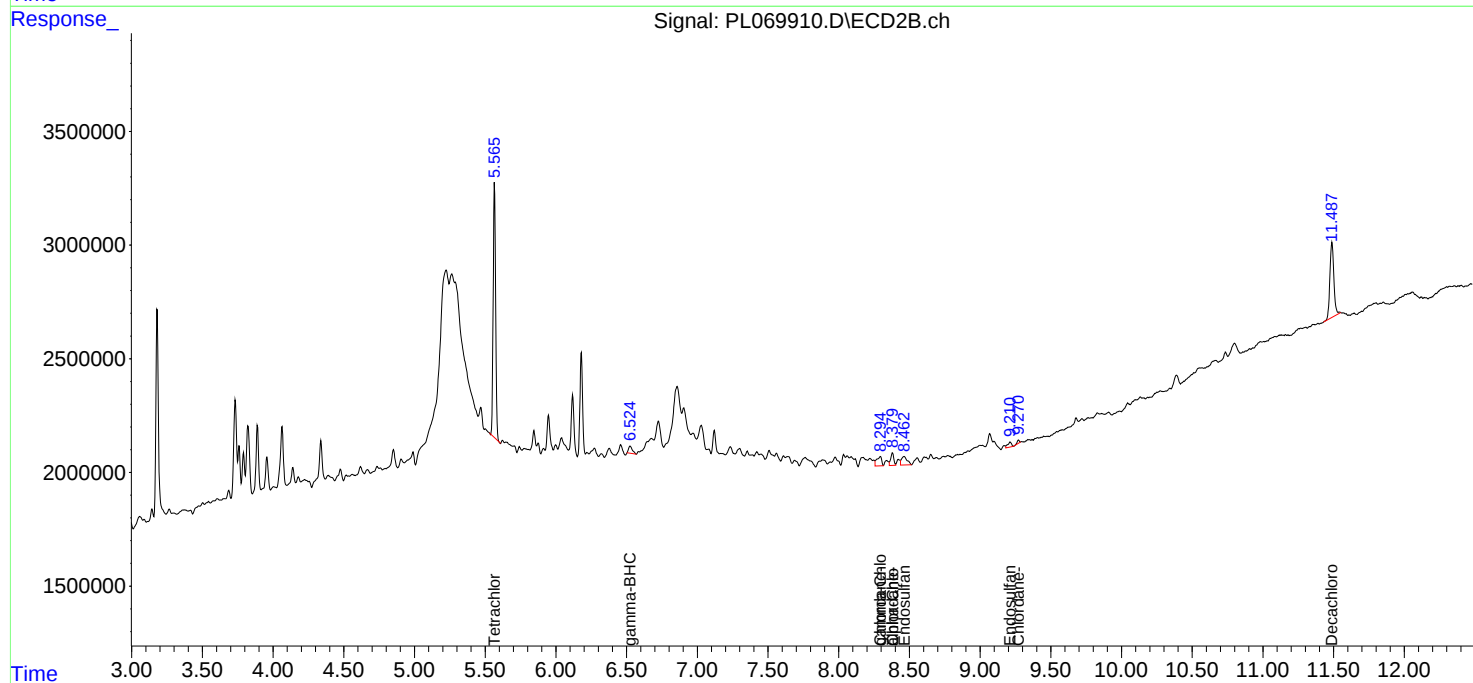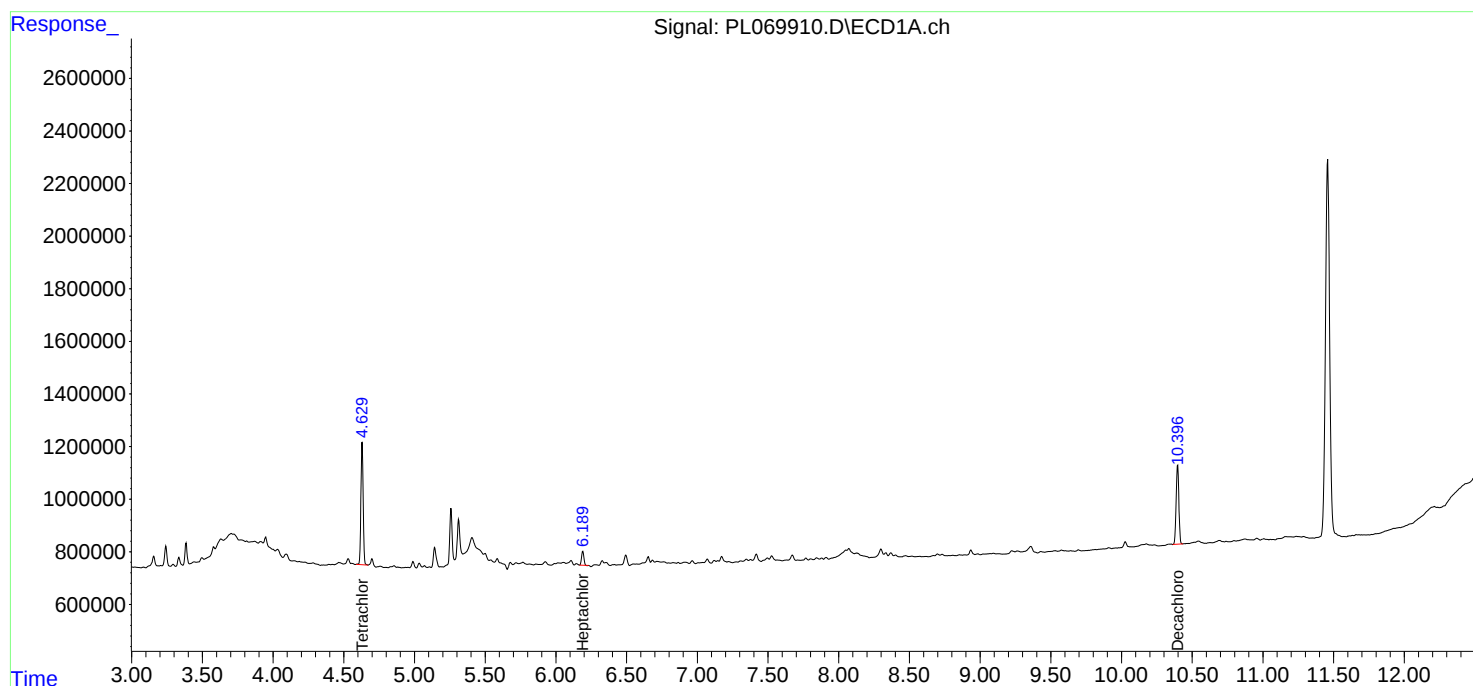


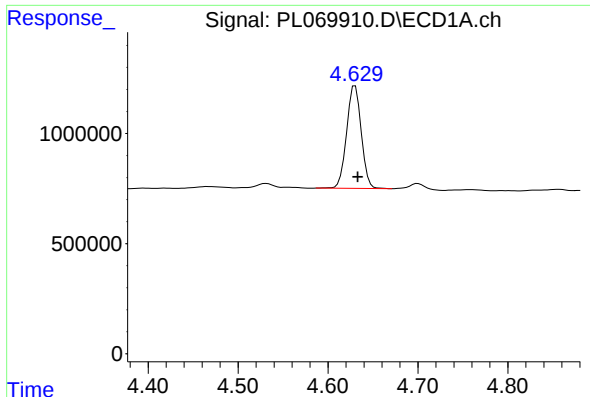

#1 Tetrachloro-m-xylene


R.T.: 4.630 min
Delta R.T.: -0.003 min
Response: 5265476
Conc: 12.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

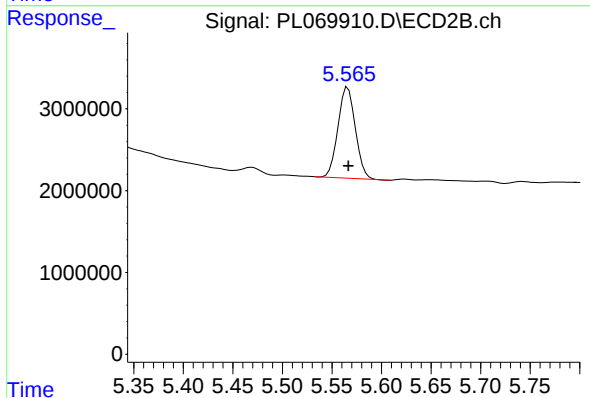


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 13485666
Conc: 11.08 ng/ml

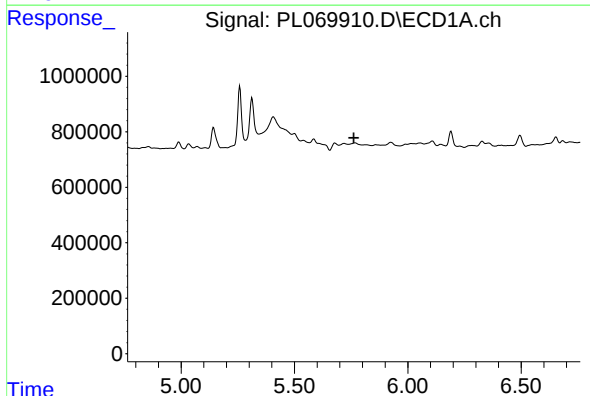


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.762 min
Response: 0
Conc: N.D.

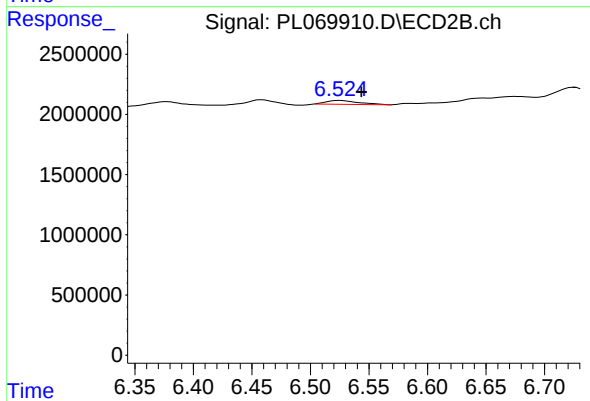

#3 gamma-BHC (Lindane)


R.T.: 6.525 min
Delta R.T.: -0.019 min
Response: 592050
Conc: 0.37 ng/ml

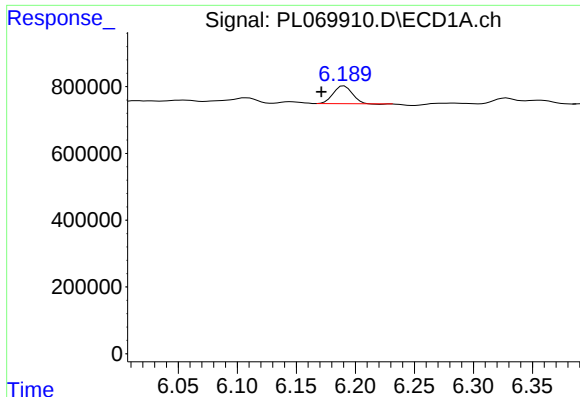

#4 Heptachlor


R.T.: 6.191 min
Delta R.T.: 0.019 min
Response: 588474
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

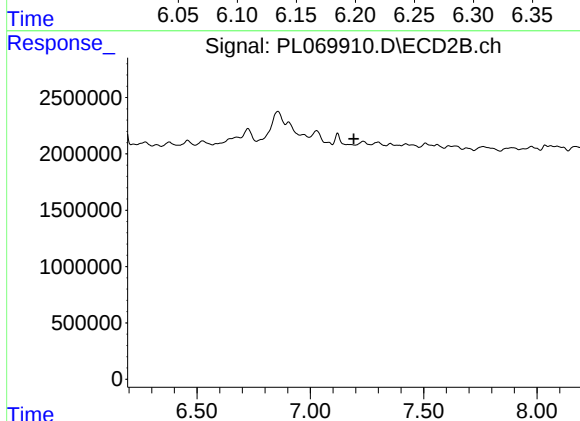


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

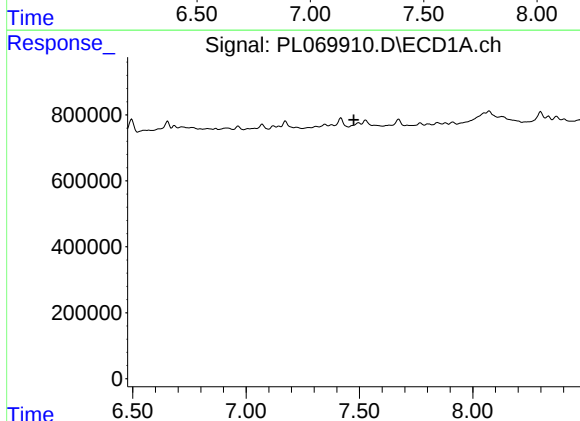


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.476 min
Response: 0
Conc: N.D.

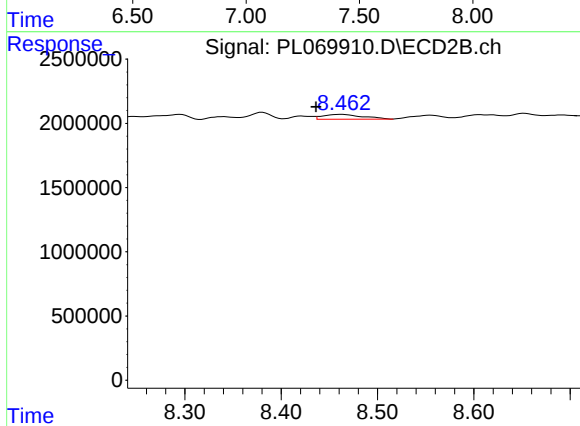

#9 Endosulfan I


R.T.: 8.463 min
Delta R.T.: 0.027 min
Response: 1061689
Conc: 0.82 ng/ml

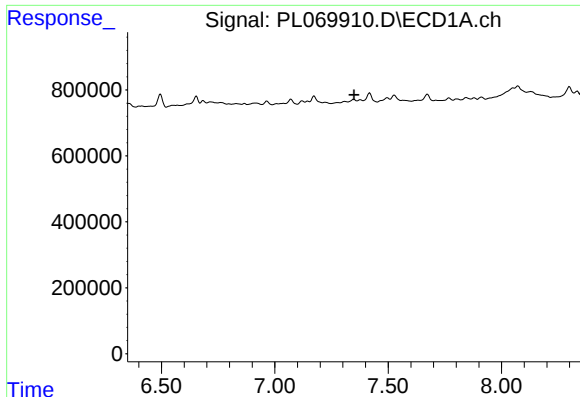

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

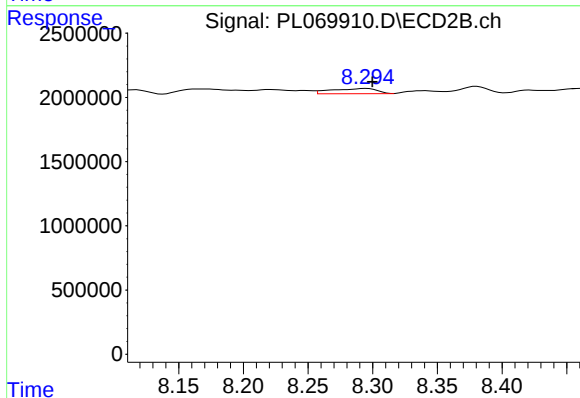


#10 gamma-Chlordane

R.T.: 8.295 min
Delta R.T.: -0.004 min
Response: 985835
Conc: 0.74 ng/ml

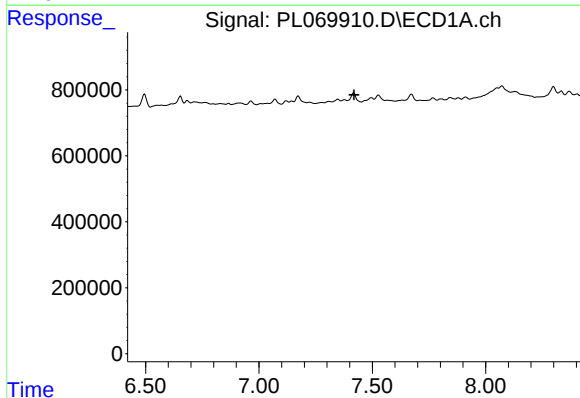


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

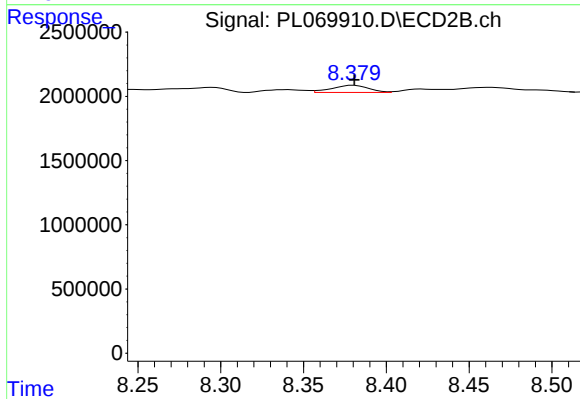

#11 alpha-Chlordane


R.T.: 8.380 min
Delta R.T.: 0.000 min
Response: 860052
Conc: 0.63 ng/ml

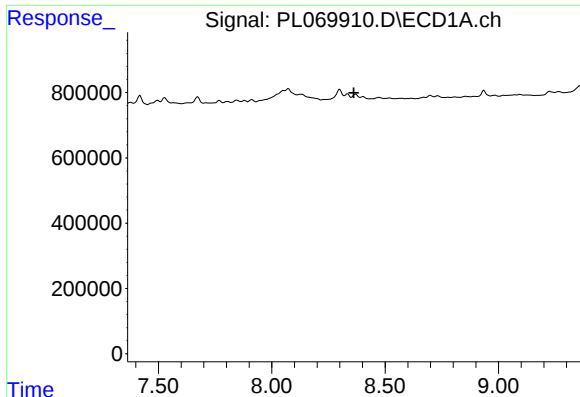

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

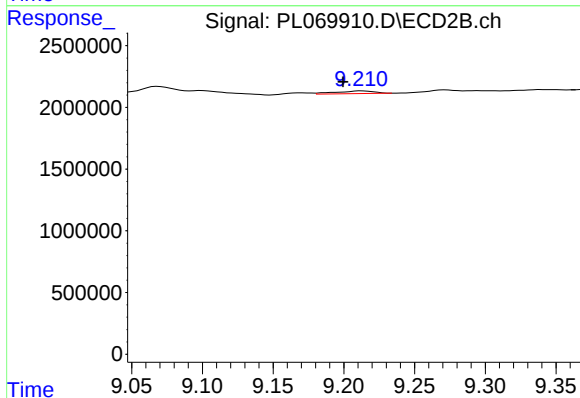


#15 Endosulfan II

R.T.: 9.213 min
Delta R.T.: 0.013 min
Response: 410096
Conc: 0.36 ng/ml

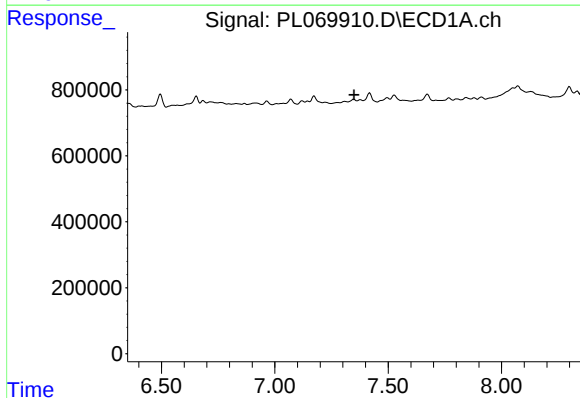


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

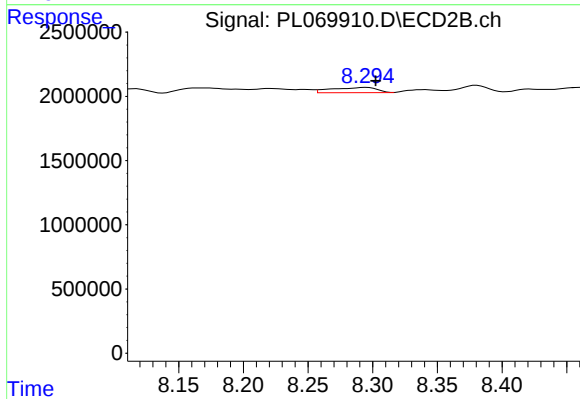

#25 Chlordane-3


R.T.: 8.295 min
Delta R.T.: -0.007 min
Response: 985835
Conc: 5.20 ng/ml

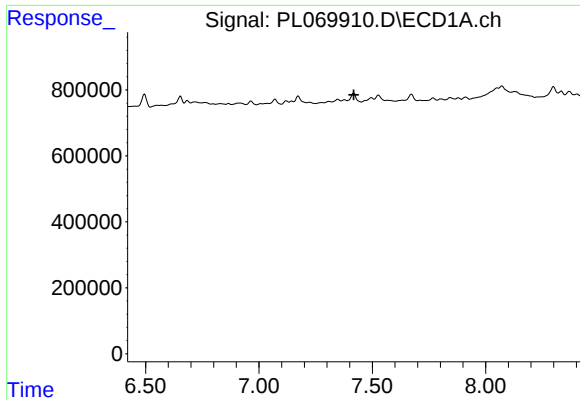

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

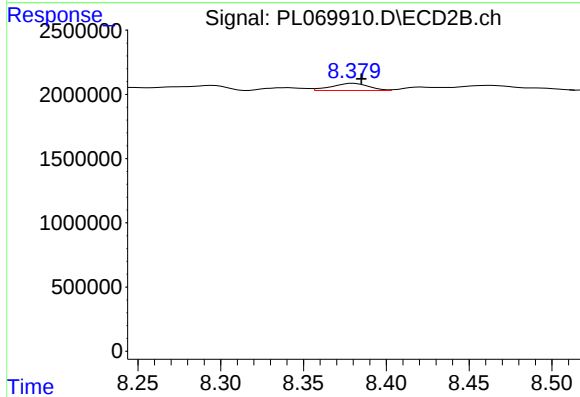


#26 Chlordane-4

R.T.: 8.380 min
Delta R.T.: -0.005 min
Response: 860052
Conc: 3.69 ng/ml

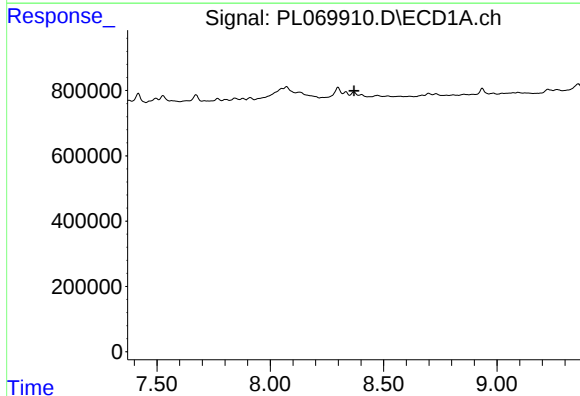


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.369 min
Response: 0
Conc: N.D.

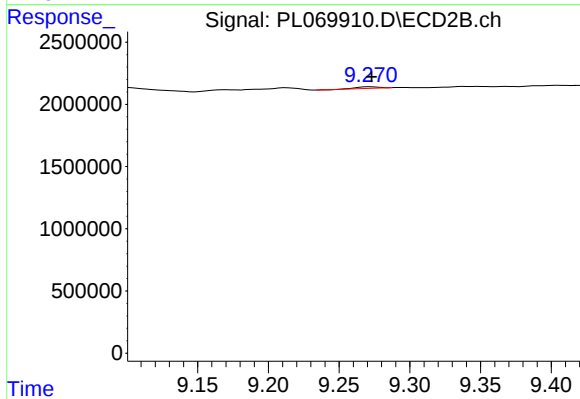

#27 Chlordane-5


R.T.: 9.272 min
Delta R.T.: -0.001 min
Response: 164325
Conc: 3.91 ng/ml

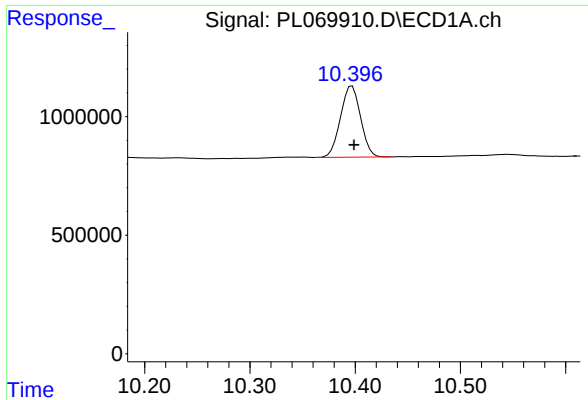

#28 Decachlorobiphenyl

R.T.: 10.397 min
Delta R.T.: -0.002 min
Response: 3992345
Conc: 5.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

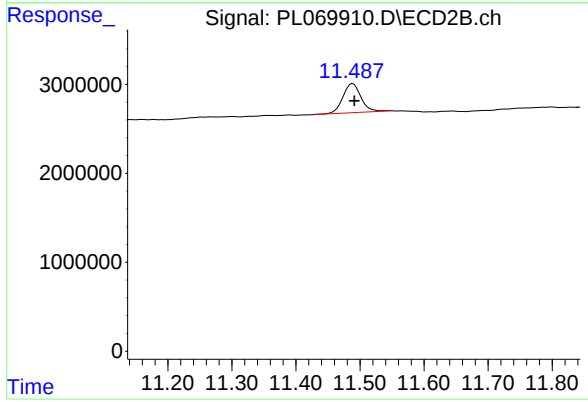

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.003 min
Response: 6418271
Conc: 5.62 ng/ml