

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092021\
 Data File : PL069920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2021 19:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 02:34:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.627	5.563	9887841	29147389	24.270	23.946
28)	SA Decachlor...	10.391	11.481	14979071	25563178	20.340	22.372
Target Compounds							
7)	B delta-BHC	0.000	7.080f	0	1406743	N.D.	0.845 #
9)	A Endosulfan I	0.000	8.441	0	41525	N.D.	0.032 #
10)	B gamma-Chl...	0.000	8.273f	0	434669	N.D.	0.325 #
11)	B alpha-Chl...	0.000	8.393	0	52817	N.D.	0.039 #
15)	B Endosulfa...	0.000	9.213	0	738737	N.D.	0.655 #
17)	MA 4,4'-DDT	0.000	9.434	0	152641	N.D.	0.136 #
21)	B Endrin ke...	0.000	10.086f	0	516635	N.D.	0.419 #
25)	Chlordane-3	0.000	8.273f	0	434669	N.D.	2.291 #
26)	Chlordane-4	0.000	8.393	0	52817	N.D.	0.227 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092021\
Data File : PL069920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2021 19:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 02:34:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

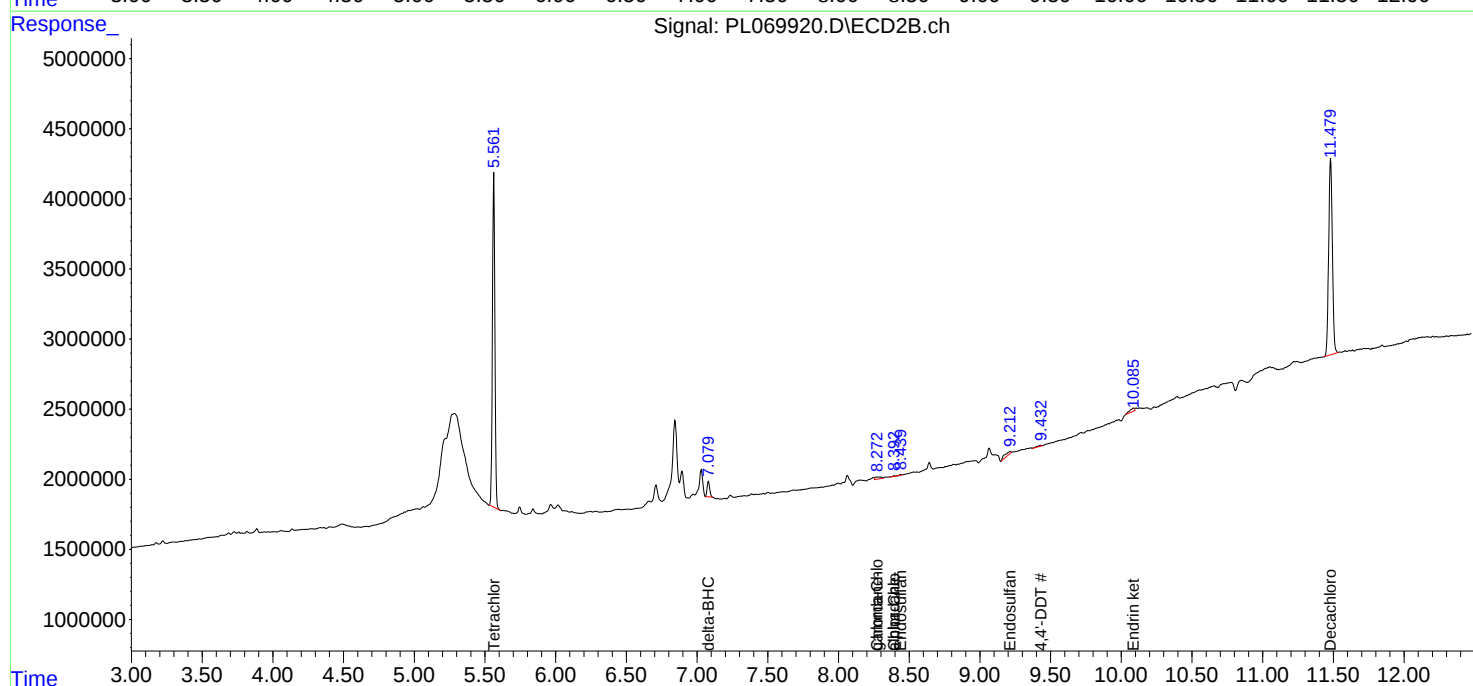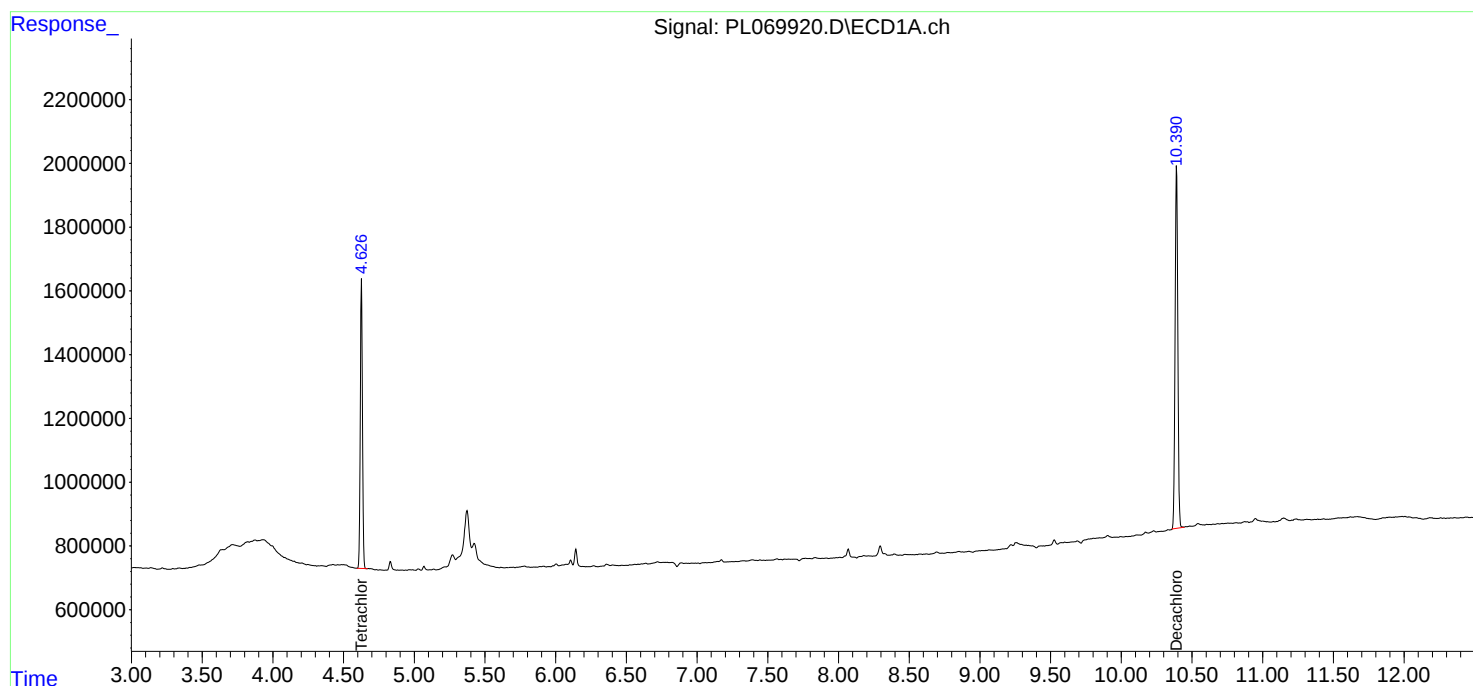


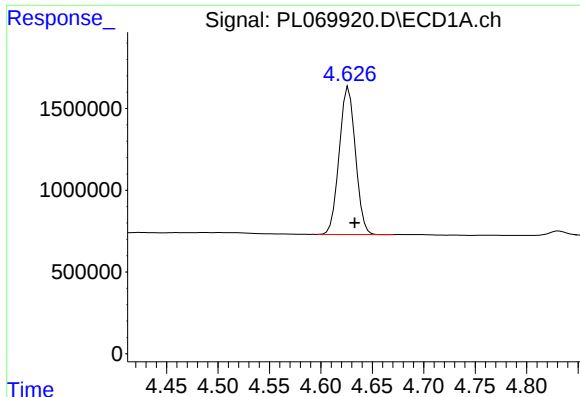

#1 Tetrachloro-m-xylene


R.T.: 4.627 min
Delta R.T.: -0.006 min
Response: 9887841
Conc: 24.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

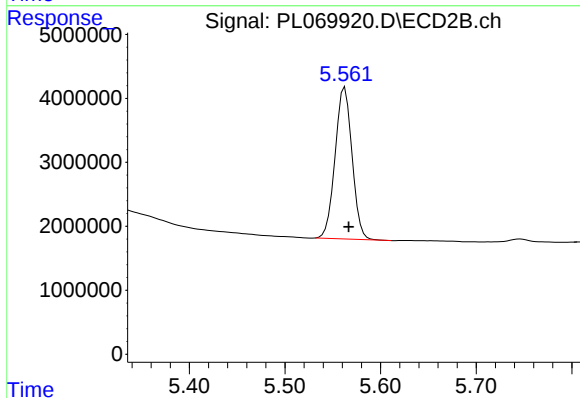


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 29147389
Conc: 23.95 ng/ml

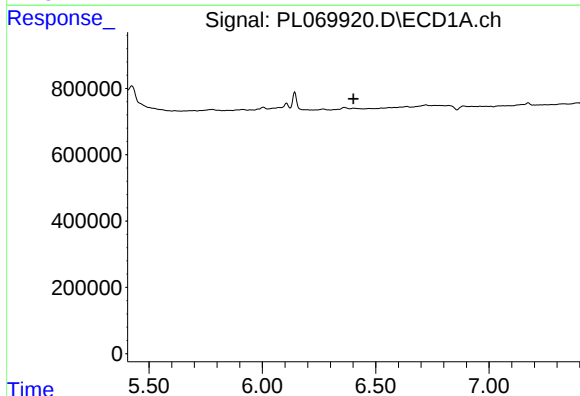


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

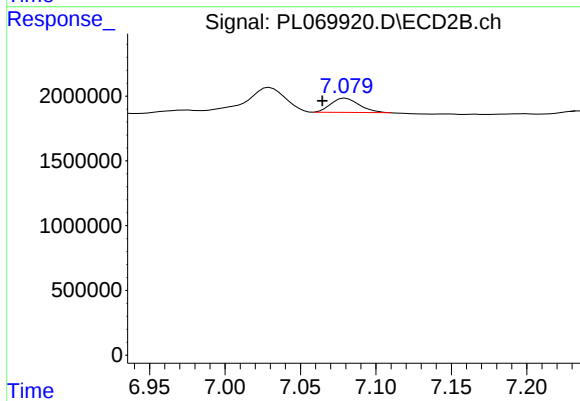

#7 delta-BHC


R.T.: 7.080 min
Delta R.T.: 0.015 min
Response: 1406743
Conc: 0.84 ng/ml

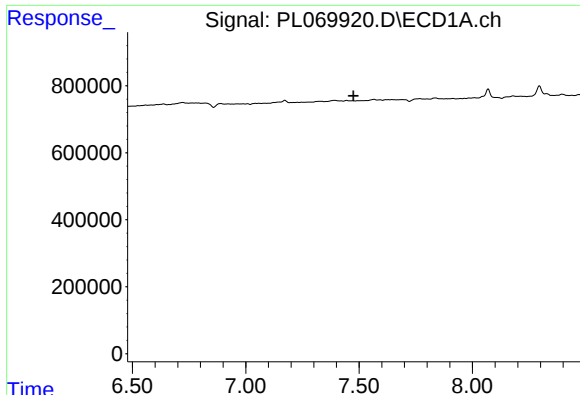

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

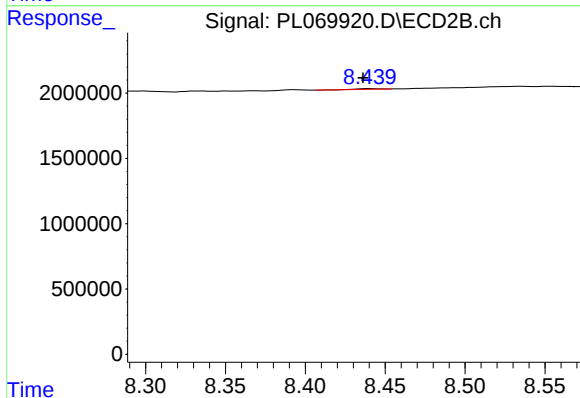


#9 Endosulfan I

R.T.: 8.441 min
Delta R.T.: 0.004 min
Response: 41525
Conc: 0.03 ng/ml

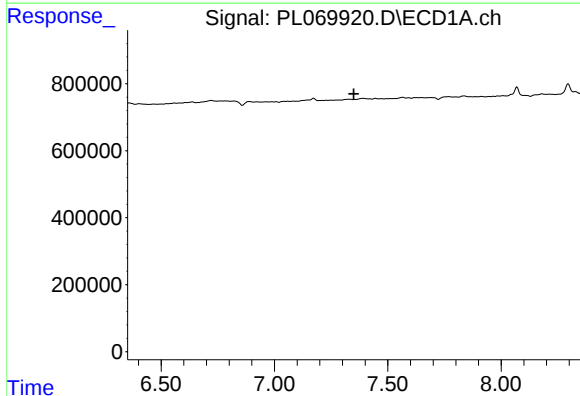


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.

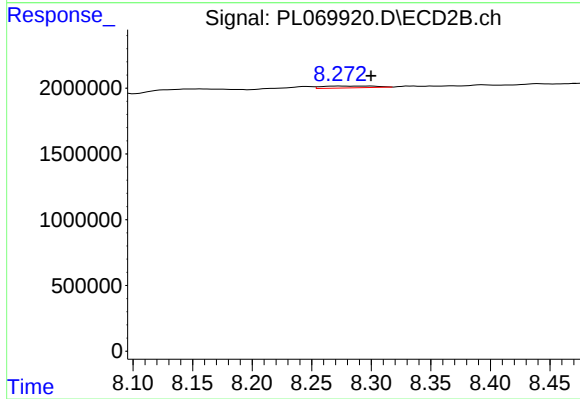

#10 gamma-Chlordane


R.T.: 8.273 min
Delta R.T.: -0.027 min
Response: 434669
Conc: 0.33 ng/ml

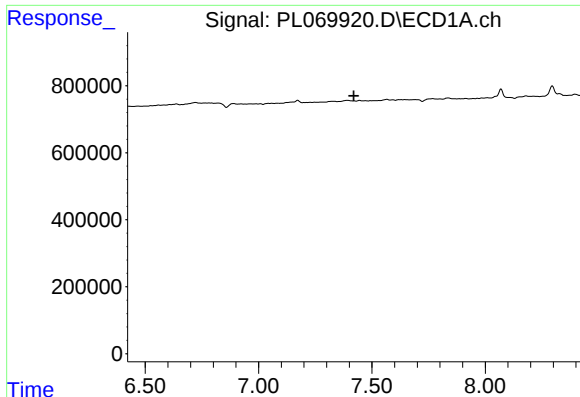

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

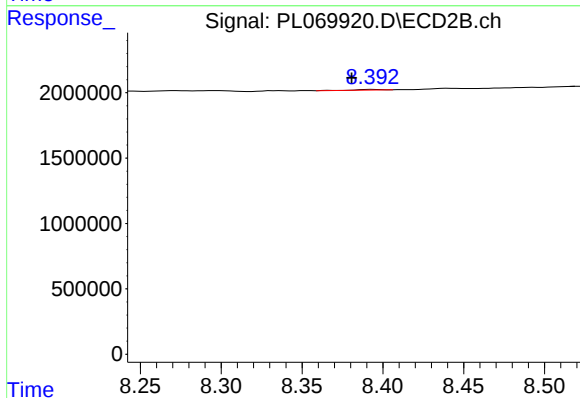


#11 alpha-Chlordane

R.T.: 8.393 min
Delta R.T.: 0.012 min
Response: 52817
Conc: 0.04 ng/ml

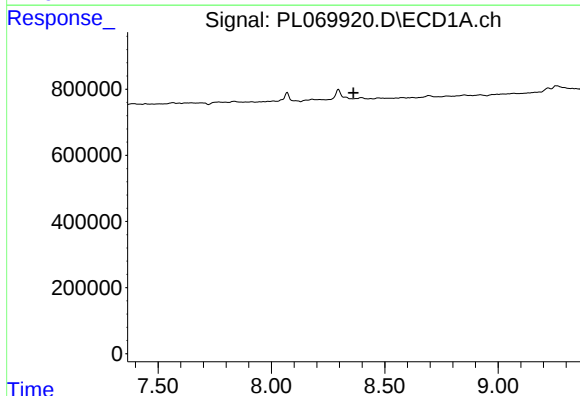


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

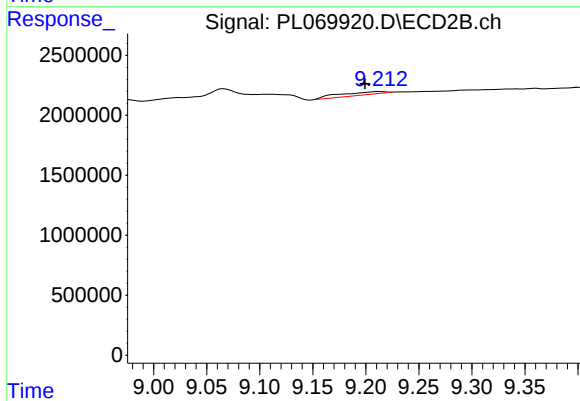

#15 Endosulfan II


R.T.: 9.213 min
Delta R.T.: 0.014 min
Response: 738737
Conc: 0.65 ng/ml

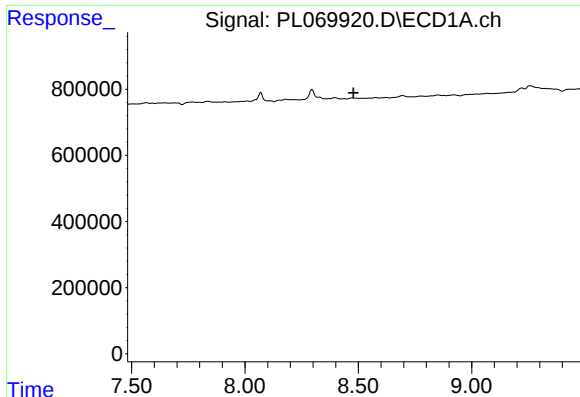

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

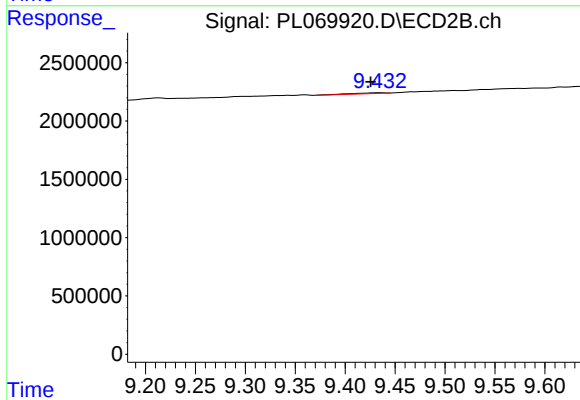


#17 4,4'-DDT

R.T.: 9.434 min
Delta R.T.: 0.009 min
Response: 152641
Conc: 0.14 ng/ml

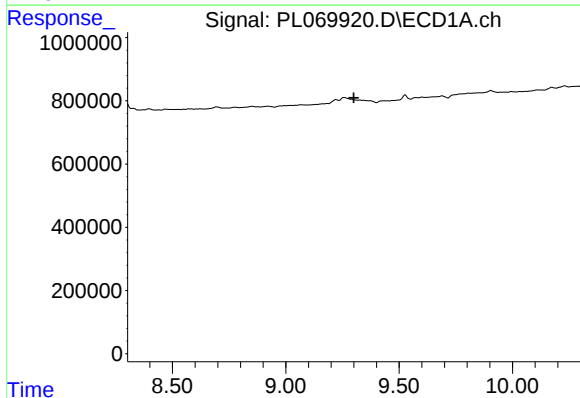


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.301 min
Response: 0
Conc: N.D.

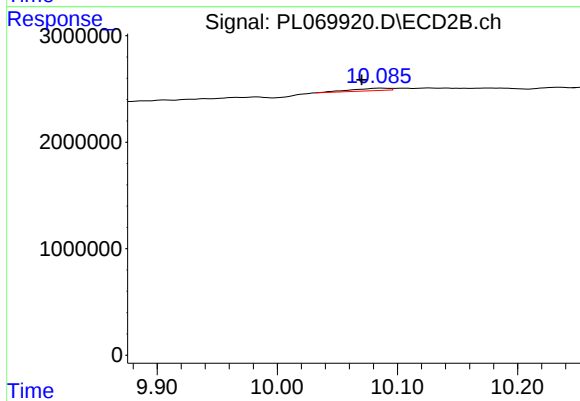

#21 Endrin ketone


R.T.: 10.086 min
Delta R.T.: 0.016 min
Response: 516635
Conc: 0.42 ng/ml

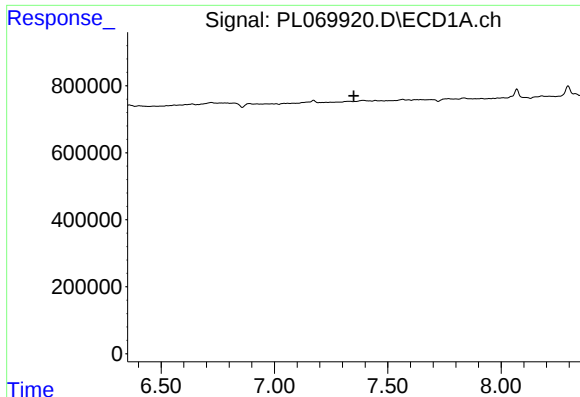

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

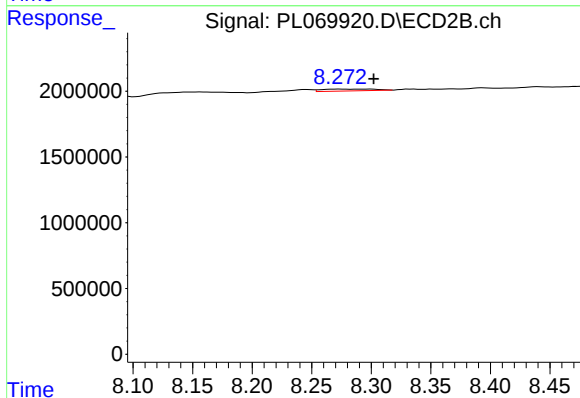


#25 Chlordane-3

R.T.: 8.273 min
Delta R.T.: -0.029 min
Response: 434669
Conc: 2.29 ng/ml

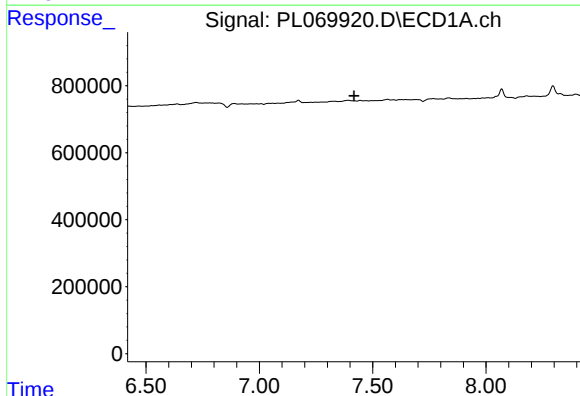


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

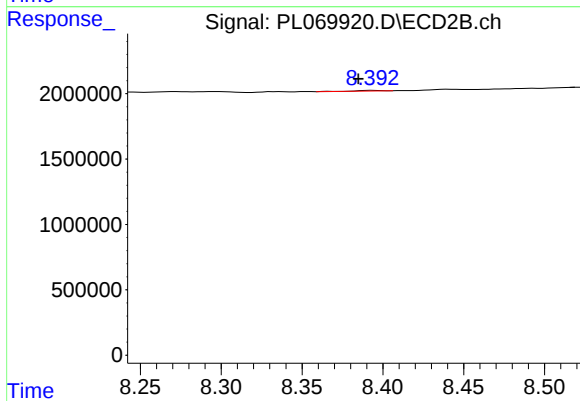

#26 Chlordane-4


R.T.: 8.393 min
Delta R.T.: 0.008 min
Response: 52817
Conc: 0.23 ng/ml

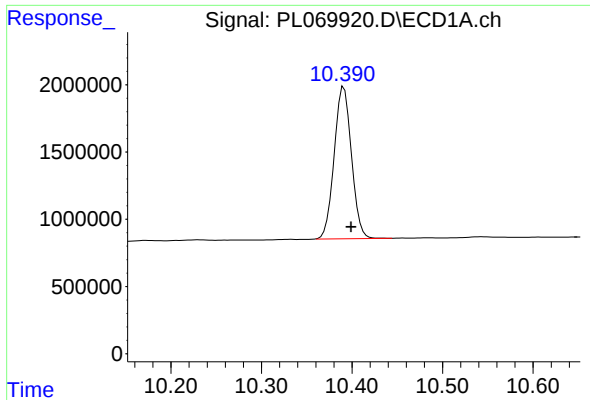

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.008 min
Response: 14979071
Conc: 20.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

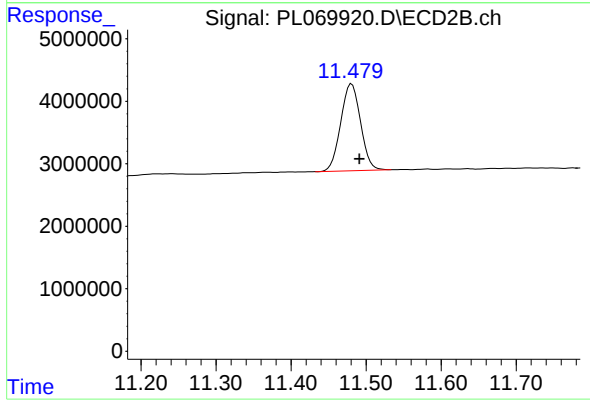

#28 Decachlorobiphenyl

R.T.: 11.481 min
Delta R.T.: -0.011 min
Response: 25563178
Conc: 22.37 ng/ml