

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092022\
 Data File : PL077849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 09:14
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 17:07:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.624	37494313	70861703	23.390	23.869
28)	SA Decachlor...	8.906	7.722	27107996	53784625	20.975	21.426
Target Compounds							
2)	A alpha-BHC	3.881	3.117	26342884	53765421	11.101	11.855
3)	MA gamma-BHC...	4.217	3.440	25256213	47011009	11.416	11.642
5)	MB Aldrin	0.000	4.064	0	212577	N.D.	0.056 #
6)	B beta-BHC	4.430	3.740	11576629	19706240	11.912	11.837
8)	B Heptachlo...	5.570	0.000	15374554	0	8.819	N.D. #
9)	A Endosulfan I	0.000	4.929	0	274499	N.D.	0.087 #
10)	B gamma-Chl...	0.000	4.793	0	1192171	N.D.	0.350 #
13)	MA Dieldrin	0.000	5.170	0	4442599	N.D.	1.340 #
14)	MA Endrin	6.461	5.446	71837918	156.4E6	51.944	54.847
15)	B Endosulfa...	6.708f	5.765f	2265252	-743484	1.640	N.D. #
16)	A 4,4'-DDD	0.000	5.604	0	460093	N.D.	0.178 #
17)	MA 4,4'-DDT	6.913	5.852	141.7E6	296.6E6	111.866	112.580
18)	B Endrin al...	6.820	5.923	1586804	4249763	1.501	2.059 #
20)	A Methoxychlor	7.394	6.429	178.7E6	364.7E6	270.597	266.281
21)	B Endrin ke...	7.542	6.642	3332852	18544332	2.412	6.124 #
25)	Chlordane-3	0.000	4.793	0	1192171	N.D.	3.466 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092022\
Data File : PL077849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 09:14
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 17:07:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

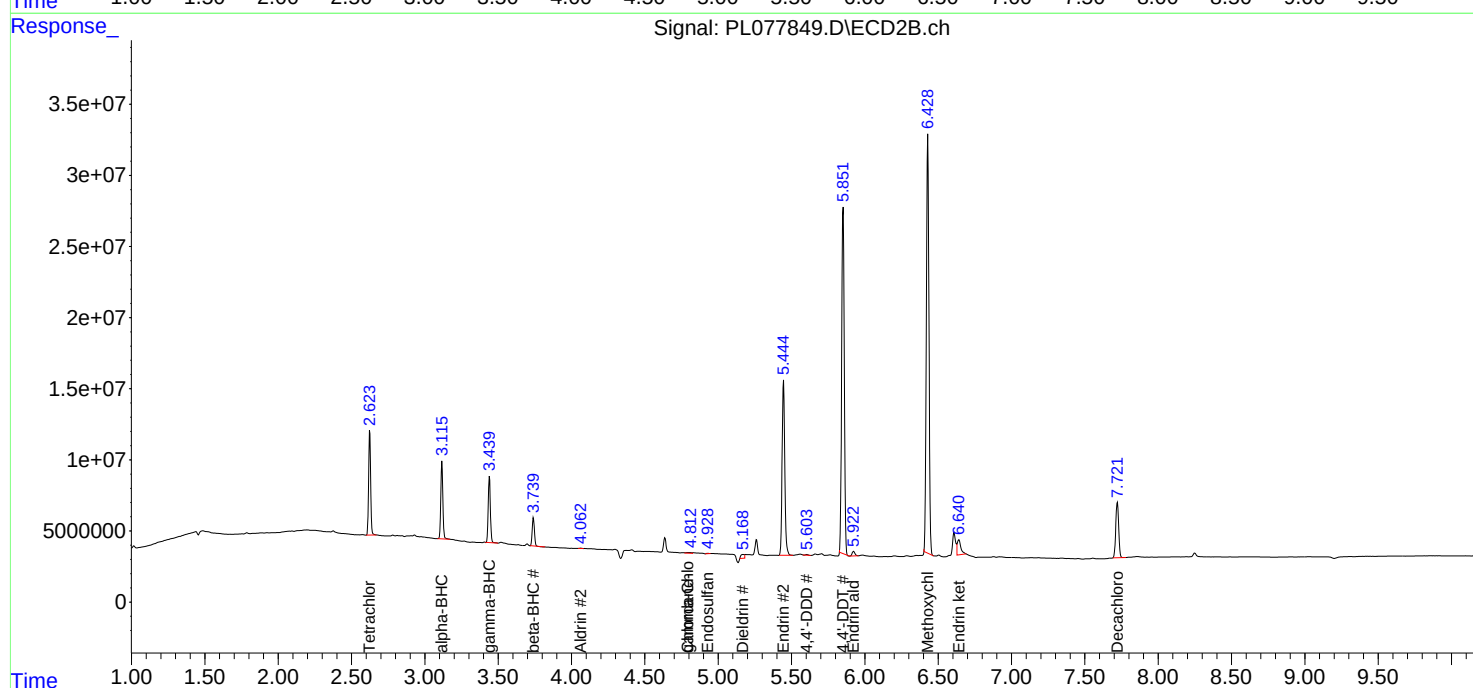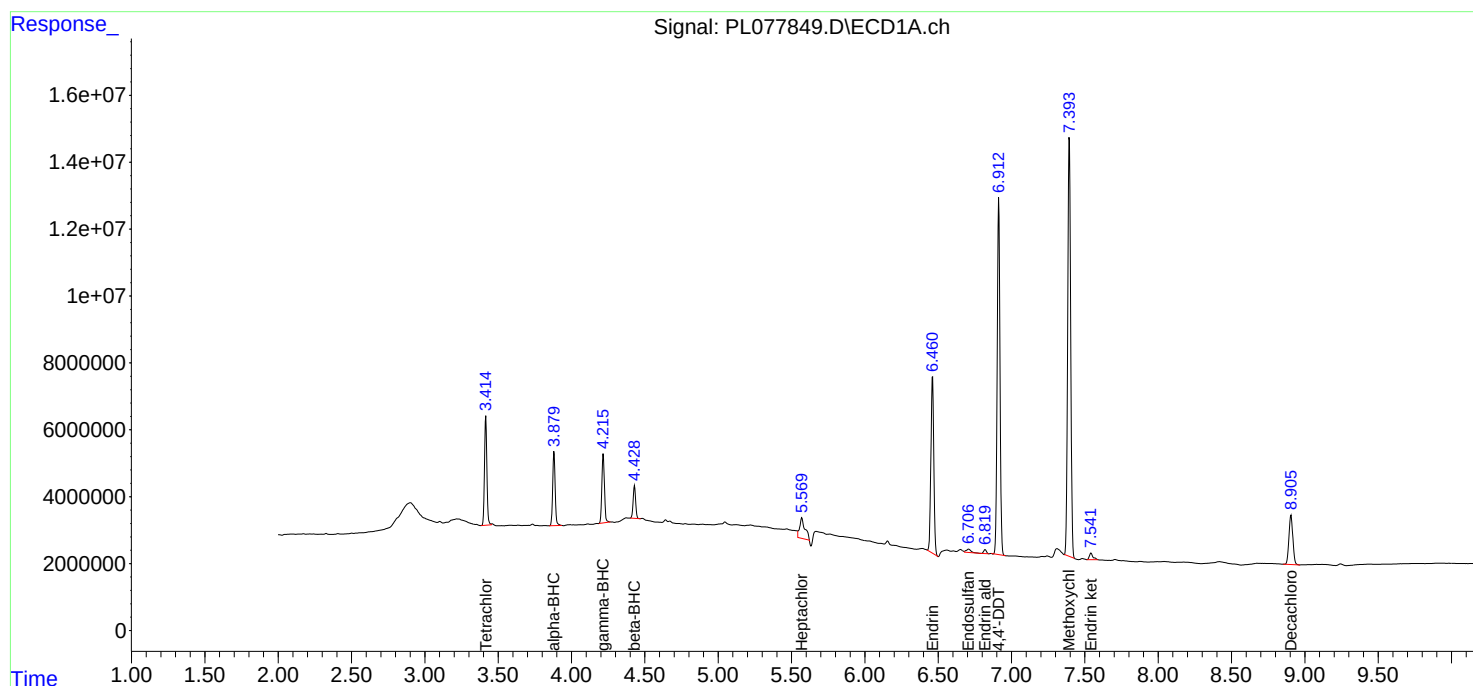


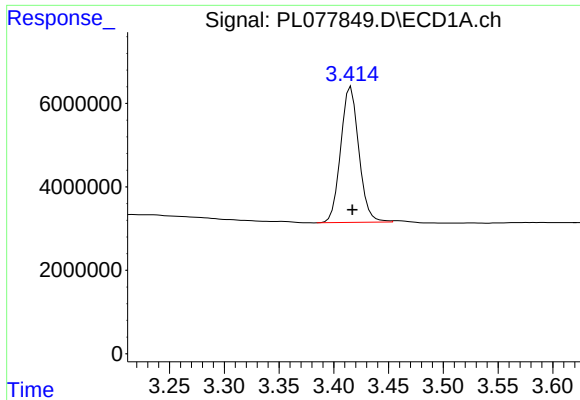

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: -0.001 min
Response: 37494313
Conc: 23.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

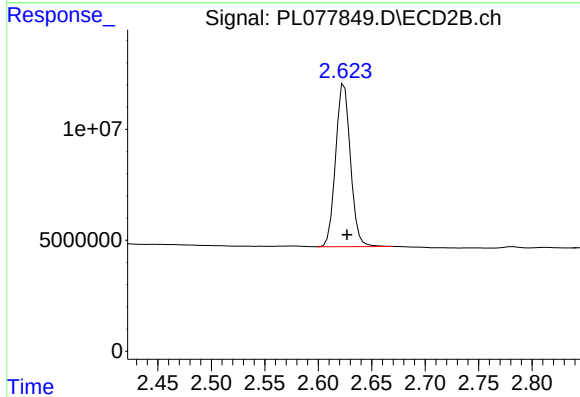


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: -0.003 min
Response: 70861703
Conc: 23.87 ng/ml

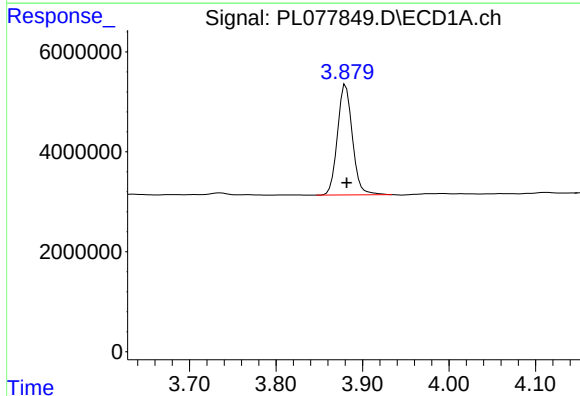


#2 alpha-BHC

R.T.: 3.881 min
Delta R.T.: -0.001 min
Response: 26342884
Conc: 11.10 ng/ml

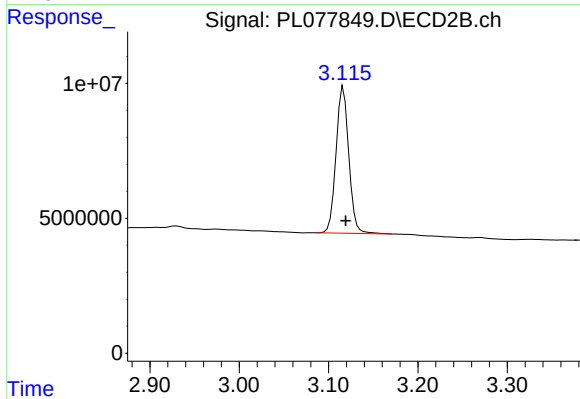

#2 alpha-BHC


R.T.: 3.117 min
Delta R.T.: -0.003 min
Response: 53765421
Conc: 11.86 ng/ml

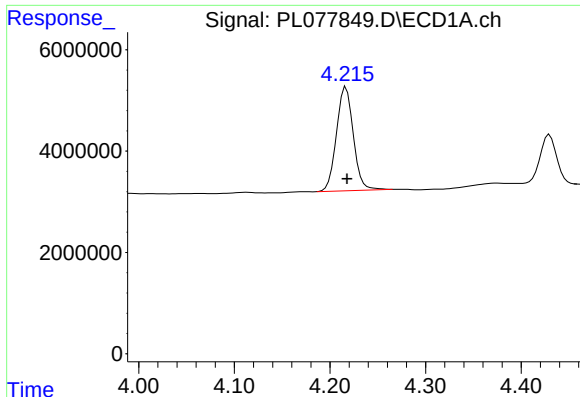

#3 gamma-BHC (Lindane)


R.T.: 4.217 min
Delta R.T.: 0.000 min
Response: 25256213
Conc: 11.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

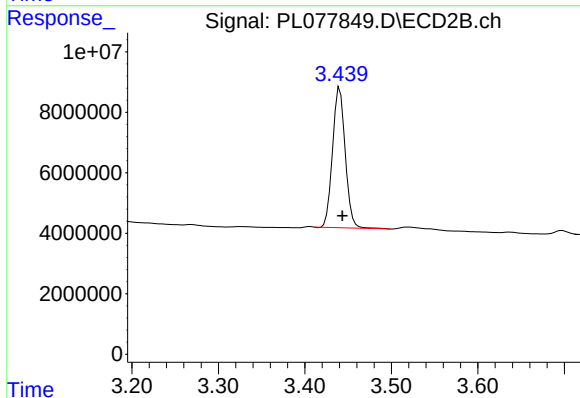


#3 gamma-BHC (Lindane)

R.T.: 3.440 min
Delta R.T.: -0.003 min
Response: 47011009
Conc: 11.64 ng/ml

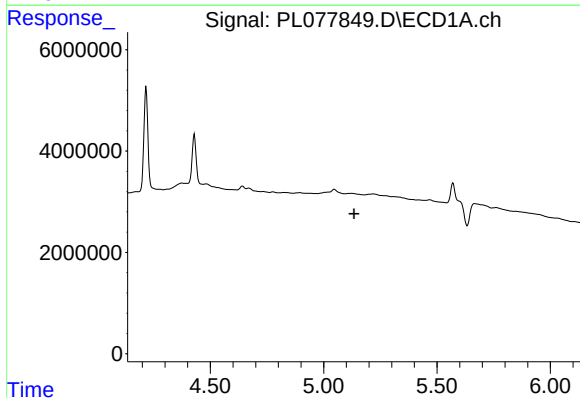


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.134 min
Response: 0
Conc: N.D.

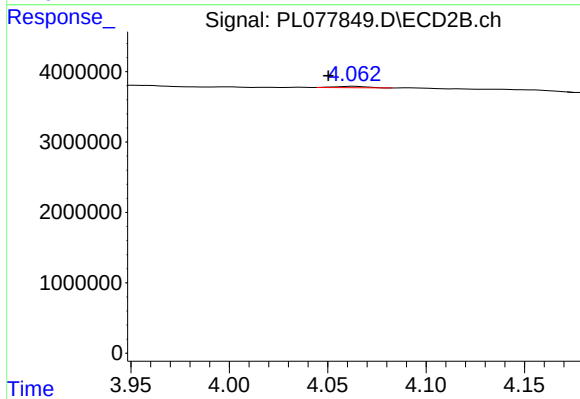

#5 Aldrin


R.T.: 4.064 min
Delta R.T.: 0.013 min
Response: 212577
Conc: 0.06 ng/ml

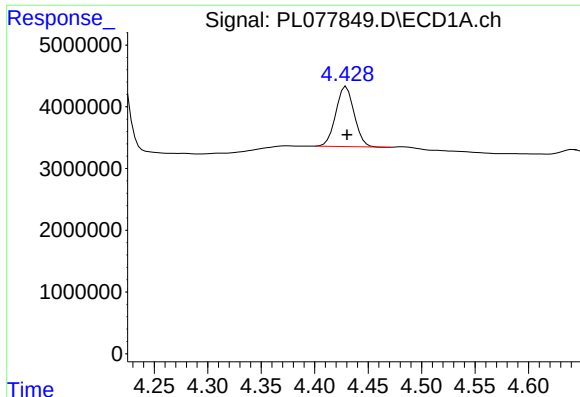

#6 beta-BHC


R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 11576629
Conc: 11.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

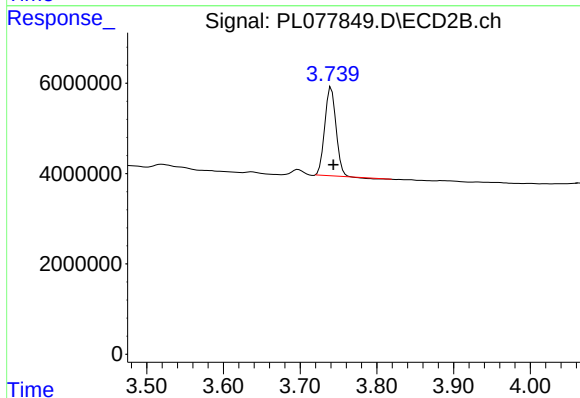


#6 beta-BHC

R.T.: 3.740 min
Delta R.T.: -0.003 min
Response: 19706240
Conc: 11.84 ng/ml

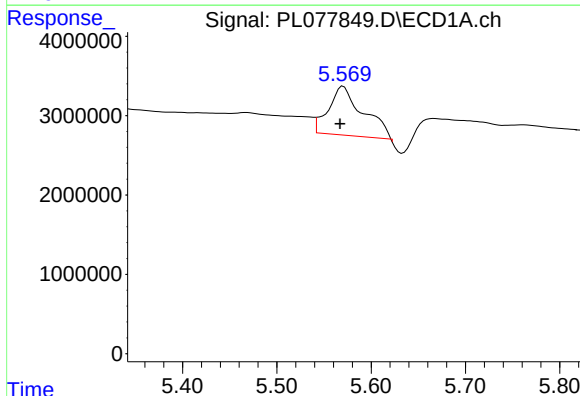


#8 Heptachlor epoxide

R.T.: 5.570 min
Delta R.T.: 0.003 min
Response: 15374554
Conc: 8.82 ng/ml

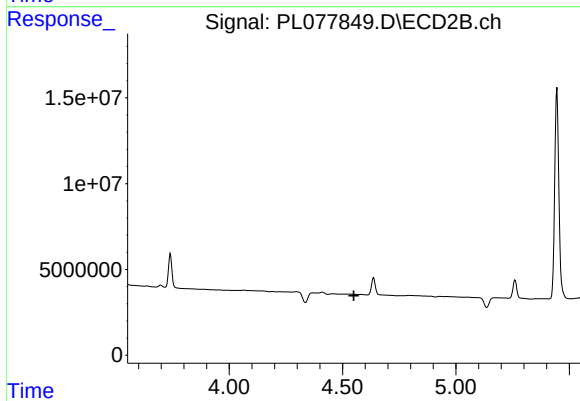

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.549 min
Response: 0
Conc: N.D.

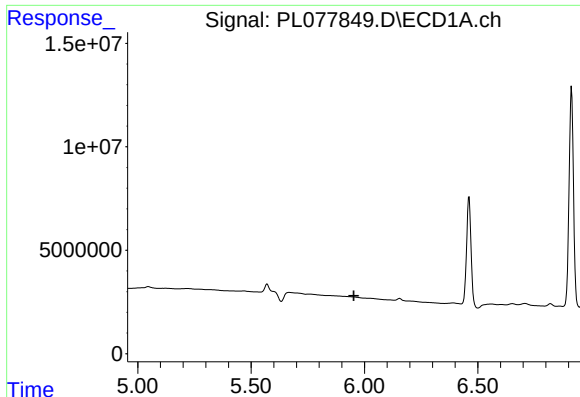

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

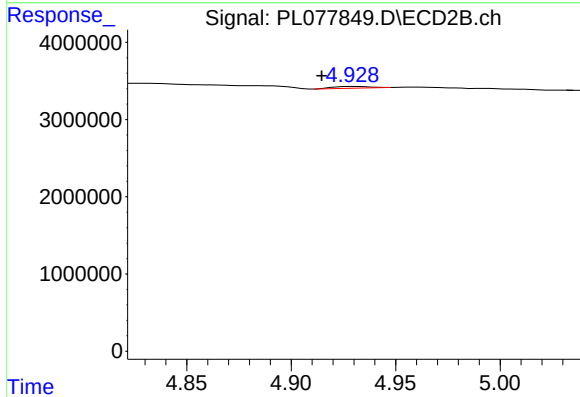


#9 Endosulfan I

R.T.: 4.929 min
Delta R.T.: 0.015 min
Response: 274499
Conc: 0.09 ng/ml

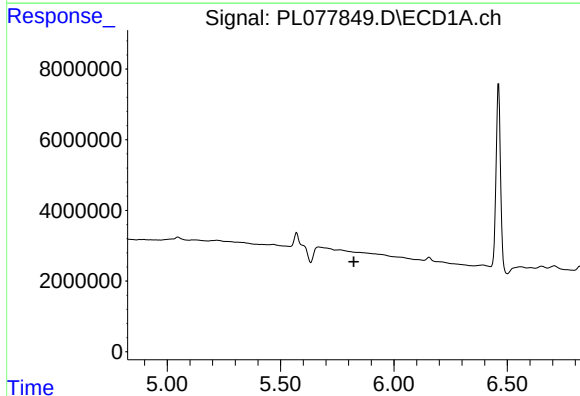


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

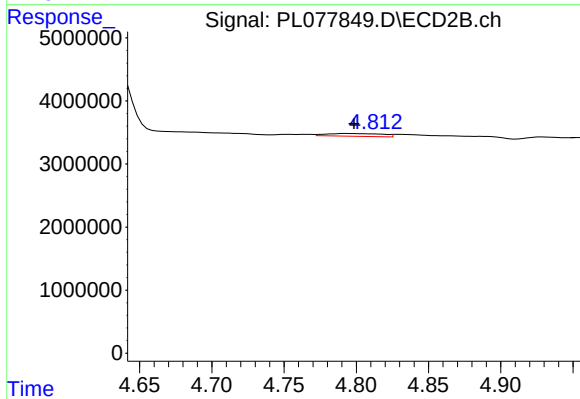

#10 gamma-Chlordane


R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 1192171
Conc: 0.35 ng/ml

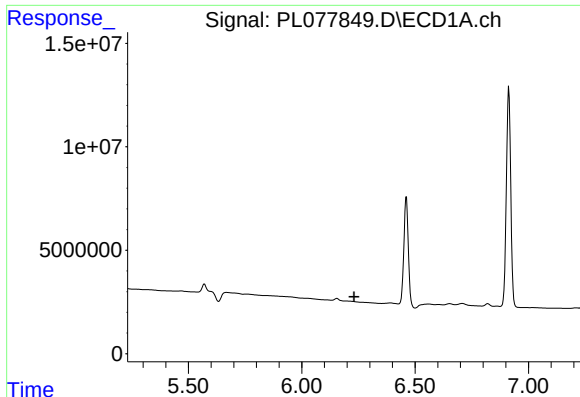

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

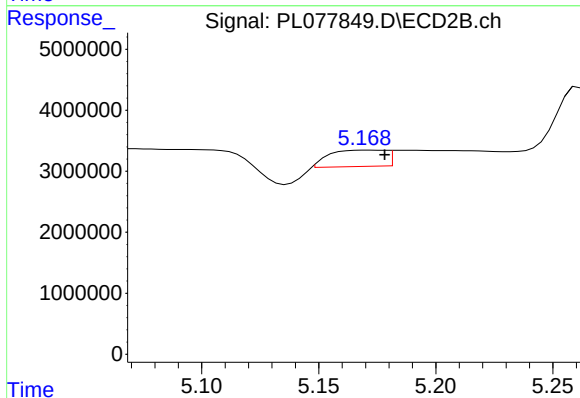


#13 Dieldrin

R.T.: 5.170 min
Delta R.T.: -0.008 min
Response: 4442599
Conc: 1.34 ng/ml

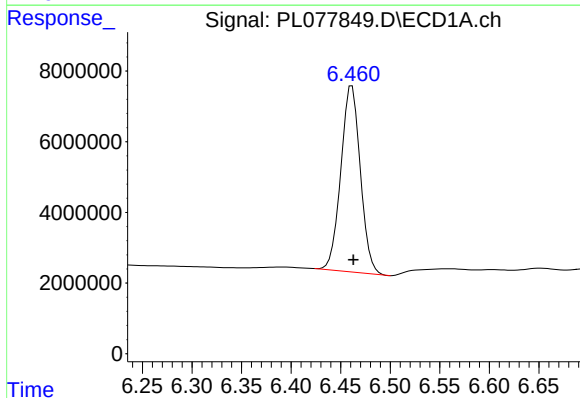


#14 Endrin

R.T.: 6.461 min
Delta R.T.: -0.001 min
Response: 71837918
Conc: 51.94 ng/ml

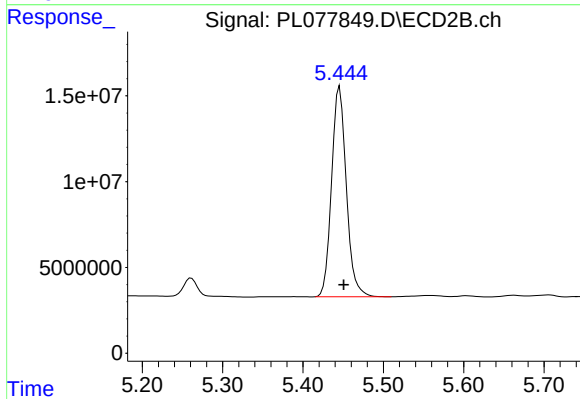

#14 Endrin


R.T.: 5.446 min
Delta R.T.: -0.005 min
Response: 156393773
Conc: 54.85 ng/ml

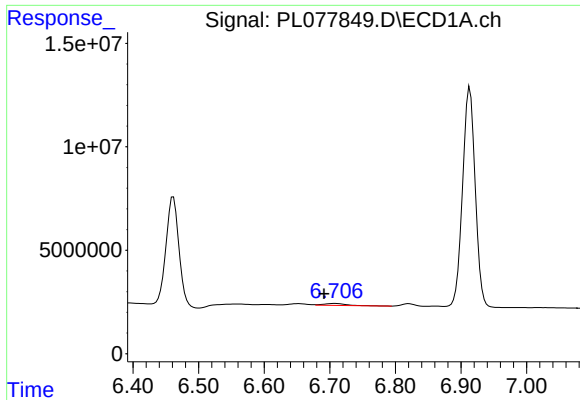

#15 Endosulfan II


R.T.: 6.708 min
Delta R.T.: 0.017 min
Response: 2265252
Conc: 1.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

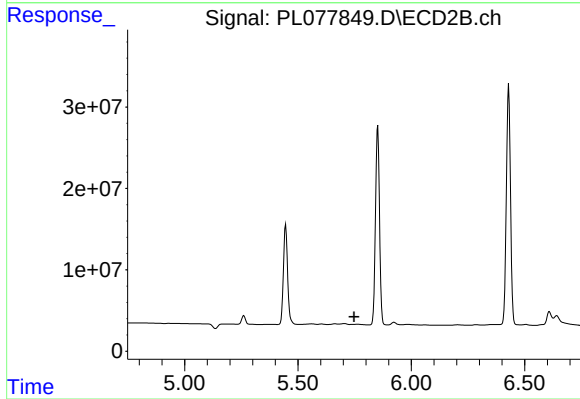


#15 Endosulfan II

R.T.: 5.765 min
Delta R.T.: 0.018 min
Response: -743484
Conc: N.D.

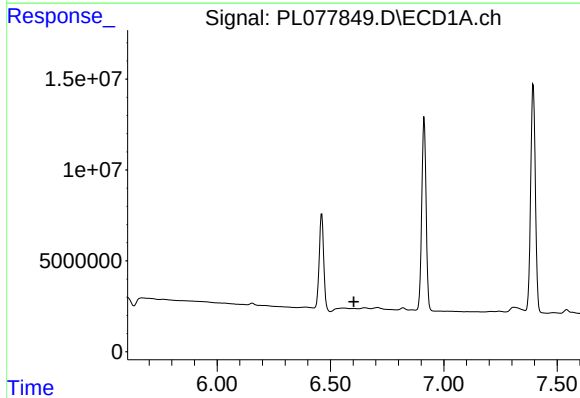


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.604 min
Response: 0
Conc: N.D.

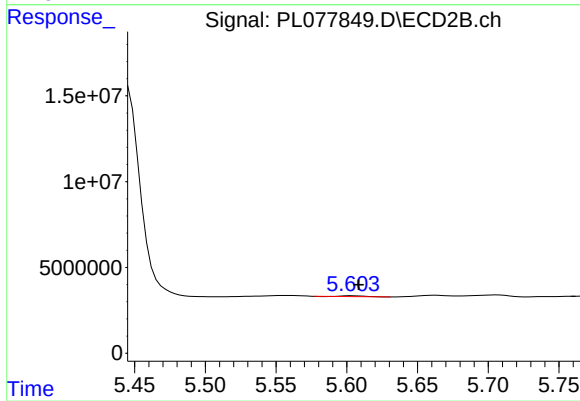

#16 4,4'-DDD


R.T.: 5.604 min
Delta R.T.: -0.004 min
Response: 460093
Conc: 0.18 ng/ml

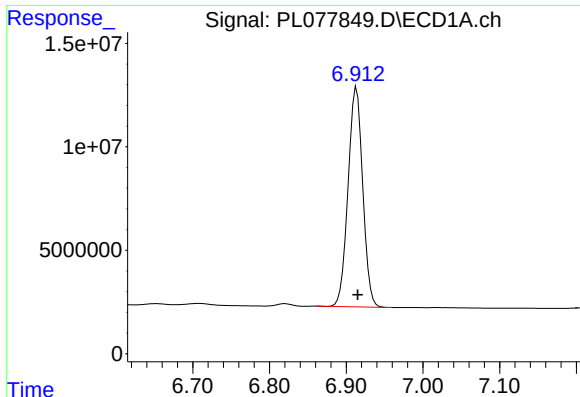

#17 4,4'-DDT


R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 141749430
Conc: 111.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

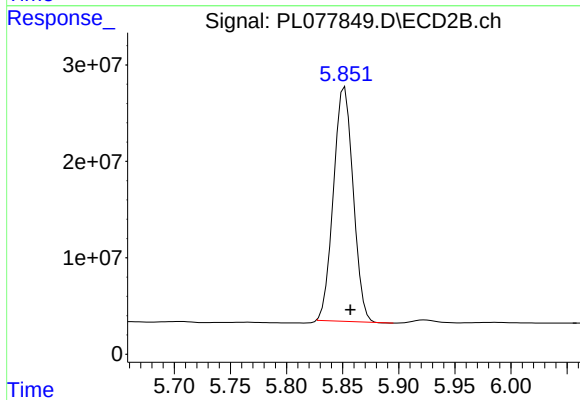


#17 4,4'-DDT

R.T.: 5.852 min
Delta R.T.: -0.005 min
Response: 296624259
Conc: 112.58 ng/ml

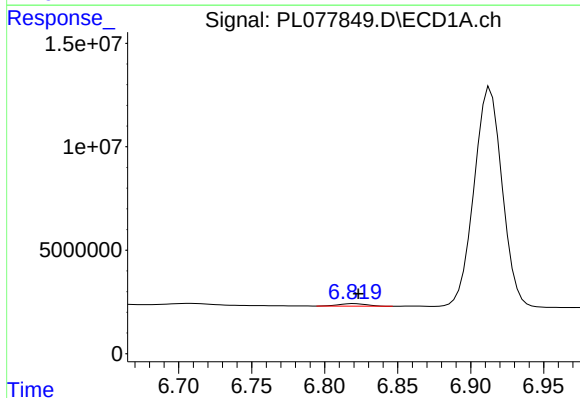


#18 Endrin aldehyde

R.T.: 6.820 min
Delta R.T.: -0.003 min
Response: 1586804
Conc: 1.50 ng/ml

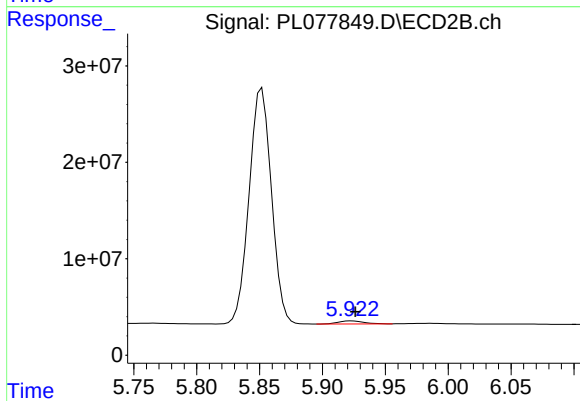

#18 Endrin aldehyde


R.T.: 5.923 min
Delta R.T.: -0.003 min
Response: 4249763
Conc: 2.06 ng/ml

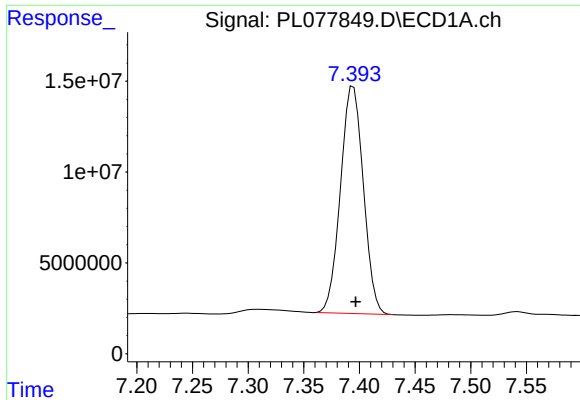

#20 Methoxychlor


R.T.: 7.394 min
Delta R.T.: -0.002 min
Response: 178716207
Conc: 270.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

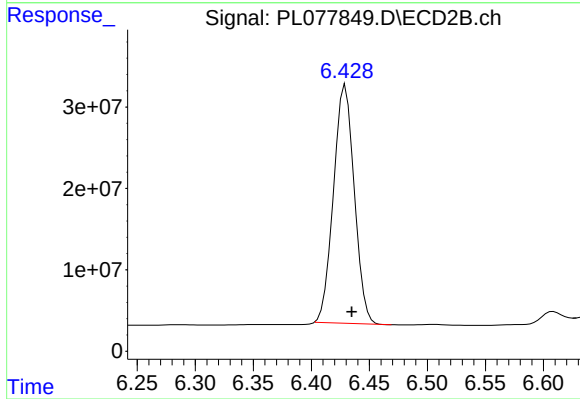


#20 Methoxychlor

R.T.: 6.429 min
Delta R.T.: -0.005 min
Response: 364652270
Conc: 266.28 ng/ml

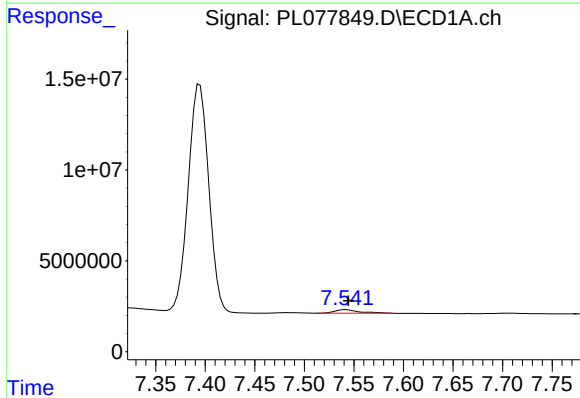


#21 Endrin ketone

R.T.: 7.542 min
Delta R.T.: -0.002 min
Response: 3332852
Conc: 2.41 ng/ml

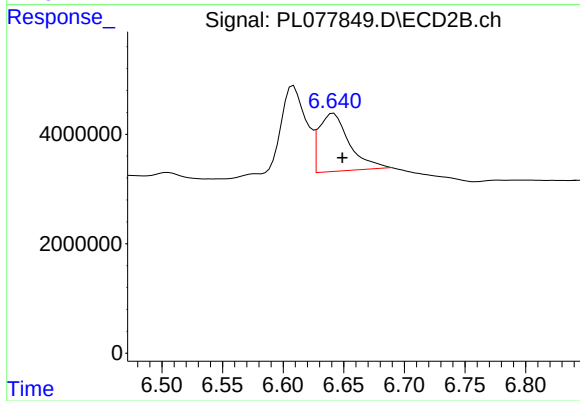

#21 Endrin ketone


R.T.: 6.642 min
Delta R.T.: -0.007 min
Response: 18544332
Conc: 6.12 ng/ml

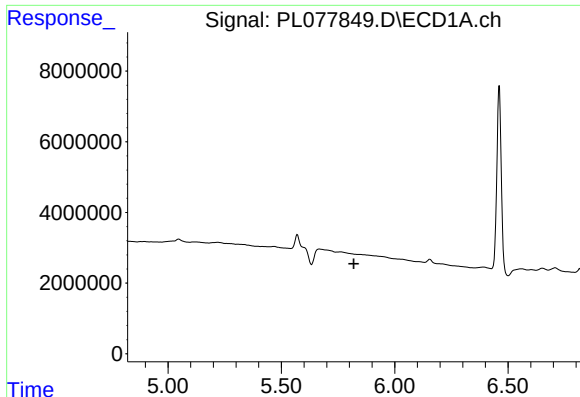

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

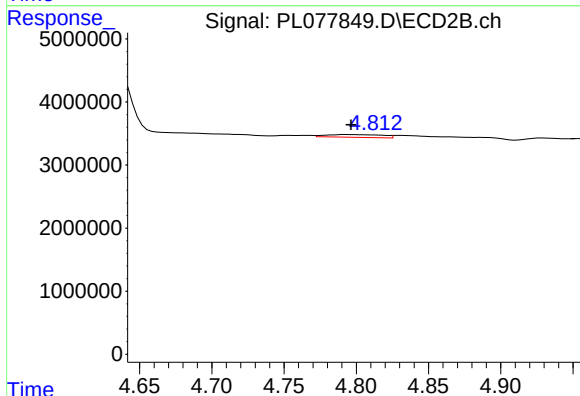


#25 Chlordane-3

R.T.: 4.793 min
Delta R.T.: -0.004 min
Response: 1192171
Conc: 3.47 ng/ml

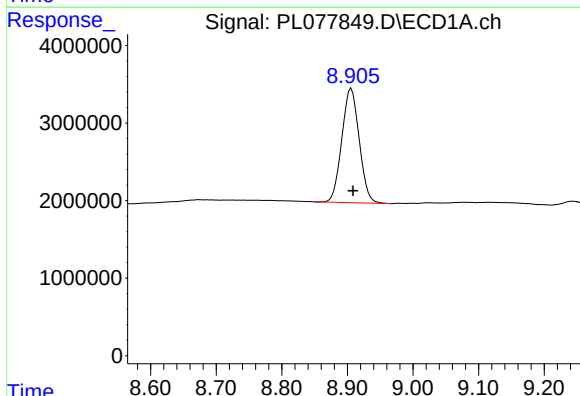

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: -0.002 min
Response: 27107996
Conc: 20.97 ng/ml

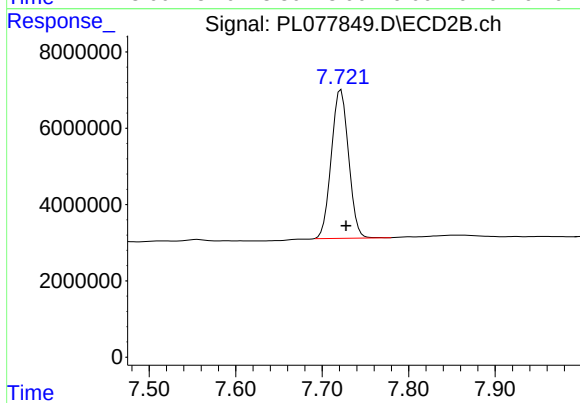

#28 Decachlorobiphenyl

R.T.: 7.722 min
Delta R.T.: -0.006 min
Response: 53784625
Conc: 21.43 ng/ml