

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092022\
 Data File : PL077852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 11:44
 Operator : AR\AJ
 Sample : PB147675BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 17:07:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	2.623	29509240	55377828	18.409	18.654
28)	SA Decachlor...	8.915	7.727	26346074	49179805	20.385	19.592
Target Compounds							
2)	A alpha-BHC	3.890	0.000	145475	0	0.061	N.D. #
3)	MA gamma-BHC...	4.221	0.000	119949	0	0.054	N.D. #
7)	B delta-BHC	4.679	0.000	557464	0	0.272	N.D. #
9)	A Endosulfan I	0.000	4.935f	0	1462843	N.D.	0.464 #
10)	B gamma-Chl...	0.000	4.792	0	331807	N.D.	0.097 #
18)	B Endrin al...	0.000	5.920	0	2754298	N.D.	1.335 #
21)	B Endrin ke...	0.000	6.652	0	3110862	N.D.	1.027 #
22)	Mirex	8.001	6.837	1086514	136350	1.035	0.063 #
25)	Chlordane-3	0.000	4.792	0	331807	N.D.	0.965 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092022\
Data File : PL077852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 11:44
Operator : AR\AJ
Sample : PB147675BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 17:07:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

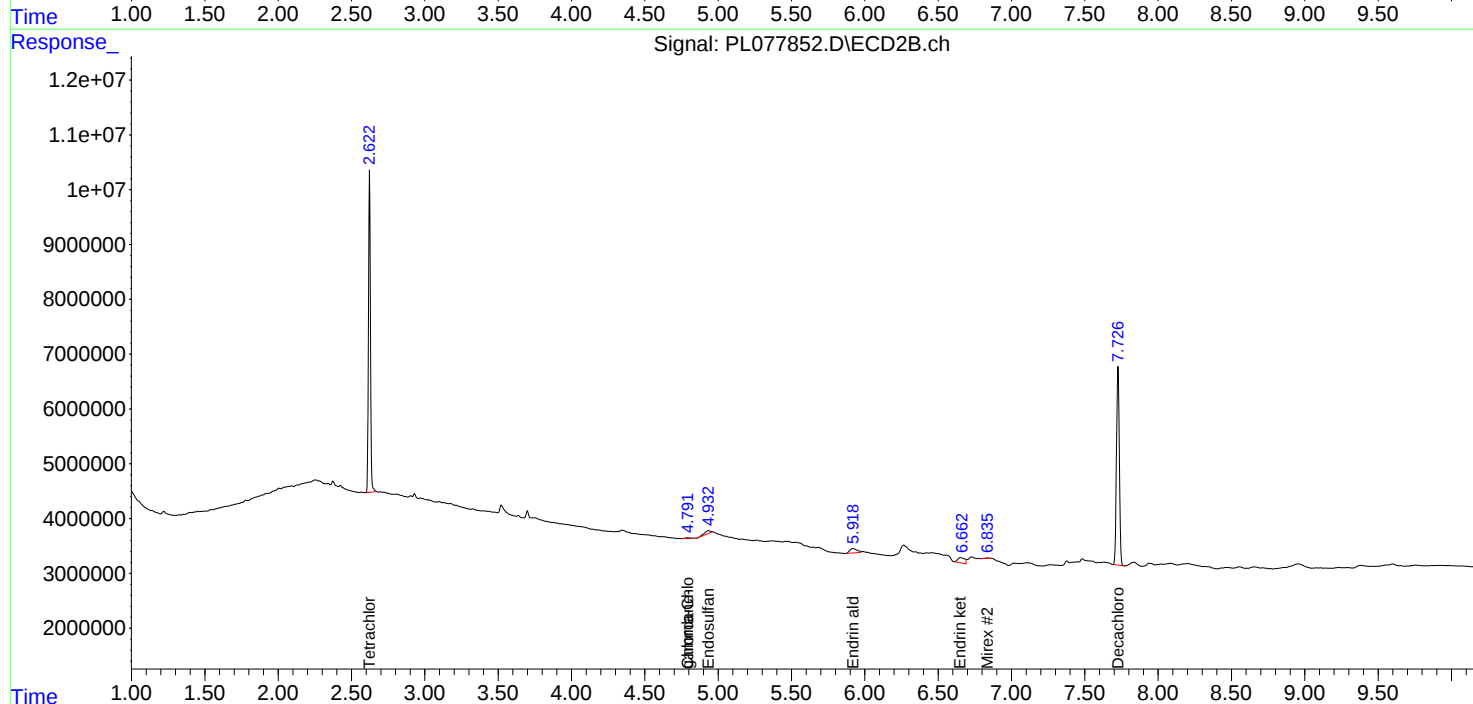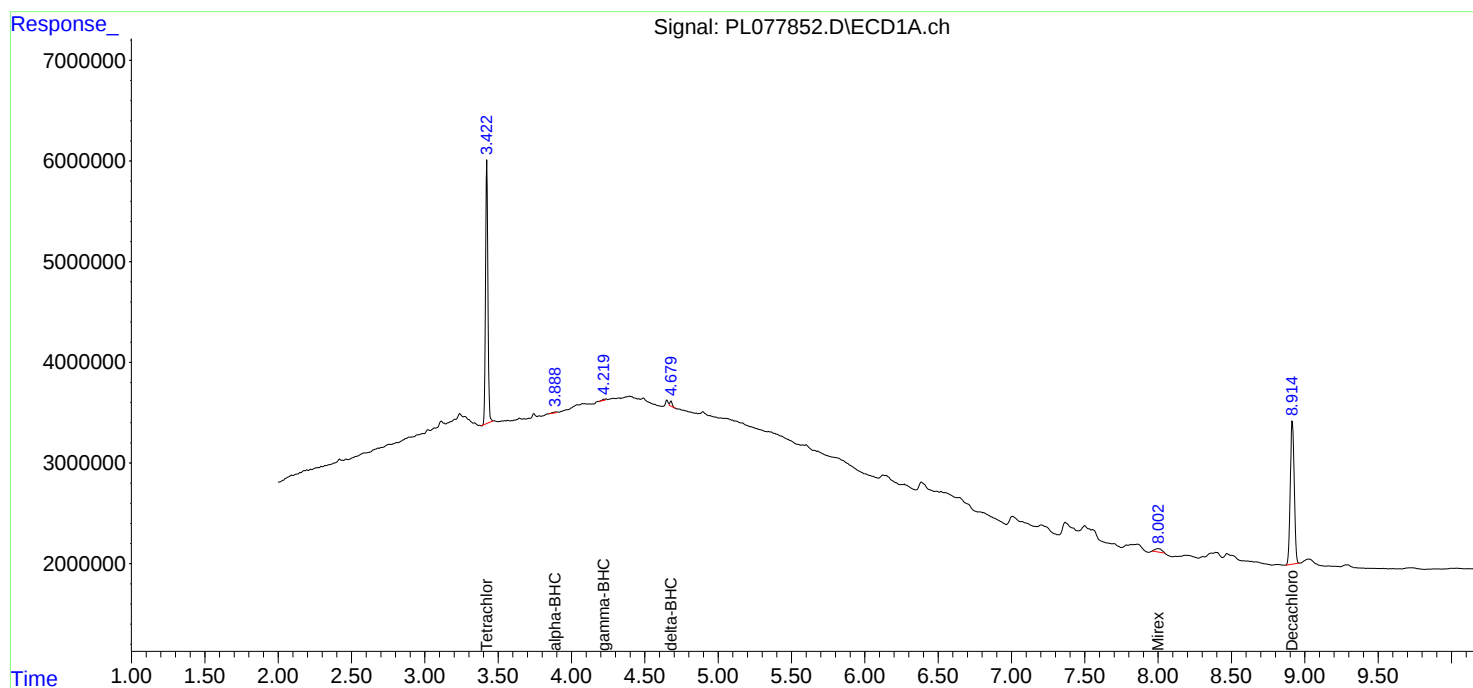


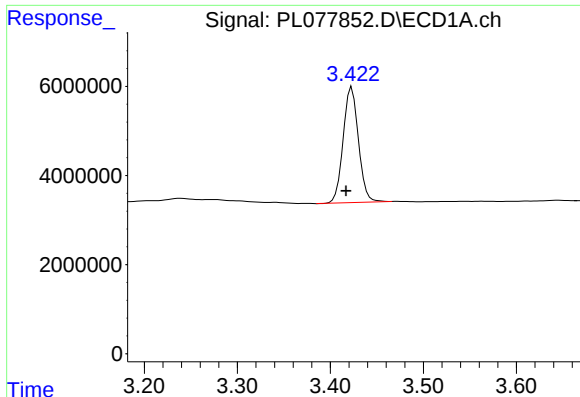

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.006 min
Response: 29509240
Conc: 18.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

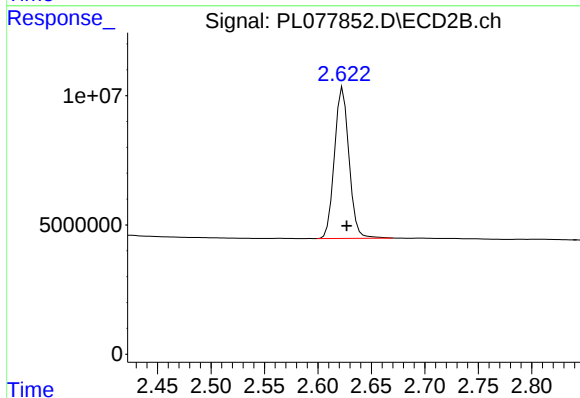


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: -0.003 min
Response: 55377828
Conc: 18.65 ng/ml

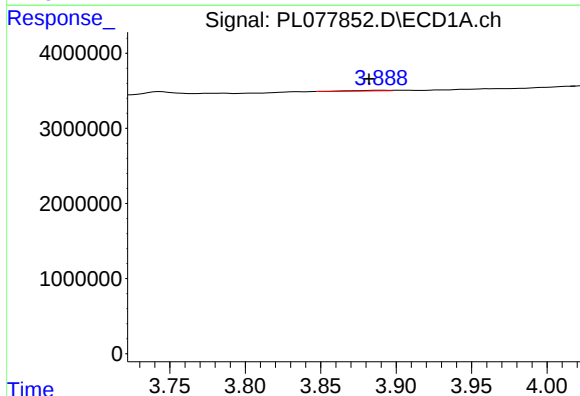


#2 alpha-BHC

R.T.: 3.890 min
Delta R.T.: 0.008 min
Response: 145475
Conc: 0.06 ng/ml

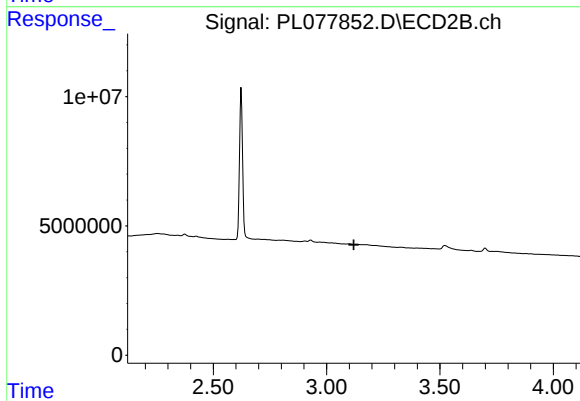

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.119 min
Response: 0
Conc: N.D.

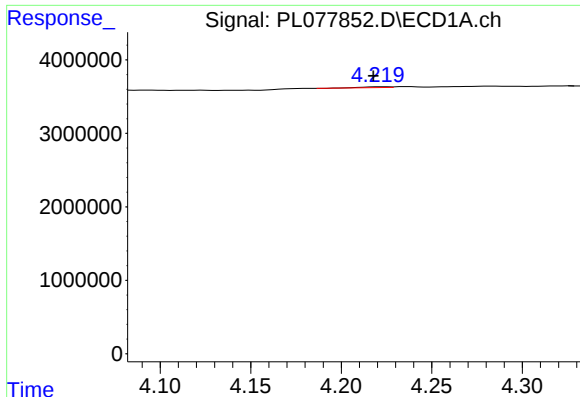

#3 gamma-BHC (Lindane)


R.T.: 4.221 min
Delta R.T.: 0.003 min
Response: 119949
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

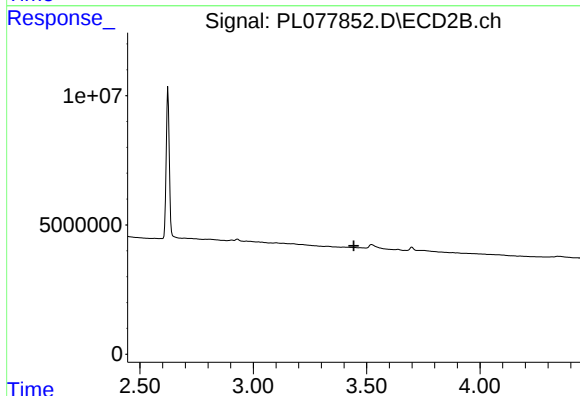


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.443 min
Response: 0
Conc: N.D.

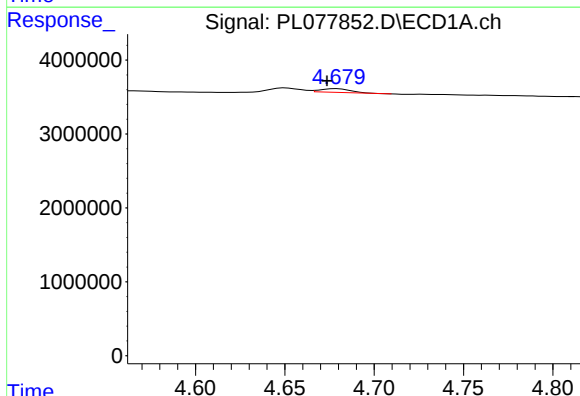


#7 delta-BHC

R.T.: 4.679 min
Delta R.T.: 0.005 min
Response: 557464
Conc: 0.27 ng/ml

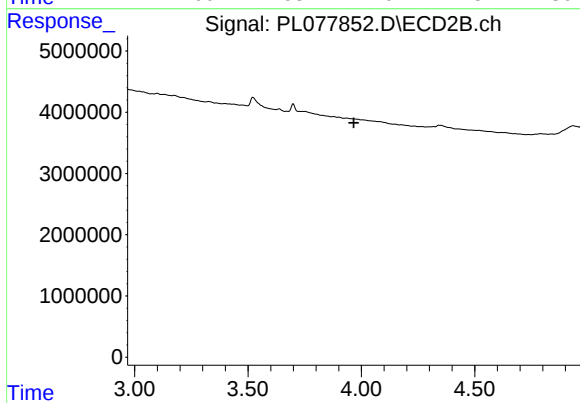

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

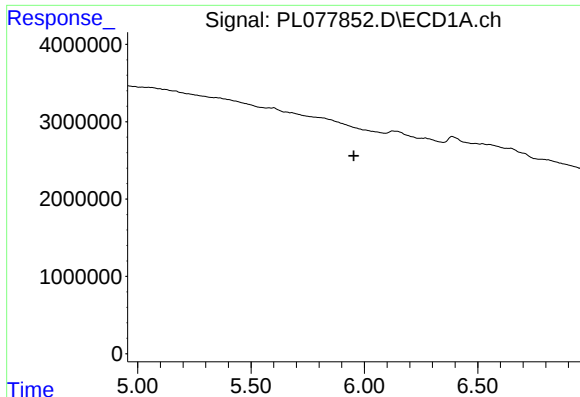

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

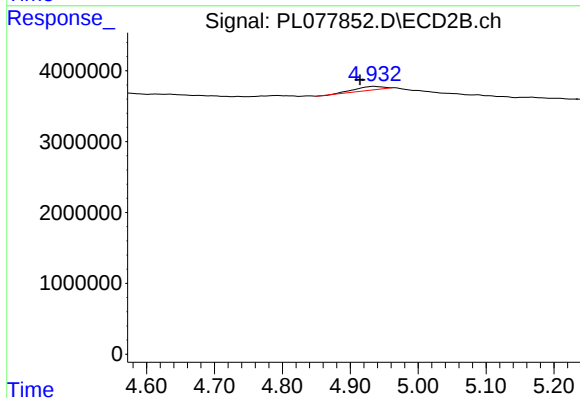


#9 Endosulfan I

R.T.: 4.935 min
Delta R.T.: 0.020 min
Response: 1462843
Conc: 0.46 ng/ml

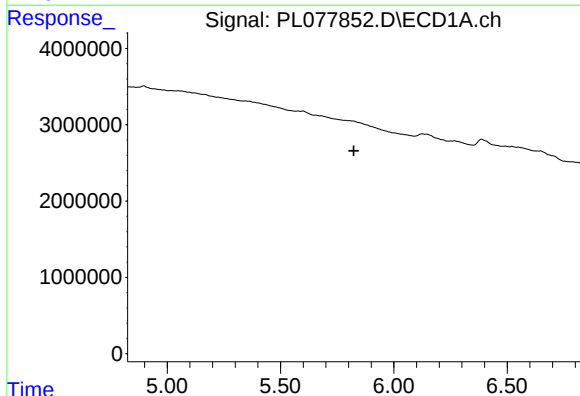


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

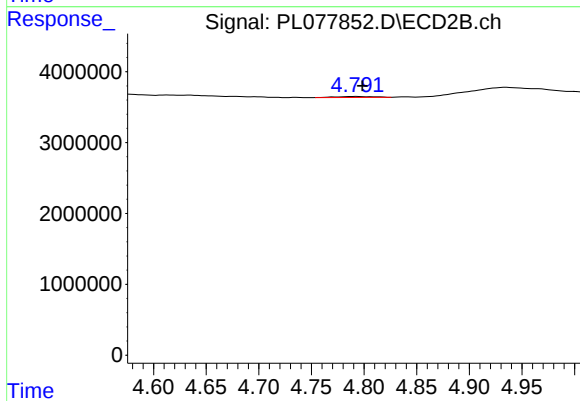

#10 gamma-Chlordane


R.T.: 4.792 min
Delta R.T.: -0.006 min
Response: 331807
Conc: 0.10 ng/ml

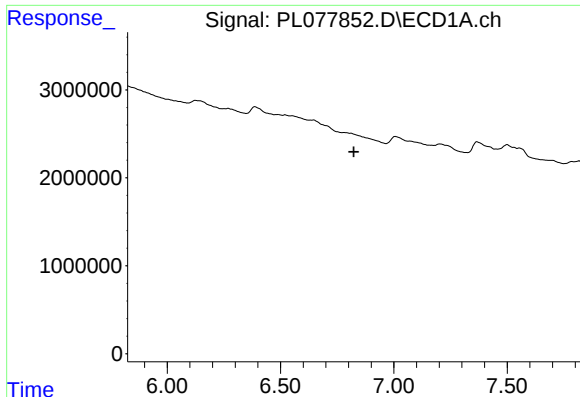

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

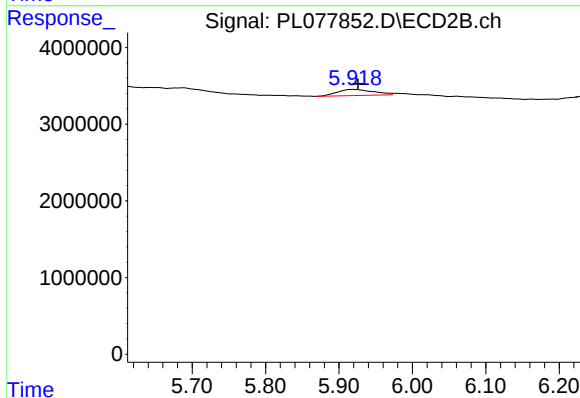


#18 Endrin aldehyde

R.T.: 5.920 min
Delta R.T.: -0.006 min
Response: 2754298
Conc: 1.33 ng/ml

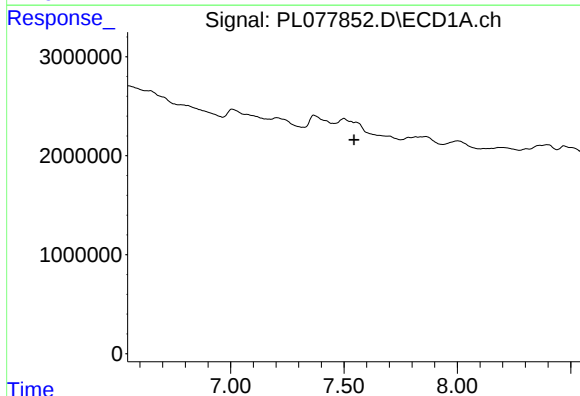


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.544 min
Response: 0
Conc: N.D.

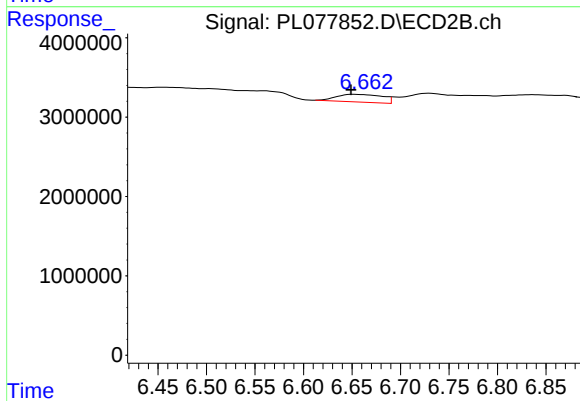

#21 Endrin ketone


R.T.: 6.652 min
Delta R.T.: 0.003 min
Response: 3110862
Conc: 1.03 ng/ml

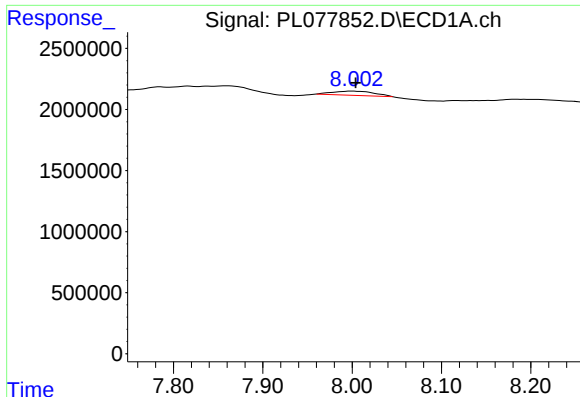

#22 Mirex


R.T.: 8.001 min
Delta R.T.: -0.003 min
Response: 1086514
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

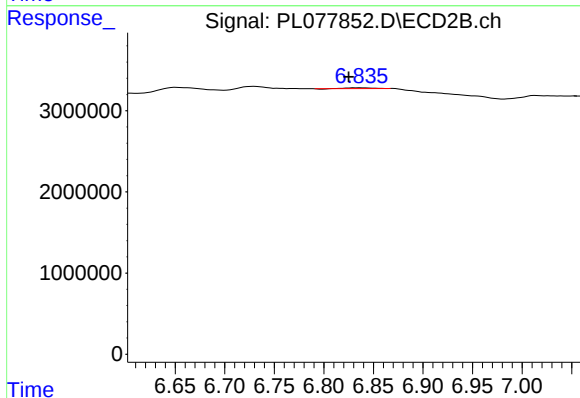


#22 Mirex

R.T.: 6.837 min
Delta R.T.: 0.012 min
Response: 136350
Conc: 0.06 ng/ml

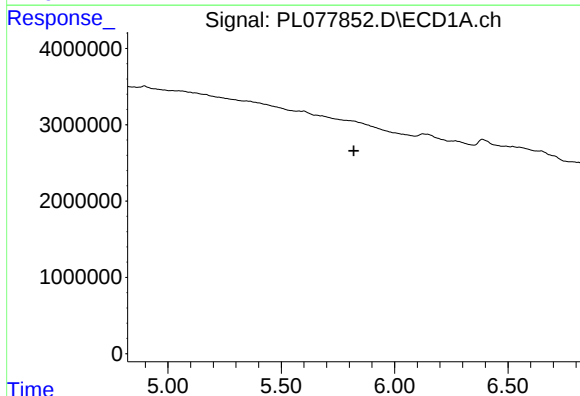


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.820 min
Response: 0
Conc: N.D.

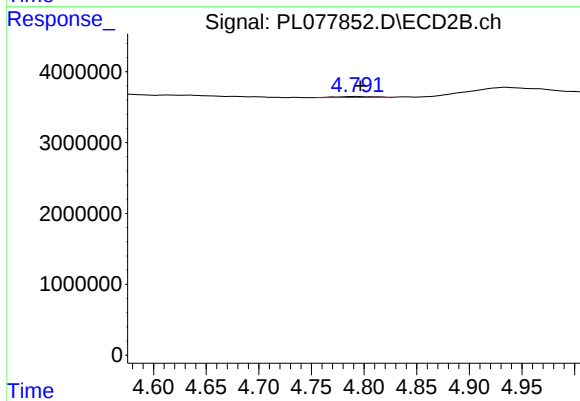

#25 Chlordane-3


R.T.: 4.792 min
Delta R.T.: -0.004 min
Response: 331807
Conc: 0.96 ng/ml

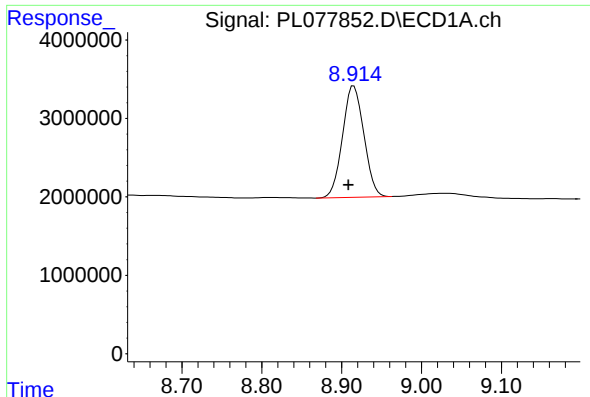

#28 Decachlorobiphenyl

R.T.: 8.915 min
Delta R.T.: 0.007 min
Response: 26346074
Conc: 20.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

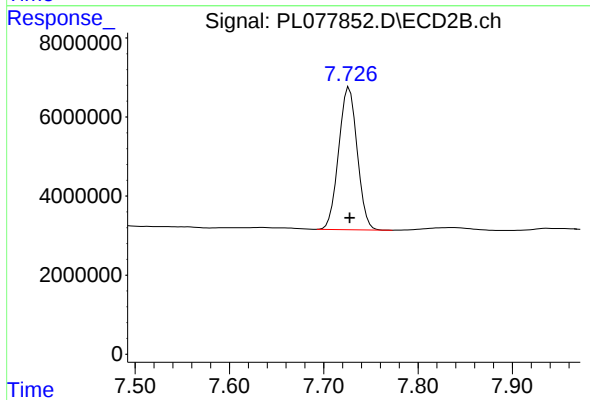

#28 Decachlorobiphenyl

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 49179805
Conc: 19.59 ng/ml