

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092022\
 Data File : PL077861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 14:36
 Operator : AR\AJ
 Sample : N4713-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-091922

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/21/2022
 Supervised By : Ankita Jodhani 09/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 17:09:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.414	2.624	17469234	38113176	10.898m	12.838
28) SA Decachlor...	8.903	7.720	19329343	34614977	14.956	13.790

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092022\
Data File : PL077861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 14:36
Operator : AR\AJ
Sample : N4713-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-03-091922


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/21/2022
Supervised By : Ankita Jodhani 09/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 17:09:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

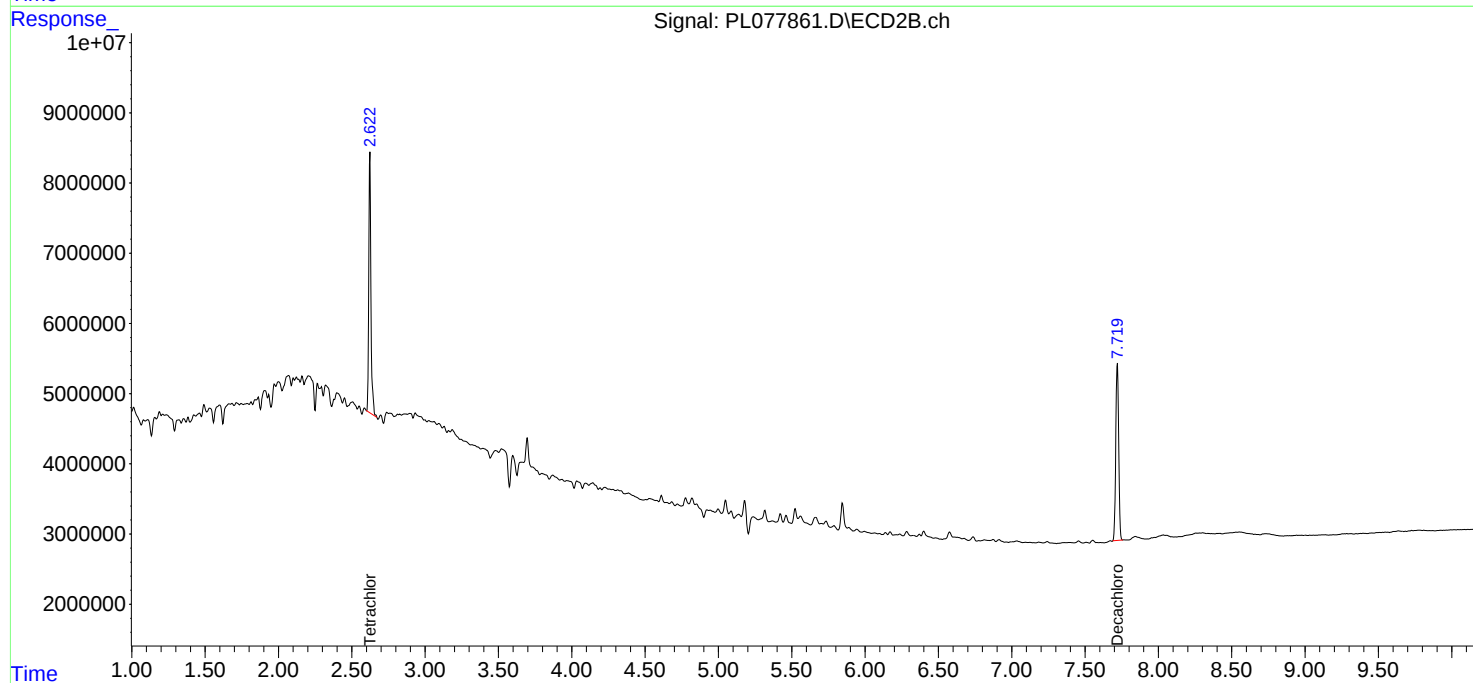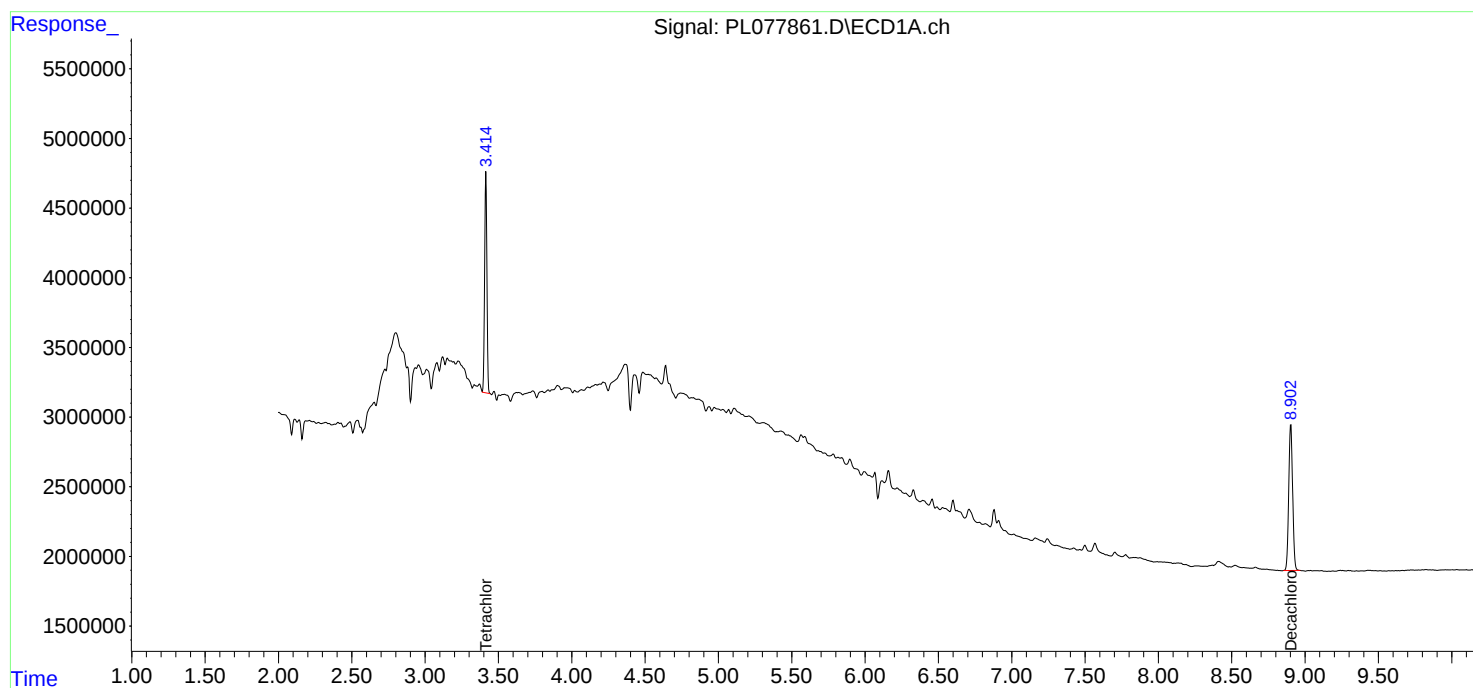

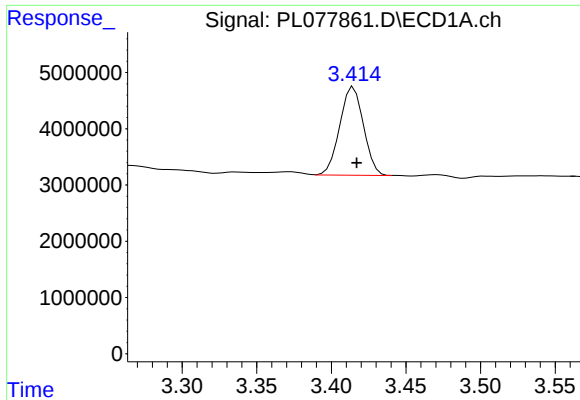


#1 Tetrachloro-m-xylene

R.T.: 3.414 min
Delta R.T.: -0.003 min
Response: 17469234
Conc: 10.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-091922


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

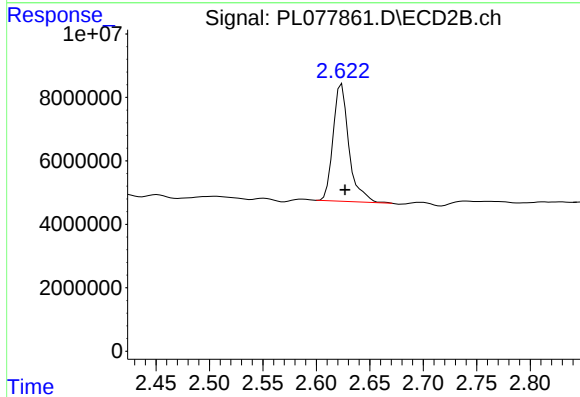


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: -0.003 min
Response: 38113176
Conc: 12.84 ng/ml

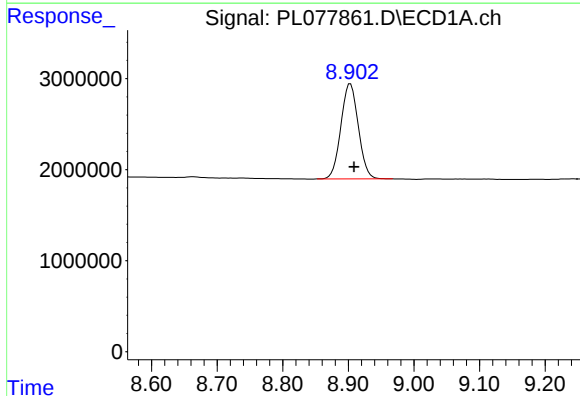

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: -0.005 min
Response: 19329343
Conc: 14.96 ng/ml

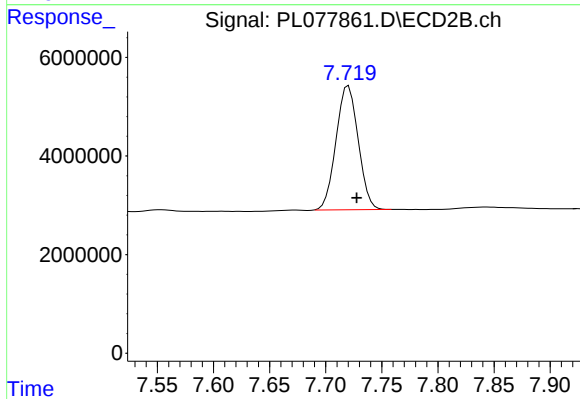

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: -0.007 min
Response: 34614977
Conc: 13.79 ng/ml