

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092023\
 Data File : PL085433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 16:08
 Operator : AR\AJ
 Sample : 04426-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/21/2023
 Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 00:17:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 10:25:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.422	2.654	47127664	24505520	14.150m	16.109
2) SA Decachlor...	8.956	7.833	83231308	45247391	24.453	23.112

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092023\
Data File : PL085433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 16:08
Operator : AR\AJ
Sample : 04426-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 00:17:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 10:25:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

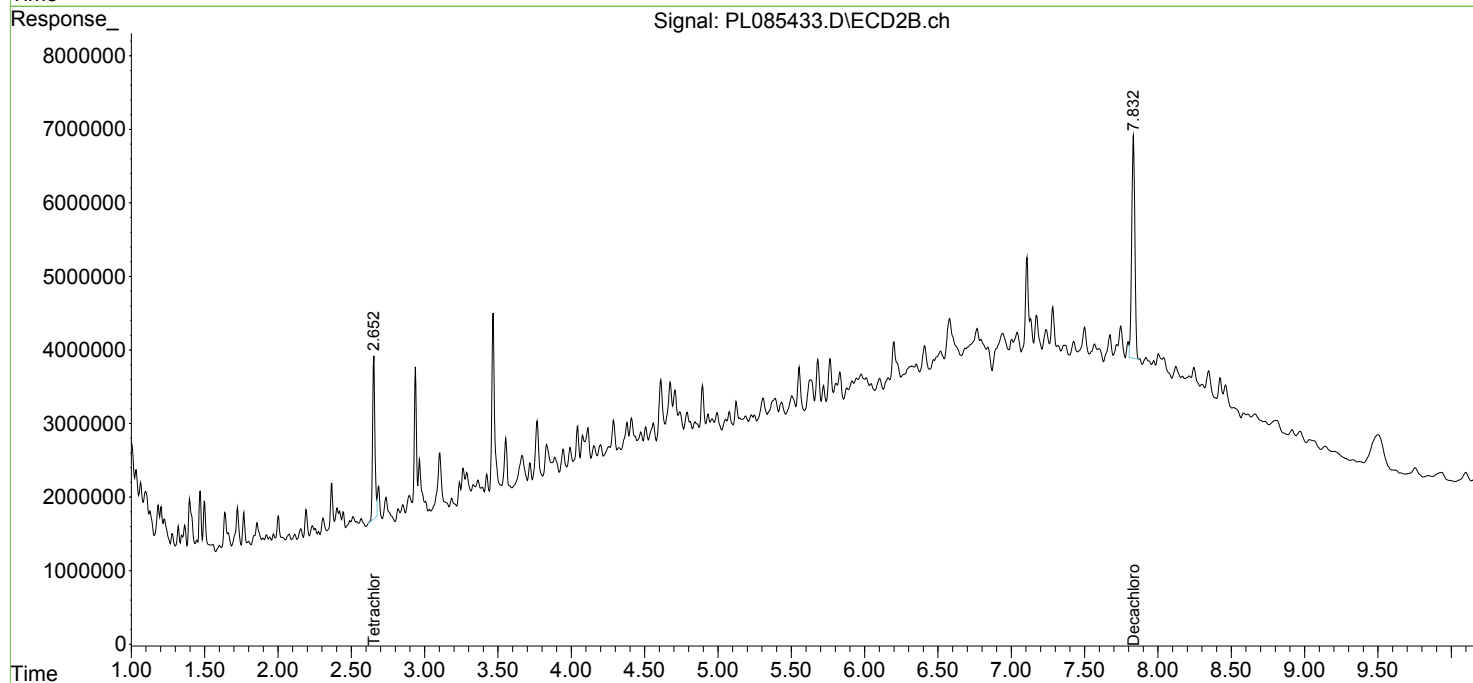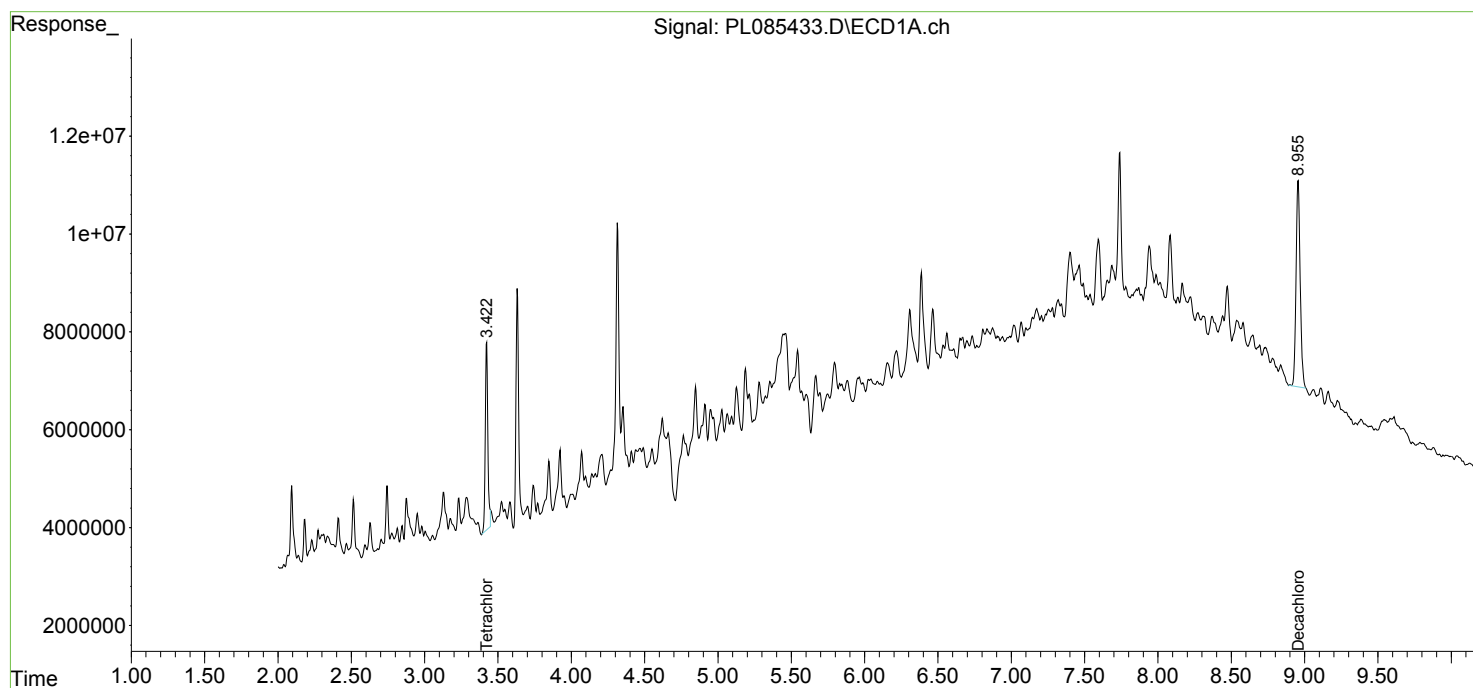

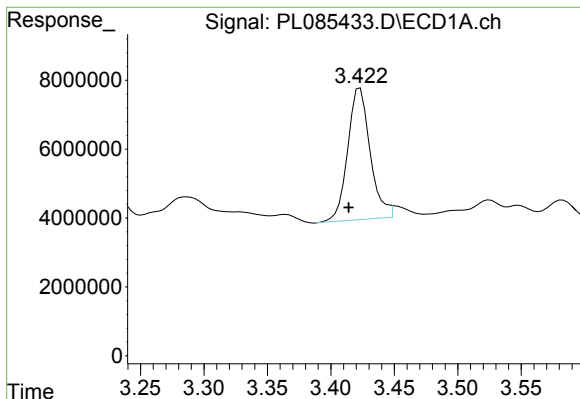


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: 0.008 min
Response: 47127664
Conc: 14.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

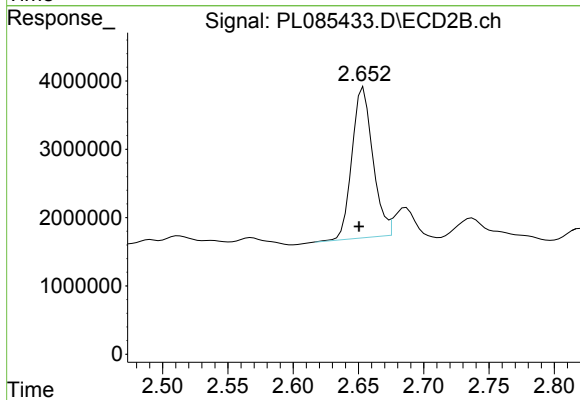


#1 Tetrachloro-m-xylene

R.T.: 2.654 min
Delta R.T.: 0.003 min
Response: 24505520
Conc: 16.11 ng/ml

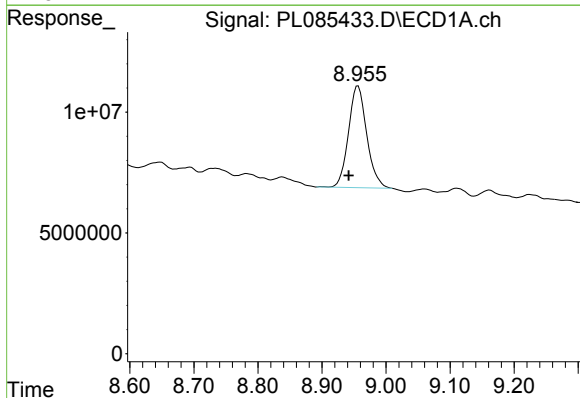

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: 0.015 min
Response: 83231308
Conc: 24.45 ng/ml

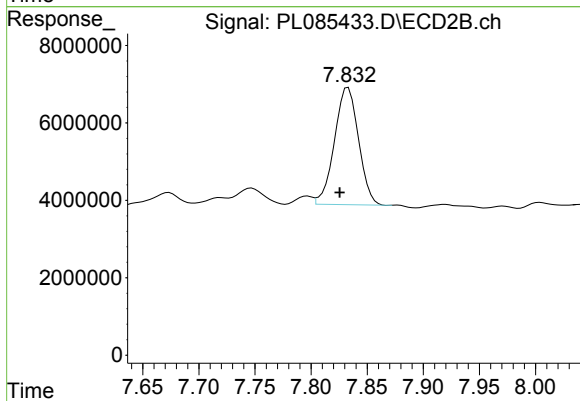

#28 Decachlorobiphenyl

R.T.: 7.833 min
Delta R.T.: 0.008 min
Response: 45247391
Conc: 23.11 ng/ml