

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092023\
 Data File : PL085441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 18:12
 Operator : AR\AJ
 Sample : 04474-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 H-2313-WATER

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/21/2023
 Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 00:23:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 10:25:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.418	2.650	53066409	26864380	15.933	17.660
28) SA Decachlor...	8.943	7.824	11753800	15155974	3.453m	7.741m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092023\
Data File : PL085441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 18:12
Operator : AR\AJ
Sample : 04474-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
H-2313-WATER


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/21/2023
Supervised By : Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 00:23:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 10:25:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

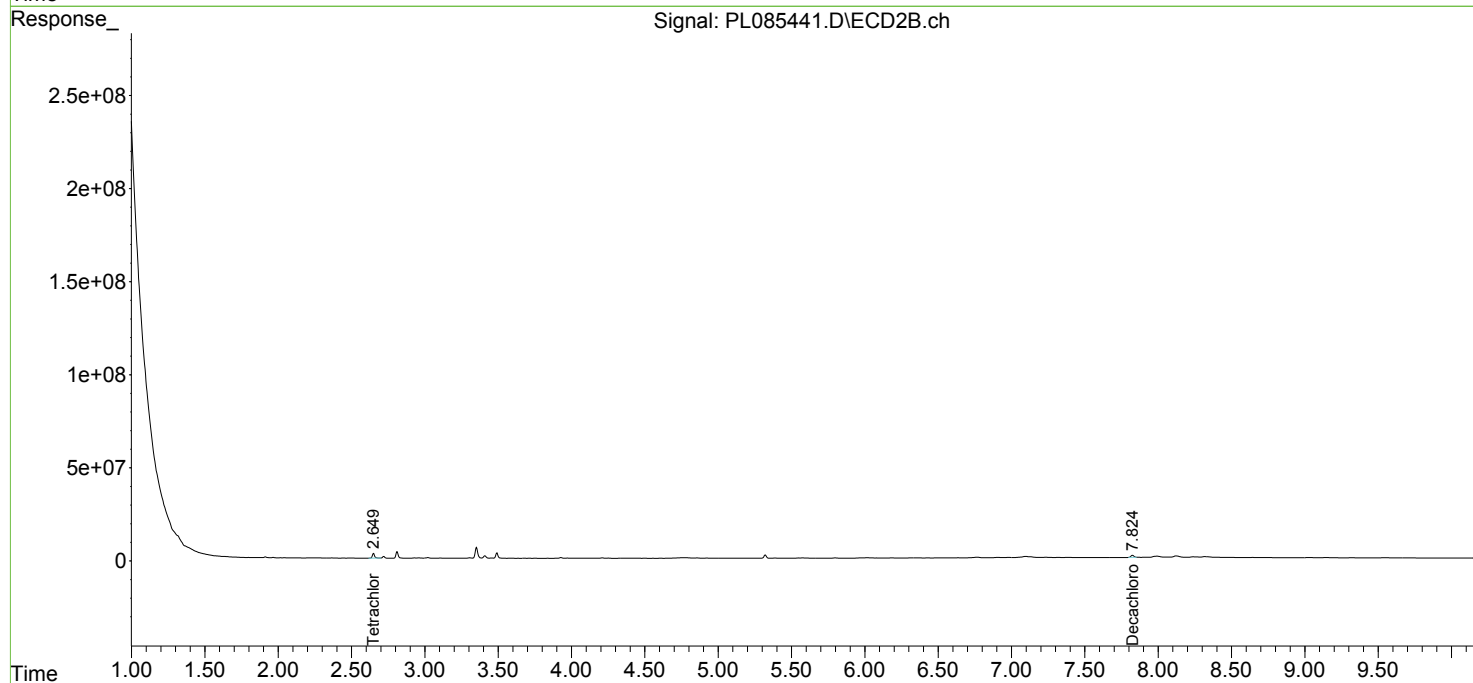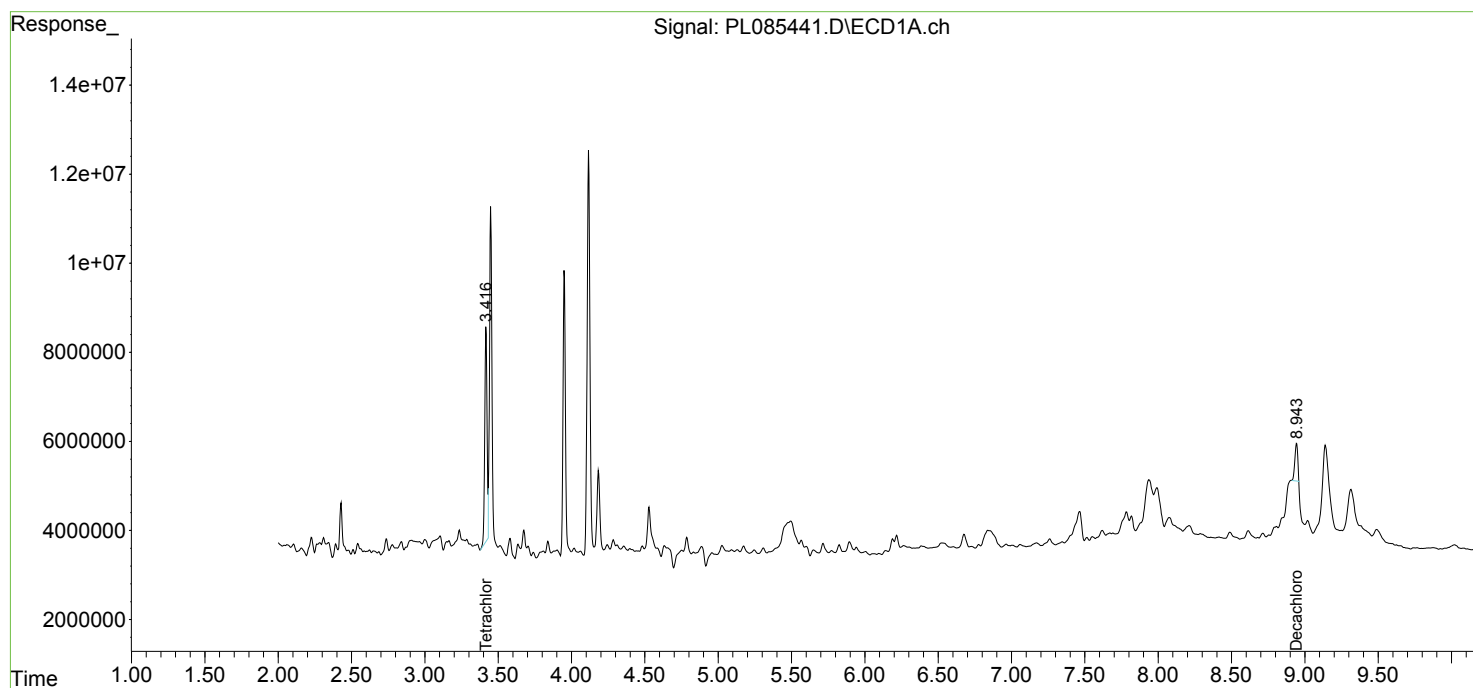

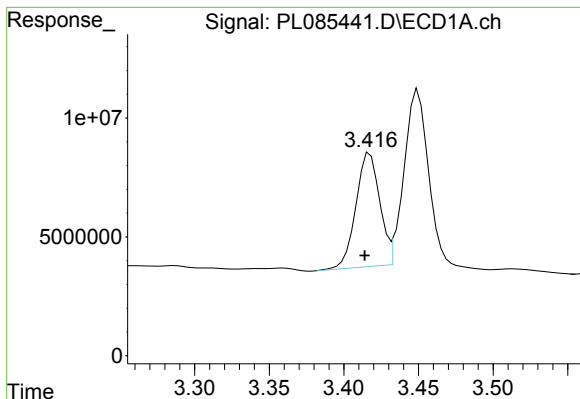


#1 Tetrachloro-m-xylene

R.T.: 3.418 min
Delta R.T.: 0.004 min
Response: 53066409
Conc: 15.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
H-2313-WATER


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

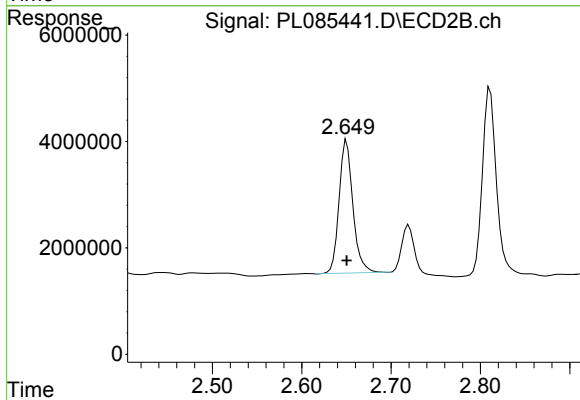


#1 Tetrachloro-m-xylene

R.T.: 2.650 min
Delta R.T.: 0.000 min
Response: 26864380
Conc: 17.66 ng/ml

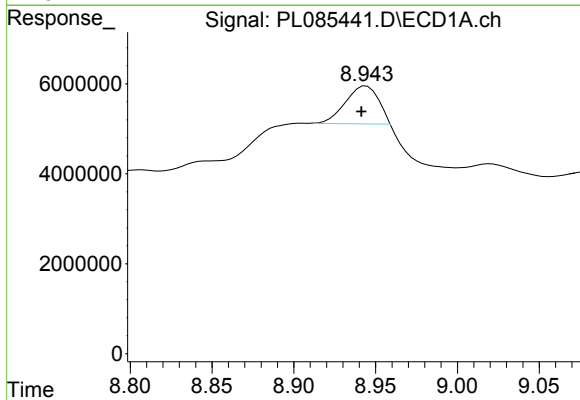

#28 Decachlorobiphenyl

R.T.: 8.943 min
Delta R.T.: 0.001 min
Response: 11753800
Conc: 3.45 ng/ml m

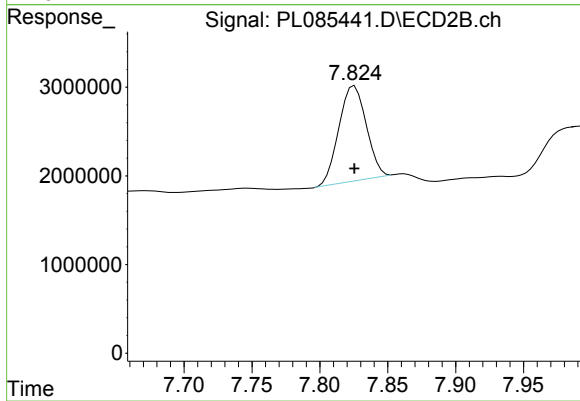

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: -0.001 min
Response: 15155974
Conc: 7.74 ng/ml m