

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092023\
 Data File : PL085448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 19:51
 Operator : AR\AJ
 Sample : 04501-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 00:29:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 20 10:25:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.650	57919213	27306966	17.390	17.951
28)	SA Decachlor...	8.948	7.824	55079679	33413844	16.182	17.067
Target Compounds							
17)	MA 4,4'-DDT	6.924	5.929	8761338	5961588	2.440	3.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092023\
Data File : PL085448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 19:51
Operator : AR\AJ
Sample : 04501-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 00:29:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091923.M
Quant Title : GC Extractables
QLast Update : Wed Sep 20 10:25:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

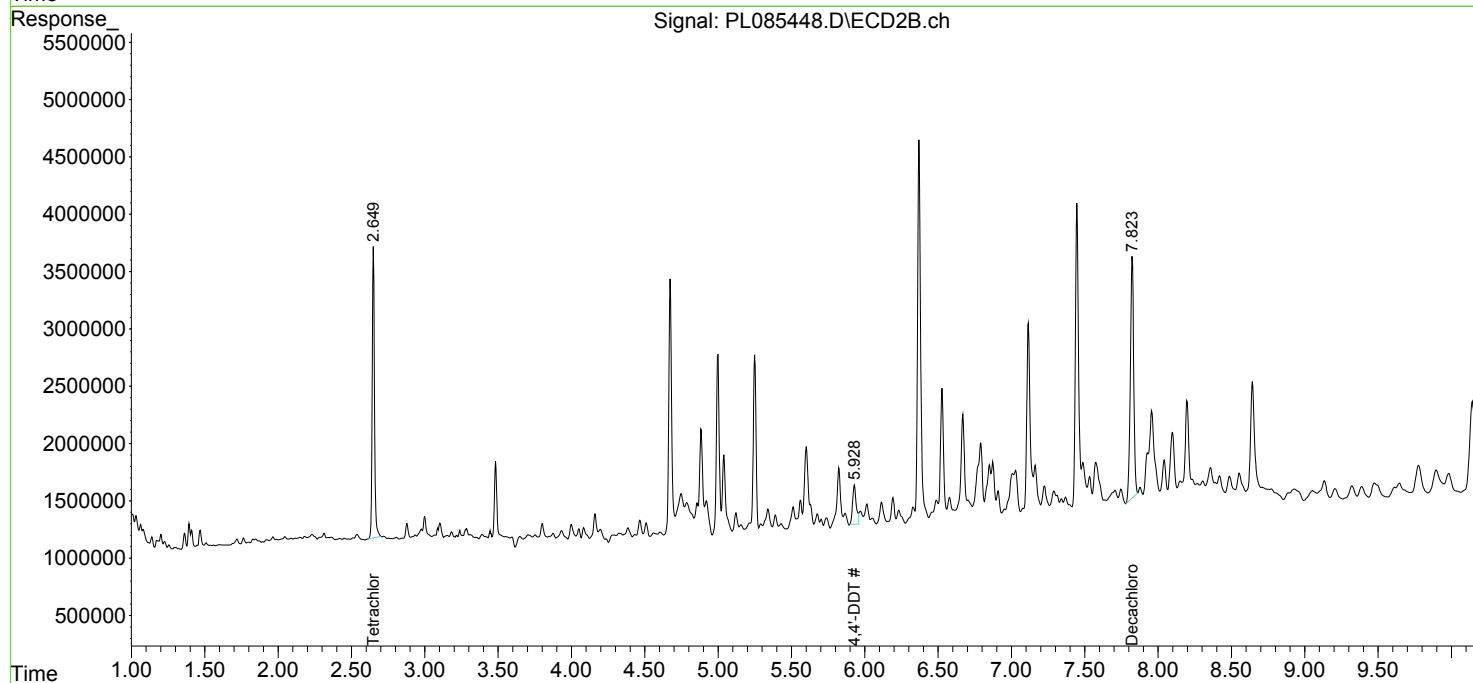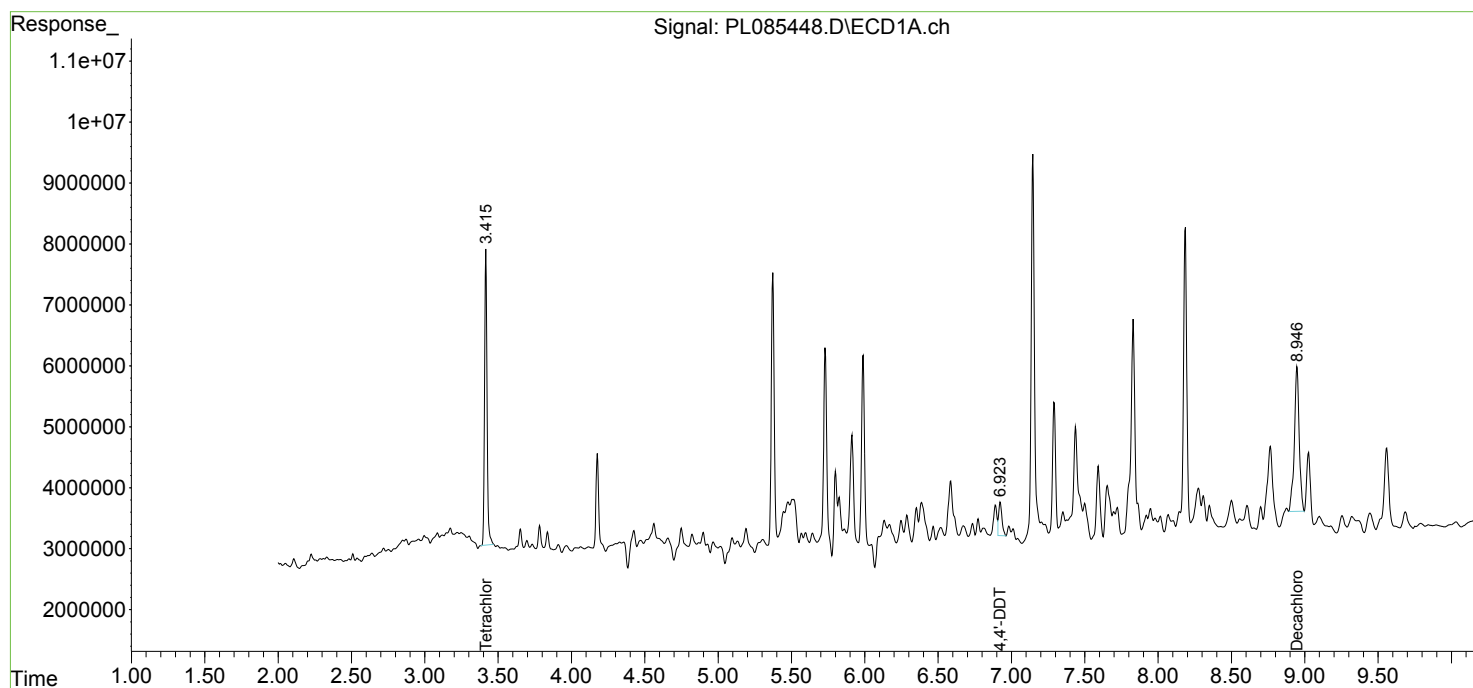


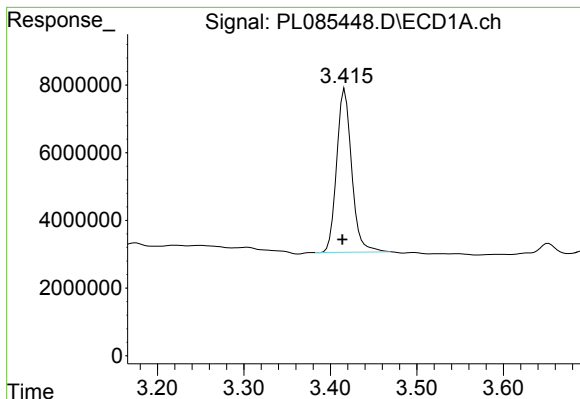

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.003 min
Response: 57919213
Conc: 17.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

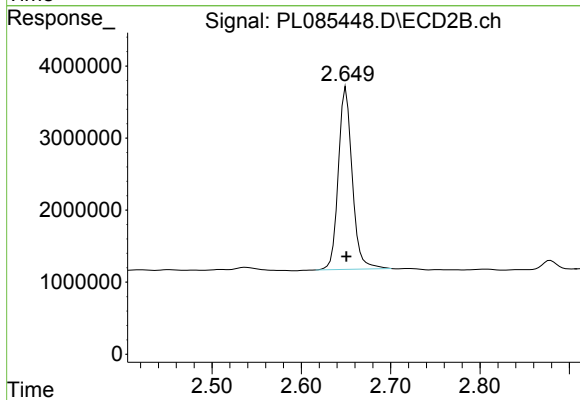


#1 Tetrachloro-m-xylene

R.T.: 2.650 min
Delta R.T.: 0.000 min
Response: 27306966
Conc: 17.95 ng/ml

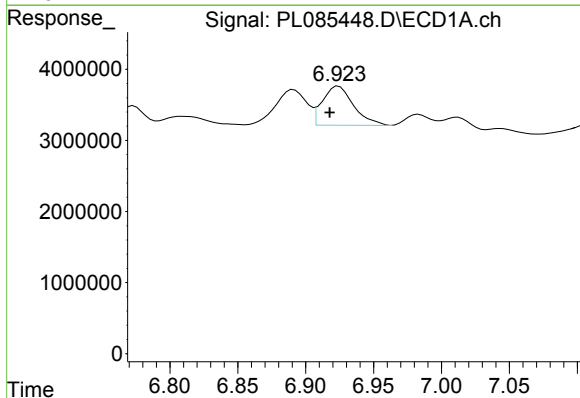


#17 4,4'-DDT

R.T.: 6.924 min
Delta R.T.: 0.007 min
Response: 8761338
Conc: 2.44 ng/ml

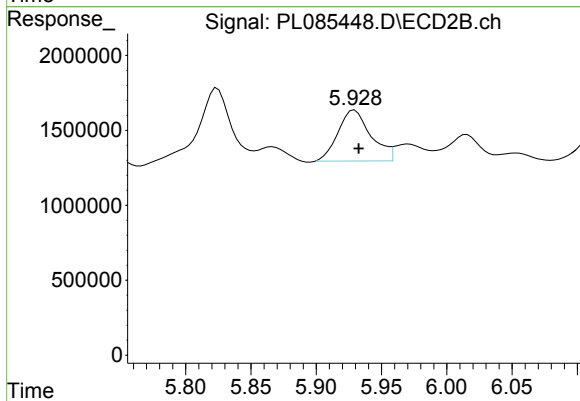

#17 4,4'-DDT


R.T.: 5.929 min
Delta R.T.: -0.003 min
Response: 5961588
Conc: 3.27 ng/ml

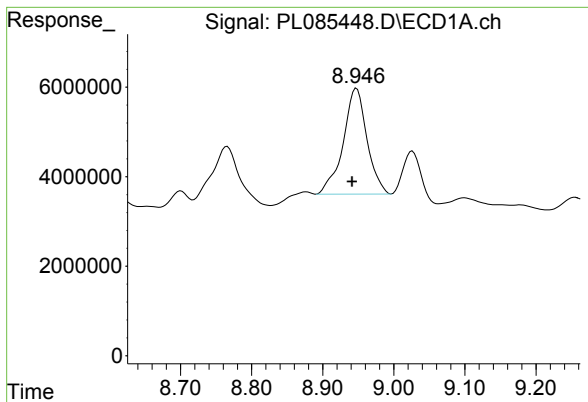

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: 0.006 min
Response: 55079679
Conc: 16.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

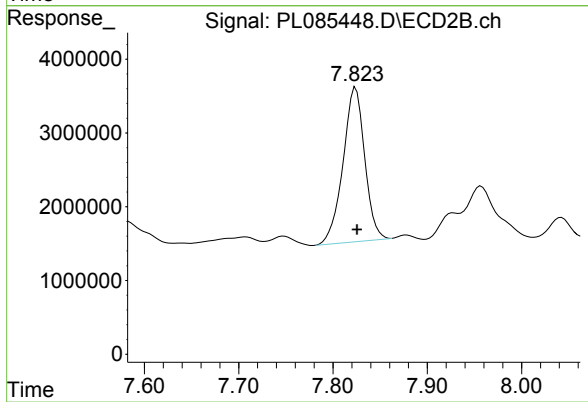

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: -0.001 min
Response: 33413844
Conc: 17.07 ng/ml