

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024--\
 Data File : PL091871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2024 22:06
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA4329

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 03:30:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 03:28:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.783	69773135	84353985	39.702	39.719
27)	SA Decachlor...	9.062	7.925	104.8E6	167.9E6	79.903	79.827
Target Compounds							
2)	A alpha-BHC	3.999	3.286	101.4E6	126.2E6	39.472	39.834
3)	MA gamma-BHC...	4.332	3.616	96649623	116.9E6	39.589	39.850
4)	MA Heptachlor	4.921	3.956	90534627	117.1E6	39.796	40.063
9)	A Endosulfan I	6.075	5.109	71407052	88556308	39.750	39.371
13)	MA Dieldrin	6.350	5.373	154.8E6	203.9E6	79.466	80.655
14)	MA Endrin	6.580	5.649	124.9E6	177.6E6	80.451	81.036
16)	A 4,4'-DDD	6.715	5.797	113.6E6	153.5E6	79.231	80.175
17)	MA 4,4'-DDT	7.029	6.048	116.9E6	164.1E6	79.553	80.534
20)	A Methoxychlor	7.505	6.623	306.1E6	421.9E6	401.032	406.449


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024--\
Data File : PL091871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2024 22:06
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 03:30:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 03:28:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

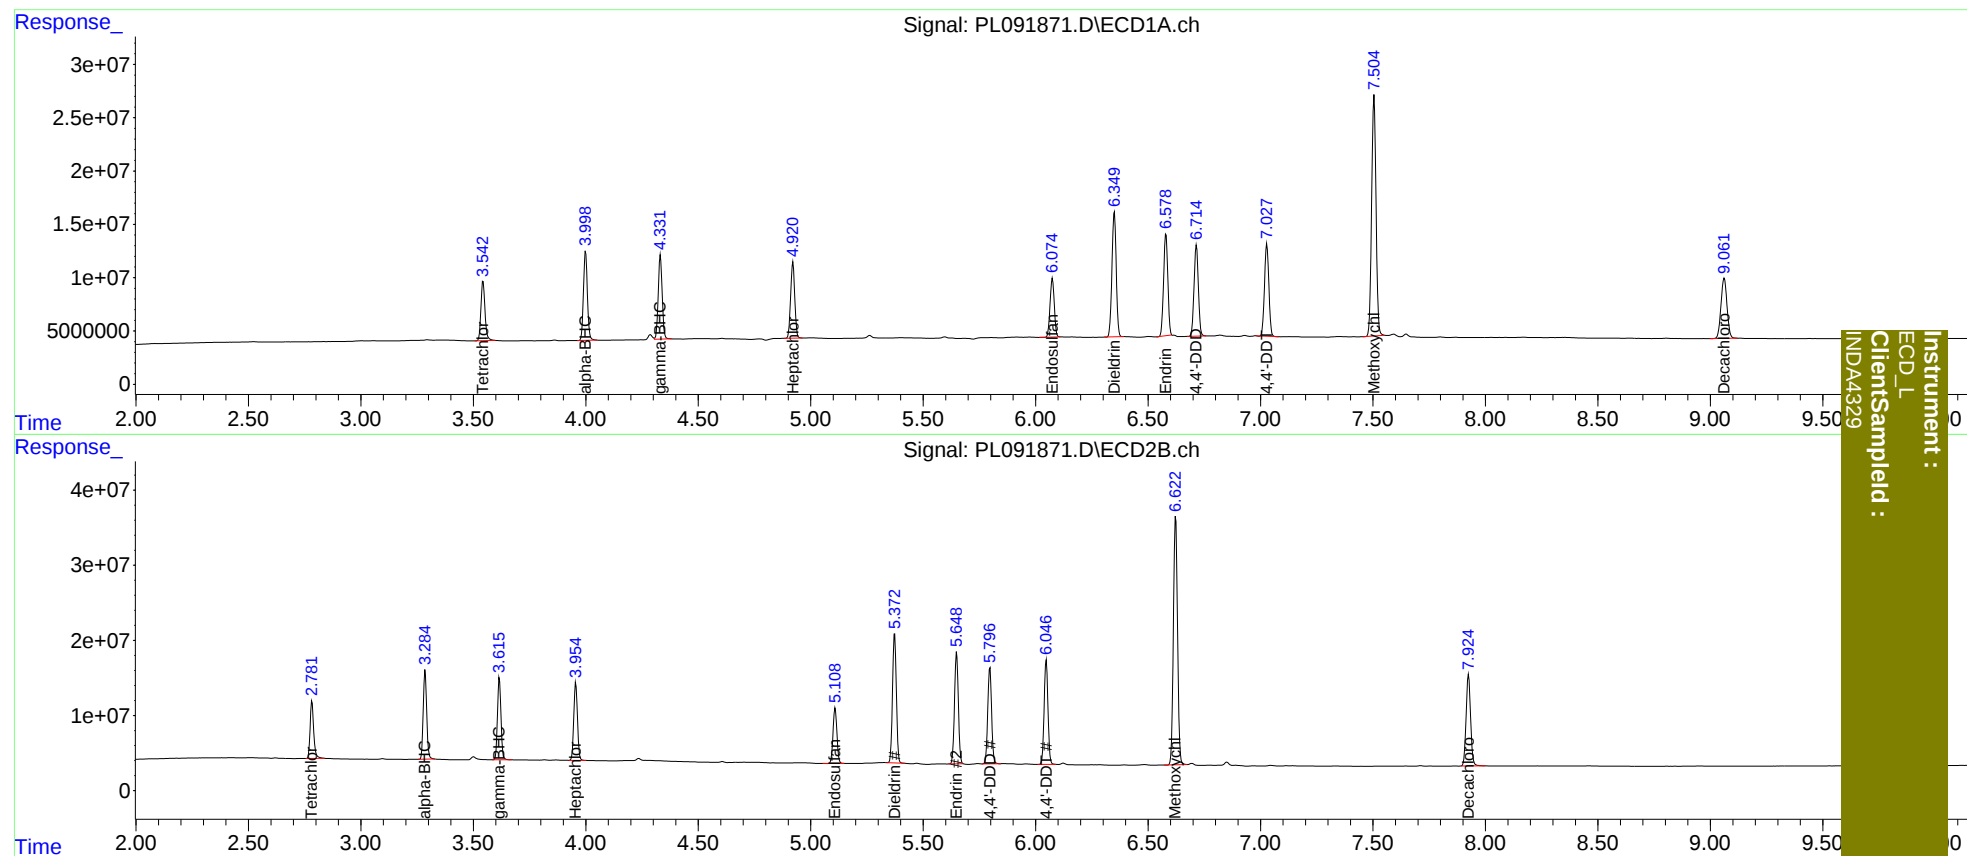


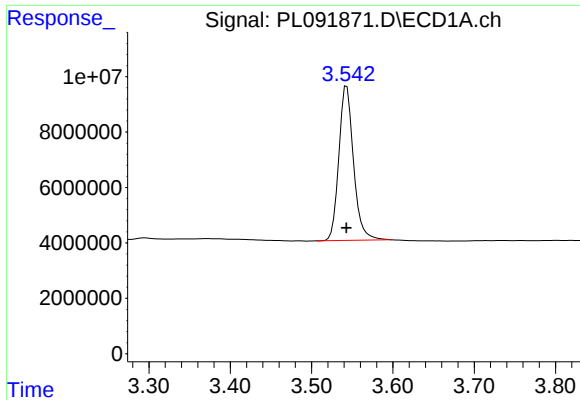

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 69773135
Conc: 39.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4329

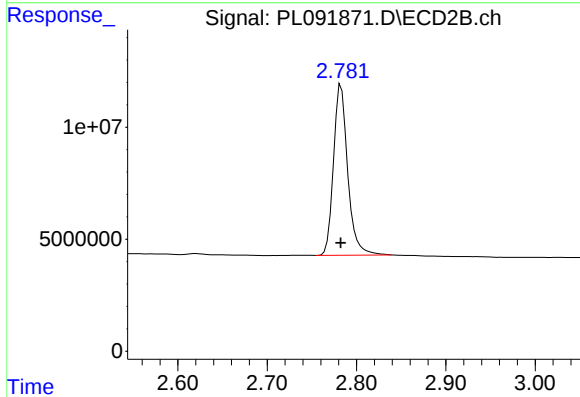


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: 0.000 min
Response: 84353985
Conc: 39.72 ng/ml

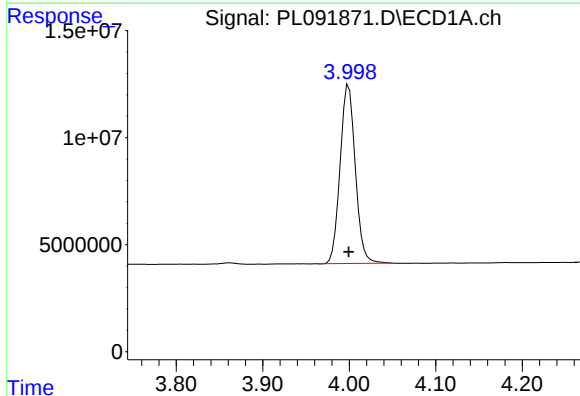


#2 alpha-BHC

R.T.: 3.999 min
Delta R.T.: 0.000 min
Response: 101401256
Conc: 39.47 ng/ml

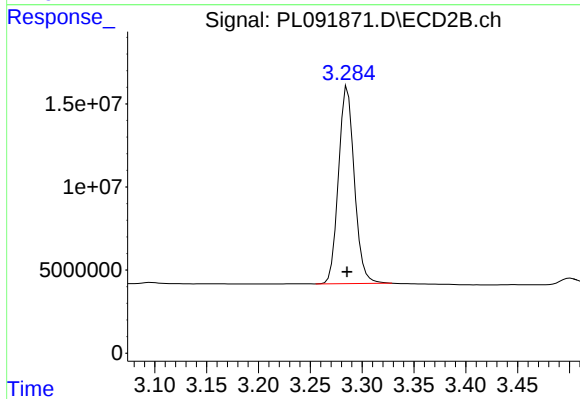

#2 alpha-BHC


R.T.: 3.286 min
Delta R.T.: 0.000 min
Response: 126183046
Conc: 39.83 ng/ml

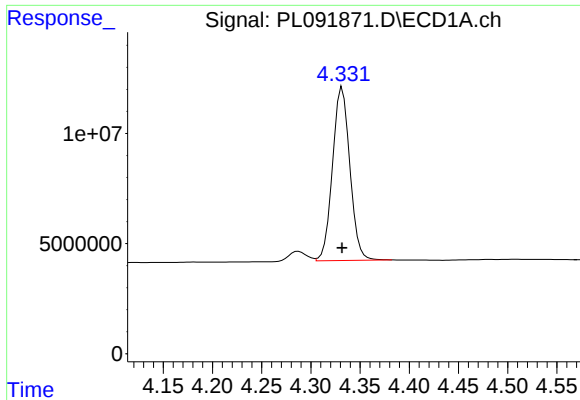

#3 gamma-BHC (Lindane)


R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 96649623
Conc: 39.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4329

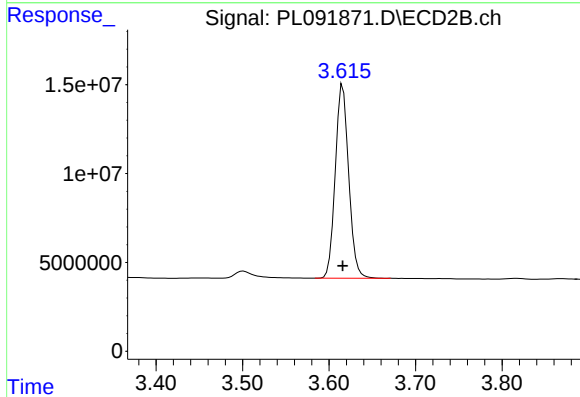


#3 gamma-BHC (Lindane)

R.T.: 3.616 min
Delta R.T.: 0.000 min
Response: 116880846
Conc: 39.85 ng/ml

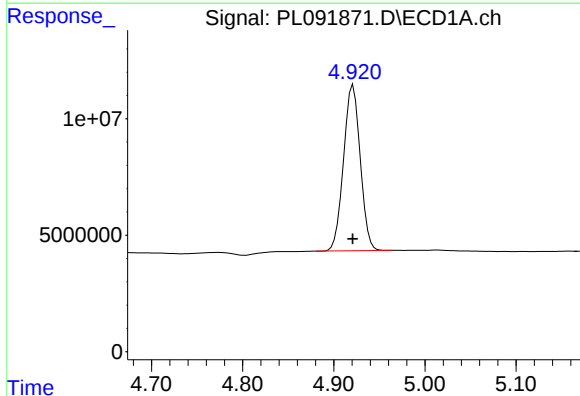


#4 Heptachlor

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 90534627
Conc: 39.80 ng/ml

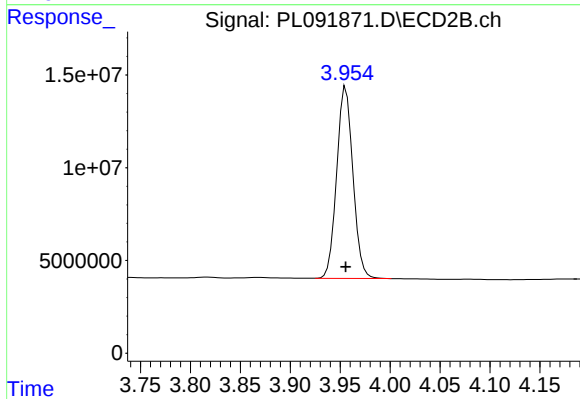

#4 Heptachlor


R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 117141776
Conc: 40.06 ng/ml

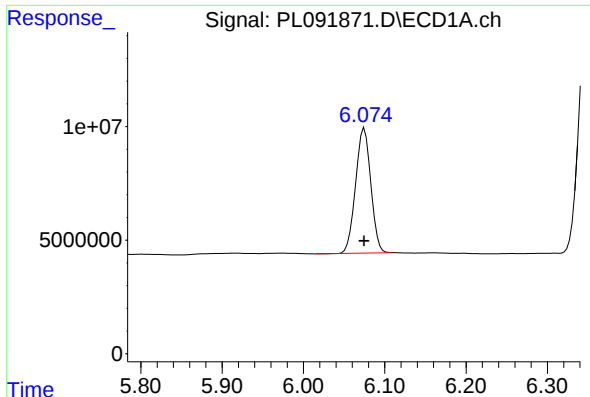

#9 Endosulfan I


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 71407052
Conc: 39.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4329

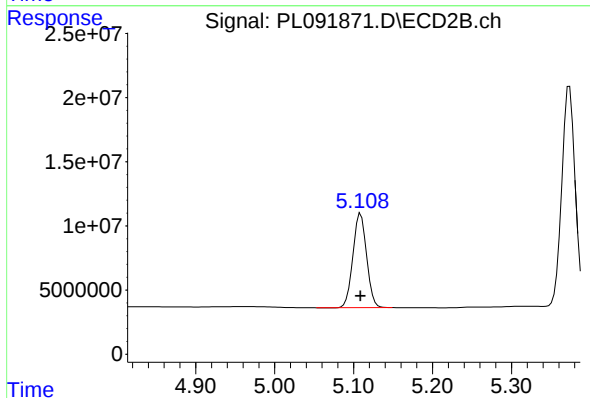


#9 Endosulfan I

R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 88556308
Conc: 39.37 ng/ml

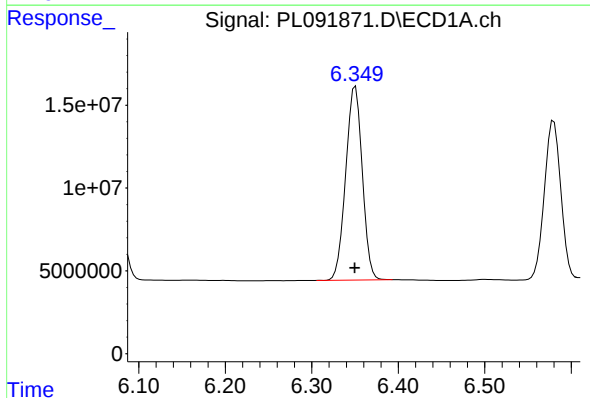


#13 Dieldrin

R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 154787149
Conc: 79.47 ng/ml

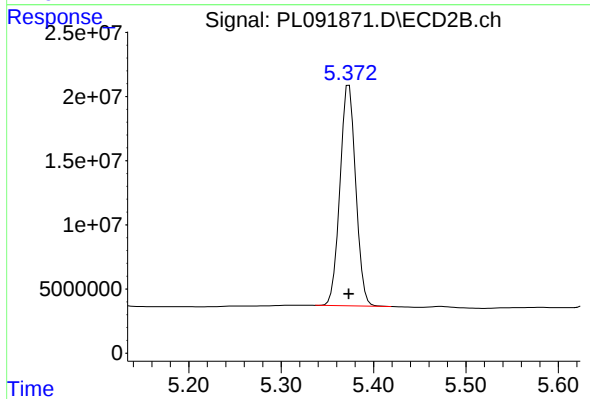

#13 Dieldrin


R.T.: 5.373 min
Delta R.T.: 0.000 min
Response: 203926202
Conc: 80.66 ng/ml

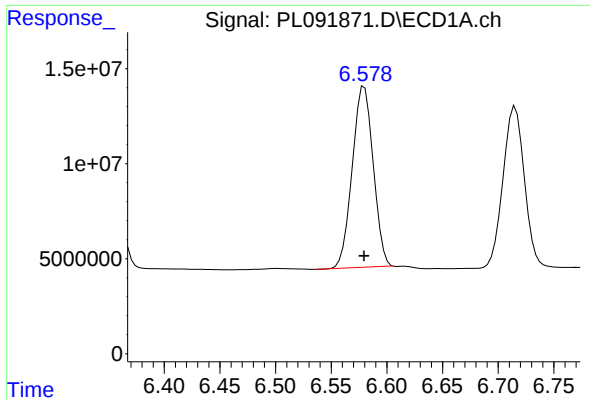

#14 Endrin


R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 124889736
Conc: 80.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4329

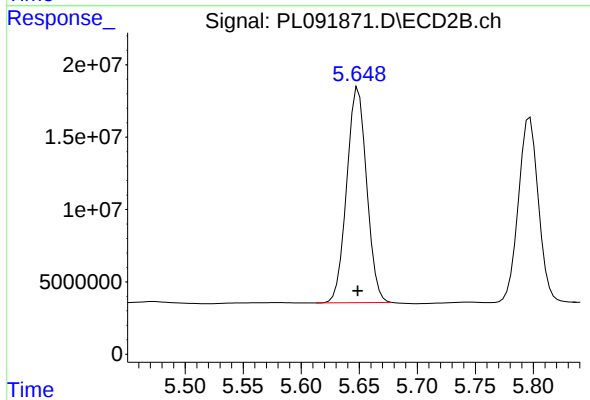


#14 Endrin

R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 177556107
Conc: 81.04 ng/ml

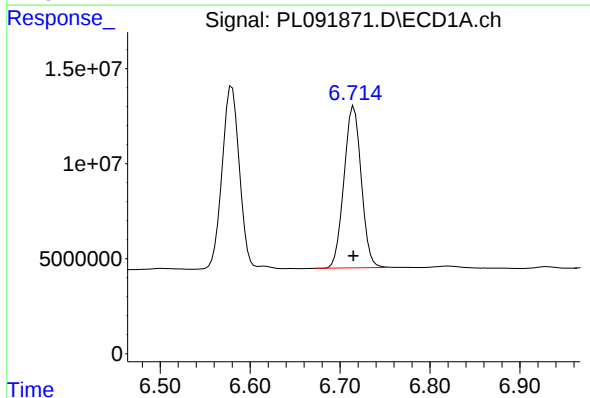


#16 4,4'-DDD

R.T.: 6.715 min
Delta R.T.: 0.000 min
Response: 113613075
Conc: 79.23 ng/ml

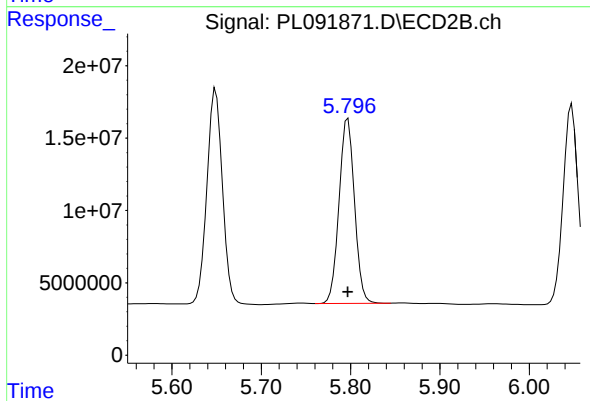

#16 4,4'-DDD


R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 153471255
Conc: 80.18 ng/ml

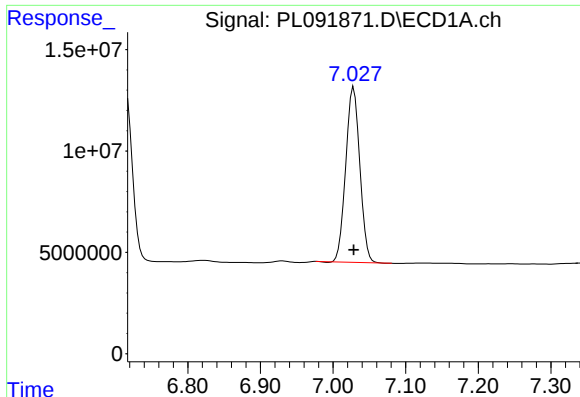

#17 4,4'-DDT


R.T.: 7.029 min
Delta R.T.: 0.000 min
Response: 116861427
Conc: 79.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4329

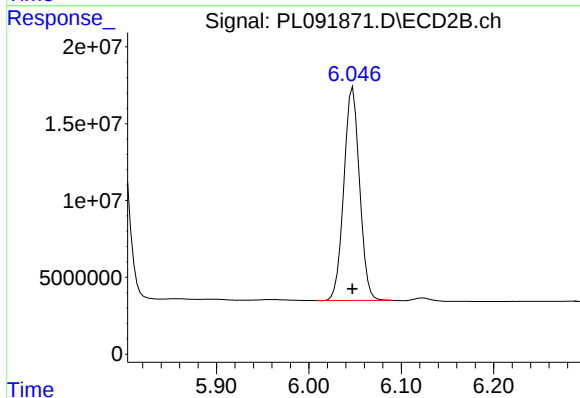


#17 4,4'-DDT

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 164140765
Conc: 80.53 ng/ml

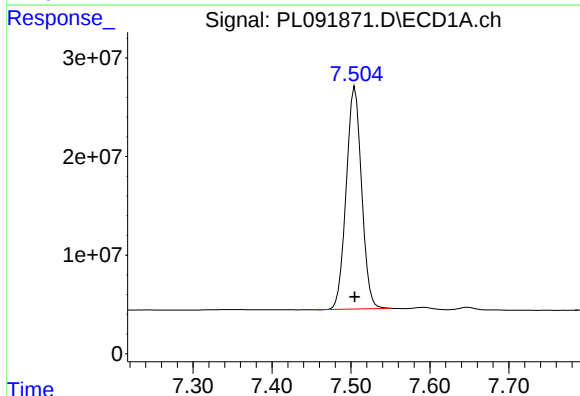


#20 Methoxychlor

R.T.: 7.505 min
Delta R.T.: 0.000 min
Response: 306102880
Conc: 401.03 ng/ml

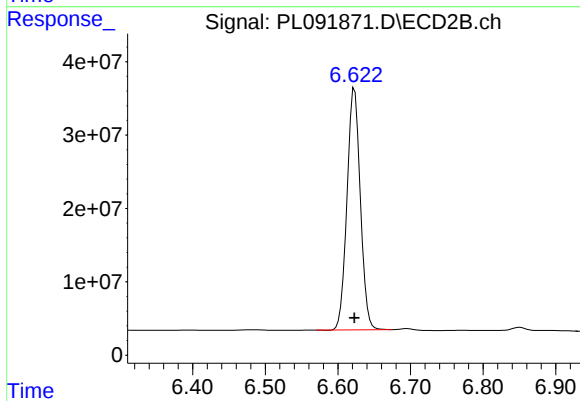

#20 Methoxychlor

R.T.: 6.623 min
Delta R.T.: 0.000 min
Response: 421915799
Conc: 406.45 ng/ml

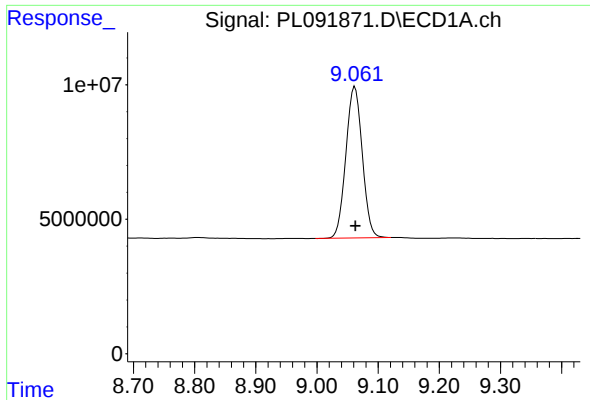

#27 Decachlorobiphenyl


R.T.: 9.062 min

Delta R.T.: 0.000 min

Response: 104849151

Conc: 79.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4329

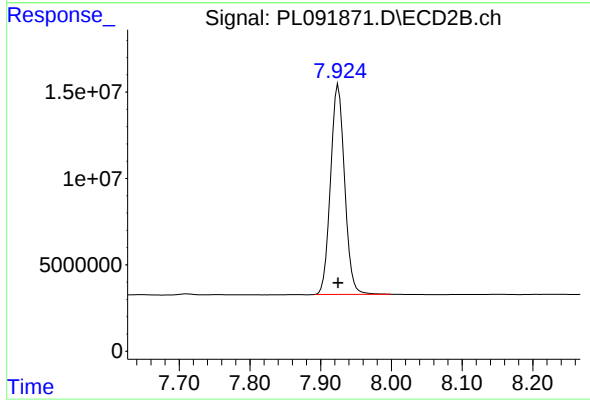

#27 Decachlorobiphenyl

R.T.: 7.925 min

Delta R.T.: 0.000 min

Response: 167912602

Conc: 79.83 ng/ml