

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024--\
 Data File : PL091873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2024 22:33
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA5331

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 03:24:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 03:22:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.783	139.6E6	173.4E6	78.865	83.360
27)	SA Decachlor...	9.062	7.925	203.5E6	334.0E6	150.409	157.608
Target Compounds							
2)	A alpha-BHC	4.000	3.287	210.4E6	271.2E6	83.860	92.085
3)	MA gamma-BHC...	4.333	3.617	197.2E6	249.9E6	81.540	91.126
4)	MA Heptachlor	4.922	3.956	182.5E6	245.4E6	80.455	88.279
9)	A Endosulfan I	6.076	5.110	142.7E6	185.0E6	78.912	84.623
13)	MA Dieldrin	6.351	5.374	316.6E6	428.9E6	165.166	180.484
14)	MA Endrin	6.580	5.650	247.5E6	364.7E6	158.860	173.389
16)	A 4,4'-DDD	6.716	5.797	233.2E6	326.0E6	165.284	182.075
17)	MA 4,4'-DDT	7.030	6.047	238.7E6	347.9E6	165.056	182.911
20)	A Methoxychlor	7.506	6.623	601.2E6	816.7E6	775.703	773.899


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024--\
Data File : PL091873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2024 22:33
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 03:24:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 03:22:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

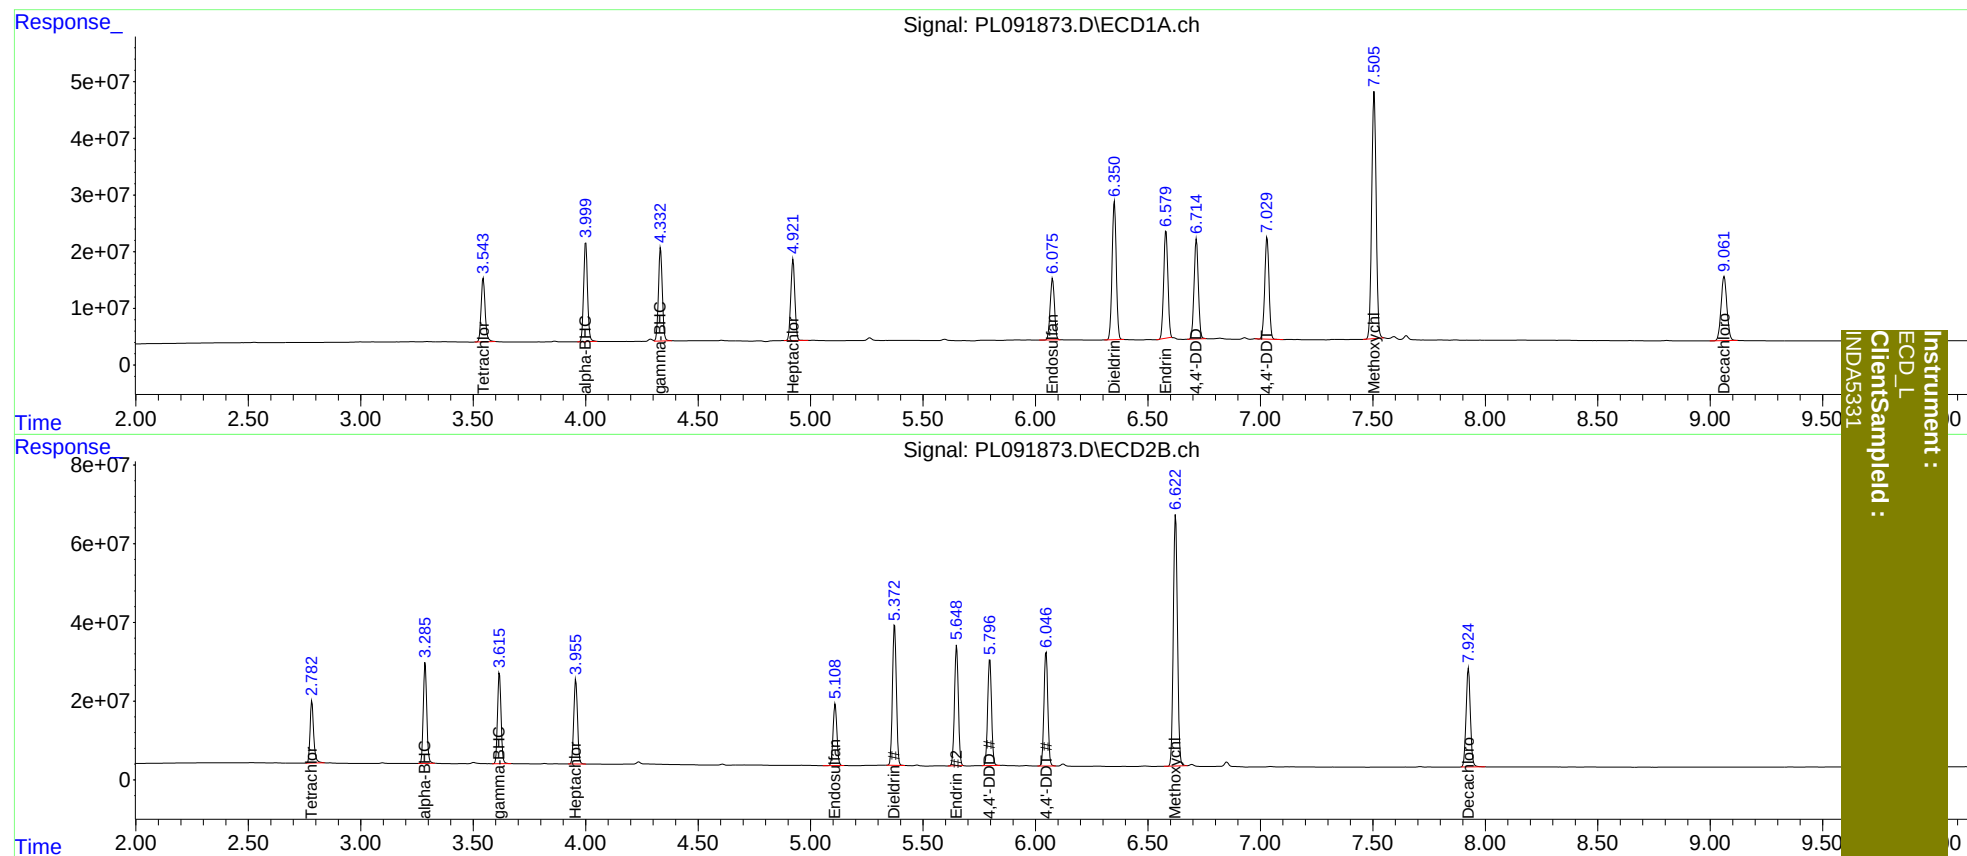


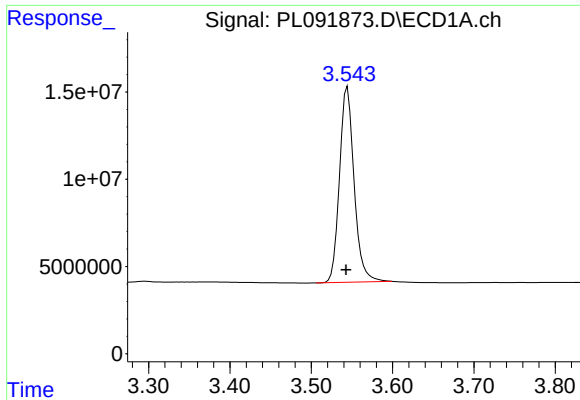

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.002 min
Response: 139587723
Conc: 78.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5331

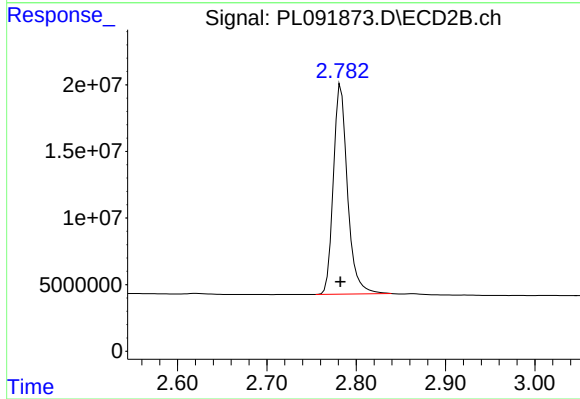


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: 0.000 min
Response: 173398030
Conc: 83.36 ng/ml

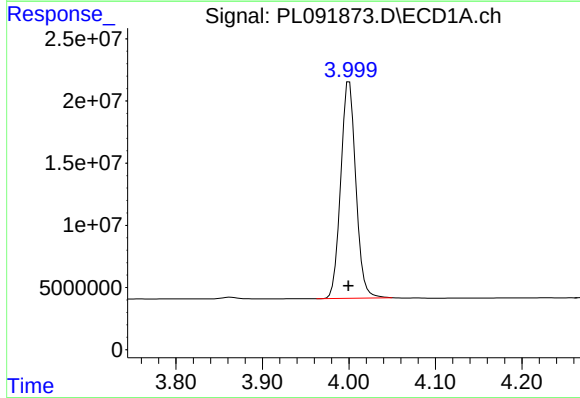


#2 alpha-BHC

R.T.: 4.000 min
Delta R.T.: 0.000 min
Response: 210356942
Conc: 83.86 ng/ml

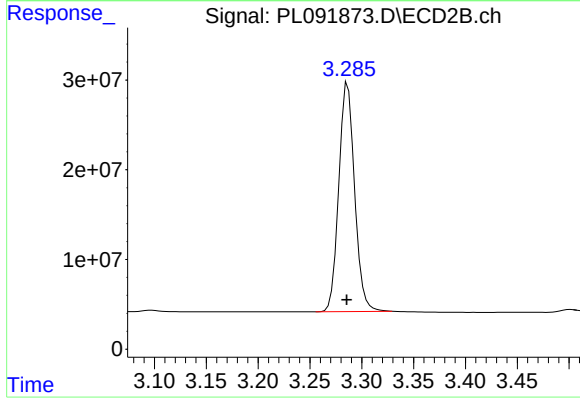

#2 alpha-BHC


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 271217132
Conc: 92.08 ng/ml

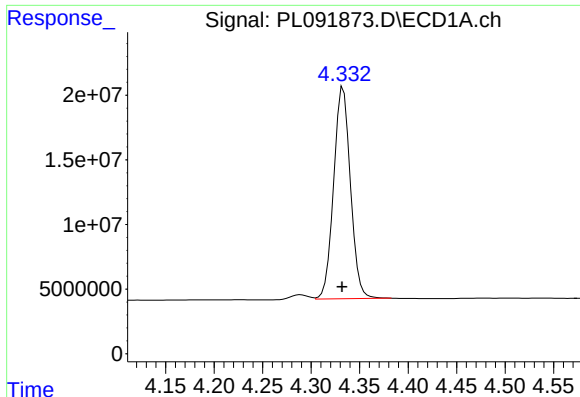

#3 gamma-BHC (Lindane)


R.T.: 4.333 min
Delta R.T.: 0.001 min
Response: 197169126
Conc: 81.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5331

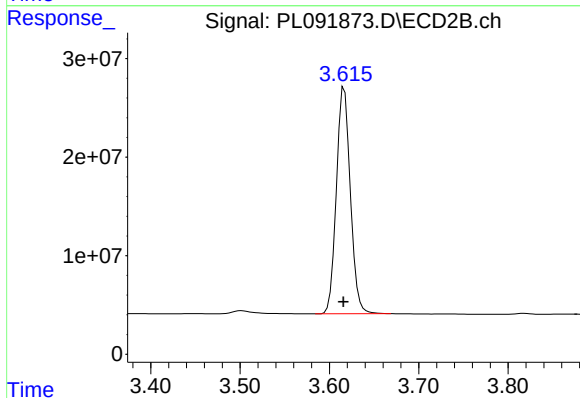


#3 gamma-BHC (Lindane)

R.T.: 3.617 min
Delta R.T.: 0.000 min
Response: 249895875
Conc: 91.13 ng/ml

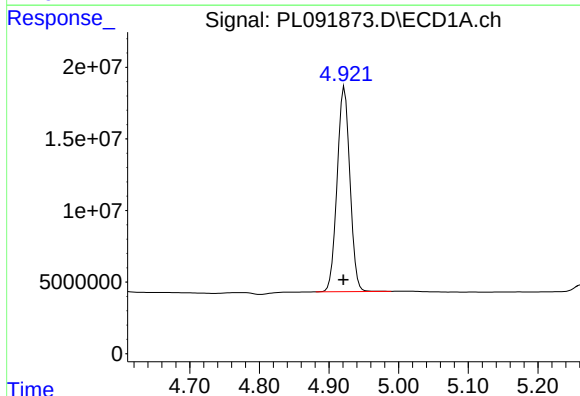


#4 Heptachlor

R.T.: 4.922 min
Delta R.T.: 0.002 min
Response: 182512335
Conc: 80.46 ng/ml

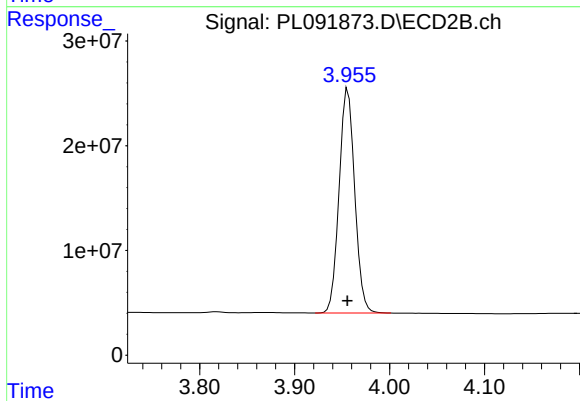

#4 Heptachlor


R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 245422894
Conc: 88.28 ng/ml

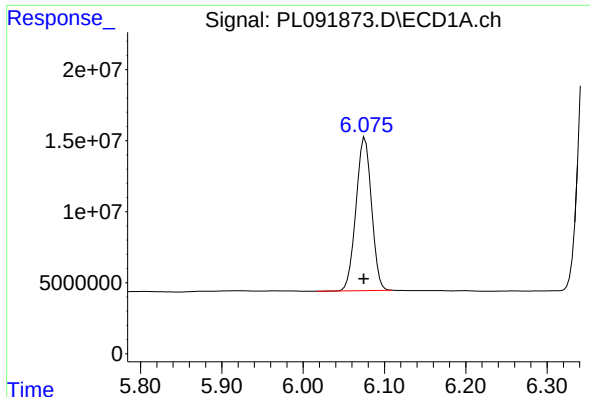

#9 Endosulfan I


R.T.: 6.076 min
Delta R.T.: 0.001 min
Response: 142726644
Conc: 78.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5331

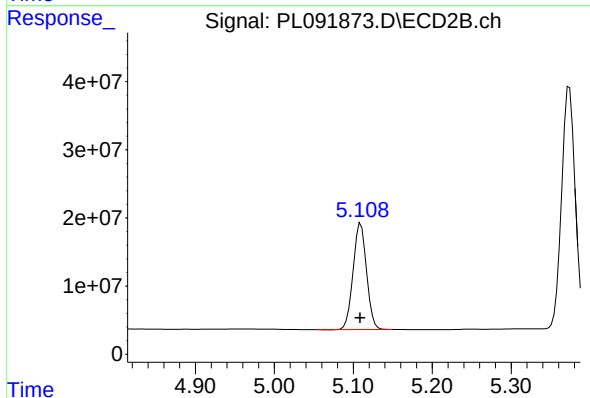


#9 Endosulfan I

R.T.: 5.110 min
Delta R.T.: 0.001 min
Response: 184995338
Conc: 84.62 ng/ml

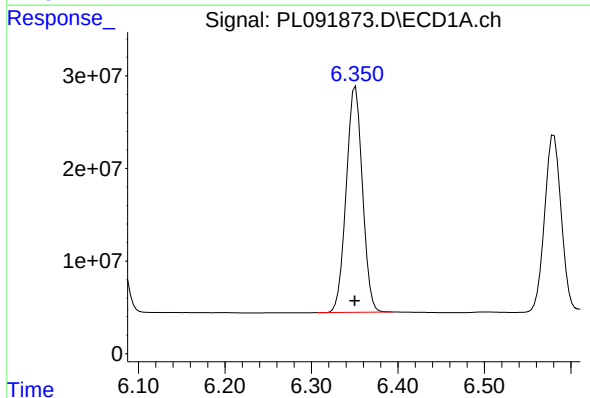


#13 Dieldrin

R.T.: 6.351 min
Delta R.T.: 0.001 min
Response: 316606948
Conc: 165.17 ng/ml

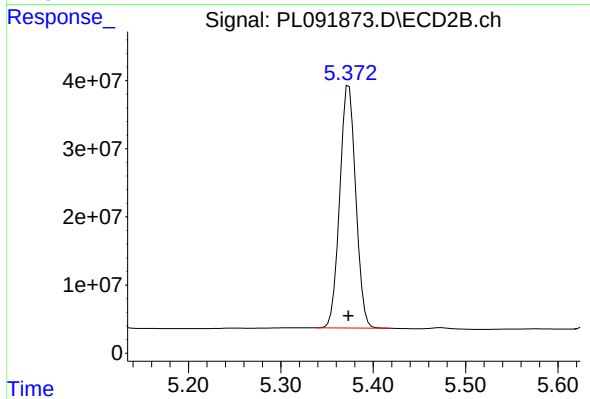

#13 Dieldrin


R.T.: 5.374 min
Delta R.T.: 0.000 min
Response: 428877007
Conc: 180.48 ng/ml

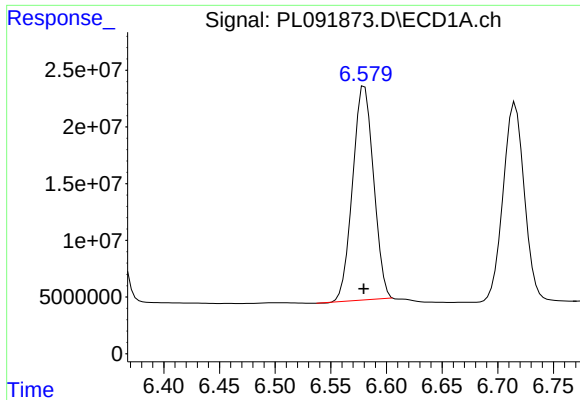

#14 Endrin


R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 247491791
Conc: 158.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5331

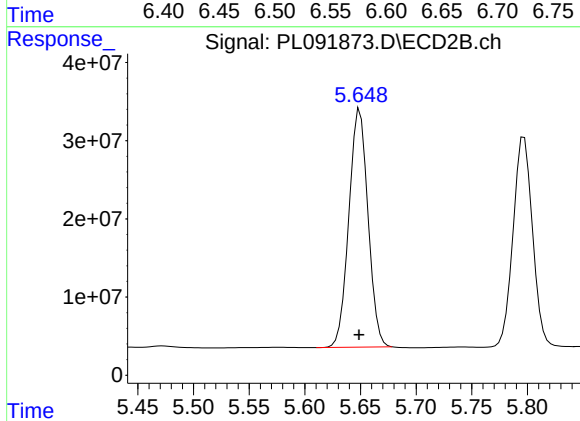


#14 Endrin

R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 364651535
Conc: 173.39 ng/ml

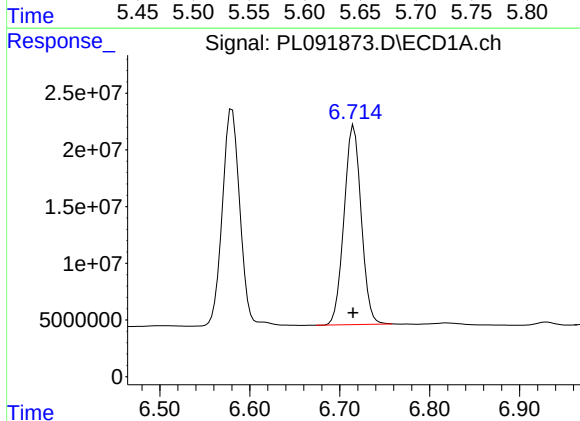


#16 4,4'-DDD

R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 233158487
Conc: 165.28 ng/ml

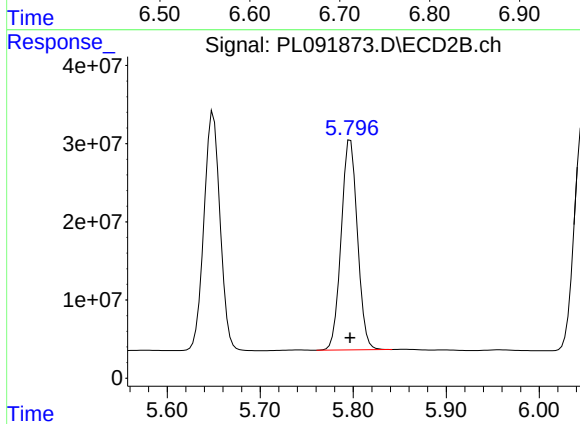

#16 4,4'-DDD


R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 326035398
Conc: 182.07 ng/ml

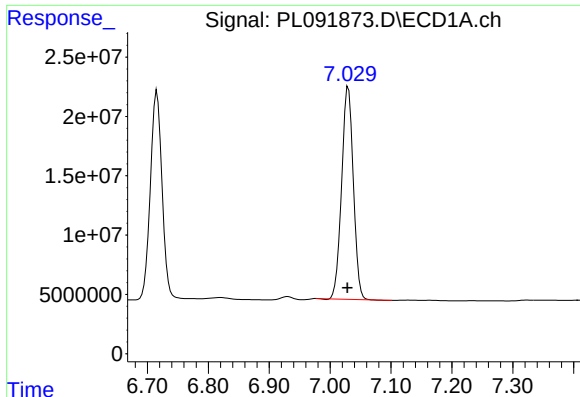

#17 4,4'-DDT


R.T.: 7.030 min
Delta R.T.: 0.001 min
Response: 238691116
Conc: 165.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5331

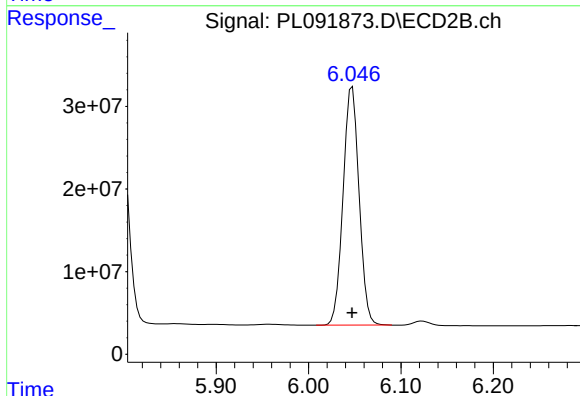


#17 4,4'-DDT

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 347893868
Conc: 182.91 ng/ml

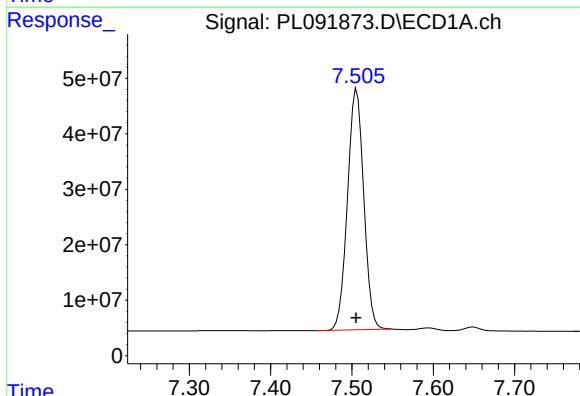


#20 Methoxychlor

R.T.: 7.506 min
Delta R.T.: 0.001 min
Response: 601215267
Conc: 775.70 ng/ml

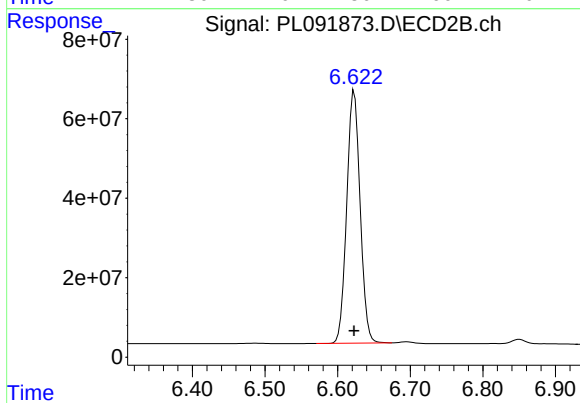

#20 Methoxychlor

R.T.: 6.623 min
Delta R.T.: 0.000 min
Response: 816671858
Conc: 773.90 ng/ml

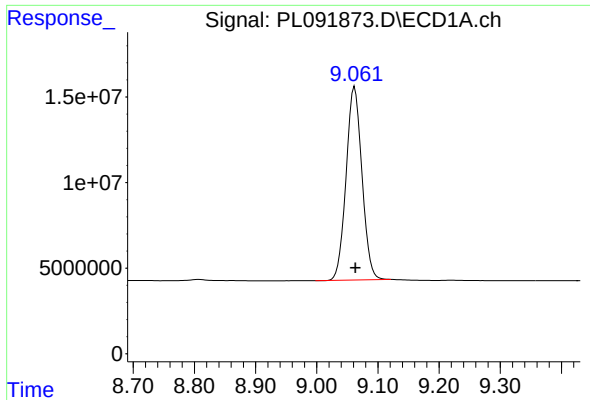

#27 Decachlorobiphenyl


R.T.: 9.062 min

Delta R.T.: -0.001 min

Response: 203465492

Conc: 150.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5331

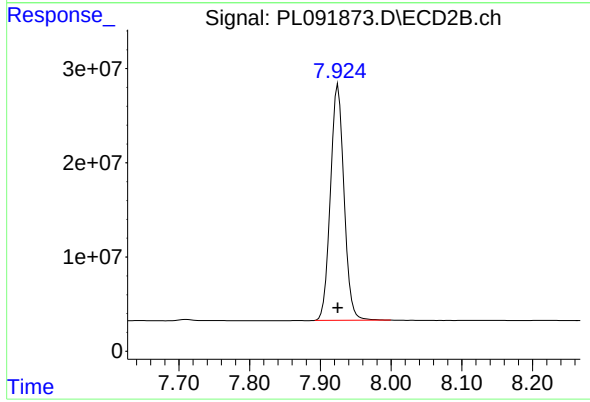

#27 Decachlorobiphenyl

R.T.: 7.925 min

Delta R.T.: 0.000 min

Response: 334019955

Conc: 157.61 ng/ml