

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024\
 Data File : PL091890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 02:22
 Operator : AR\AJ
 Sample : P3879-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DDC78

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2024
 Supervised By :mohammad ahmed 09/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 07:28:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.797	195.5E6	9389.9E6	111.948m	4411.501m#
2) SA Decachlor...	9.059	7.925	22235250	46462303	16.548m	21.836 #
Target Compounds						
2) A alpha-BHC	4.000	3.286	705.2E6	848.5E6	277.548	283.540
5) MB Aldrin	5.277	4.247	69324819	47906863	30.878	18.299 #
7) B delta-BHC	4.777	4.145	762.2E6	834.1E6	312.296	289.254

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024\
Data File : PL091890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 02:22
Operator : AR\AJ
Sample : P3879-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 07:28:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

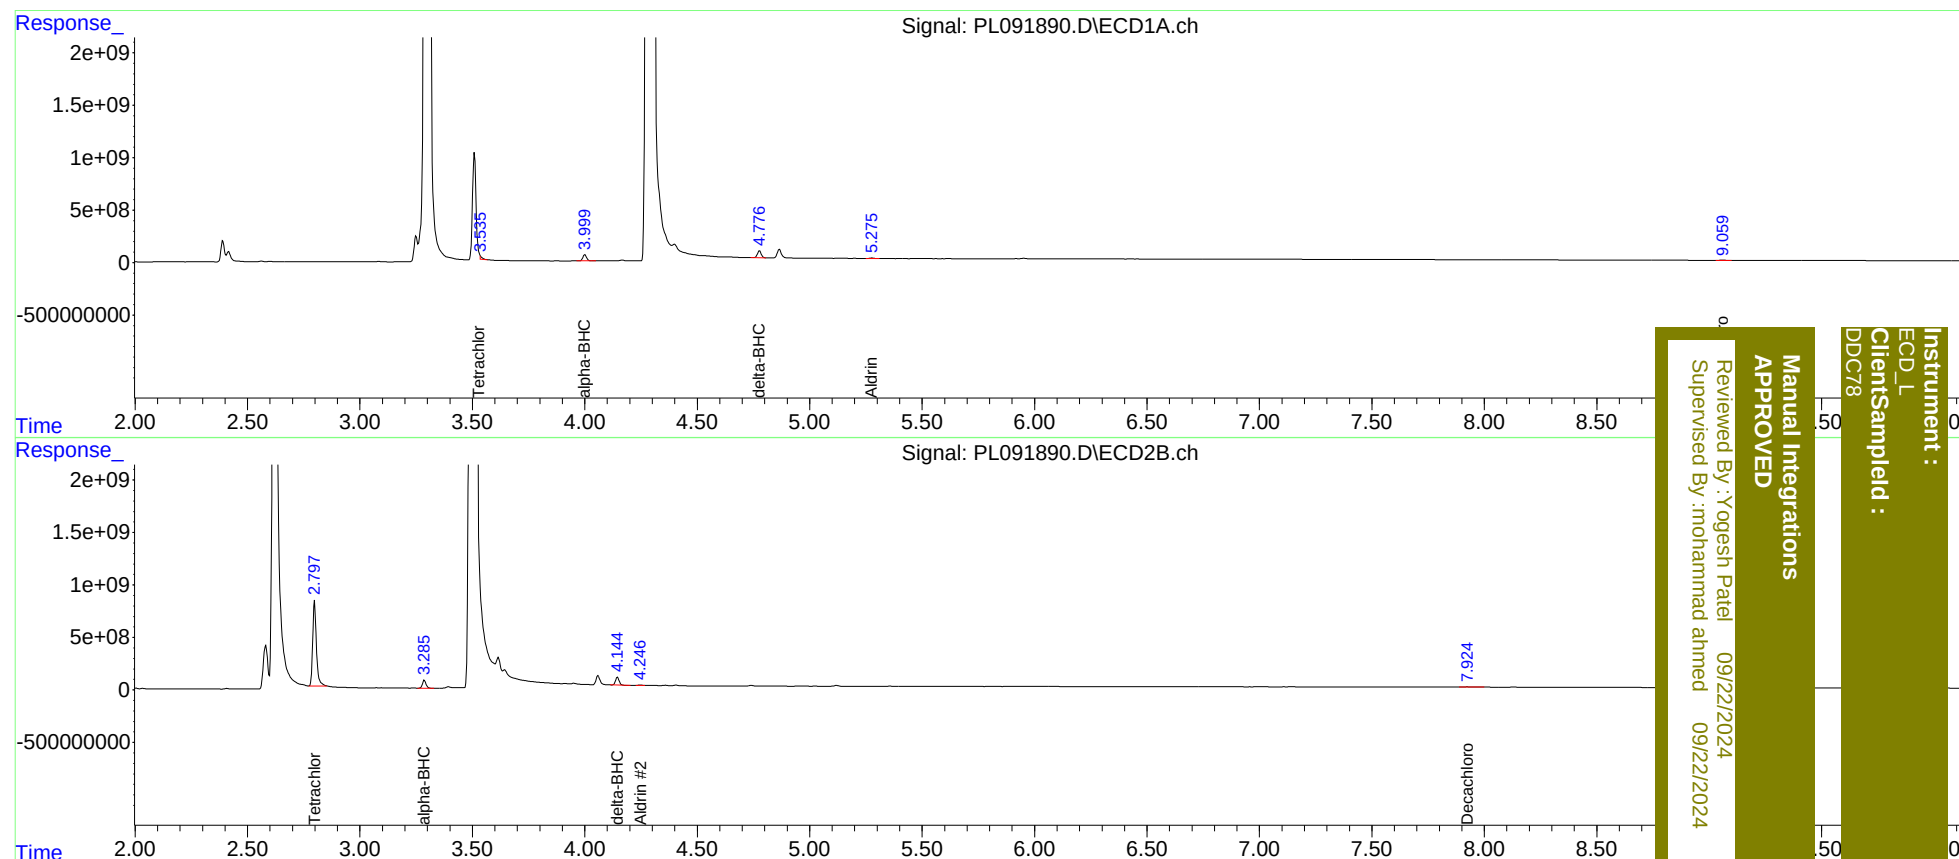

Instrument :
ECD_L
ClientSampled :
DDC78

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 09/22/2024
Supervised By : mohammad ahmed 09/22/2024