

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024\
 Data File : PL091893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 03:02
 Operator : AR\AJ
 Sample : P3879-11
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DCVZ9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2024
 Supervised By :mohammad ahmed 09/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 07:30:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.800	546.8E6	27547.7E6	313.087m	12942.309 #
2) SA Decachlor...	9.060	7.926	18241912	31183490	13.576m	14.656
Target Compounds						
2) A alpha-BHC	4.001	3.287	451.6E6	621.5E6	177.745	207.700
6) B beta-BHC	4.530	3.917	25757391	24604708	22.249m	18.990m
7) B delta-BHC	4.777	4.146	591.8E6	699.9E6	242.462	242.735
16) A 4,4'-DDD	6.697	5.798	149.9E6	191.1E6	105.158m	104.586m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024\
Data File : PL091893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 03:02
Operator : AR\AJ
Sample : P3879-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 07:30:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

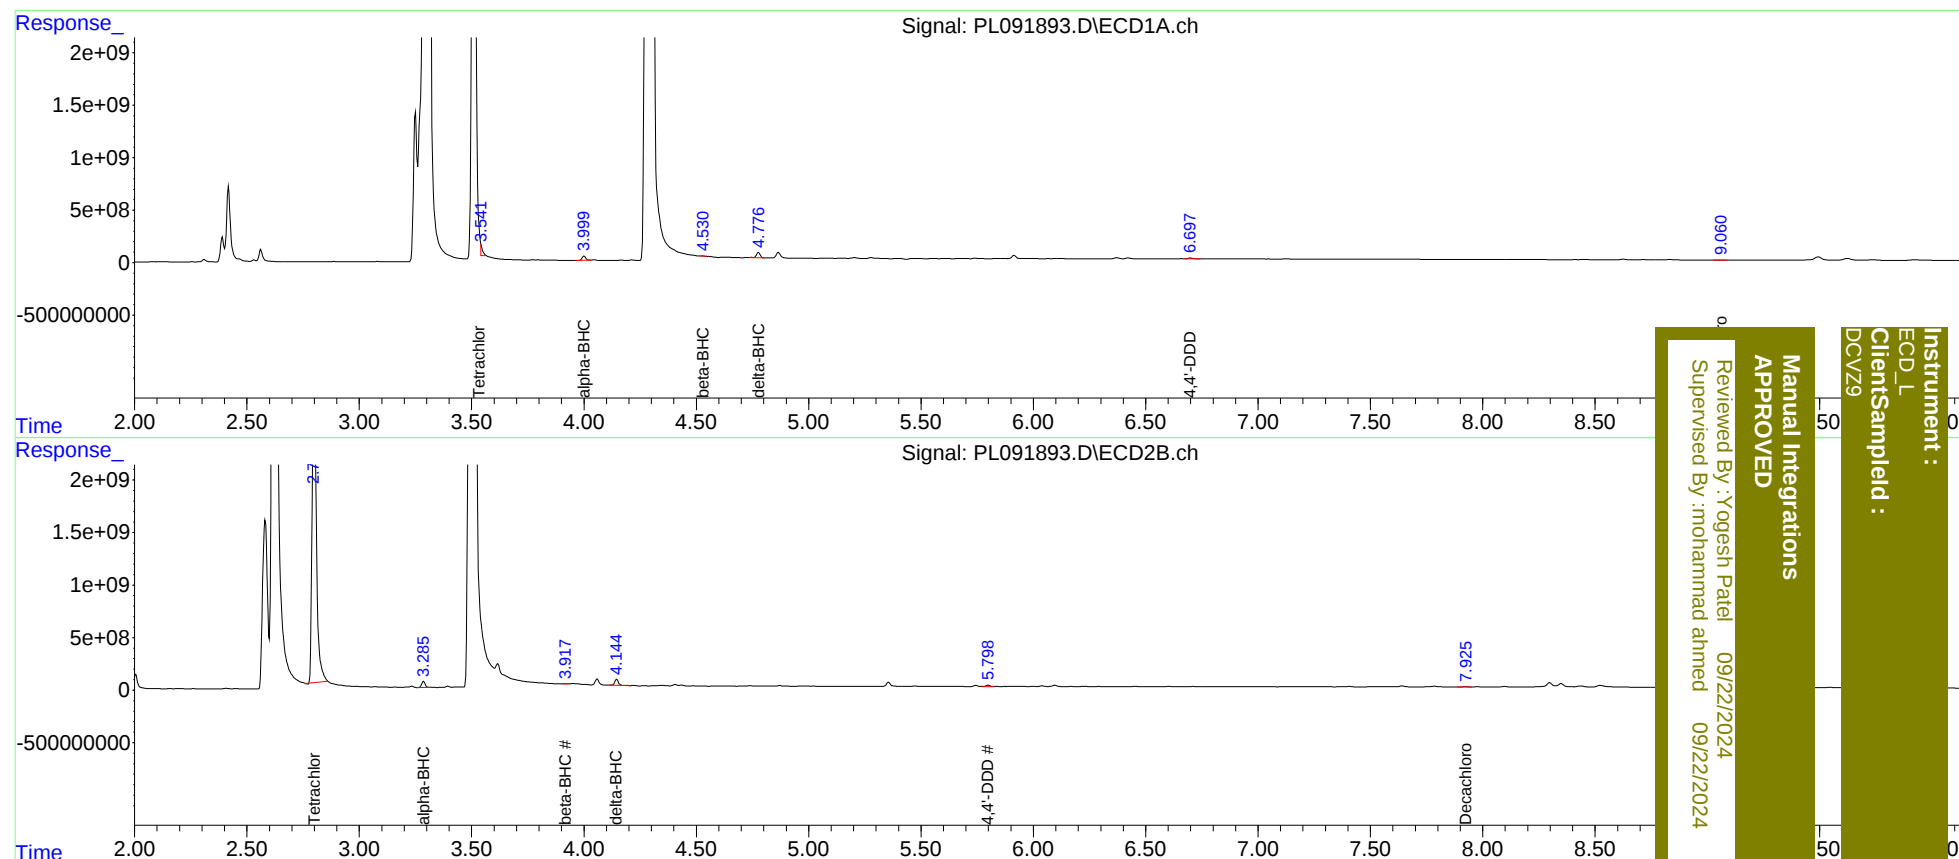

Reviewed By : Yogesh Patel 09/22/2024
Supervised By : mohammad ahmed 09/22/2024

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
DCVZ9