

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024\
 Data File : PL091888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 01:55
 Operator : AR\AJ
 Sample : P3879-06MS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DDC59MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2024
 Supervised By :mohammad ahmed 09/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 07:28:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.533	2.798	383.8E6	14196.0E6	219.730m	6669.474m#
27)	SA Decachlor...	9.062	7.925	25878140	41231666	19.259	19.378
Target Compounds							
2)	A alpha-BHC	4.001	3.287	665.1E6	837.1E6	261.734	279.749
3)	MA gamma-BHC...	4.269f	3.615	81123.4E6	1527.0E6	32993.263m	546.819m#
4)	MA Heptachlor	4.920	3.957	81589314	133.7E6	35.879m	47.739 #
5)	MB Aldrin	5.266	4.239	118.6E6	173.7E6	52.830	66.360 #
6)	B beta-BHC	4.528	3.918	58086638	141.4E6	50.174m	109.123m#
7)	B delta-BHC	4.778	4.146	762.4E6	910.8E6	312.375	315.869
8)	B Heptachlo...	5.689	4.740	147.4E6	245.2E6	72.372	100.021m#
9)	A Endosulfan I	6.074	5.119	75942175	416.5E6	41.898m	191.853 #
10)	B trans-Chl...	5.952	4.990	388.1E6	109.3E6	199.244	45.364 #
11)	B cis-Chlor...	6.023	5.053	140.7E6	107.5E6	69.310m	44.843 #
12)	B 4,4'-DDE	6.199	5.240	271.0E6	235.4E6	151.265	100.168m#
13)	MA Dieldrin	6.351	5.374	233.2E6	385.0E6	120.147	161.203 #
14)	MA Endrin	6.580	5.649	174.5E6	223.9E6	109.604	104.071
15)	B Endosulfa...	6.801	5.942	166.9E6	207.3E6	94.186	97.840m
16)	A 4,4'-DDD	6.715	5.797	165.4E6	207.0E6	116.029	113.273
17)	MA 4,4'-DDT	7.030	6.048	151.7E6	207.2E6	103.219	106.766
18)	B Endrin al...	6.931	6.122	132.1E6	166.2E6	103.750	107.596m
19)	B Endosulfa...	7.164	6.346	162.5E6	203.3E6	98.643	98.626
20)	A Methoxychlor	7.505	6.623	382.1E6	497.2E6	491.978	475.401
21)	B Endrin ke...	7.650	6.852	187.7E6	231.4E6	103.457	99.821

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092024\
Data File : PL091888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 01:55
Operator : AR\AJ
Sample : P3879-06MS
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 07:28:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

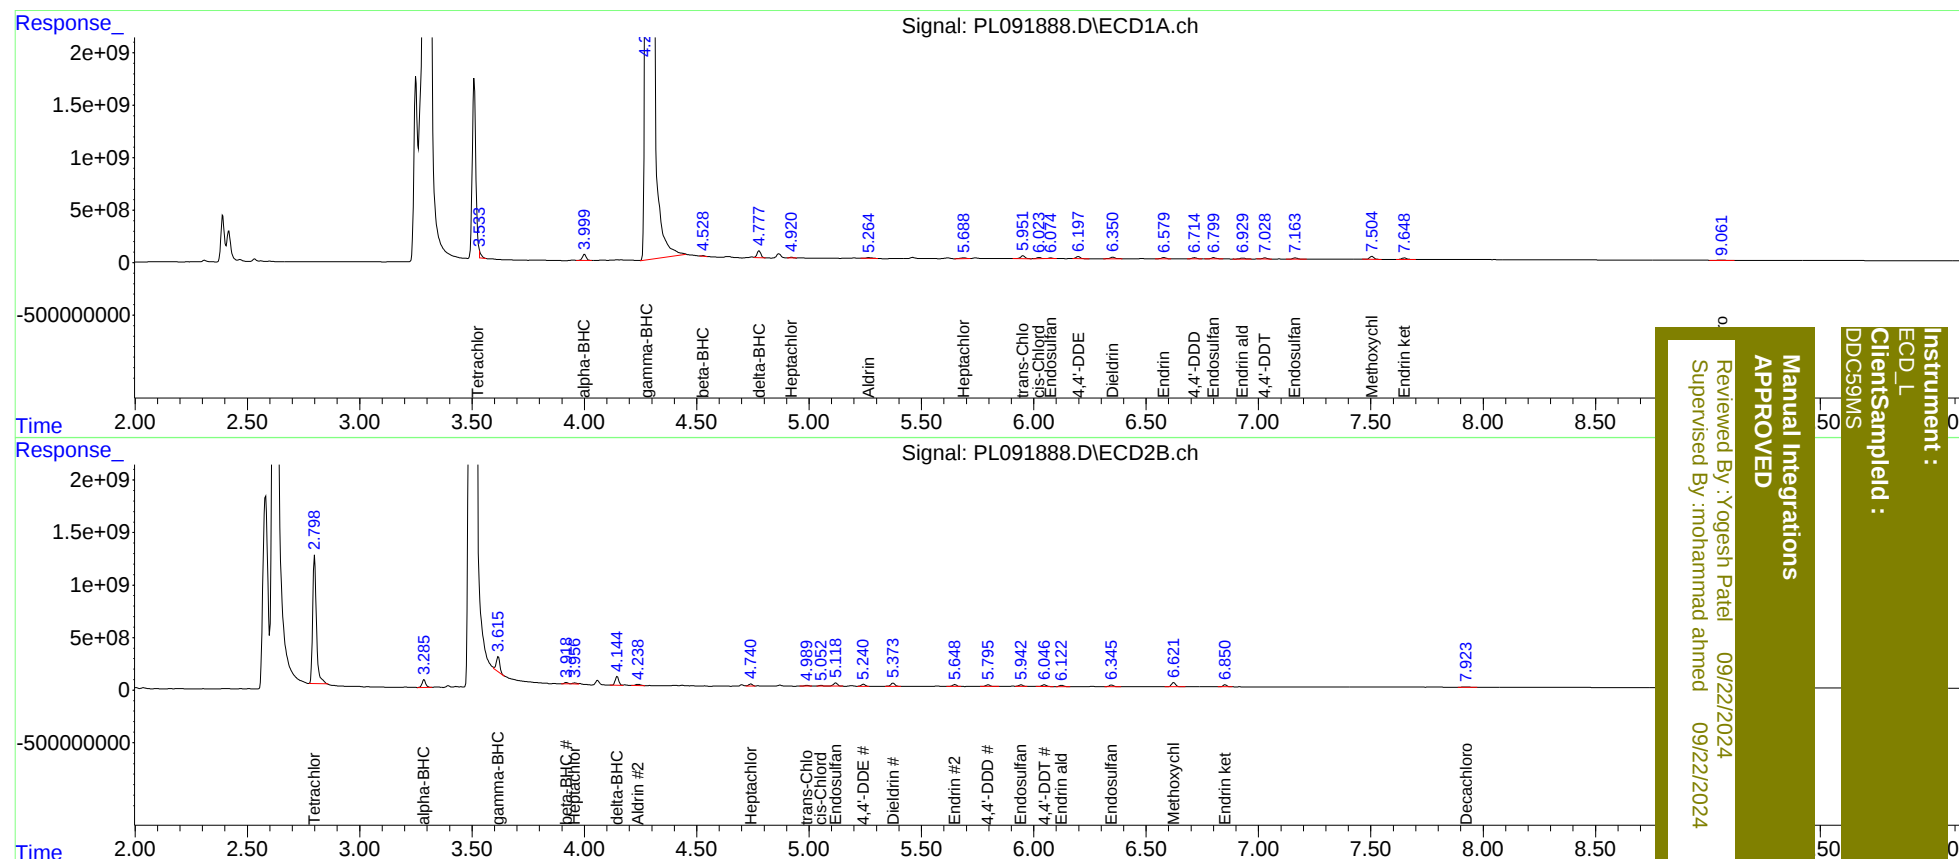

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 09/22/2024
Supervised By : mohammad ahmed 09/22/2024

Instrument :
ECD_L
ClientSampled :
DDC59MS