

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
 Data File : PL097268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2025 16:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:42:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.824	70468568	105.0E6	15.566	15.973
28)	SA Decachlor...	9.001	7.984	56635933	97364753	17.308	17.107
Target Compounds							
15)	B Endosulfa...	6.730	0.000	7804371	0	1.587	N.D. #
18)	B Endrin al...	0.000	6.168	0	13471912	N.D.	2.524 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
Data File : PL097268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2025 16:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:42:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

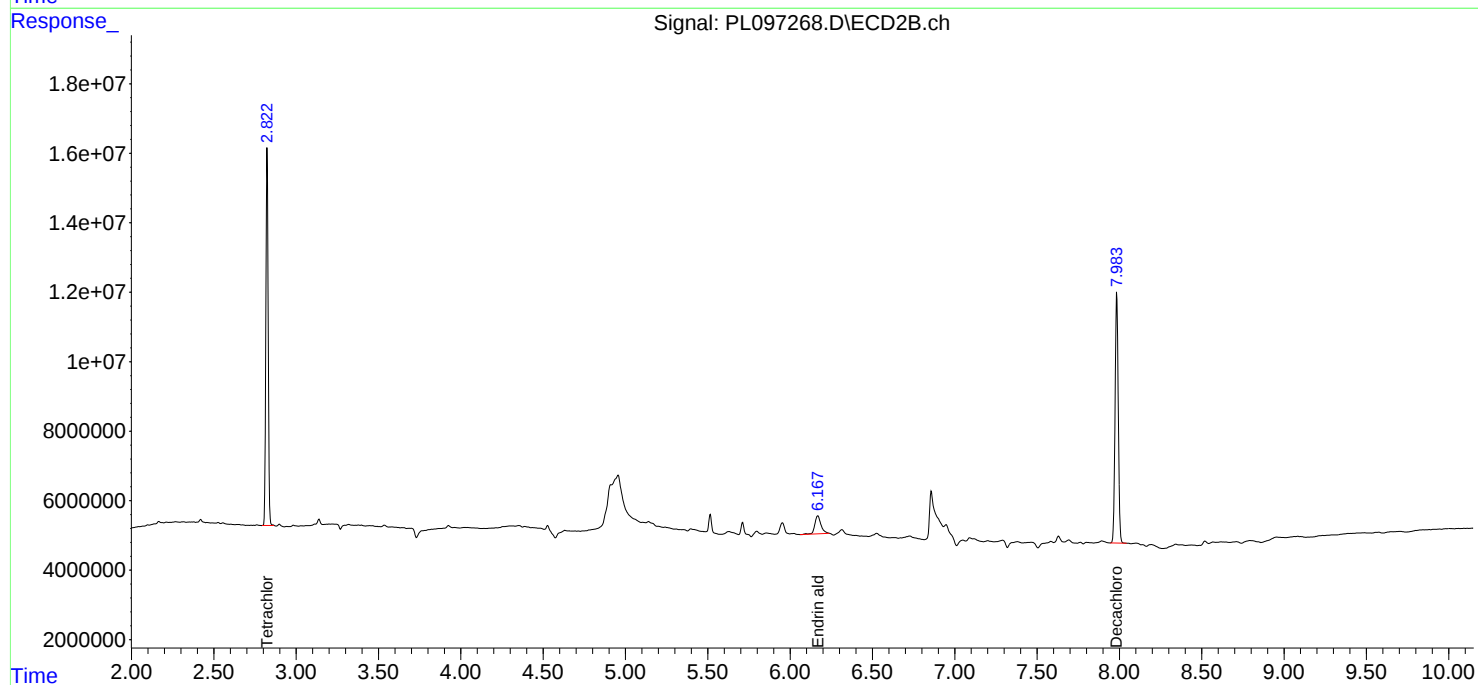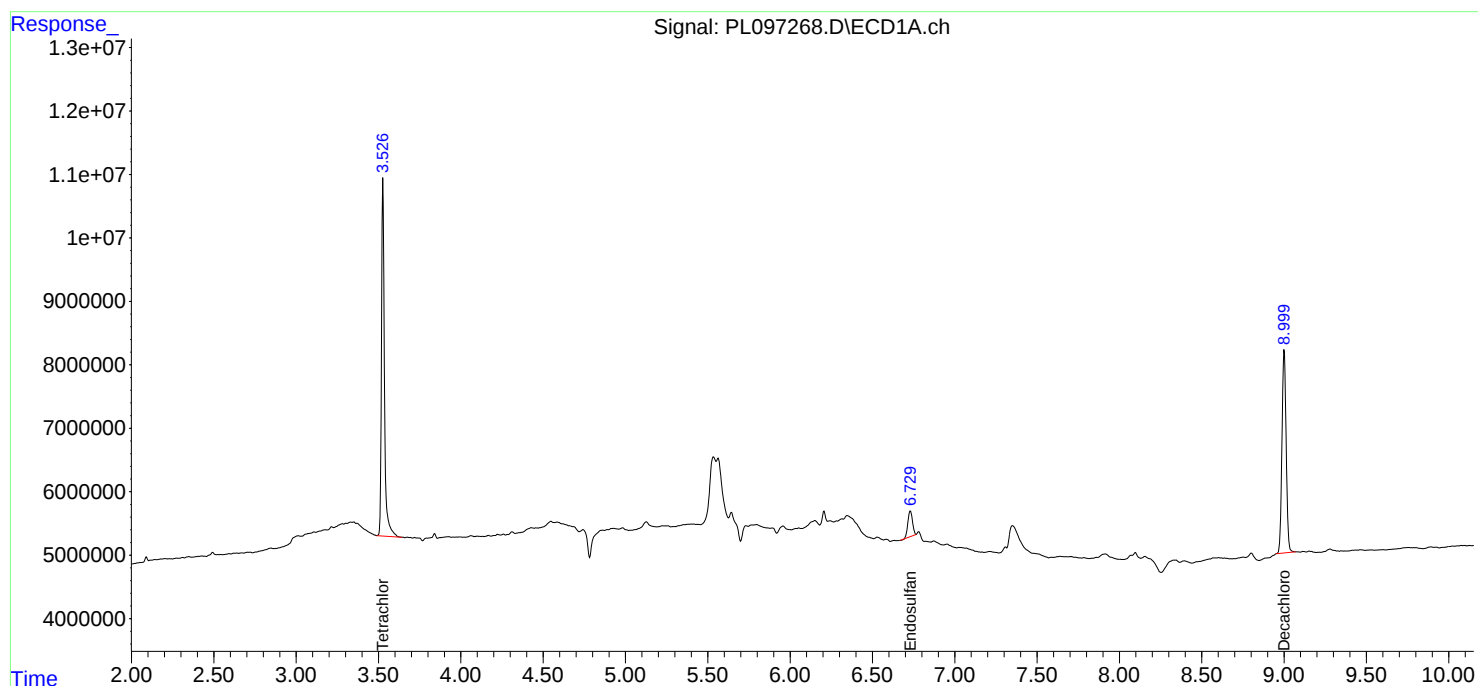


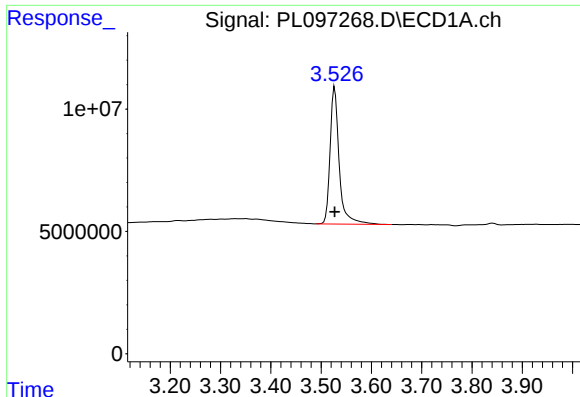

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 70468568
Conc: 15.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

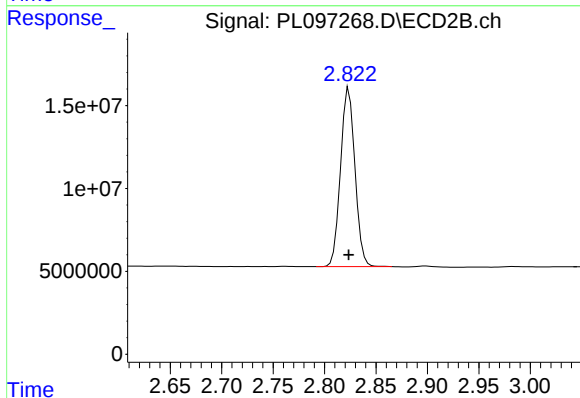


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 105031523
Conc: 15.97 ng/ml

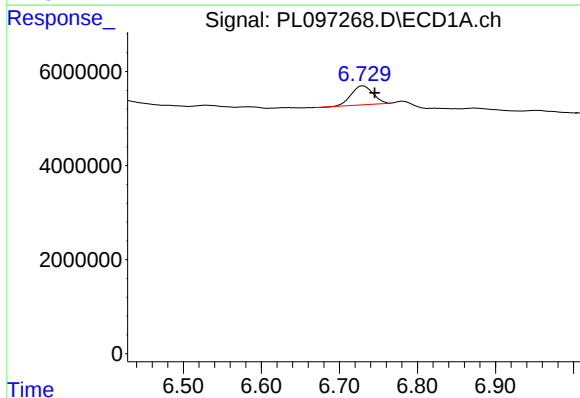


#15 Endosulfan II

R.T.: 6.730 min
Delta R.T.: -0.015 min
Response: 7804371
Conc: 1.59 ng/ml

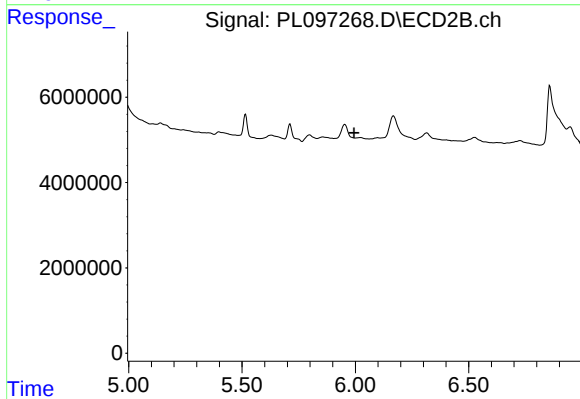

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.994 min
Response: 0
Conc: N.D.

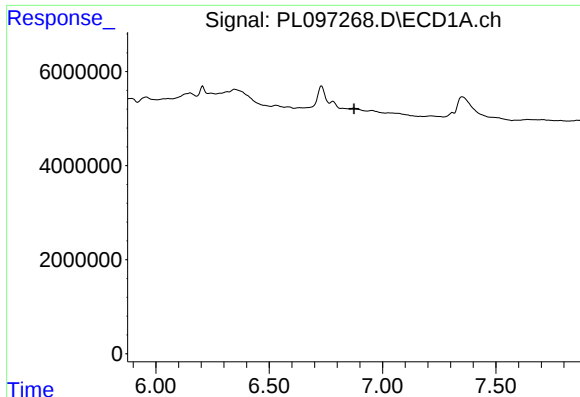

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

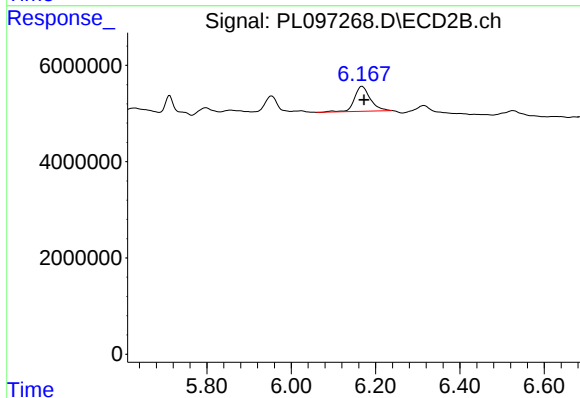


#18 Endrin aldehyde

R.T.: 6.168 min
Delta R.T.: -0.004 min
Response: 13471912
Conc: 2.52 ng/ml

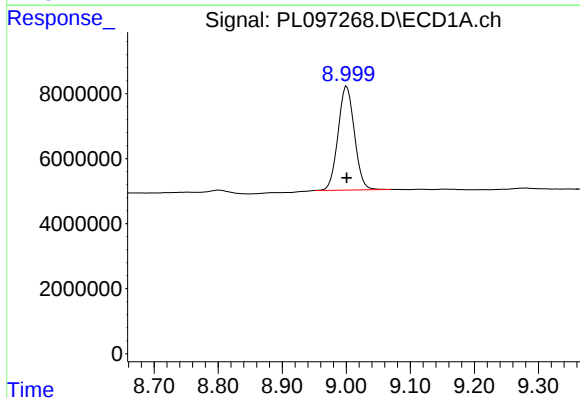

#28 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.000 min
Response: 56635933
Conc: 17.31 ng/ml

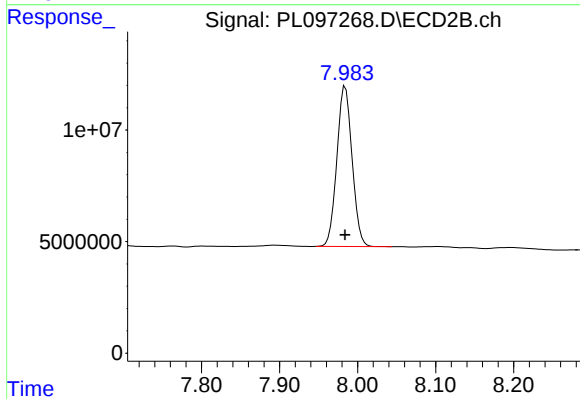

#28 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: 0.000 min
Response: 97364753
Conc: 17.11 ng/ml