

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
 Data File : PL097277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2025 18:28
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:25:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:24:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	2.823	274.3E6	532.9E6	75.672	76.064
28)	SA Decachlor...	9.001	7.984	192.4E6	341.0E6	73.542	73.095
Target Compounds							
23)	Chlordane-1	4.681	3.833	156.3E6	191.1E6	755.703	758.033
24)	Chlordane-2	5.204	4.412	160.7E6	210.6E6	743.598	740.720
25)	Chlordane-3	5.907	5.045	624.4E6	657.7E6	767.330	749.383
26)	Chlordane-4	5.991	5.108	754.4E6	576.9E6	760.435	752.709
27)	Chlordane-5	6.828	6.002	123.0E6	221.3E6	754.896	756.597



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
Data File : PL097277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2025 18:28
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:25:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:24:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

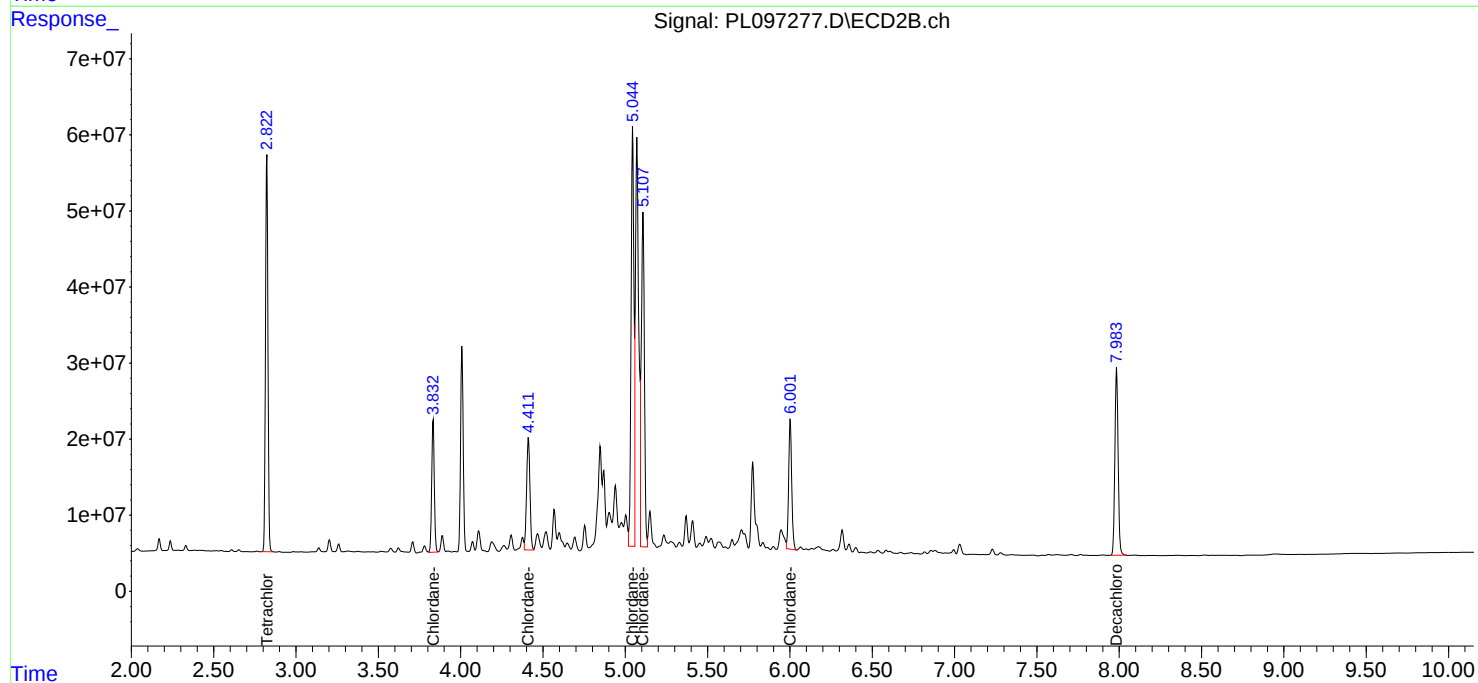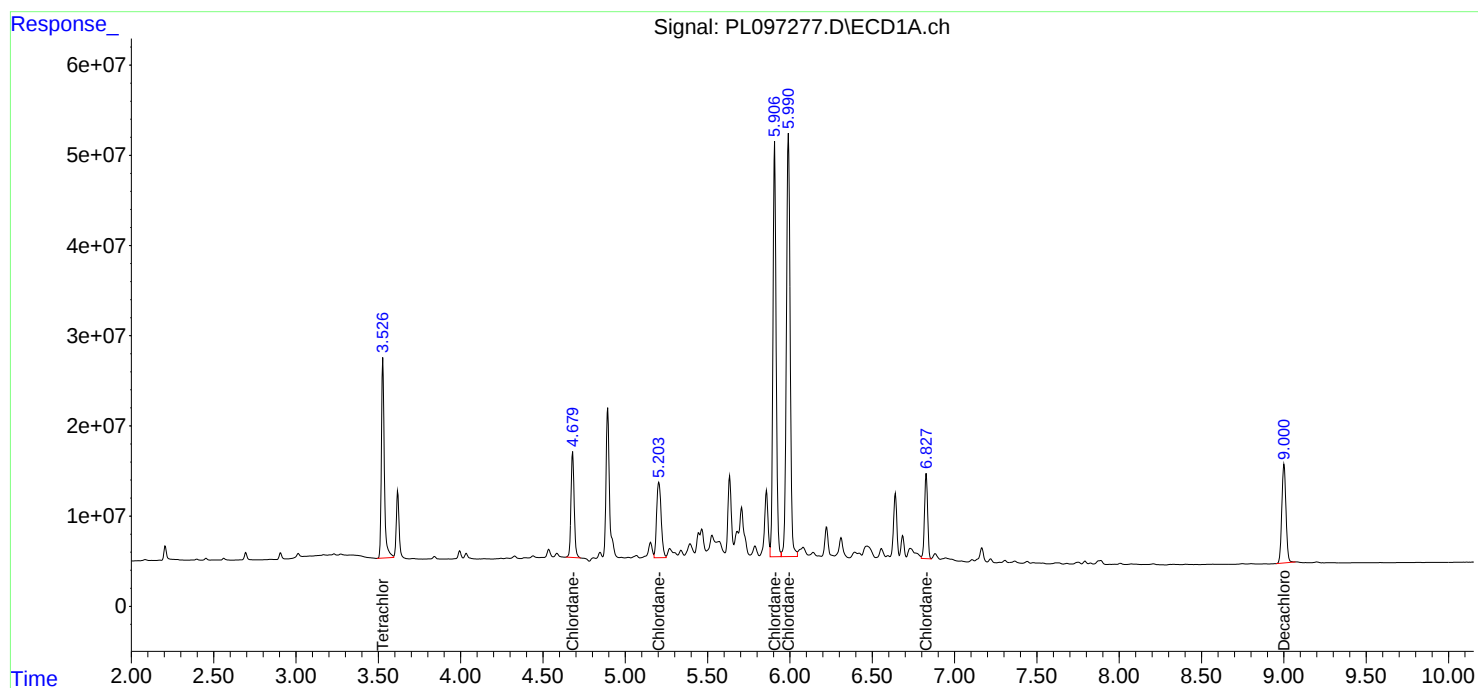


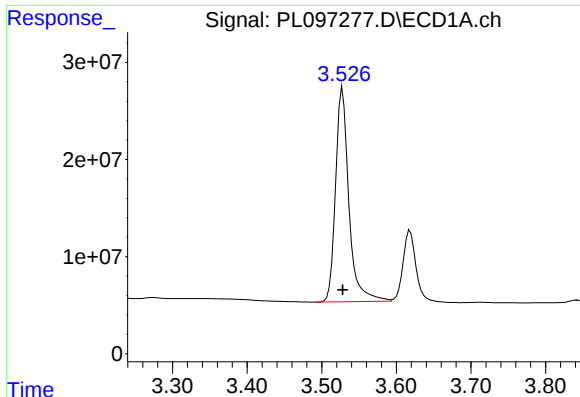

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 274252346
Conc: 75.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

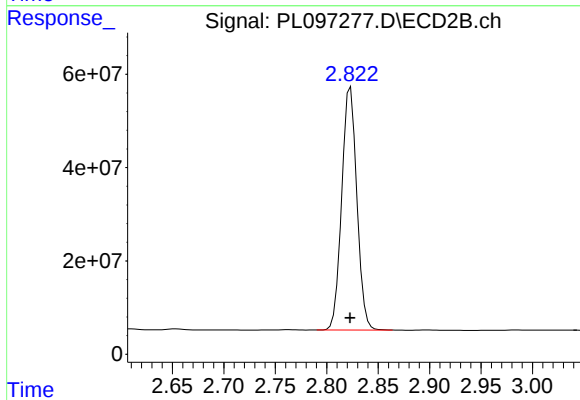


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 532896536
Conc: 76.06 ng/ml

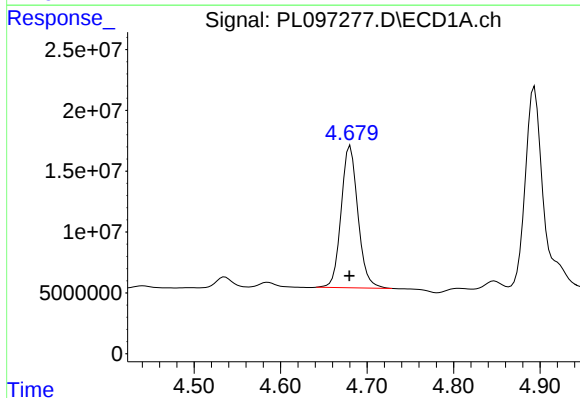


#23 Chlordane-1

R.T.: 4.681 min
Delta R.T.: 0.000 min
Response: 156317594
Conc: 755.70 ng/ml

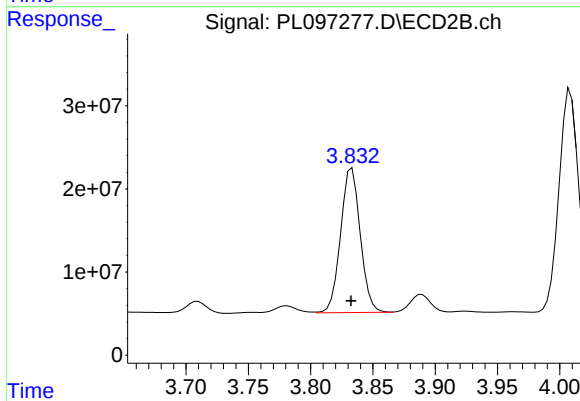

#23 Chlordane-1


R.T.: 3.833 min
Delta R.T.: 0.000 min
Response: 191143594
Conc: 758.03 ng/ml

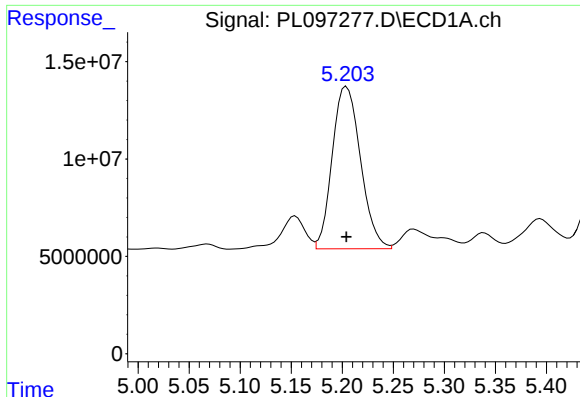

#24 Chlordane-2


R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 160688486
Conc: 743.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

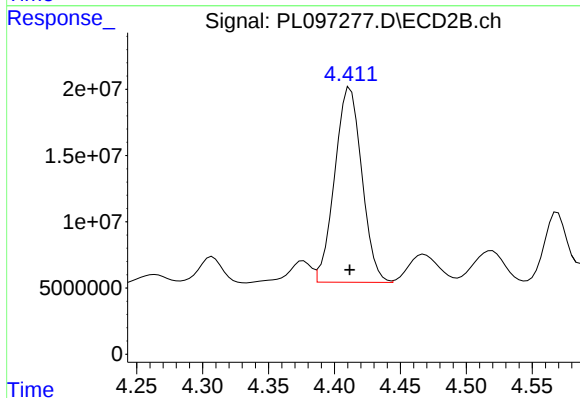


#24 Chlordane-2

R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 210590686
Conc: 740.72 ng/ml

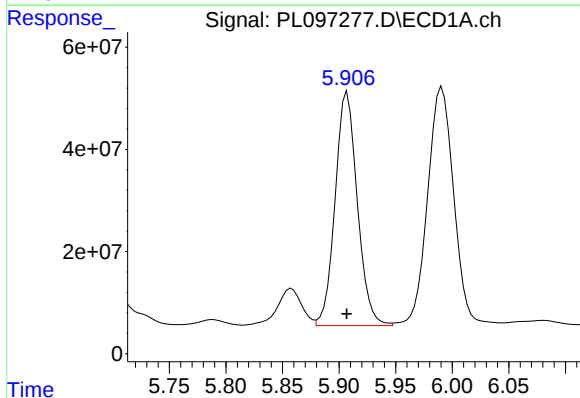


#25 Chlordane-3

R.T.: 5.907 min
Delta R.T.: 0.000 min
Response: 624417781
Conc: 767.33 ng/ml

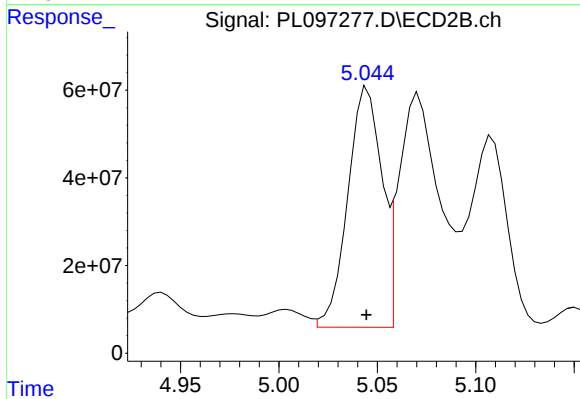

#25 Chlordane-3


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 657685163
Conc: 749.38 ng/ml

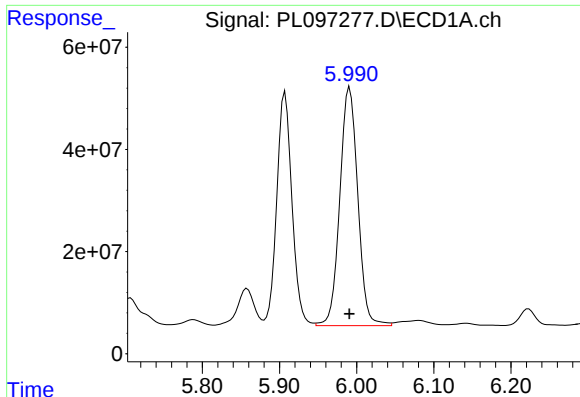

#26 Chlordane-4


R.T.: 5.991 min
Delta R.T.: 0.000 min
Response: 754386034
Conc: 760.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

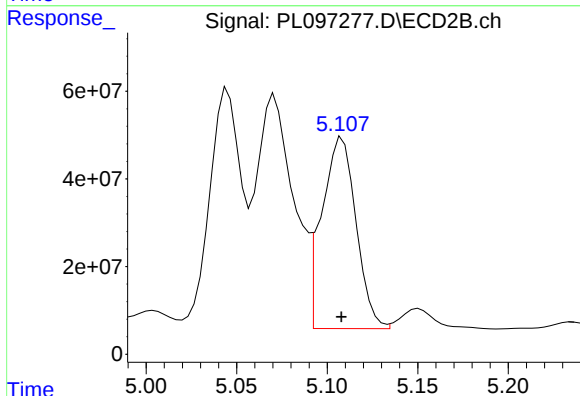


#26 Chlordane-4

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 576929725
Conc: 752.71 ng/ml

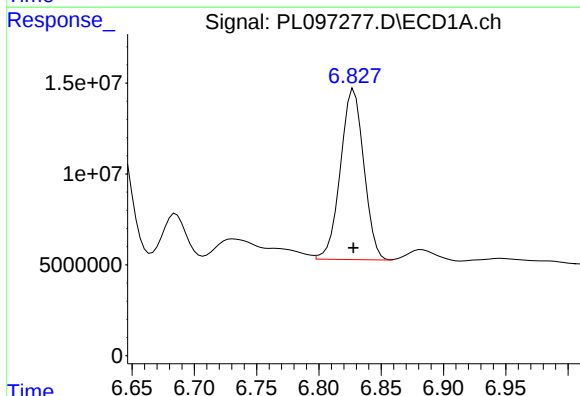


#27 Chlordane-5

R.T.: 6.828 min
Delta R.T.: 0.000 min
Response: 122956380
Conc: 754.90 ng/ml

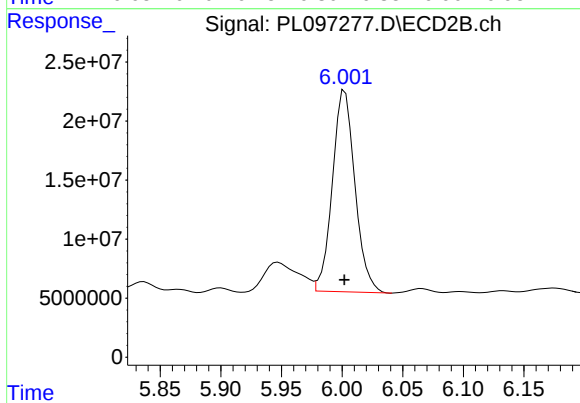

#27 Chlordane-5


R.T.: 6.002 min
Delta R.T.: 0.000 min
Response: 221330336
Conc: 756.60 ng/ml

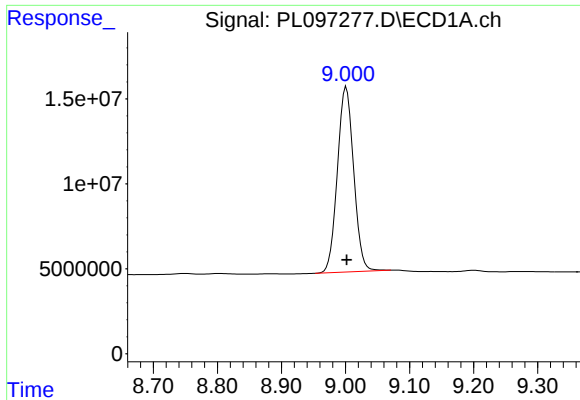

#28 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.000 min
Response: 192402228
Conc: 73.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

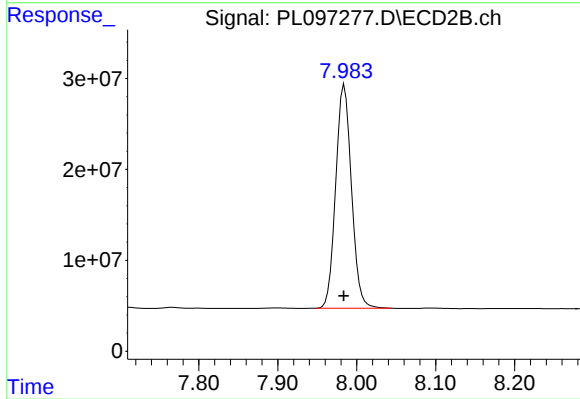

#28 Decachlorobiphenyl

R.T.: 7.984 min
Delta R.T.: 0.000 min
Response: 340998210
Conc: 73.10 ng/ml