

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
 Data File : PL097276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2025 18:14
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:25:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:24:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	2.823	369.7E6	711.5E6	102.020	101.550
28)	SA Decachlor...	9.001	7.985	259.0E6	456.4E6	99.008	97.839
Target Compounds							
23)	Chlordane-1	4.680	3.833	211.8E6	254.3E6	1023.904	1008.576
24)	Chlordane-2	5.203	4.412	213.8E6	279.8E6	989.458	984.039
25)	Chlordane-3	5.907	5.045	844.1E6	876.7E6	1037.331	998.970
26)	Chlordane-4	5.991	5.108	1020.8E6	771.5E6	1028.991	1006.591
27)	Chlordane-5	6.828	6.002	166.9E6	300.3E6	1024.830	1026.621



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
Data File : PL097276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2025 18:14
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:25:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:24:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

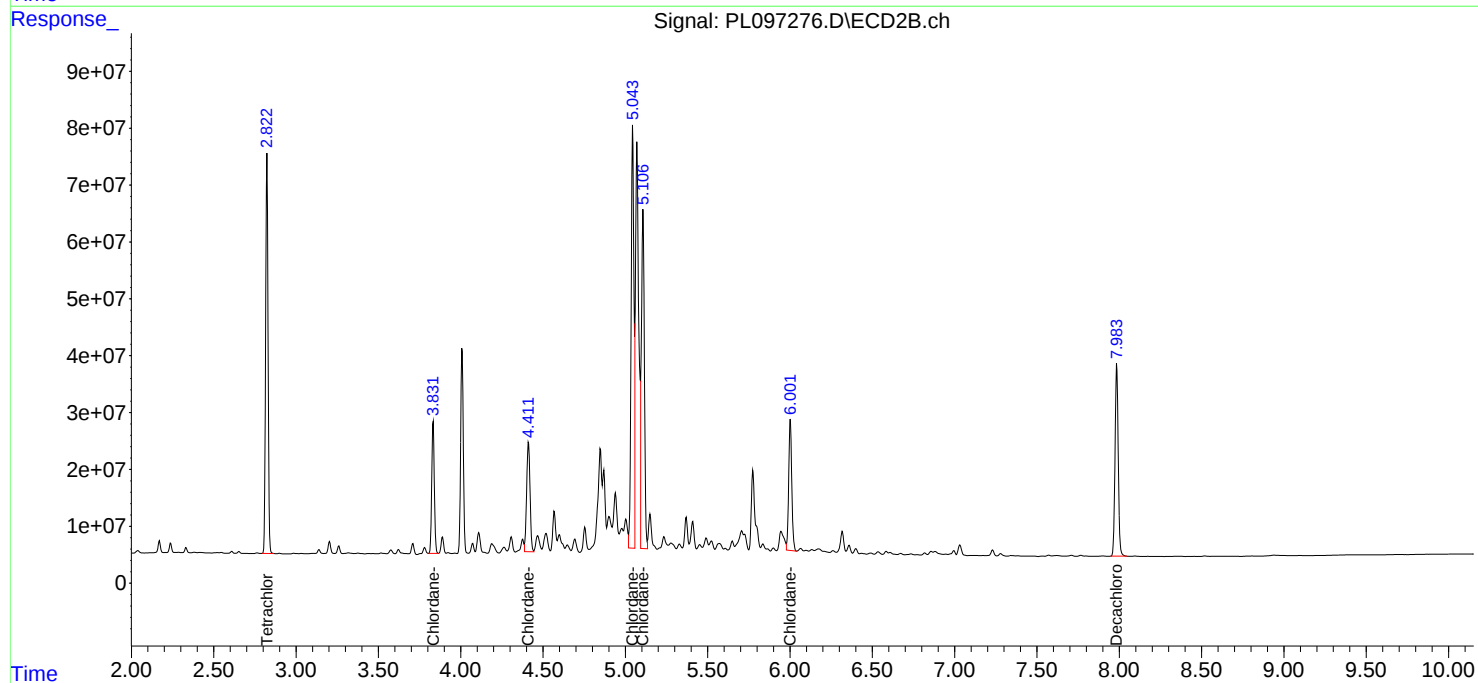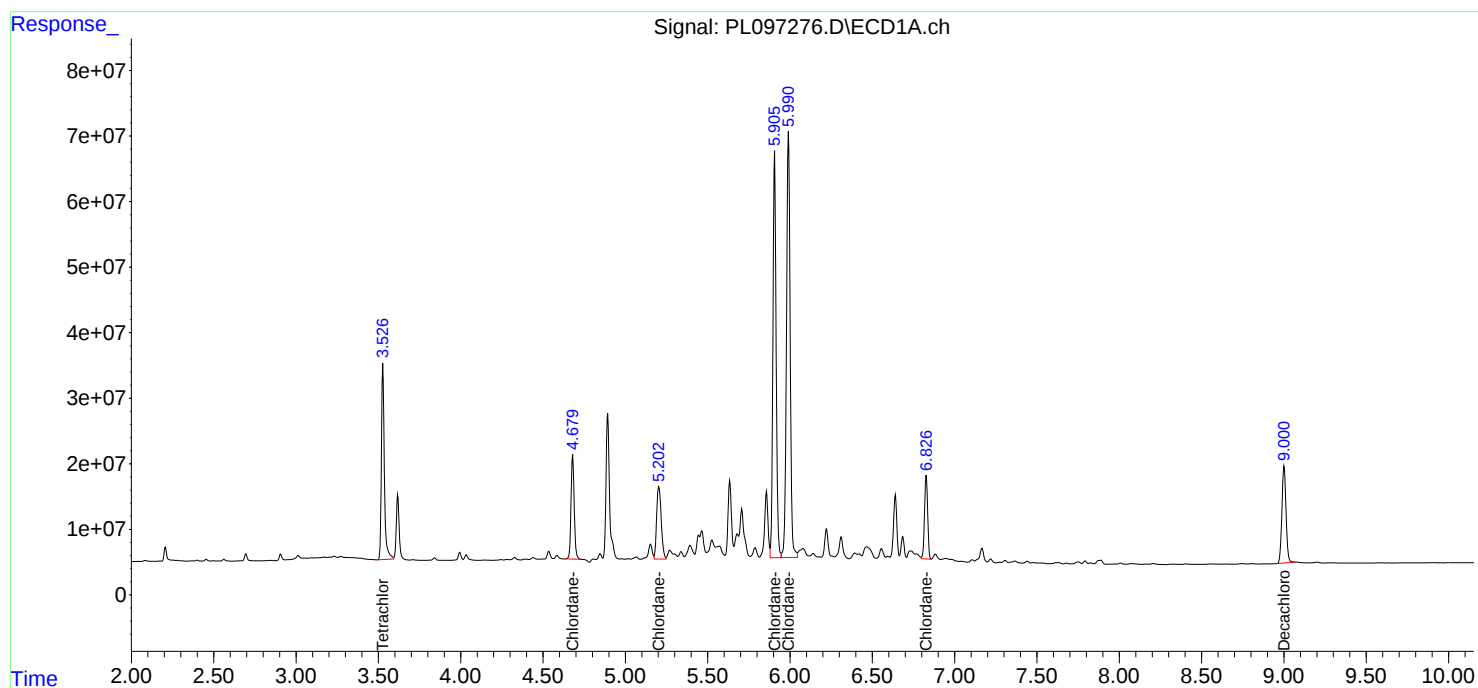


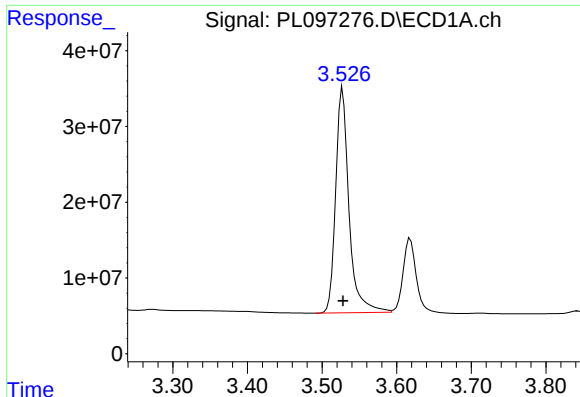

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 369743986
Conc: 102.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

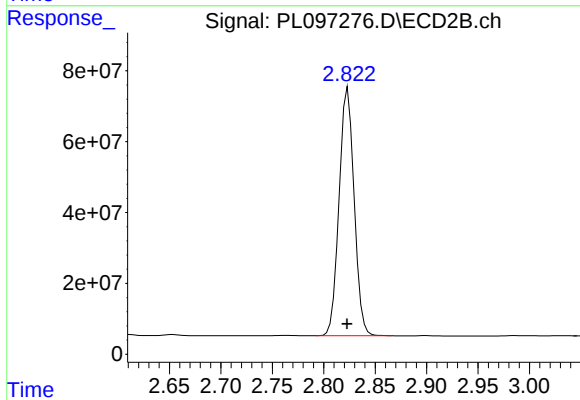


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 711452864
Conc: 101.55 ng/ml

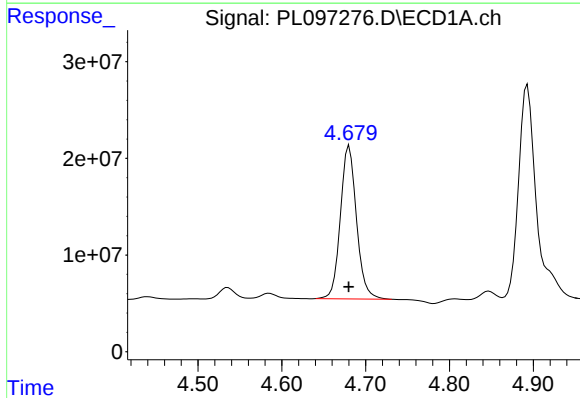


#23 Chlordane-1

R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 211795112
Conc: 1023.90 ng/ml

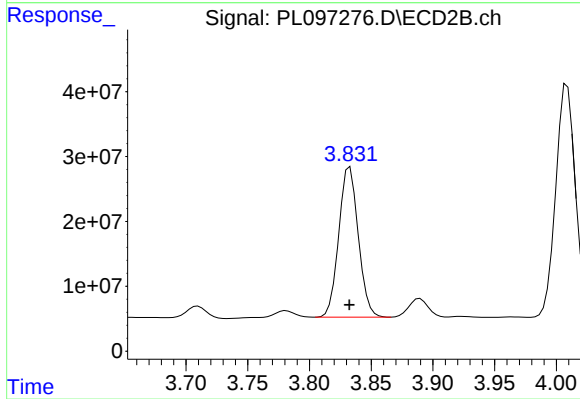

#23 Chlordane-1


R.T.: 3.833 min
Delta R.T.: 0.000 min
Response: 254320022
Conc: 1008.58 ng/ml

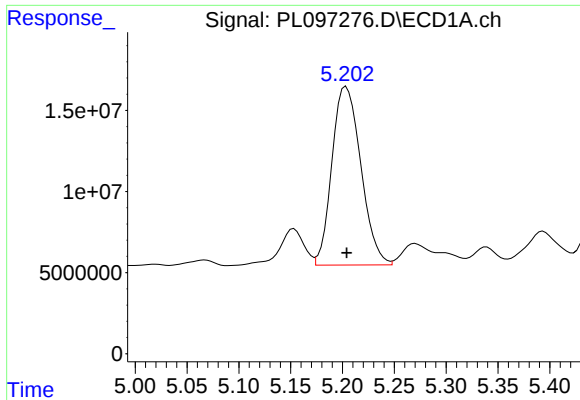

#24 Chlordane-2


R.T.: 5.203 min
Delta R.T.: 0.000 min
Response: 213817836
Conc: 989.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

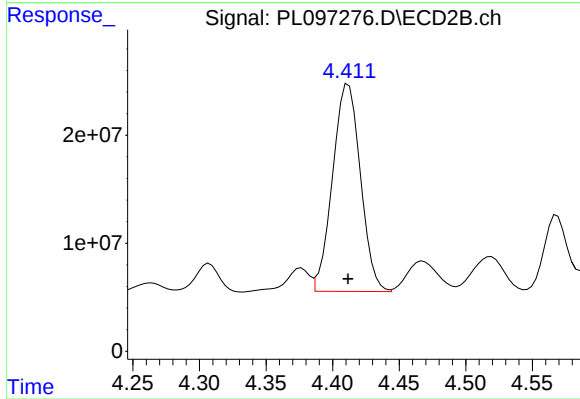


#24 Chlordane-2

R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 279767634
Conc: 984.04 ng/ml

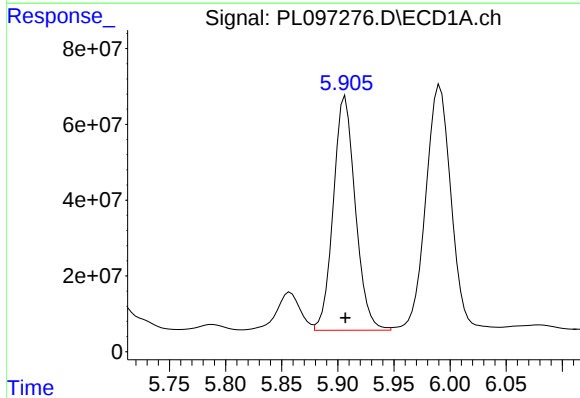


#25 Chlordane-3

R.T.: 5.907 min
Delta R.T.: 0.000 min
Response: 844132802
Conc: 1037.33 ng/ml

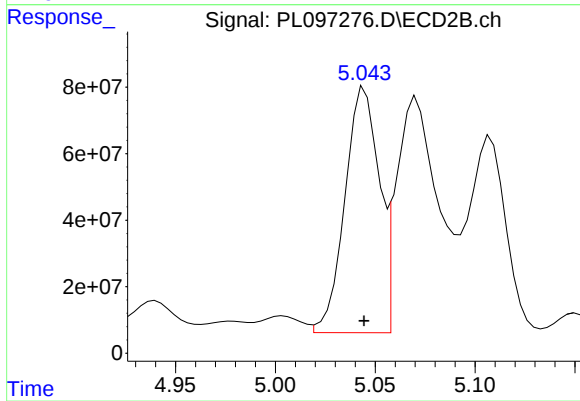

#25 Chlordane-3


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 876731409
Conc: 998.97 ng/ml

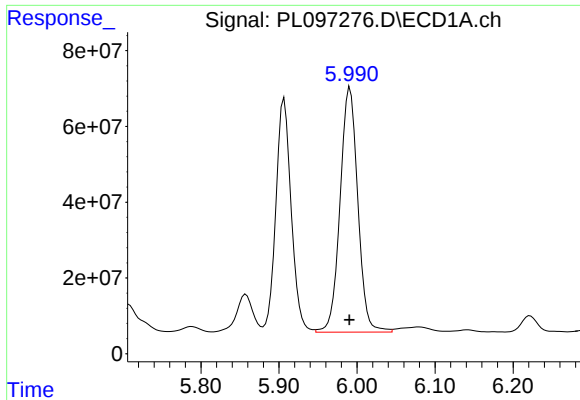

#26 Chlordane-4


R.T.: 5.991 min
Delta R.T.: 0.000 min
Response: 1020805608
Conc: 1028.99 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

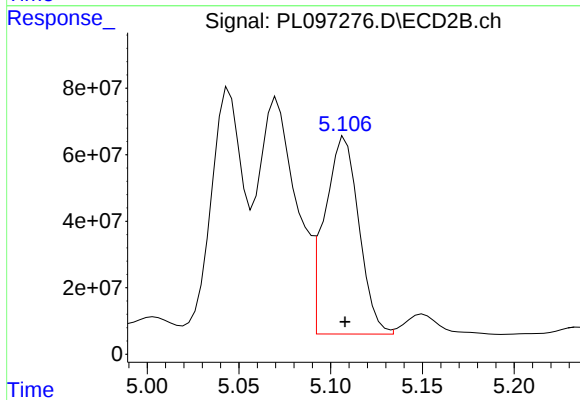


#26 Chlordane-4

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 771523105
Conc: 1006.59 ng/ml

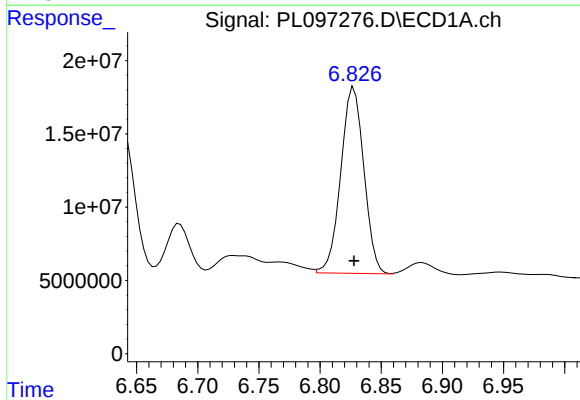


#27 Chlordane-5

R.T.: 6.828 min
Delta R.T.: 0.000 min
Response: 166922807
Conc: 1024.83 ng/ml

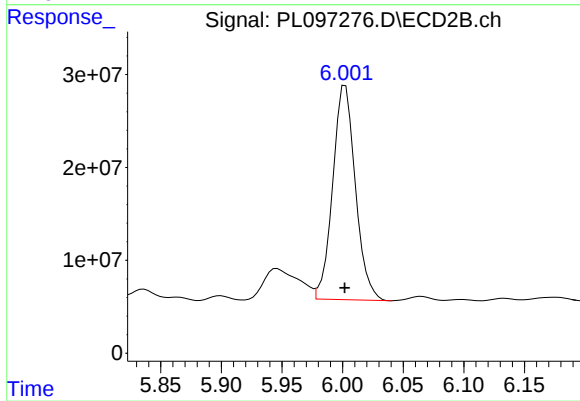

#27 Chlordane-5


R.T.: 6.002 min
Delta R.T.: 0.000 min
Response: 300321307
Conc: 1026.62 ng/ml

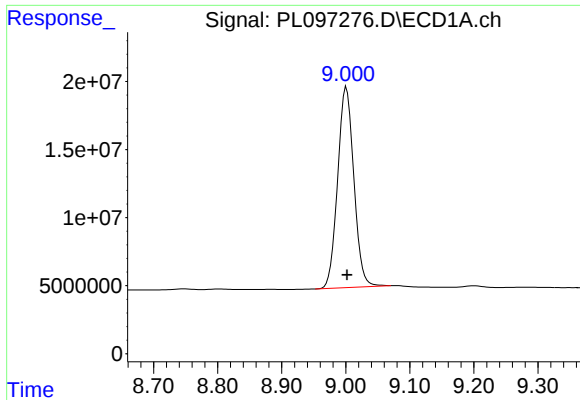

#28 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.000 min
Response: 259026560
Conc: 99.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

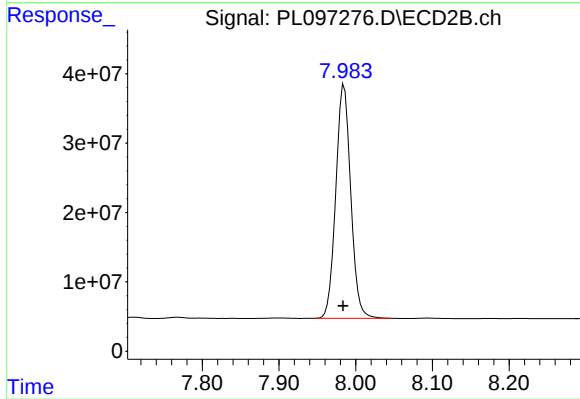

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: 0.001 min
Response: 456429722
Conc: 97.84 ng/ml