

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
 Data File : PL097279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2025 18:55
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:25:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:24:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.823	92961241	176.7E6	25.650	25.217
28)	SA Decachlor...	9.001	7.984	68343440	122.2E6	26.123	26.186
Target Compounds							
23)	Chlordane-1	4.680	3.833	53048556	63412421	256.458	251.479
24)	Chlordane-2	5.204	4.412	56610080	74787331	261.967	263.053
25)	Chlordane-3	5.907	5.045	201.3E6	222.8E6	247.413	253.815
26)	Chlordane-4	5.991	5.108	245.0E6	192.3E6	246.934	250.900
27)	Chlordane-5	6.828	6.002	42246305	74302927	259.373	253.998


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092025\
Data File : PL097279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2025 18:55
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:25:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:24:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

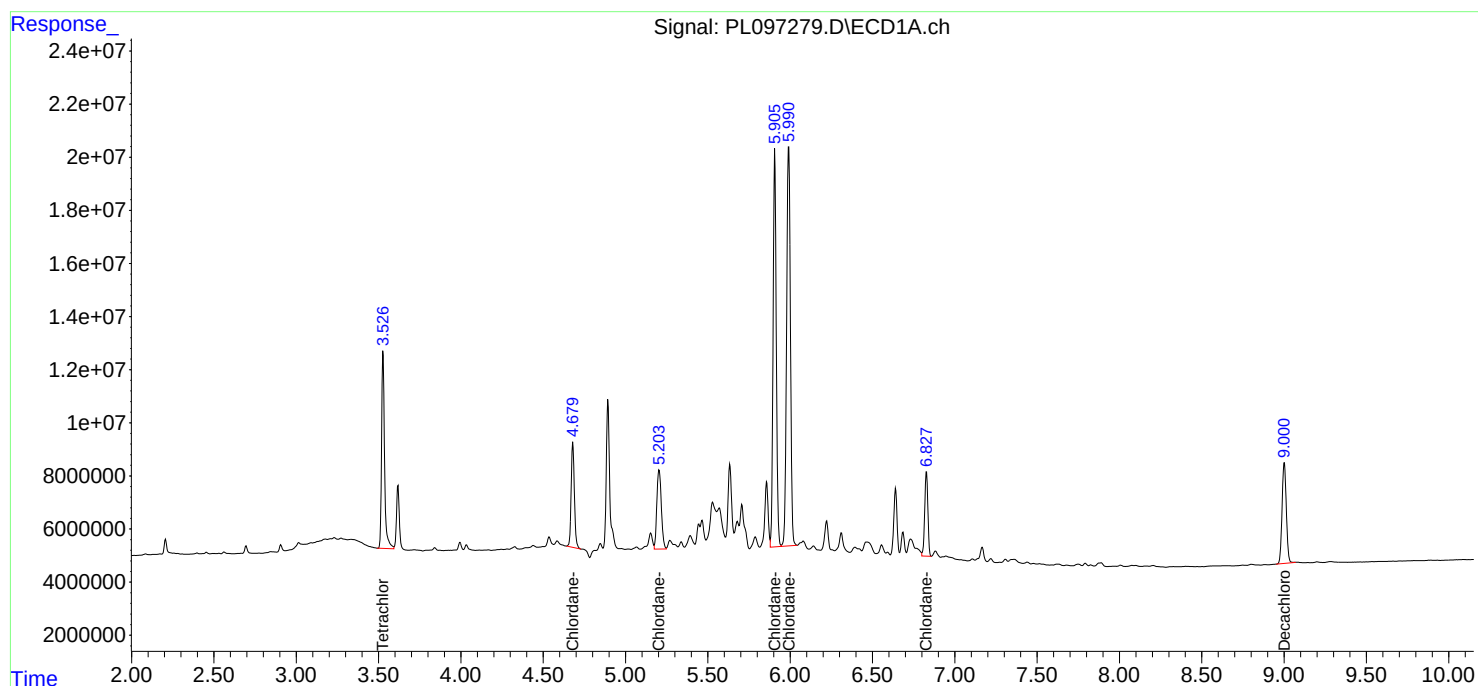


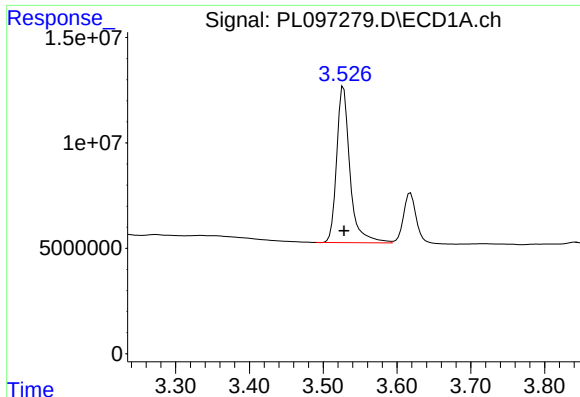

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 92961241
Conc: 25.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

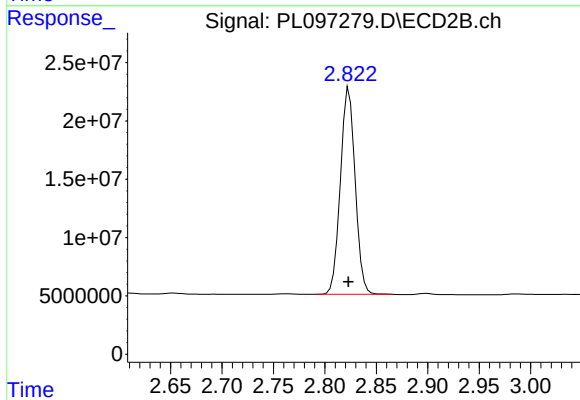


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 176667328
Conc: 25.22 ng/ml

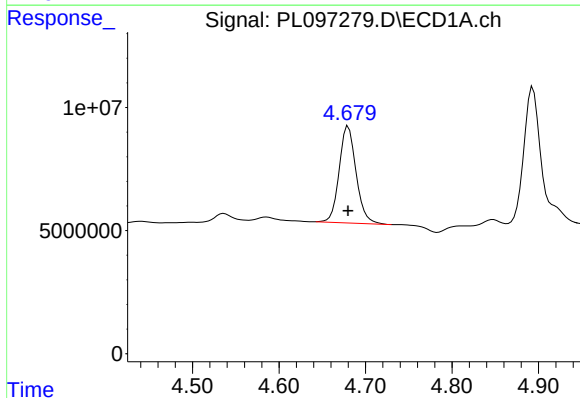


#23 Chlordane-1

R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 53048556
Conc: 256.46 ng/ml

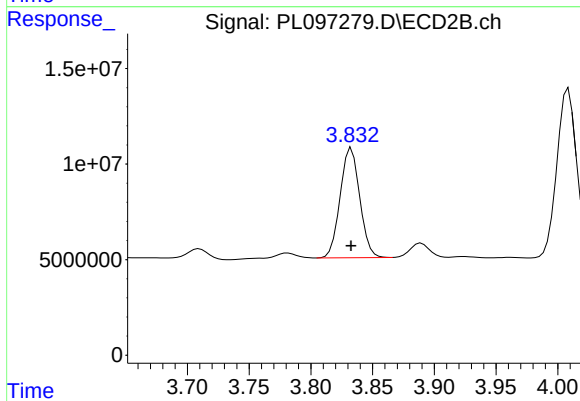

#23 Chlordane-1


R.T.: 3.833 min
Delta R.T.: 0.000 min
Response: 63412421
Conc: 251.48 ng/ml

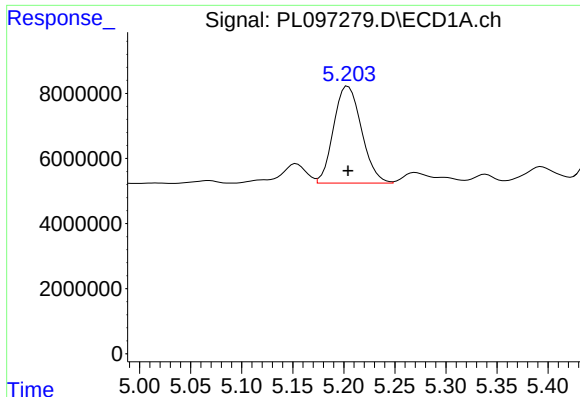

#24 Chlordane-2


R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 56610080
Conc: 261.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

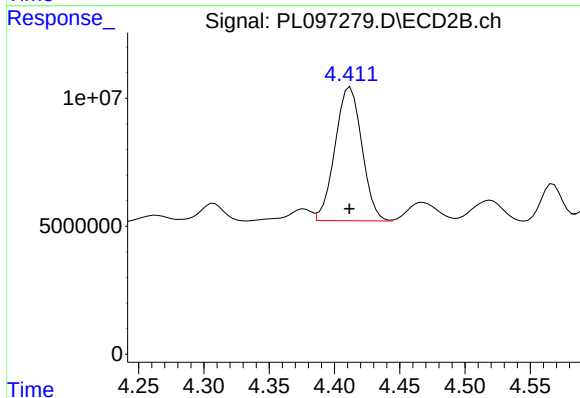


#24 Chlordane-2

R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 74787331
Conc: 263.05 ng/ml

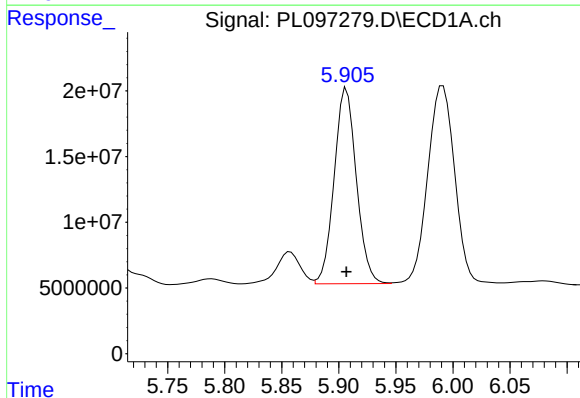


#25 Chlordane-3

R.T.: 5.907 min
Delta R.T.: 0.000 min
Response: 201333389
Conc: 247.41 ng/ml

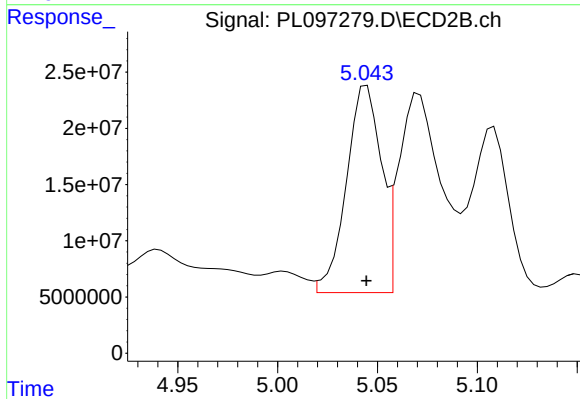

#25 Chlordane-3


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 222757291
Conc: 253.82 ng/ml

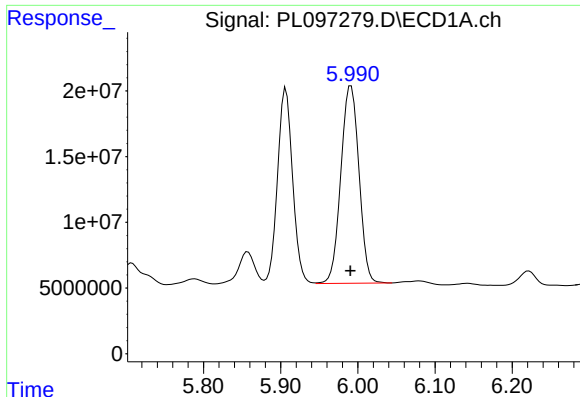

#26 Chlordane-4


R.T.: 5.991 min
Delta R.T.: 0.000 min
Response: 244969718
Conc: 246.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

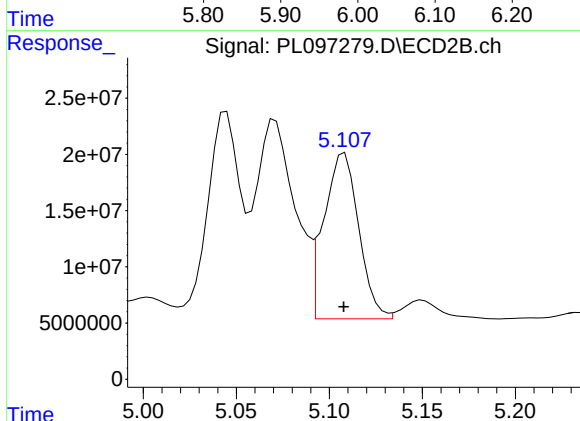


#26 Chlordane-4

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 192307377
Conc: 250.90 ng/ml

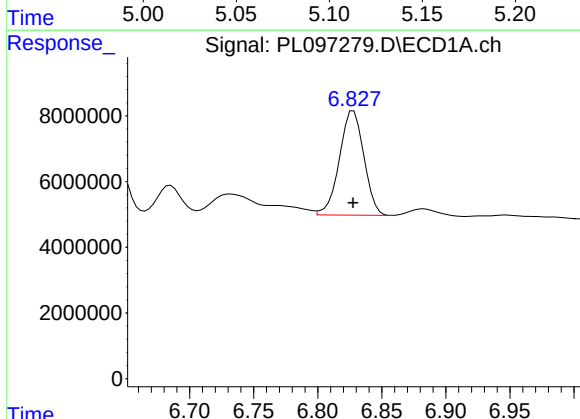


#27 Chlordane-5

R.T.: 6.828 min
Delta R.T.: 0.000 min
Response: 42246305
Conc: 259.37 ng/ml

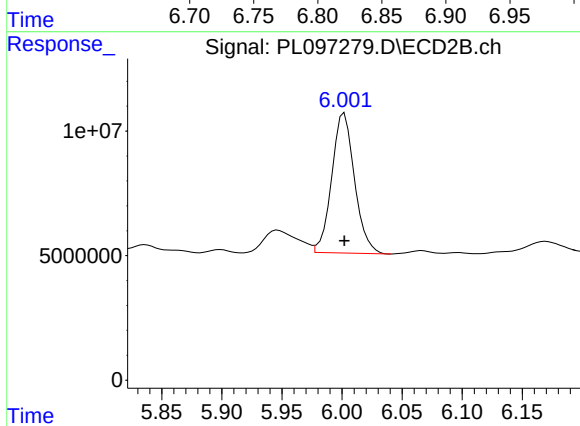

#27 Chlordane-5

R.T.: 6.002 min
Delta R.T.: 0.000 min
Response: 74302927
Conc: 254.00 ng/ml

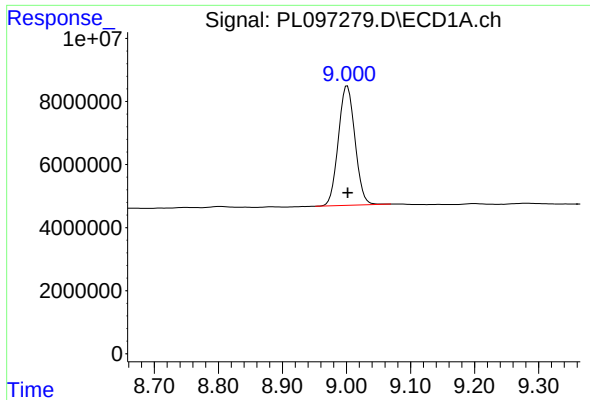

#28 Decachlorobiphenyl


R.T.: 9.001 min

Delta R.T.: 0.000 min

Response: 68343440

Conc: 26.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

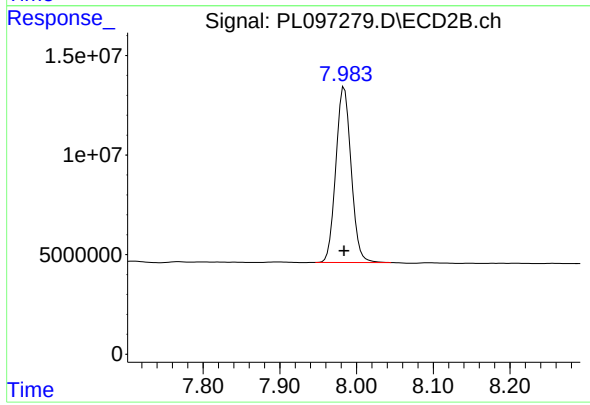

#28 Decachlorobiphenyl

R.T.: 7.984 min

Delta R.T.: 0.000 min

Response: 122159280

Conc: 26.19 ng/ml