

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092118\
 Data File : PL040171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2018 10:14
 Operator : AJ\SJ
 Sample : J4979-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 10:32:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.901	103.8E6	39068934	13.388	12.244
28)	SA Decachlor...	7.953	8.888	122.6E6	50380196	14.718	18.549 #
Target Compounds							
3)	MA gamma-BHC...	4.015	0.000	57422574	0	5.018	N.D. #
5)	MB Aldrin	4.515	0.000	44393045	0	4.028	N.D. #
7)	B delta-BHC	0.000	4.947	0	15062846	N.D.	3.787 #
8)	B Heptachlo...	0.000	5.764	0	28008853	N.D.	7.082 #
15)	B Endosulfa...	5.992f	0.000	367.9E6	0	38.395	N.D. #
16)	A 4,4'-DDD	0.000	6.638f	0	90147614	N.D.	31.182 #
23)	Chlordane-1	0.000	4.947	0	15062846	N.D.	97.276 #
27)	Chlordane-5	5.992	0.000	367.9E6	0	992.214	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092118\
Data File : PL040171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2018 10:14
Operator : AJ\SJ
Sample : J4979-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 10:32:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

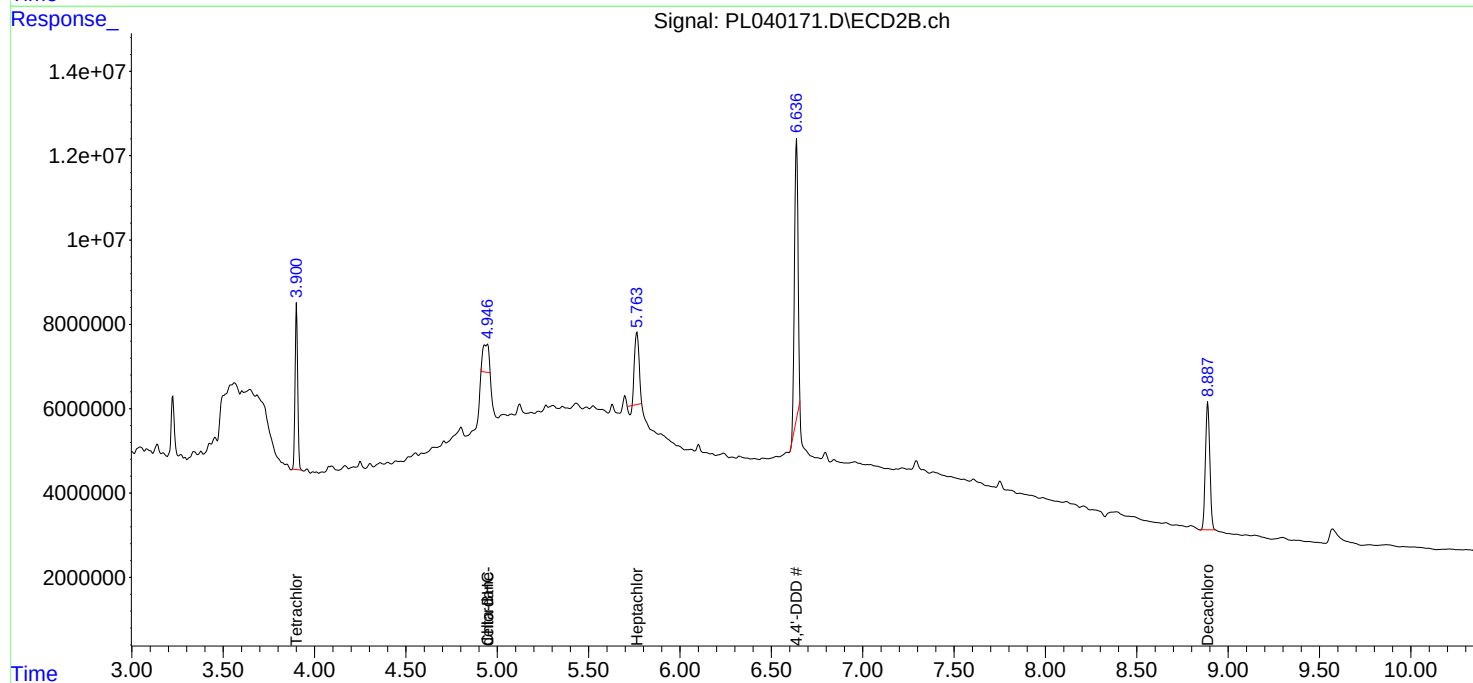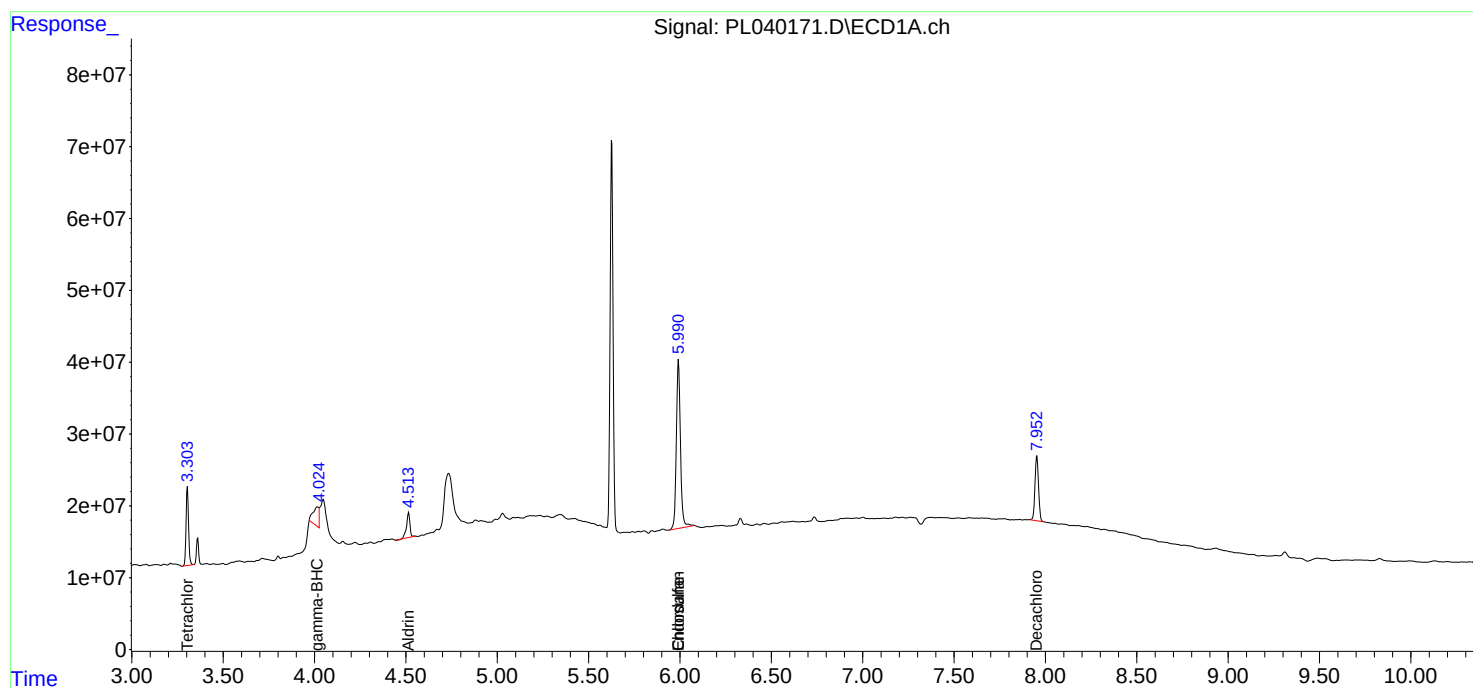


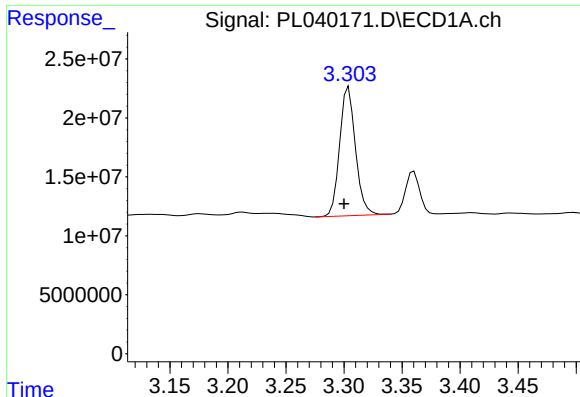

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: 0.004 min
Response: 103820659
Conc: 13.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

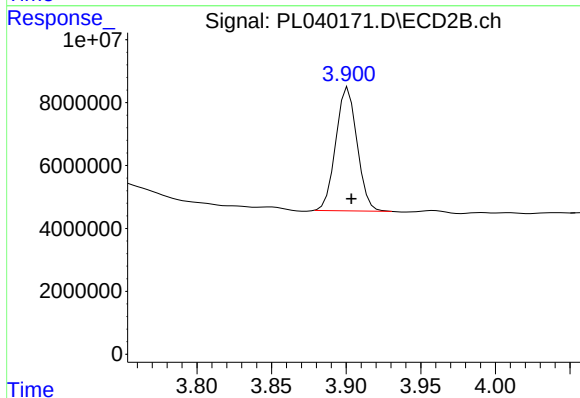


#1 Tetrachloro-m-xylene

R.T.: 3.901 min
Delta R.T.: -0.002 min
Response: 39068934
Conc: 12.24 ng/ml

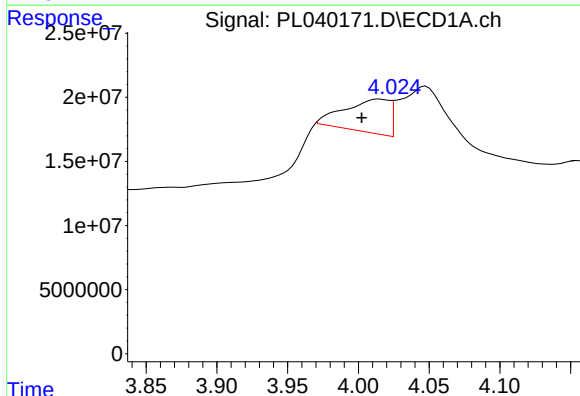


#3 gamma-BHC (Lindane)

R.T.: 4.015 min
Delta R.T.: 0.012 min
Response: 57422574
Conc: 5.02 ng/ml

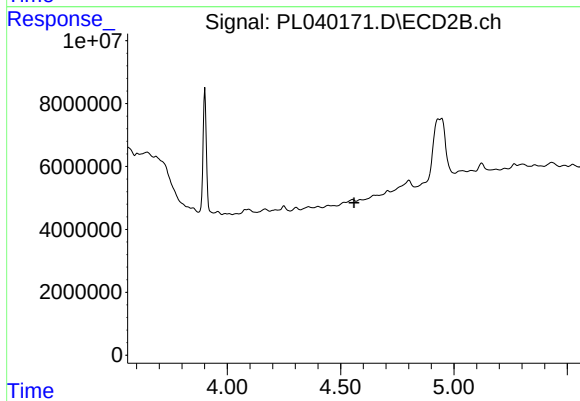

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.559 min
Response: 0
Conc: N.D.

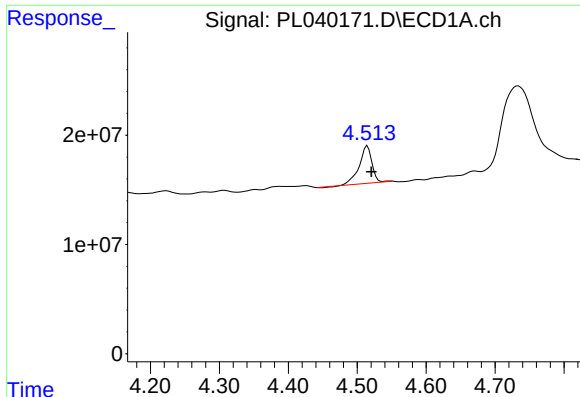

#5 Aldrin


R.T.: 4.515 min
Delta R.T.: -0.006 min
Response: 44393045
Conc: 4.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

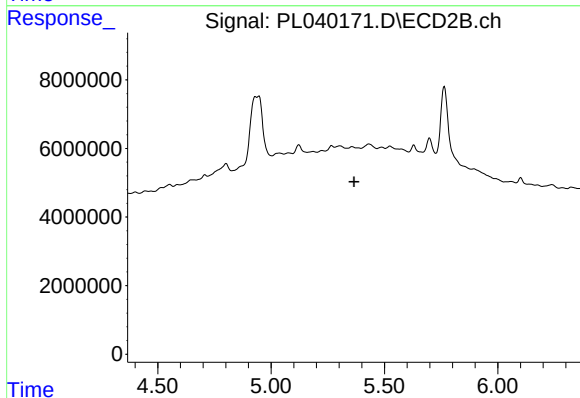


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.367 min
Response: 0
Conc: N.D.

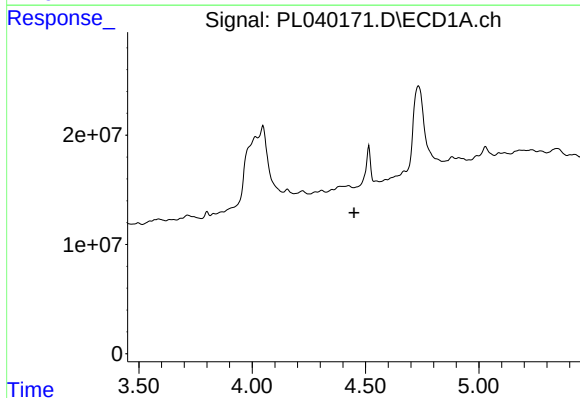


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

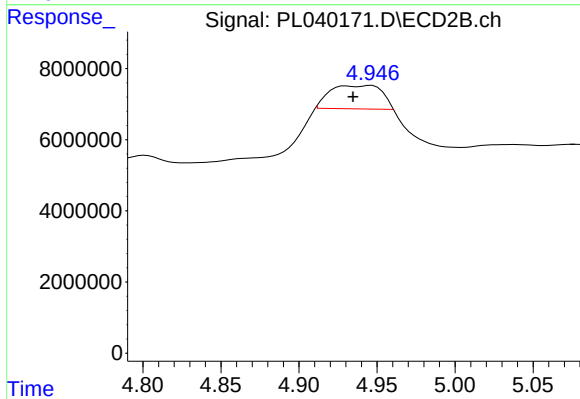

#7 delta-BHC


R.T.: 4.947 min
Delta R.T.: 0.012 min
Response: 15062846
Conc: 3.79 ng/ml

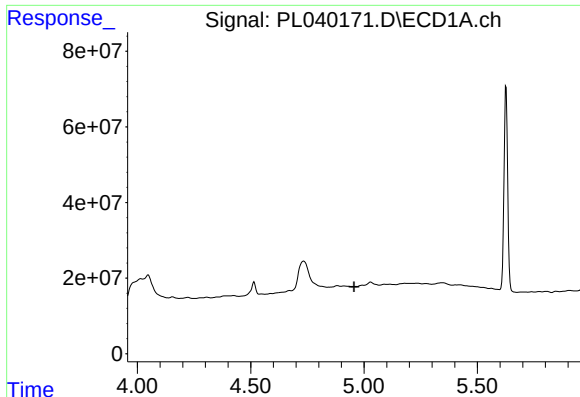

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

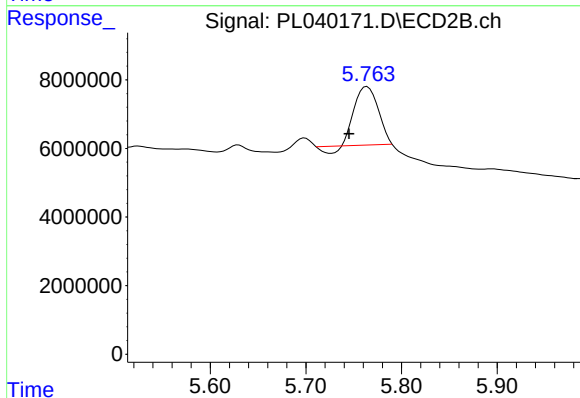


#8 Heptachlor epoxide

R.T.: 5.764 min
Delta R.T.: 0.019 min
Response: 28008853
Conc: 7.08 ng/ml

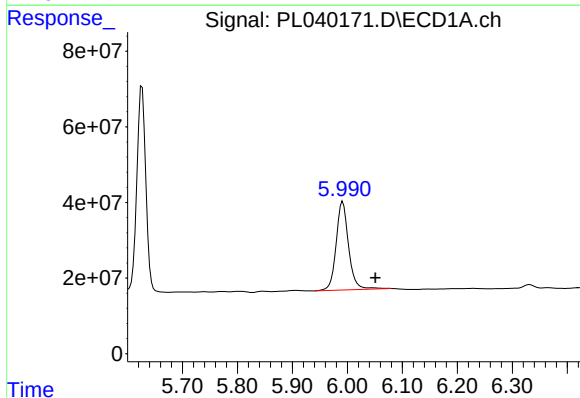


#15 Endosulfan II

R.T.: 5.992 min
Delta R.T.: -0.059 min
Response: 367865791
Conc: 38.40 ng/ml

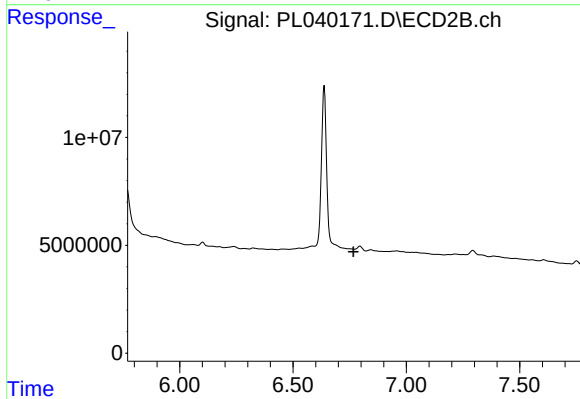

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.767 min
Response: 0
Conc: N.D.

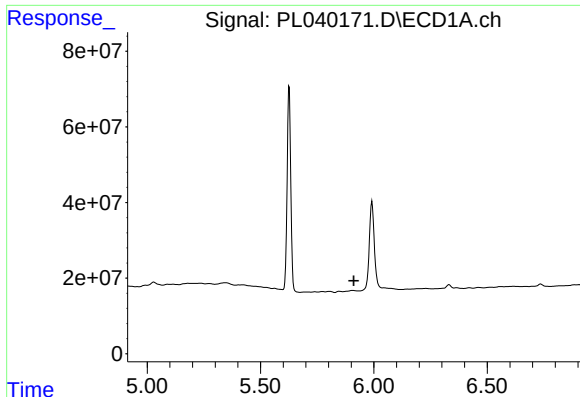

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

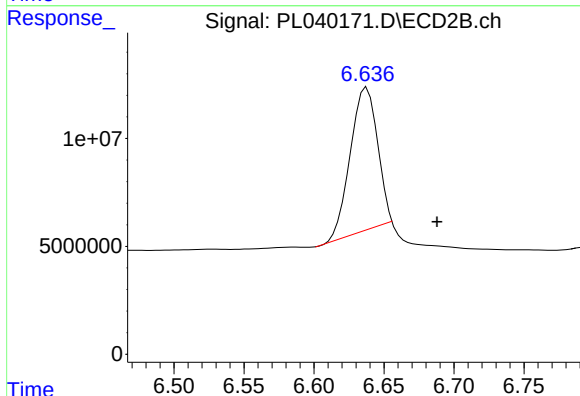


#16 4,4'-DDD

R.T.: 6.638 min
Delta R.T.: -0.050 min
Response: 90147614
Conc: 31.18 ng/ml

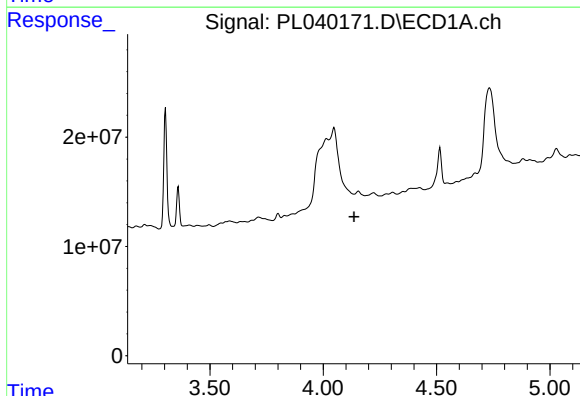


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.136 min
Response: 0
Conc: N.D.

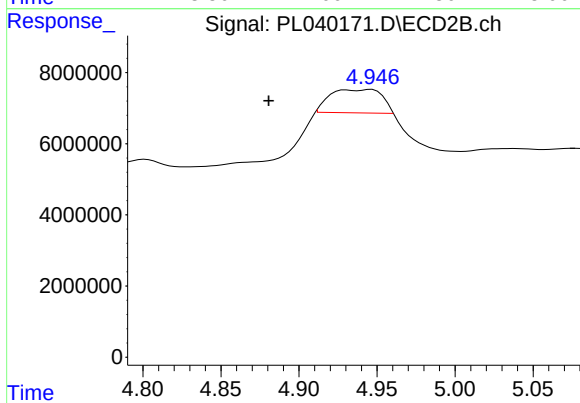

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.066 min
Response: 15062846
Conc: 97.28 ng/ml

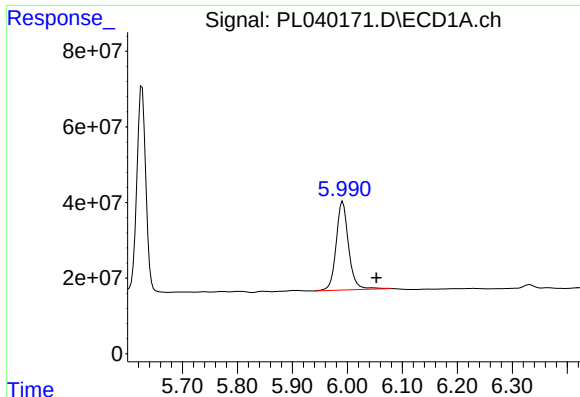

#27 Chlordane-5


R.T.: 5.992 min
Delta R.T.: -0.061 min
Response: 367865791
Conc: 992.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

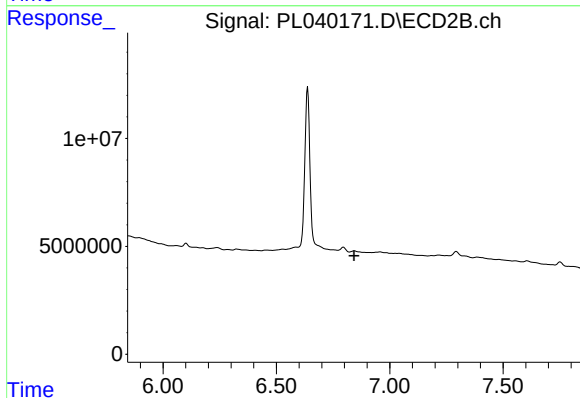


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.842 min
Response: 0
Conc: N.D.

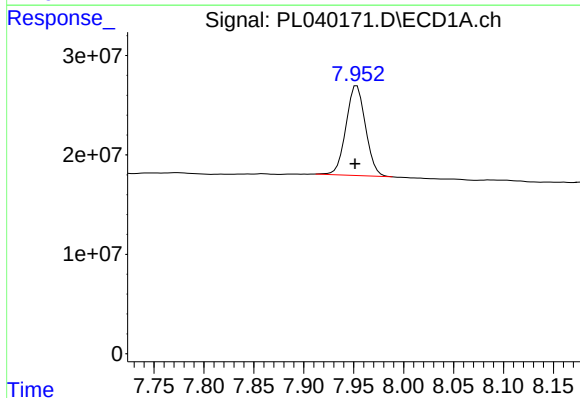

#28 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 122641536
Conc: 14.72 ng/ml

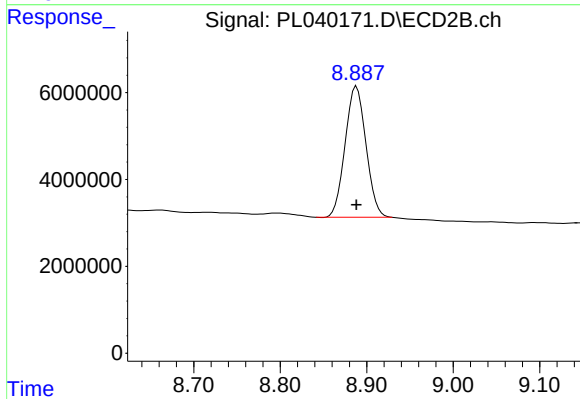

#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.000 min
Response: 50380196
Conc: 18.55 ng/ml