

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092118\
 Data File : PL040177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2018 11:39
 Operator : AJ\SJ
 Sample : J4987-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 22:44:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 14 23:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.298	3.902	111.4E6	45829639	14.368	14.363
28)	SA Decachlor...	7.949	8.887	91077339	35725871	10.930	13.154
Target Compounds							
2)	A alpha-BHC	0.000	4.308f	0	5545283	N.D.	1.072 #
3)	MA gamma-BHC...	4.042f	0.000	173.8E6	0	15.183	N.D. #
7)	B delta-BHC	0.000	4.946	0	7871784	N.D.	1.979 #
8)	B Heptachlo...	0.000	5.768	0	12396456	N.D.	3.134 #
15)	B Endosulfa...	5.990f	0.000	250.1E6	0	26.103	N.D. #
16)	A 4,4'-DDD	0.000	6.640f	0	47497337	N.D.	16.430 #
23)	Chlordane-1	0.000	4.946	0	7871784	N.D.	50.836 #
27)	Chlordane-5	5.990	0.000	250.1E6	0	674.559	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092118\
Data File : PL040177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2018 11:39
Operator : AJ\SJ
Sample : J4987-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 22:44:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091418.M
Quant Title : GC Extractables
QLast Update : Fri Sep 14 23:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

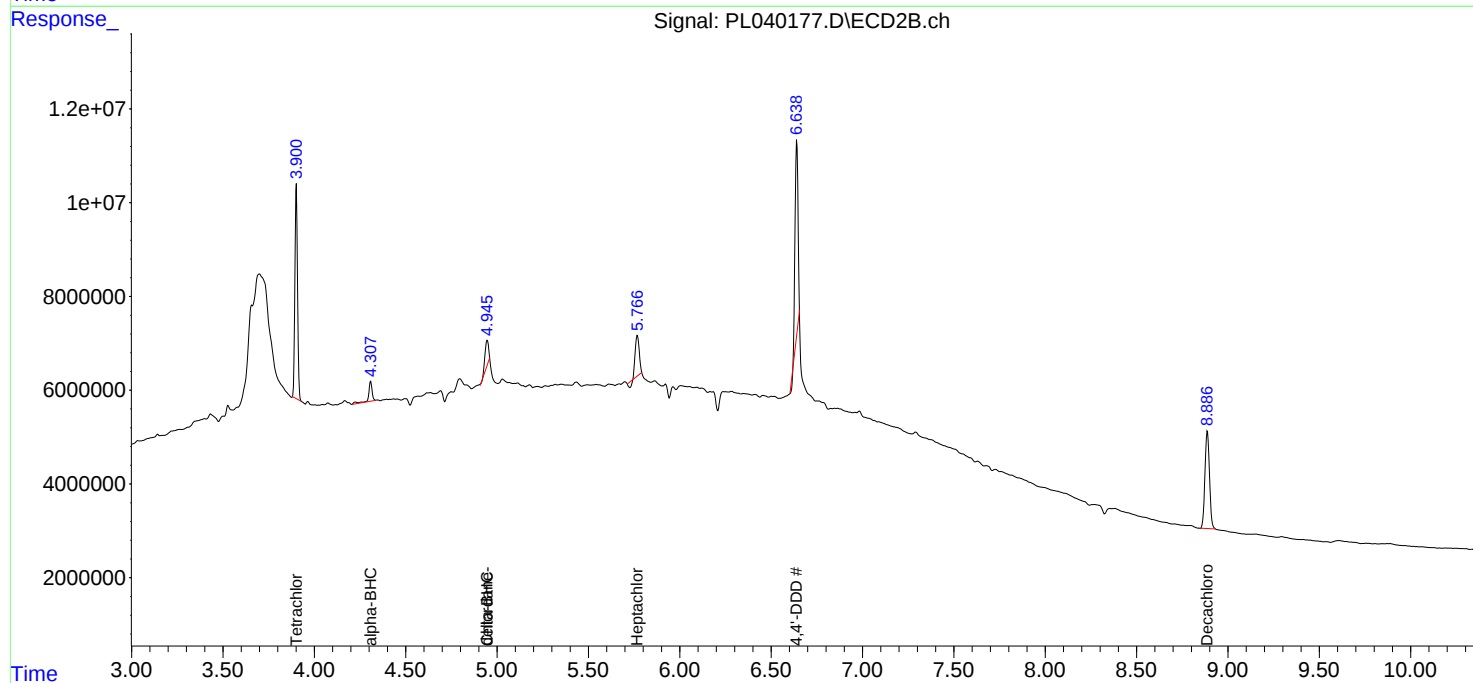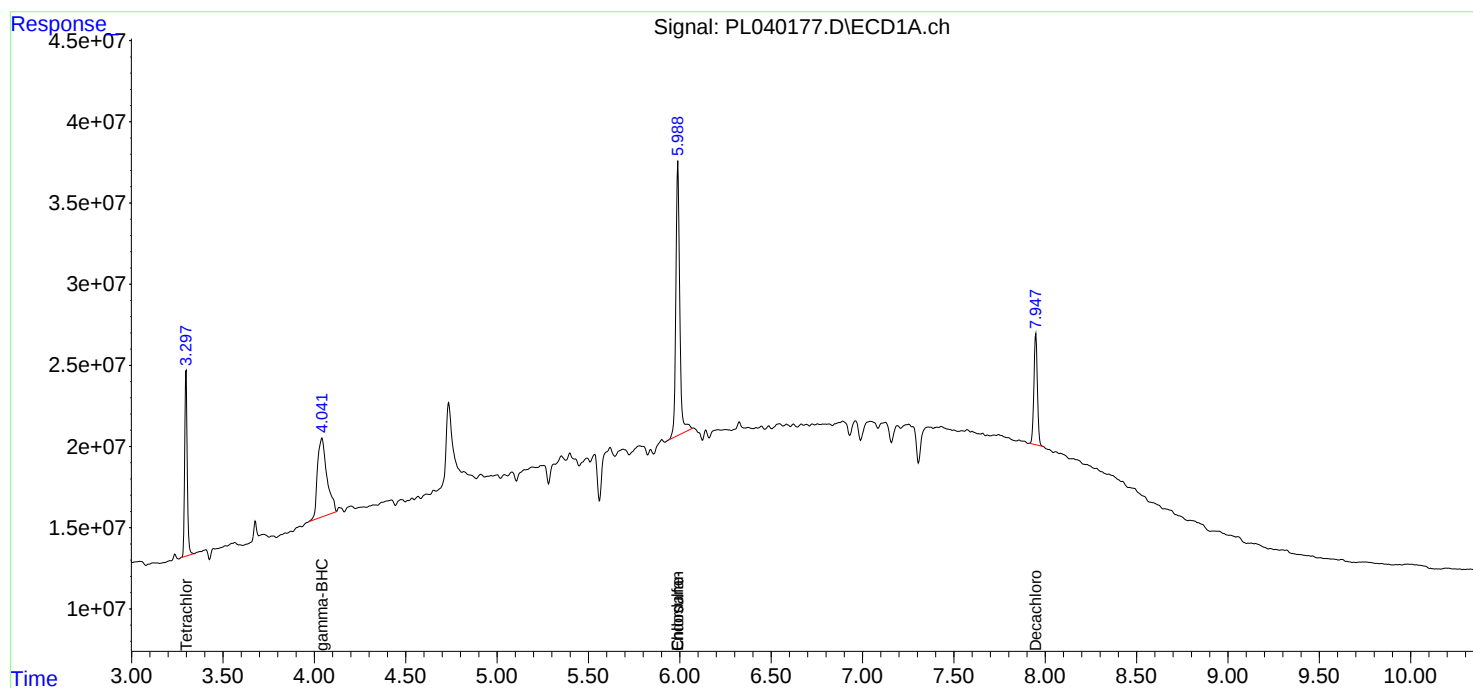


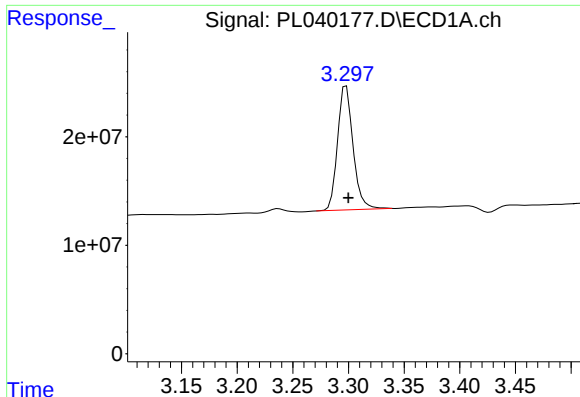

#1 Tetrachloro-m-xylene


R.T.: 3.298 min
Delta R.T.: -0.002 min
Response: 111421807
Conc: 14.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

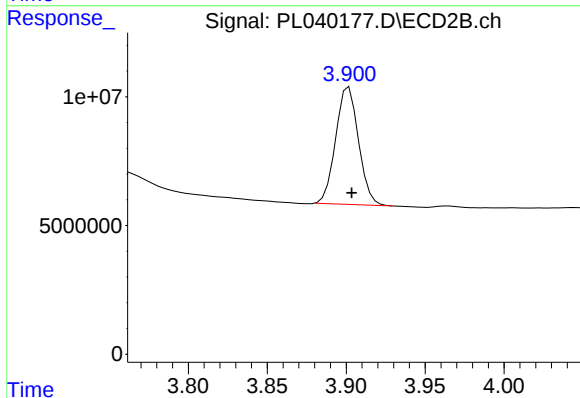


#1 Tetrachloro-m-xylene

R.T.: 3.902 min
Delta R.T.: -0.002 min
Response: 45829639
Conc: 14.36 ng/ml

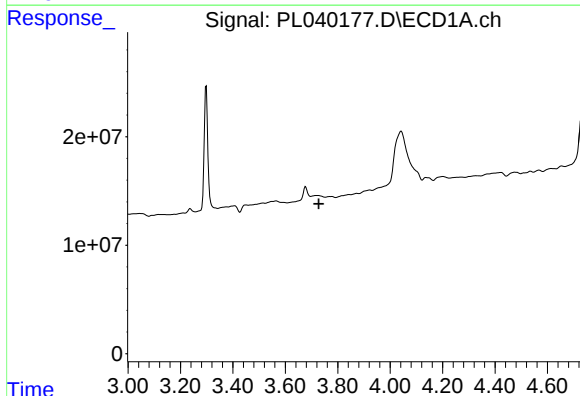


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.727 min
Response: 0
Conc: N.D.

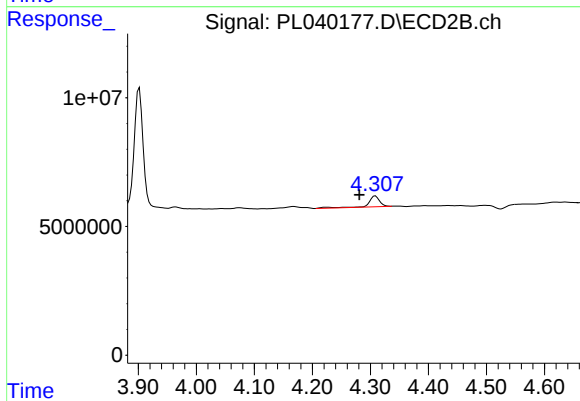

#2 alpha-BHC


R.T.: 4.308 min
Delta R.T.: 0.027 min
Response: 5545283
Conc: 1.07 ng/ml

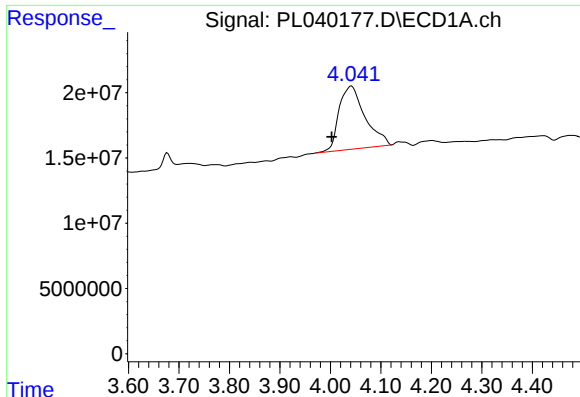

#3 gamma-BHC (Lindane)


R.T.: 4.042 min
Delta R.T.: 0.039 min
Response: 173760713
Conc: 15.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

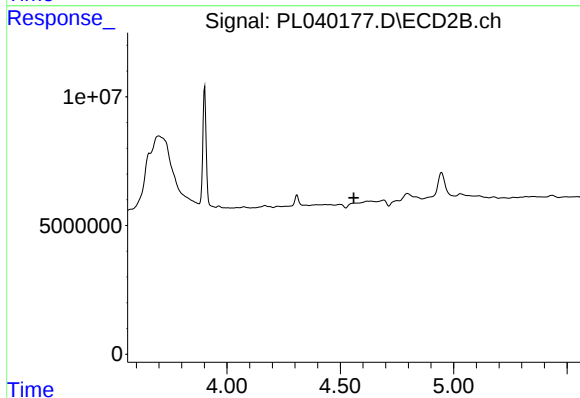


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

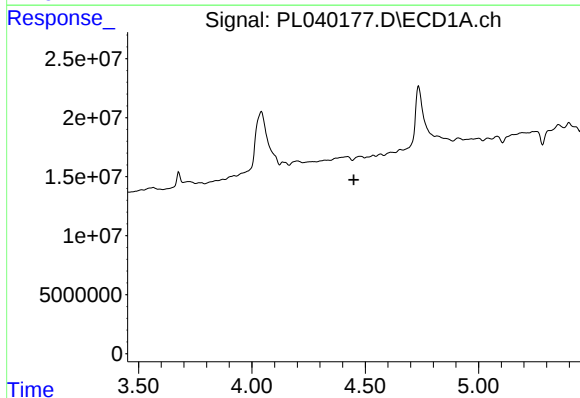


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

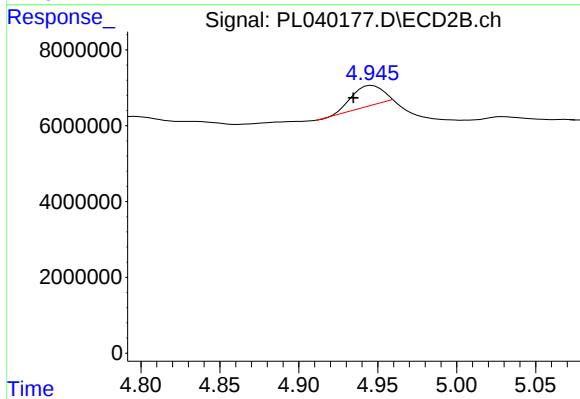

#7 delta-BHC


R.T.: 4.946 min
Delta R.T.: 0.012 min
Response: 7871784
Conc: 1.98 ng/ml

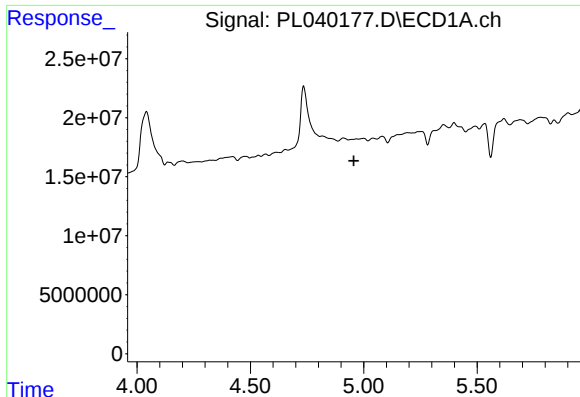

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

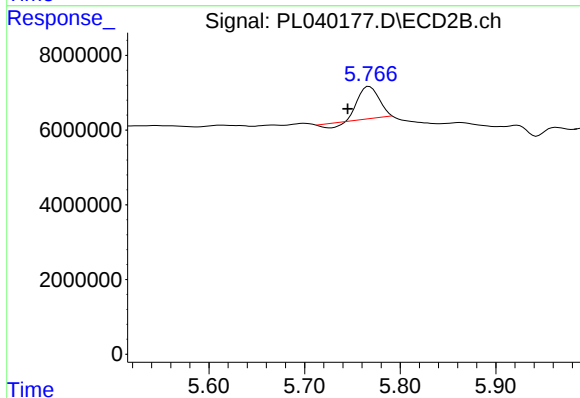


#8 Heptachlor epoxide

R.T.: 5.768 min
Delta R.T.: 0.023 min
Response: 12396456
Conc: 3.13 ng/ml

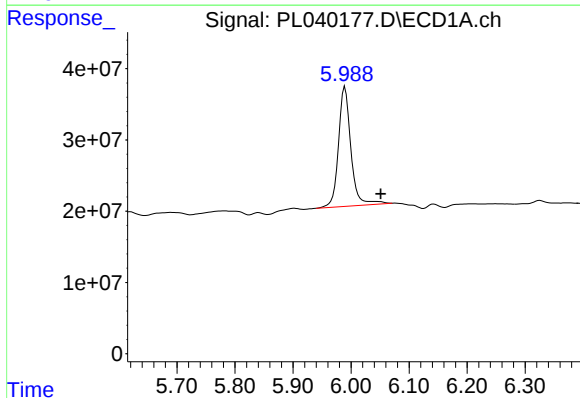


#15 Endosulfan II

R.T.: 5.990 min
Delta R.T.: -0.061 min
Response: 250094610
Conc: 26.10 ng/ml

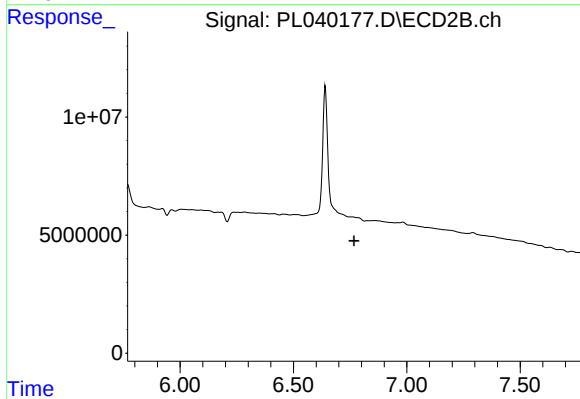

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.767 min
Response: 0
Conc: N.D.

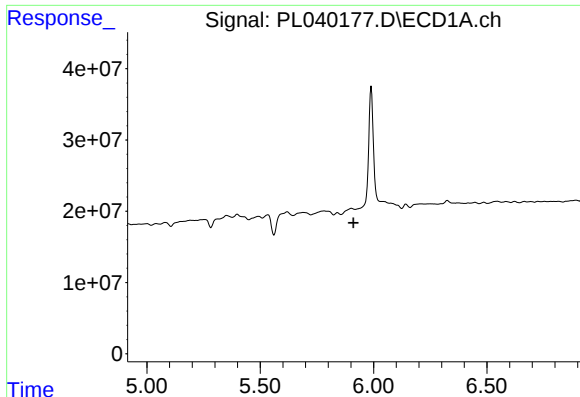

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

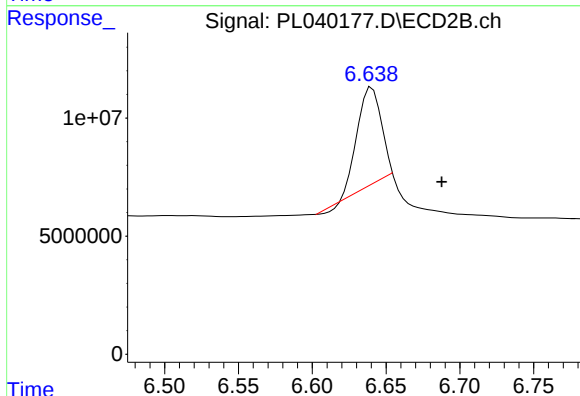


#16 4,4'-DDD

R.T.: 6.640 min
Delta R.T.: -0.047 min
Response: 47497337
Conc: 16.43 ng/ml

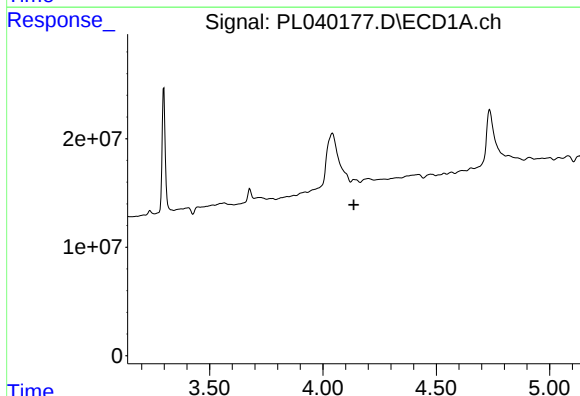


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.136 min
Response: 0
Conc: N.D.

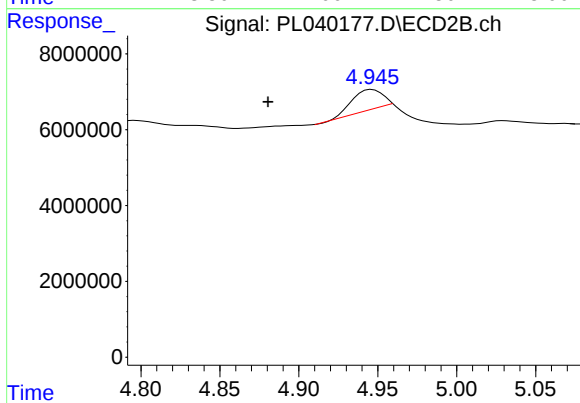

#23 Chlordane-1


R.T.: 4.946 min
Delta R.T.: 0.066 min
Response: 7871784
Conc: 50.84 ng/ml

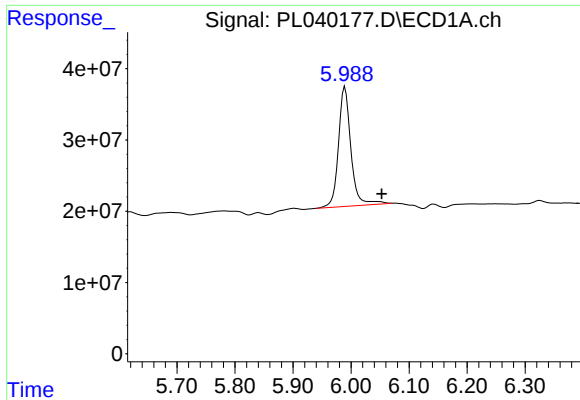

#27 Chlordane-5


R.T.: 5.990 min
Delta R.T.: -0.063 min
Response: 250094610
Conc: 674.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

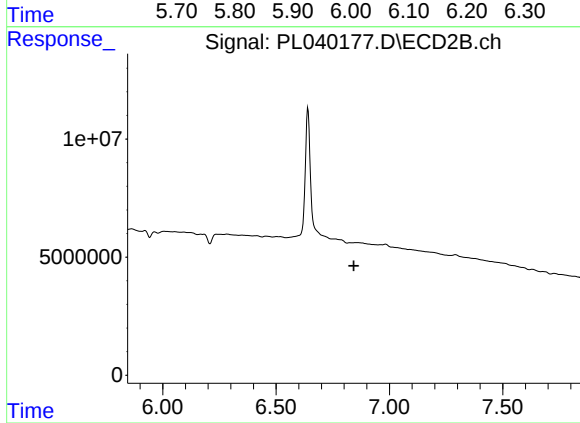


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.842 min
Response: 0
Conc: N.D.

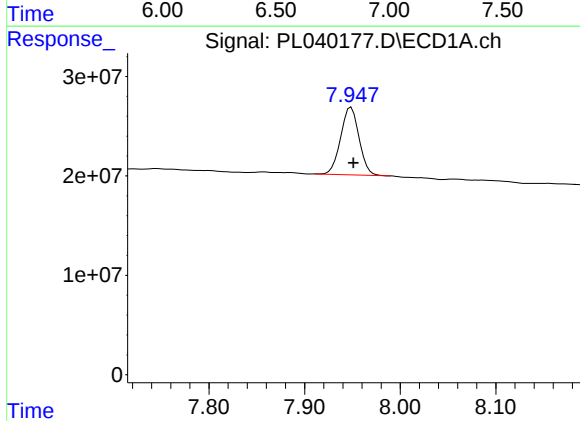

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: -0.003 min
Response: 91077339
Conc: 10.93 ng/ml

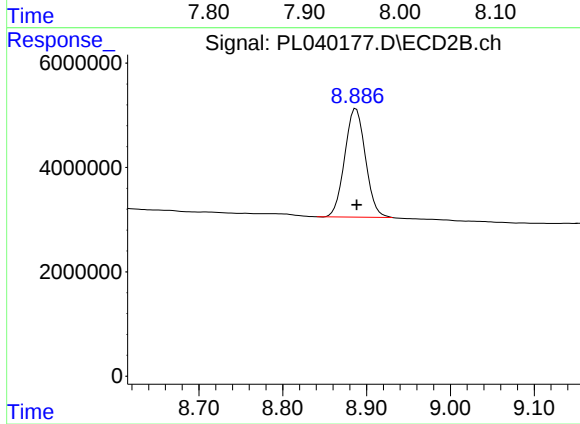

#28 Decachlorobiphenyl

R.T.: 8.887 min
Delta R.T.: 0.000 min
Response: 35725871
Conc: 13.15 ng/ml