

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092120\
 Data File : PL061623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2020 10:32
 Operator : DD\AJ
 Sample : L4074-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 15:20:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	23523781	37355779	13.639	12.144
28)	SA Decachlor...	8.207	9.090	19842631	26224994	11.894	11.091
Target Compounds							
3)	MA gamma-BHC...	0.000	4.688	0	4068552	N.D.	0.948 #
9)	A Endosulfan I	5.515	0.000	2290518	0	1.331	N.D. #
13)	MA Dieldrin	0.000	6.493	0	3940549	N.D.	1.202 #
15)	B Endosulfa...	6.276	0.000	1156779	0	0.676	N.D. #
16)	A 4,4'-DDD	0.000	6.846	0	7858757	N.D.	3.060 #
17)	MA 4,4'-DDT	6.371	7.114f	2675978	3758546	1.949	1.502
19)	B Endosulfa...	6.657	0.000	3307926	0	2.010	N.D. #
20)	A Methoxychlor	6.903f	0.000	6990428	0	8.166	N.D. #
27)	Chlordane-5	6.276	0.000	1156779	0	20.581	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092120\
Data File : PL061623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2020 10:32
Operator : DD\AJ
Sample : L4074-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 15:20:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

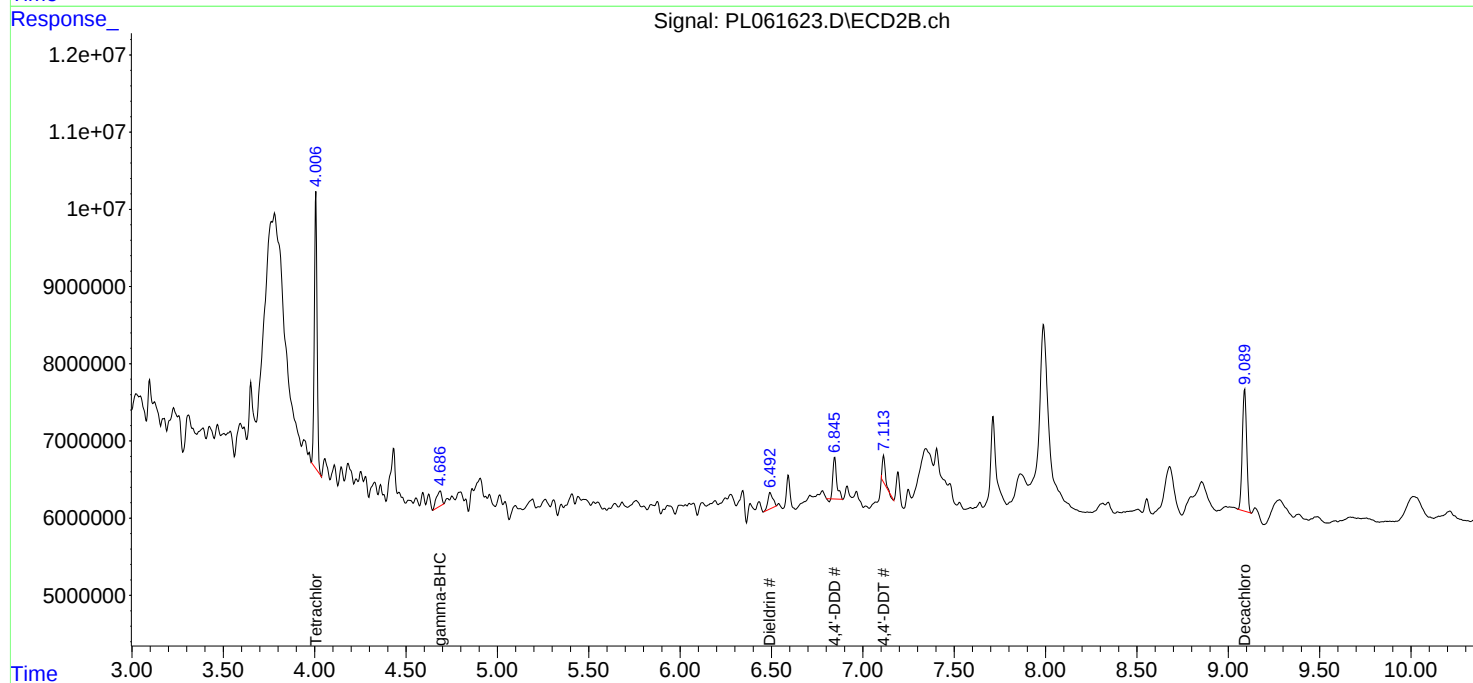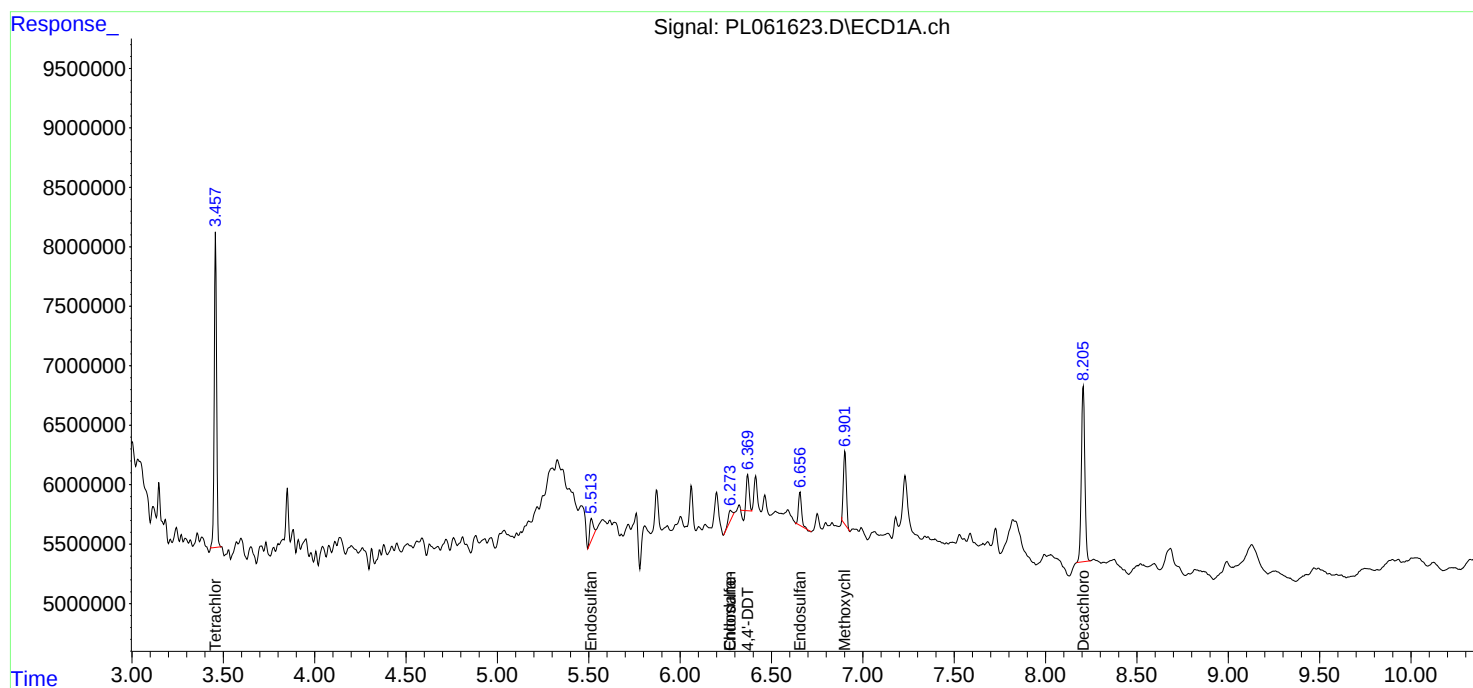


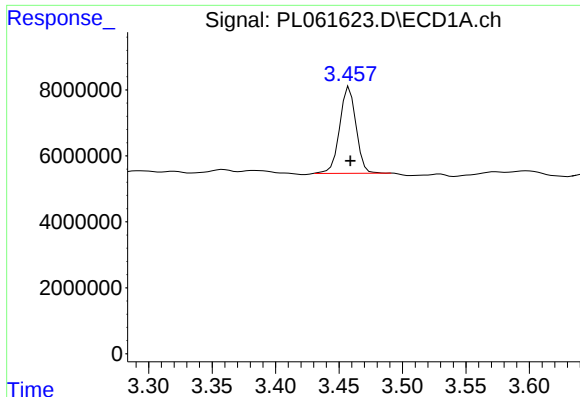

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 23523781
Conc: 13.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

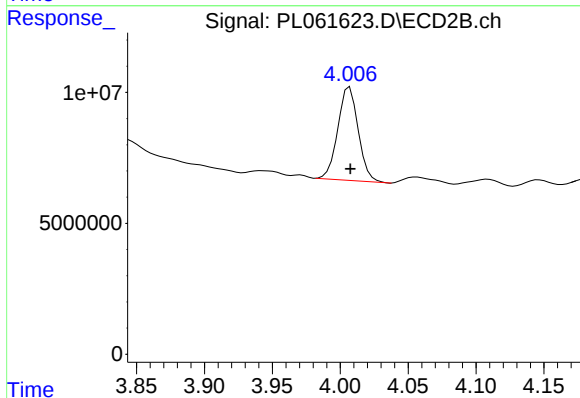


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 37355779
Conc: 12.14 ng/ml

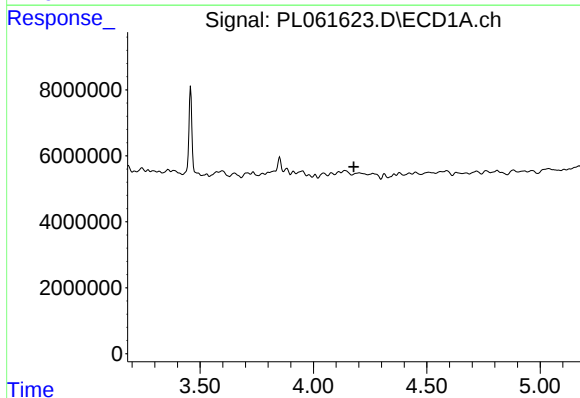


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.178 min
Response: 0
Conc: N.D.

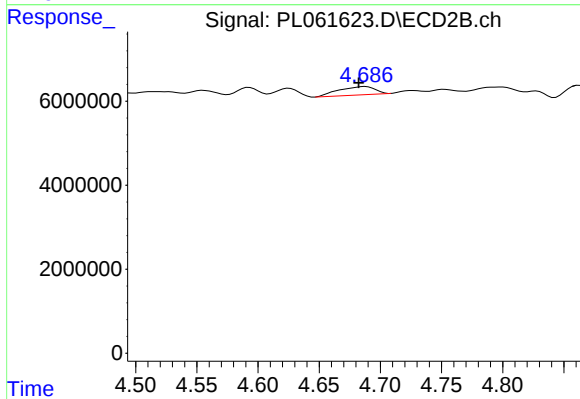

#3 gamma-BHC (Lindane)


R.T.: 4.688 min
Delta R.T.: 0.006 min
Response: 4068552
Conc: 0.95 ng/ml

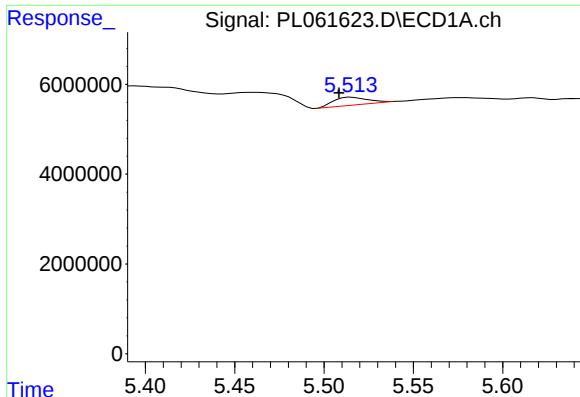

#9 Endosulfan I


R.T.: 5.515 min
Delta R.T.: 0.007 min
Response: 2290518
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

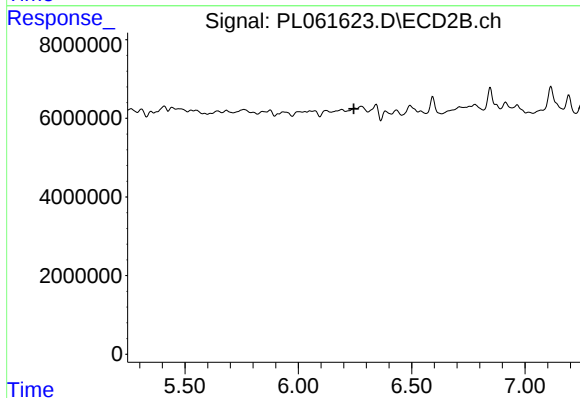


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

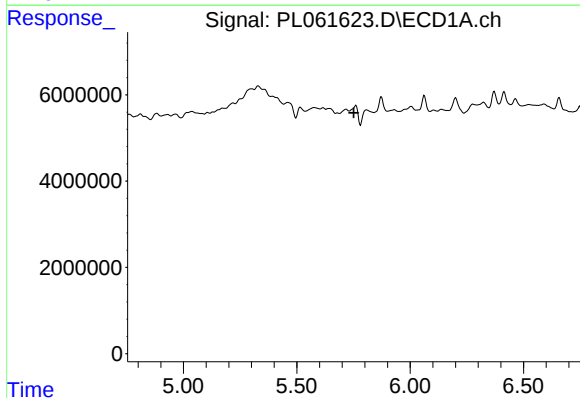


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.752 min
Response: 0
Conc: N.D.

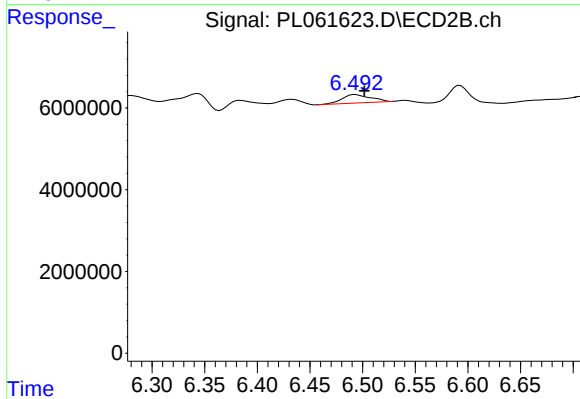

#13 Dieldrin


R.T.: 6.493 min
Delta R.T.: -0.009 min
Response: 3940549
Conc: 1.20 ng/ml

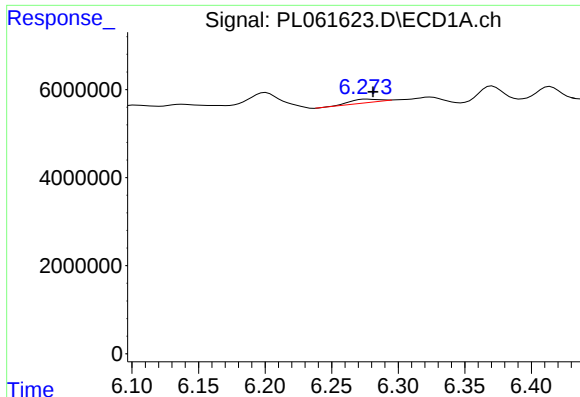

#15 Endosulfan II


R.T.: 6.276 min
Delta R.T.: -0.005 min
Response: 1156779
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

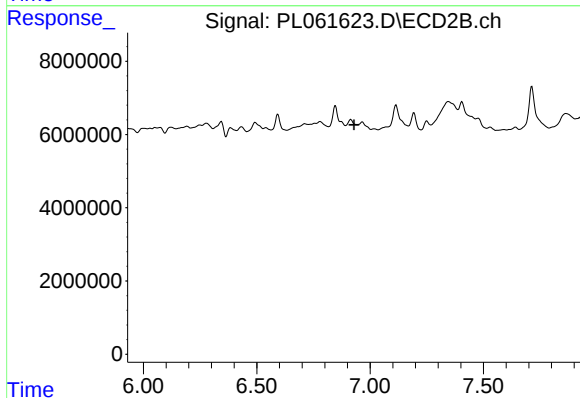


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.930 min
Response: 0
Conc: N.D.

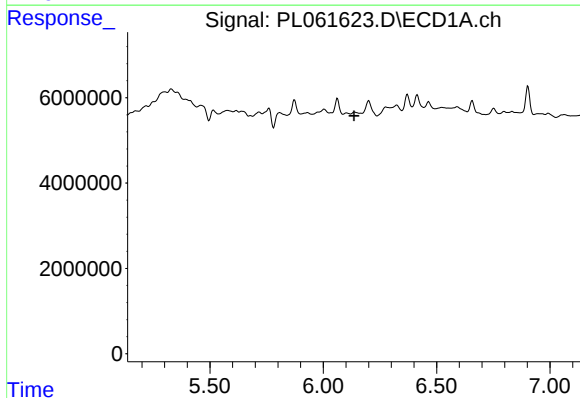


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

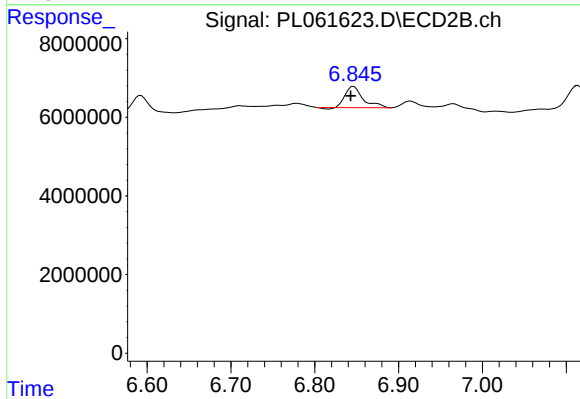

#16 4,4'-DDD


R.T.: 6.846 min
Delta R.T.: 0.004 min
Response: 7858757
Conc: 3.06 ng/ml

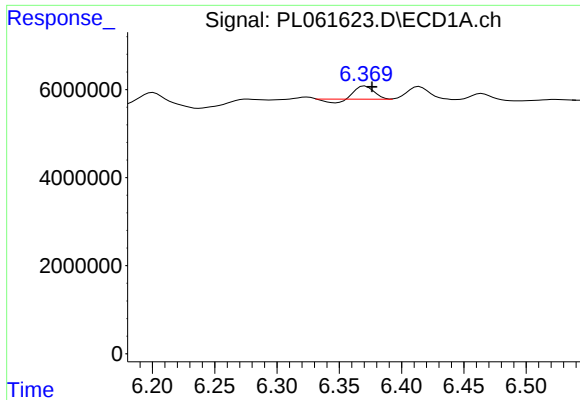

#17 4,4'-DDT


R.T.: 6.371 min
Delta R.T.: -0.006 min
Response: 2675978
Conc: 1.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

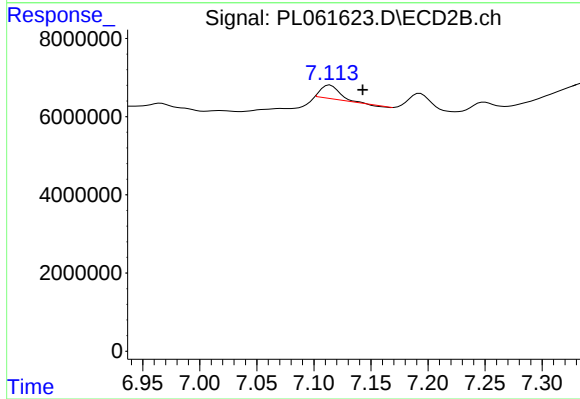


#17 4,4'-DDT

R.T.: 7.114 min
Delta R.T.: -0.029 min
Response: 3758546
Conc: 1.50 ng/ml

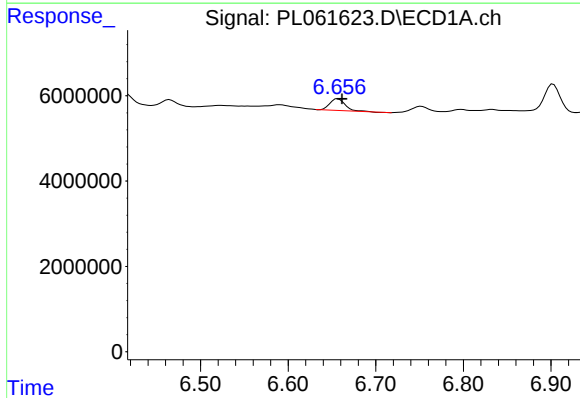


#19 Endosulfan Sulfate

R.T.: 6.657 min
Delta R.T.: -0.005 min
Response: 3307926
Conc: 2.01 ng/ml

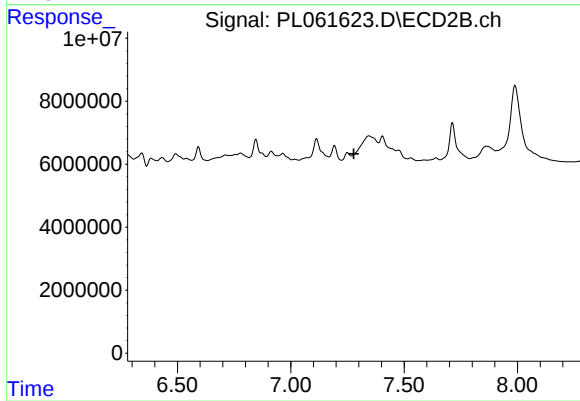

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

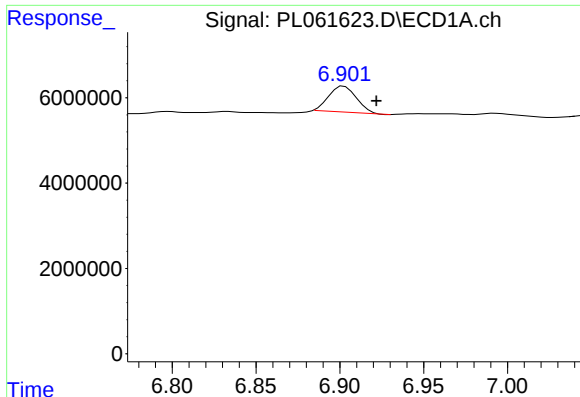

#20 Methoxychlor


R.T.: 6.903 min
Delta R.T.: -0.019 min
Response: 6990428
Conc: 8.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

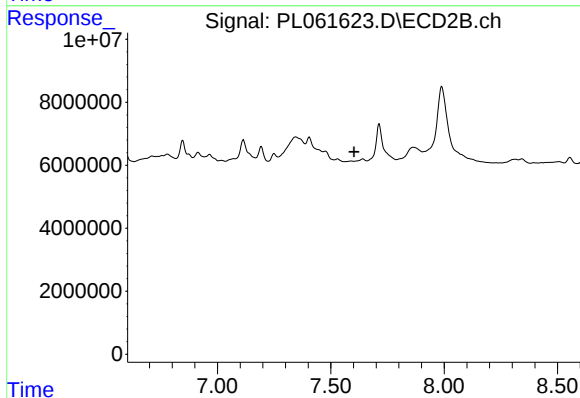


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.603 min
Response: 0
Conc: N.D.

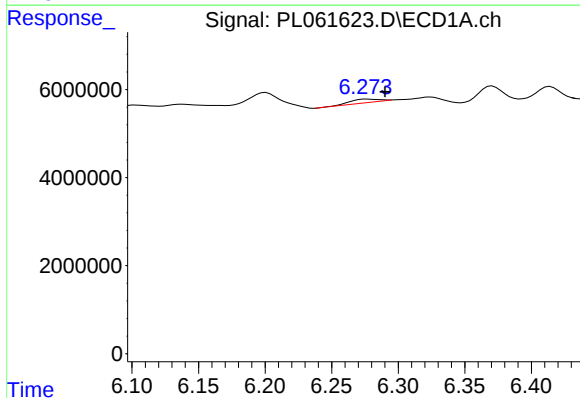


#27 Chlordane-5

R.T.: 6.276 min
Delta R.T.: -0.014 min
Response: 1156779
Conc: 20.58 ng/ml

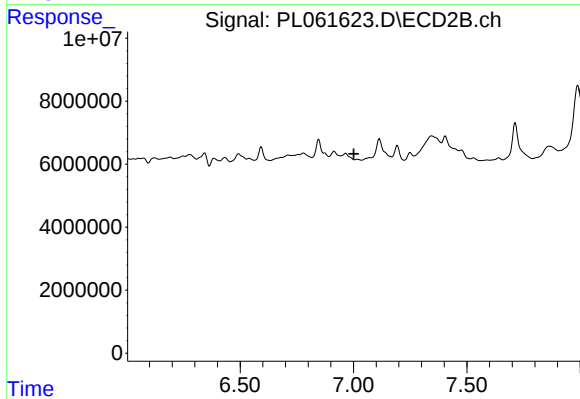

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.002 min
Response: 0
Conc: N.D.

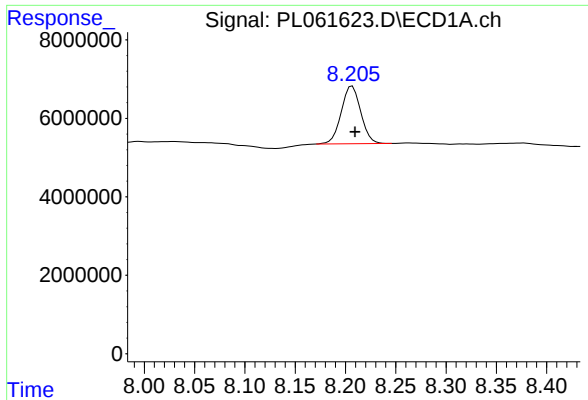

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.003 min
Response: 19842631
Conc: 11.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

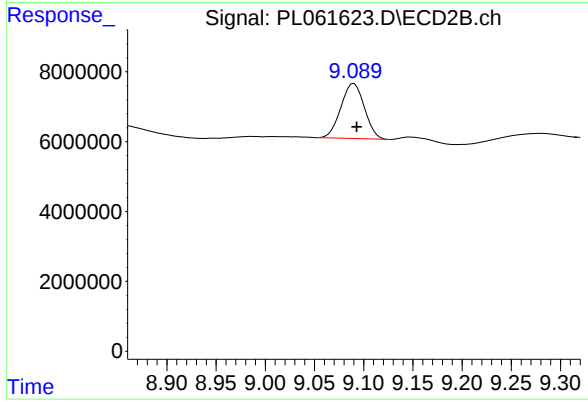

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: -0.003 min
Response: 26224994
Conc: 11.09 ng/ml