

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092120\
 Data File : PL061628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2020 12:45
 Operator : DD\AJ
 Sample : L3869-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-091820

Manual Integrations
 APPROVED

Ankita
 9/22/2020 12:32:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 15:21:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.457	4.007	29086690	42286059	16.865m	13.747
28) SA Decachlor...	8.206	9.087	20805247	33282041	12.471	14.075m
Target Compounds						
17) MA 4,4'-DDT	6.371	7.139	3076069	2429654	2.240m	0.971m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092120\
Data File : PL061628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2020 12:45
Operator : DD\AJ
Sample : L3869-06
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-091820


Manual Integrations
APPROVED

Ankita
9/22/2020 12:32:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 15:21:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

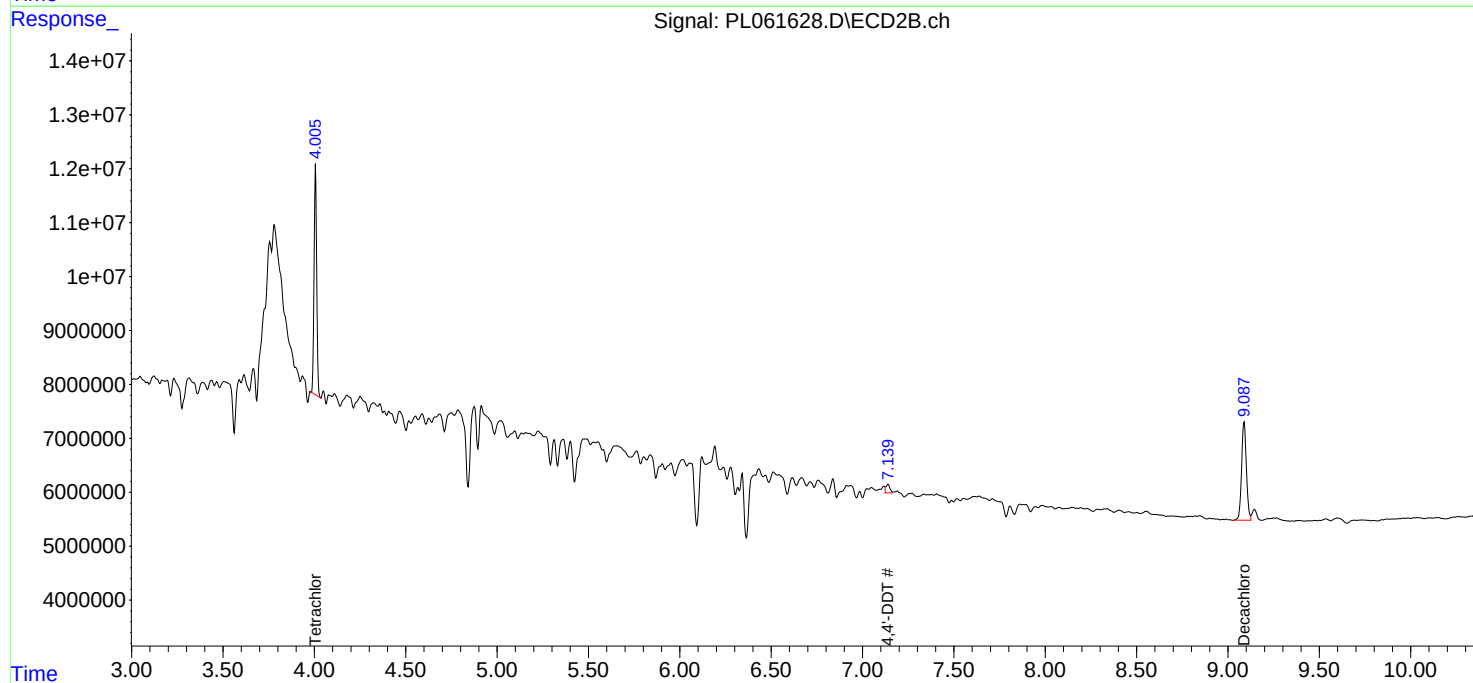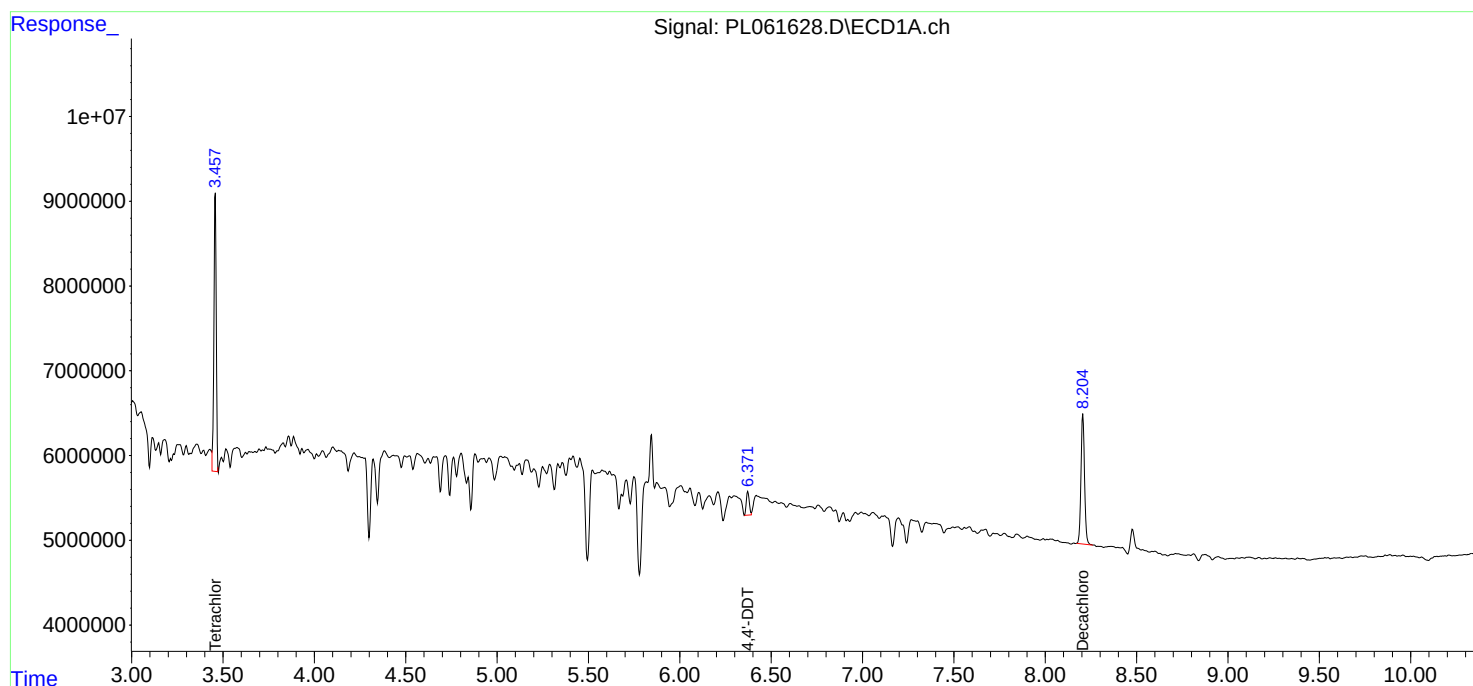

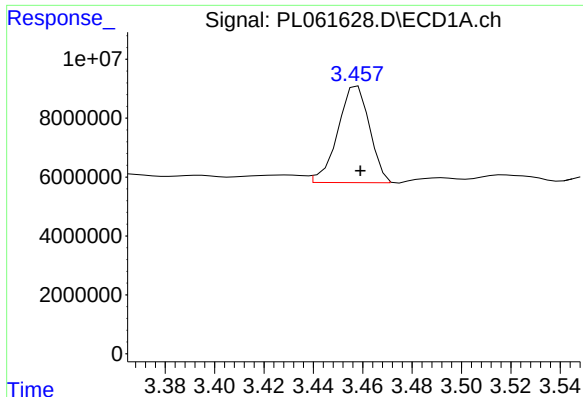


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: -0.002 min
Response: 29086690
Conc: 16.86 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-02-091820


Manual Integrations
APPROVED

Ankita
9/22/2020 12:32:55 PM

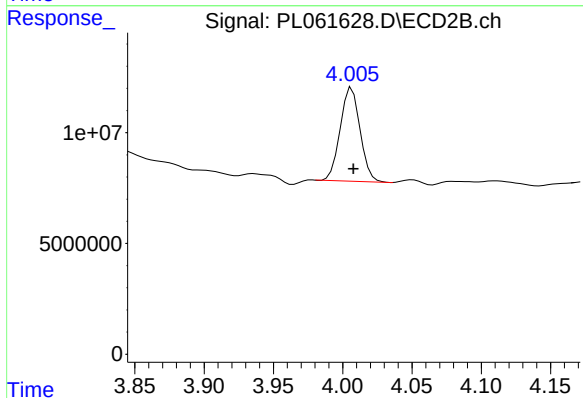


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.001 min
Response: 42286059
Conc: 13.75 ng/ml

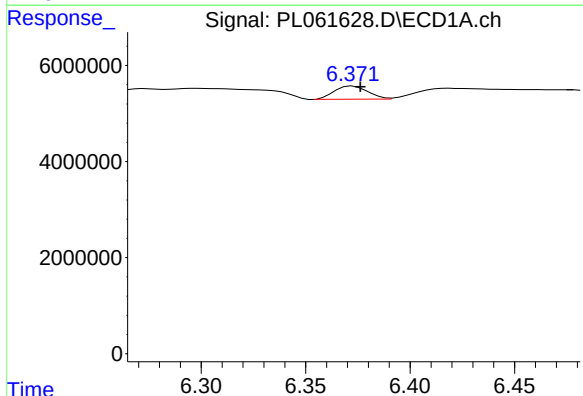


#17 4,4'-DDT

R.T.: 6.371 min
Delta R.T.: -0.005 min
Response: 3076069
Conc: 2.24 ng/ml m

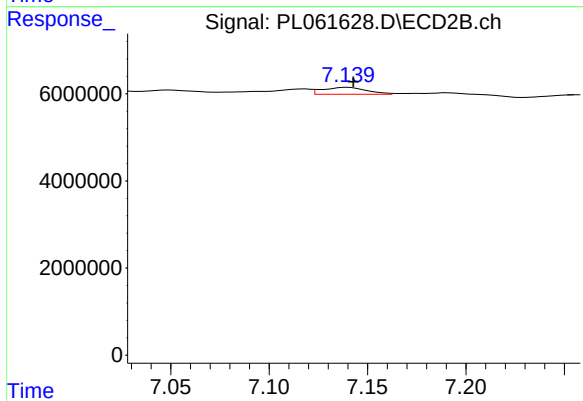

#17 4,4'-DDT

R.T.: 7.139 min
Delta R.T.: -0.004 min
Response: 2429654
Conc: 0.97 ng/ml m

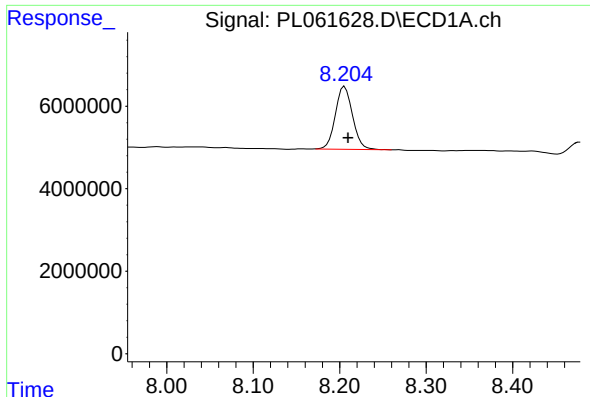


#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.004 min
Response: 20805247
Conc: 12.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-091820

Manual Integrations
APPROVED

Ankita
9/22/2020 12:32:55 PM

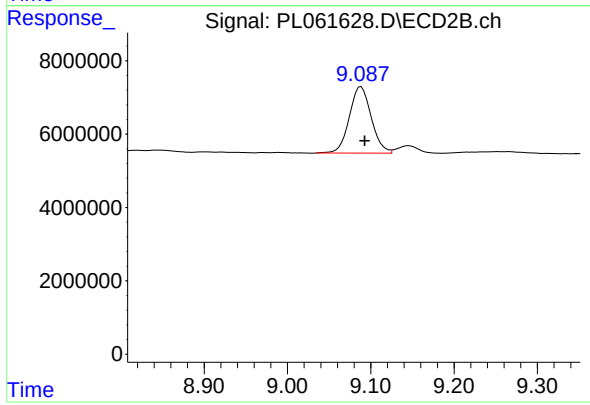

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: -0.006 min
Response: 33282041
Conc: 14.08 ng/ml m