

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
 Data File : PL069944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2021 17:26
 Operator : AR\AJ
 Sample : M3772-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 04:16:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.628	5.563	7520016	23163710	18.458	19.030
28)	SA Decachlor...	10.391	11.480	11579087	21224586	15.723	18.575
Target Compounds							
7)	B delta-BHC	0.000	7.080f	0	1961887	N.D.	1.178 #
10)	B gamma-Chl...	0.000	8.290	0	493833	N.D.	0.370 #
15)	B Endosulfa...	0.000	9.213	0	376980	N.D.	0.334 #
23)	Chlordane-1	0.000	6.970f	0	28861	N.D.	0.703 #
25)	Chlordane-3	0.000	8.290	0	493833	N.D.	2.603 #
27)	Chlordane-5	0.000	9.279	0	31963	N.D.	0.760 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
Data File : PL069944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2021 17:26
Operator : AR\AJ
Sample : M3772-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 04:16:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

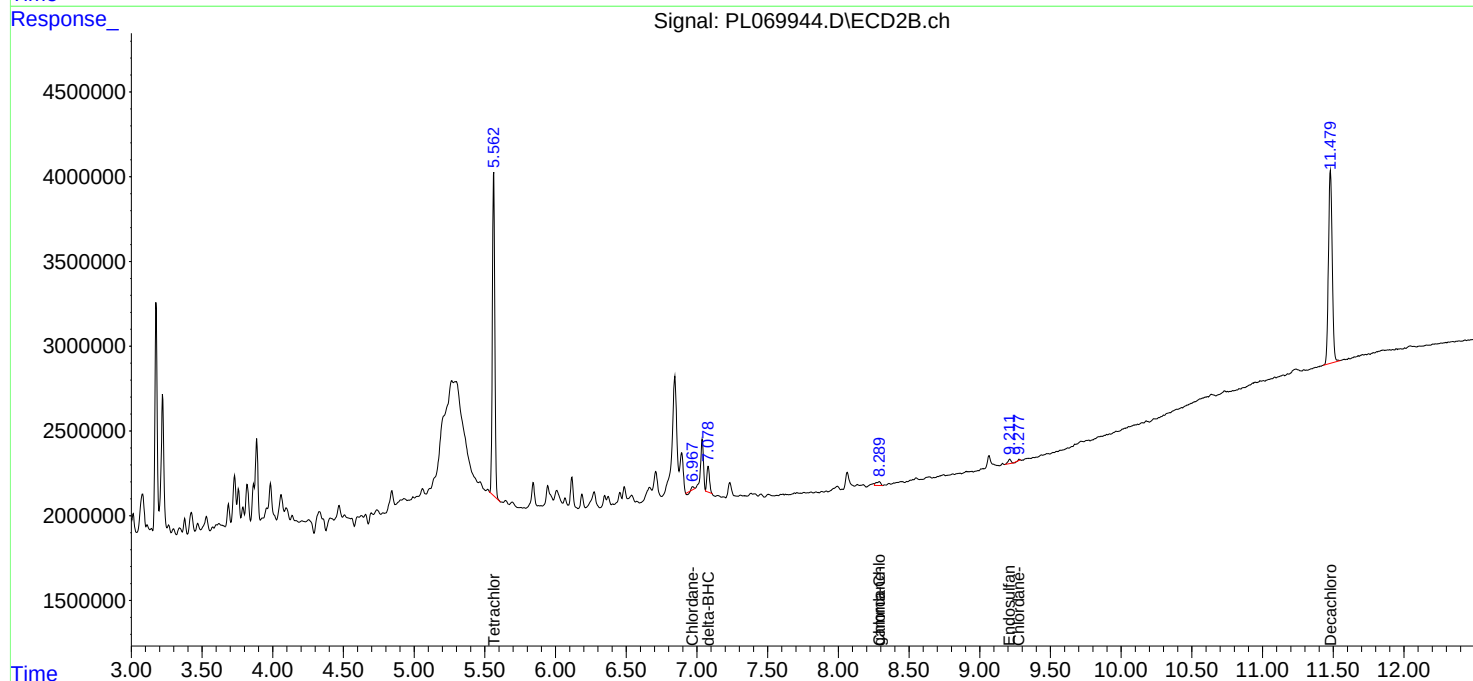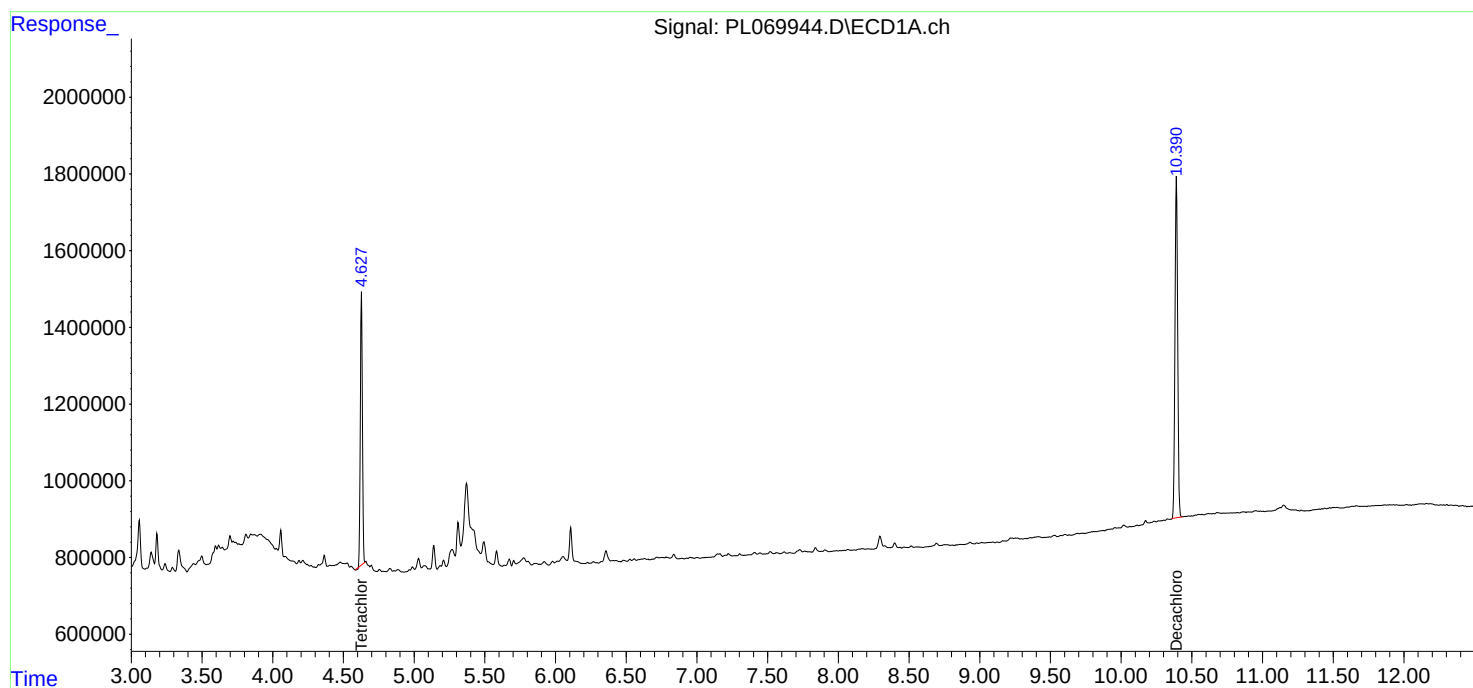


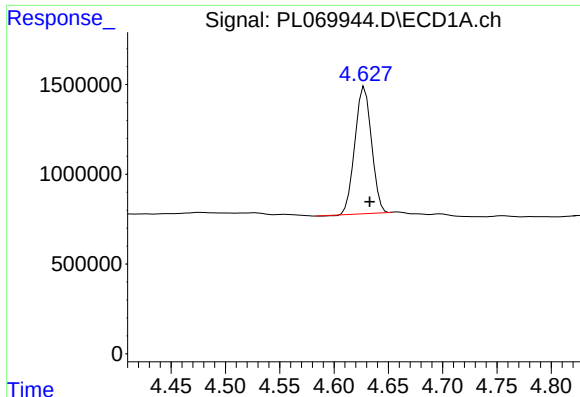

#1 Tetrachloro-m-xylene


R.T.: 4.628 min
Delta R.T.: -0.005 min
Response: 7520016
Conc: 18.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

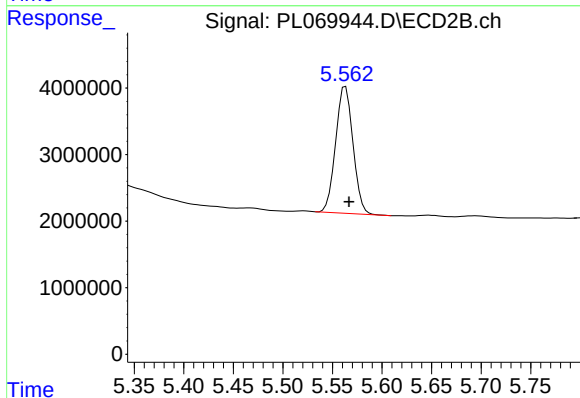


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.003 min
Response: 23163710
Conc: 19.03 ng/ml

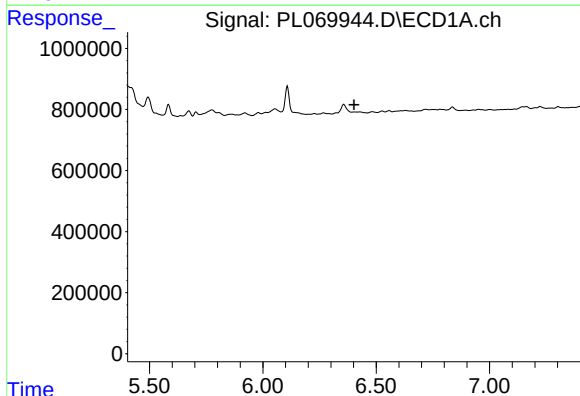


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

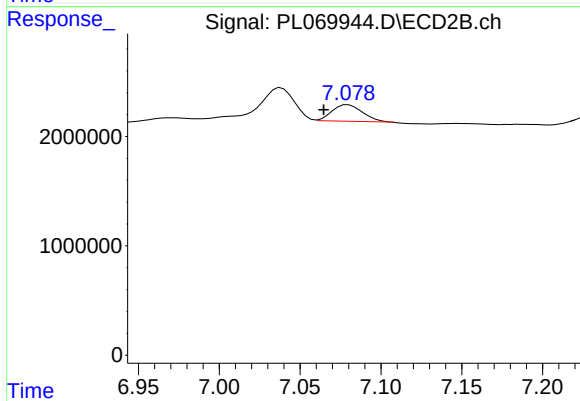

#7 delta-BHC


R.T.: 7.080 min
Delta R.T.: 0.015 min
Response: 1961887
Conc: 1.18 ng/ml

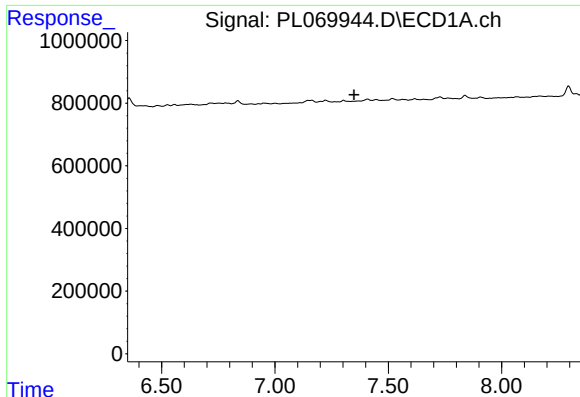

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

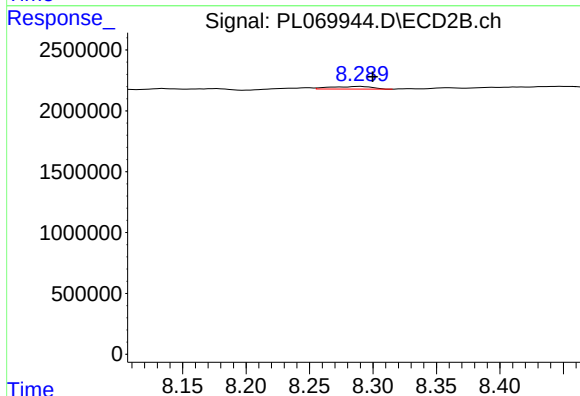


#10 gamma-Chlordane

R.T.: 8.290 min
Delta R.T.: -0.009 min
Response: 493833
Conc: 0.37 ng/ml

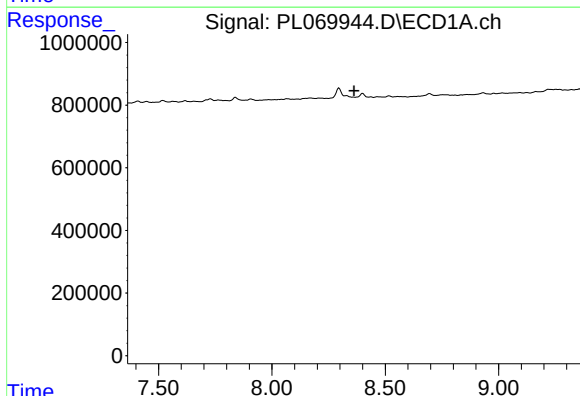


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

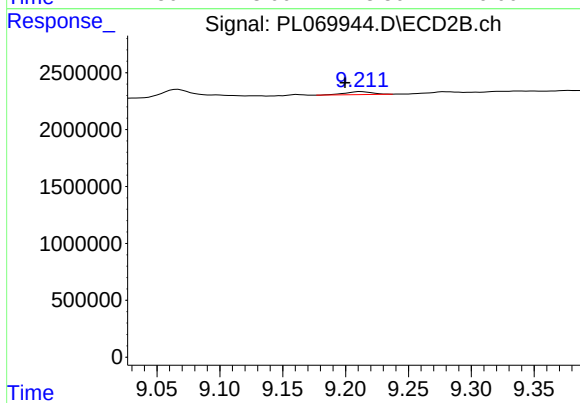

#15 Endosulfan II


R.T.: 9.213 min
Delta R.T.: 0.013 min
Response: 376980
Conc: 0.33 ng/ml

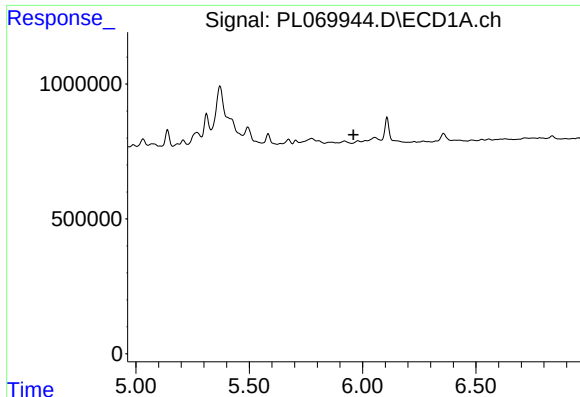

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

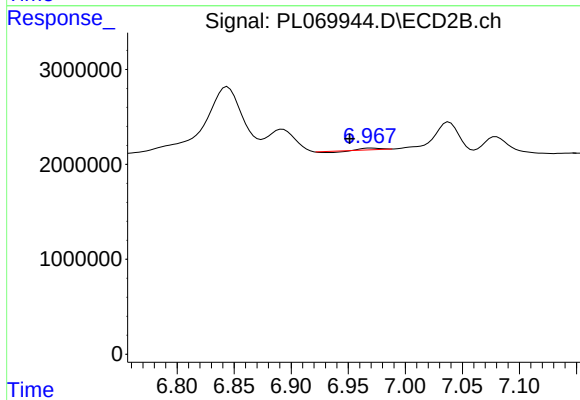


#23 Chlordane-1

R.T.: 6.970 min
Delta R.T.: 0.019 min
Response: 28861
Conc: 0.70 ng/ml

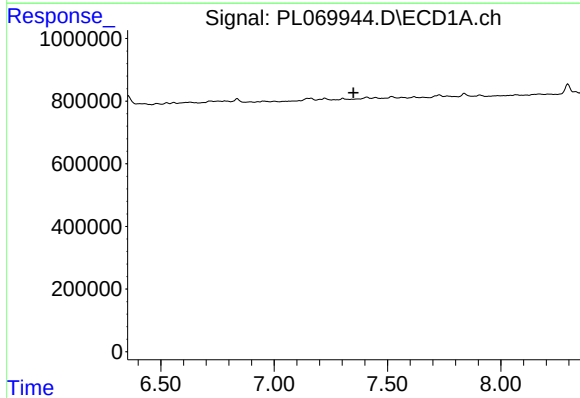


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.

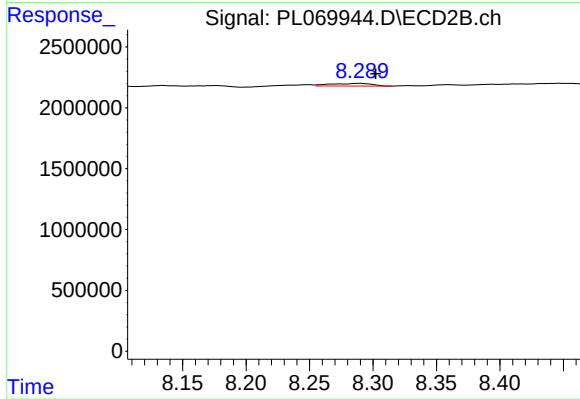

#25 Chlordane-3


R.T.: 8.290 min
Delta R.T.: -0.012 min
Response: 493833
Conc: 2.60 ng/ml

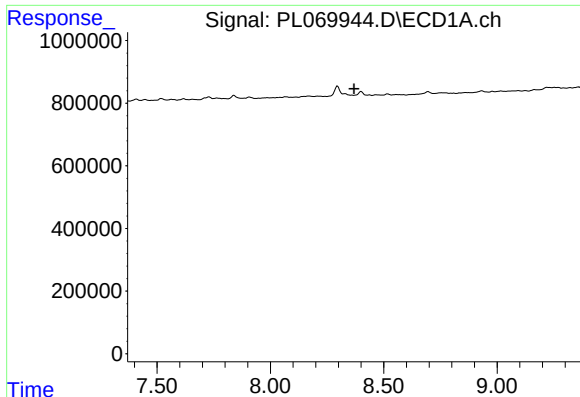

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

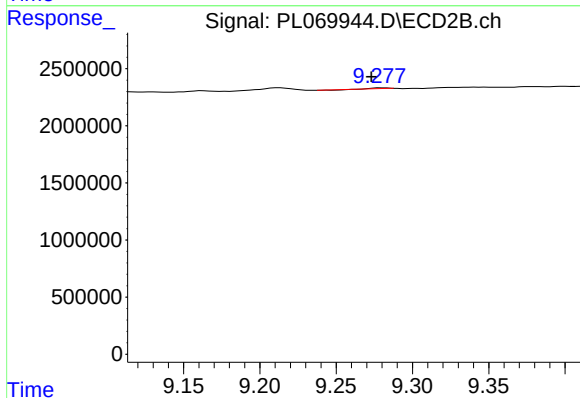


#27 Chlordane-5

R.T.: 9.279 min
Delta R.T.: 0.006 min
Response: 31963
Conc: 0.76 ng/ml

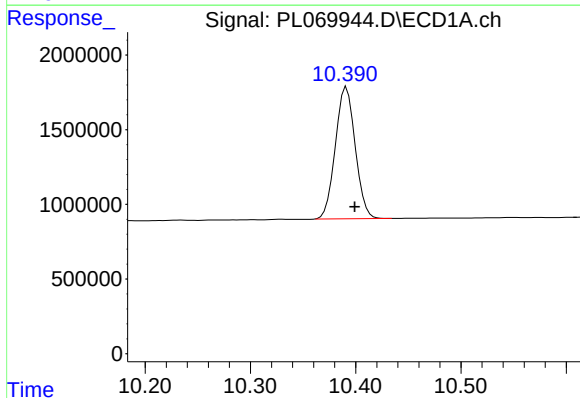

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.008 min
Response: 11579087
Conc: 15.72 ng/ml

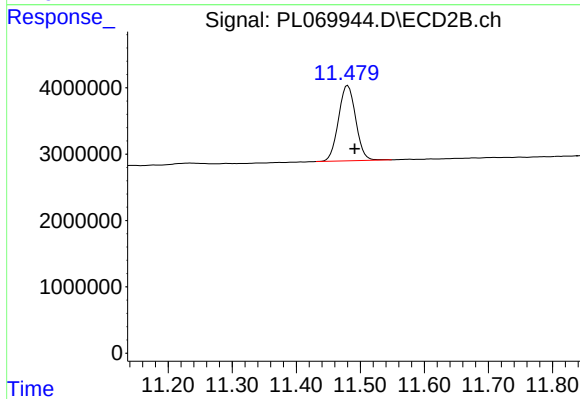

#28 Decachlorobiphenyl

R.T.: 11.480 min
Delta R.T.: -0.011 min
Response: 21224586
Conc: 18.58 ng/ml