

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
 Data File : PL069947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2021 18:16
 Operator : AR\AJ
 Sample : M3823-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 04:17:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.628	5.563	8167245	24111943	20.046	19.809
28)	SA Decachlor...	10.391	11.480	12149293	22238564	16.498	19.462
Target Compounds							
7)	B delta-BHC	0.000	7.079	0	5044685	N.D.	3.029 #
9)	A Endosulfan I	0.000	8.435	0	255840	N.D.	0.198 #
11)	B alpha-Chl...	0.000	8.388	0	490642	N.D.	0.360 #
20)	A Methoxychlor	0.000	9.896	0	585024	N.D.	0.969 #
23)	Chlordane-1	0.000	6.972f	0	31767	N.D.	0.774 #
26)	Chlordane-4	0.000	8.388	0	490642	N.D.	2.107 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091212\
Data File : PL069947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2021 18:16
Operator : AR\AJ
Sample : M3823-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 04:17:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

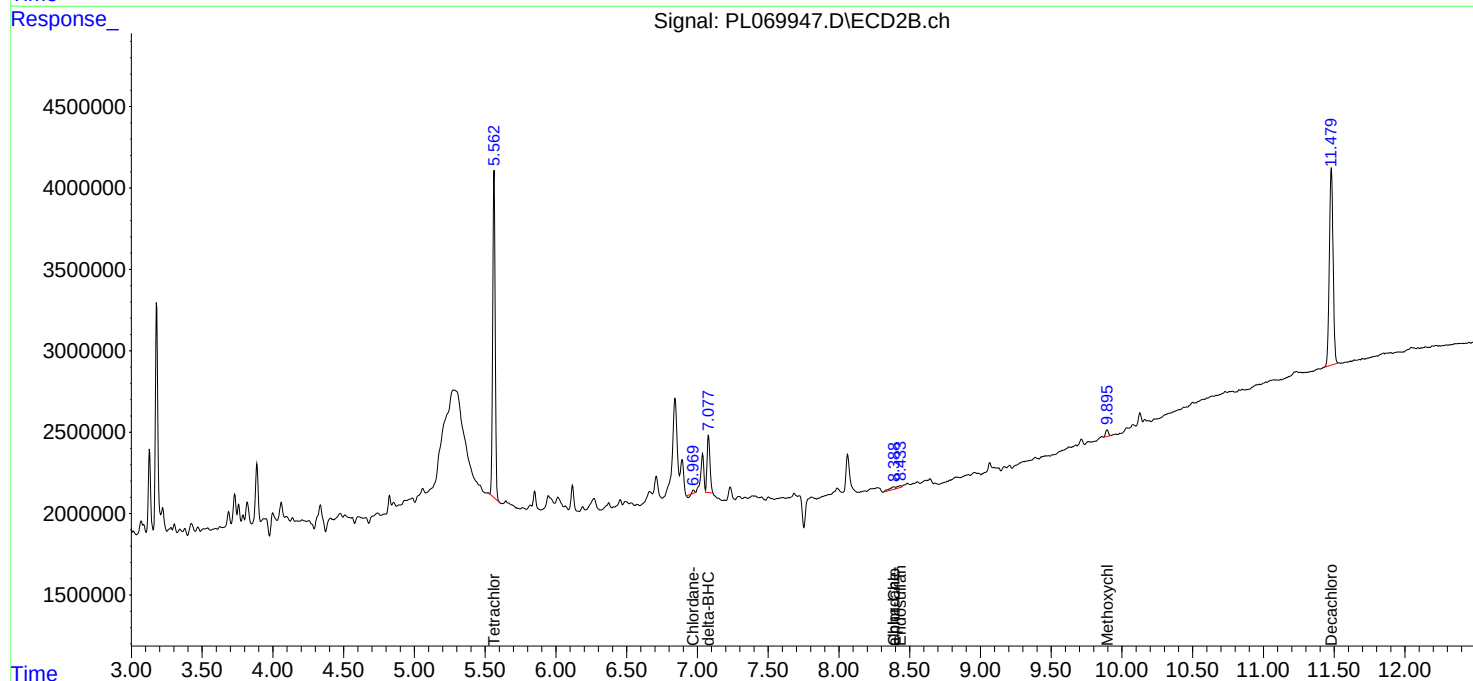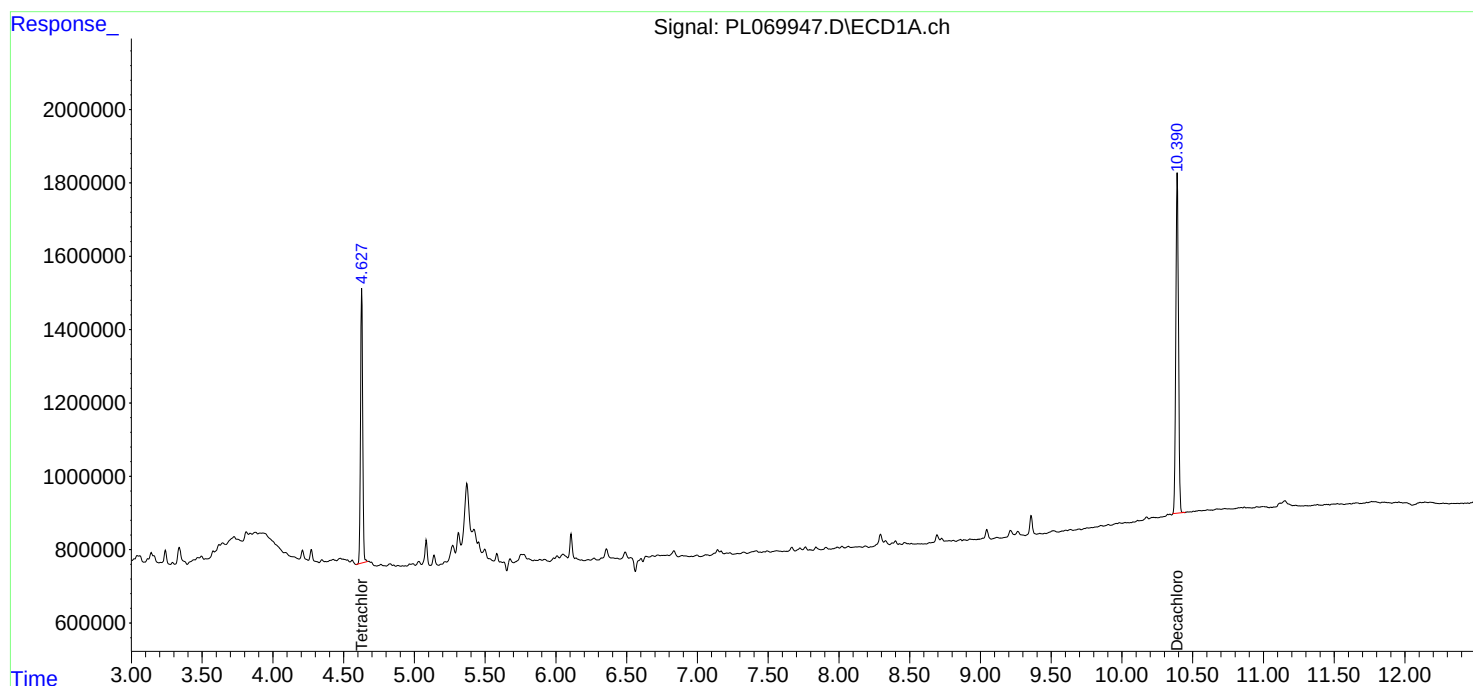


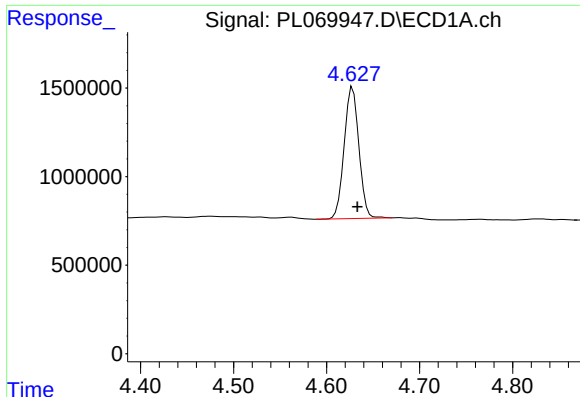

#1 Tetrachloro-m-xylene


R.T.: 4.628 min
Delta R.T.: -0.005 min
Response: 8167245
Conc: 20.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

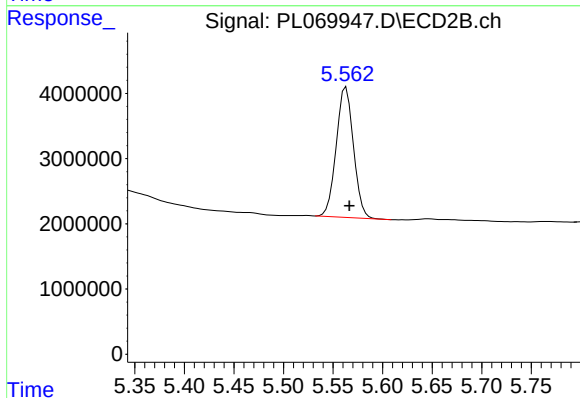


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.003 min
Response: 24111943
Conc: 19.81 ng/ml

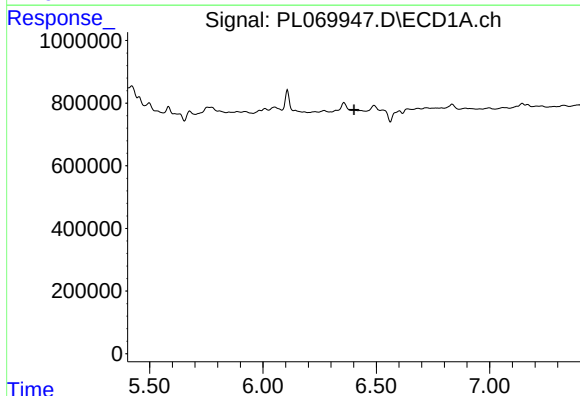


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

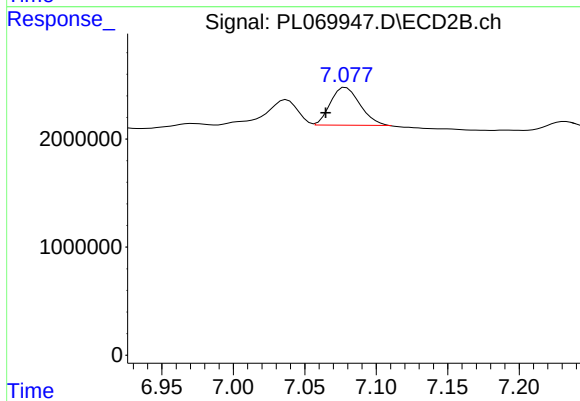

#7 delta-BHC


R.T.: 7.079 min
Delta R.T.: 0.014 min
Response: 5044685
Conc: 3.03 ng/ml

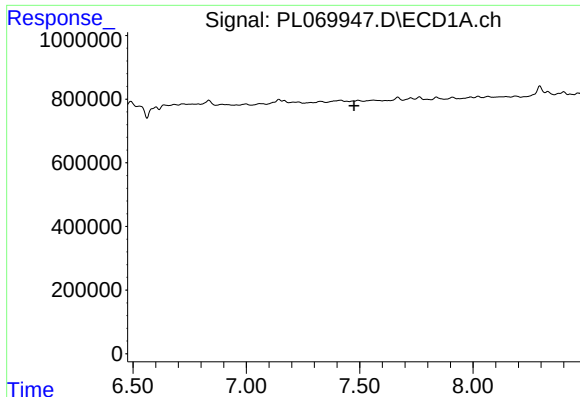

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

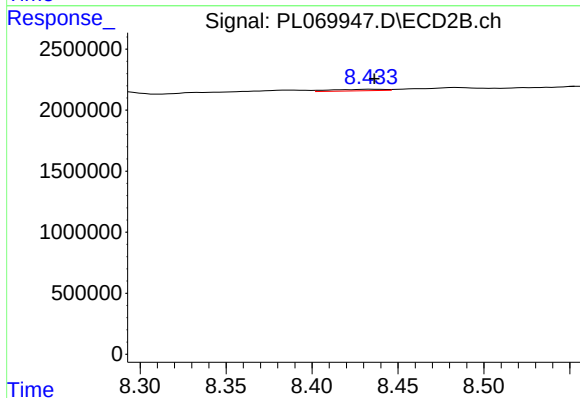


#9 Endosulfan I

R.T.: 8.435 min
Delta R.T.: -0.001 min
Response: 255840
Conc: 0.20 ng/ml

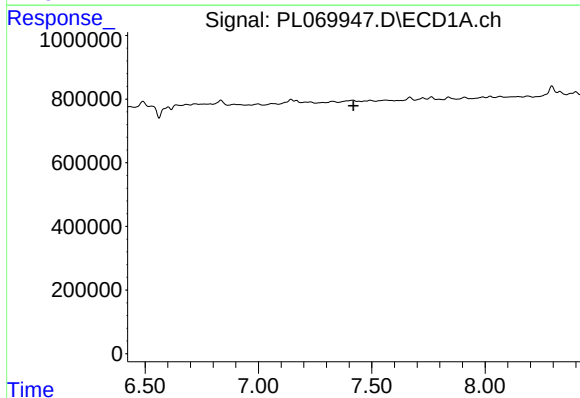


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

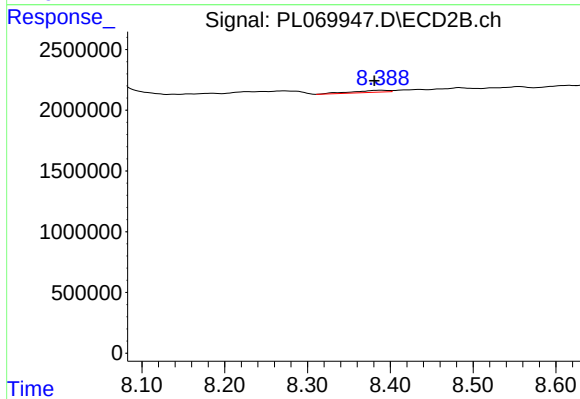

#11 alpha-Chlordane


R.T.: 8.388 min
Delta R.T.: 0.007 min
Response: 490642
Conc: 0.36 ng/ml

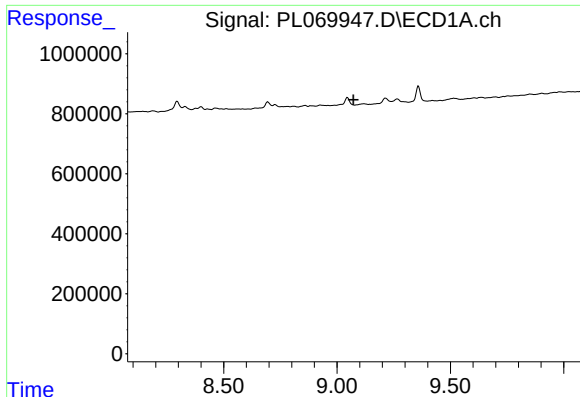

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

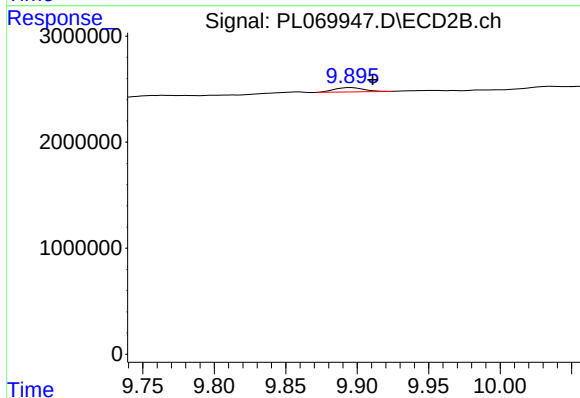


#20 Methoxychlor

R.T.: 9.896 min
Delta R.T.: -0.015 min
Response: 585024
Conc: 0.97 ng/ml

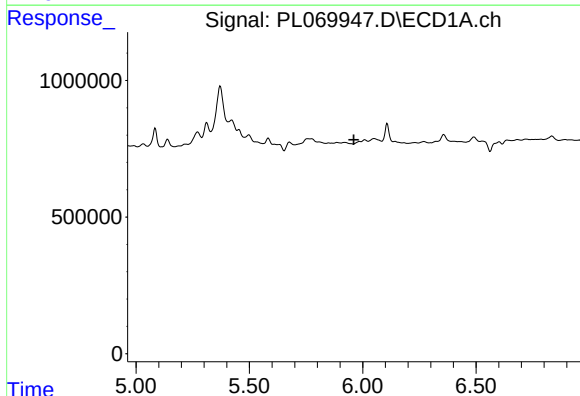


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

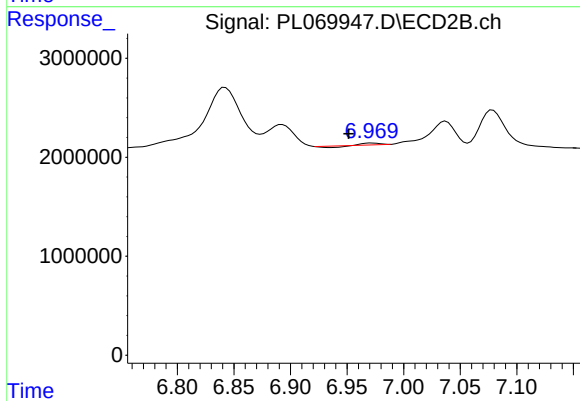

#23 Chlordane-1


R.T.: 6.972 min
Delta R.T.: 0.020 min
Response: 31767
Conc: 0.77 ng/ml

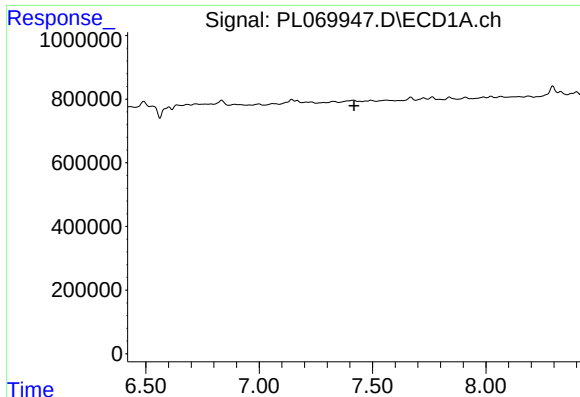

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

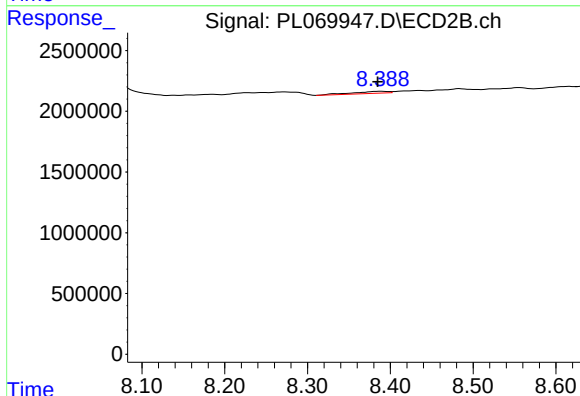


#26 Chlordane-4

R.T.: 8.388 min
Delta R.T.: 0.003 min
Response: 490642
Conc: 2.11 ng/ml

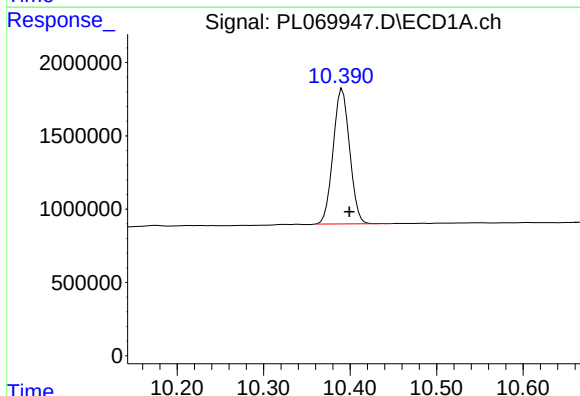

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.008 min
Response: 12149293
Conc: 16.50 ng/ml

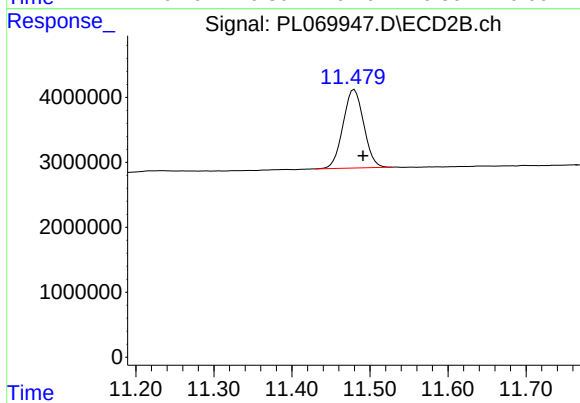

#28 Decachlorobiphenyl

R.T.: 11.480 min
Delta R.T.: -0.011 min
Response: 22238564
Conc: 19.46 ng/ml