

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
 Data File : PL069948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2021 18:33
 Operator : AR\AJ
 Sample : M3823-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 04:17:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.628	5.563	7488332	21645478	18.380	17.782
28)	SA Decachlor...	10.392	11.480	10338290	18871053	14.038	16.515
Target Compounds							
7)	B delta-BHC	0.000	7.079	0	6742614	N.D.	4.048 #
10)	B gamma-Chl...	0.000	8.288	0	867856	N.D.	0.650 #
11)	B alpha-Chl...	0.000	8.380	0	565747	N.D.	0.416 #
15)	B Endosulfa...	0.000	9.198	0	874739	N.D.	0.776 #
16)	A 4,4'-DDD	0.000	9.098	0	914159	N.D.	0.859 #
20)	A Methoxychlor	9.046f	9.895f	789655	1554336	2.105	2.575
21)	B Endrin ke...	0.000	10.076	0	1119438	N.D.	0.908 #
25)	Chlordane-3	0.000	8.288	0	867856	N.D.	4.575 #
26)	Chlordane-4	0.000	8.380	0	565747	N.D.	2.430 #
27)	Chlordane-5	0.000	9.254f	0	169479	N.D.	4.030 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
Data File : PL069948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2021 18:33
Operator : AR\AJ
Sample : M3823-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 04:17:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

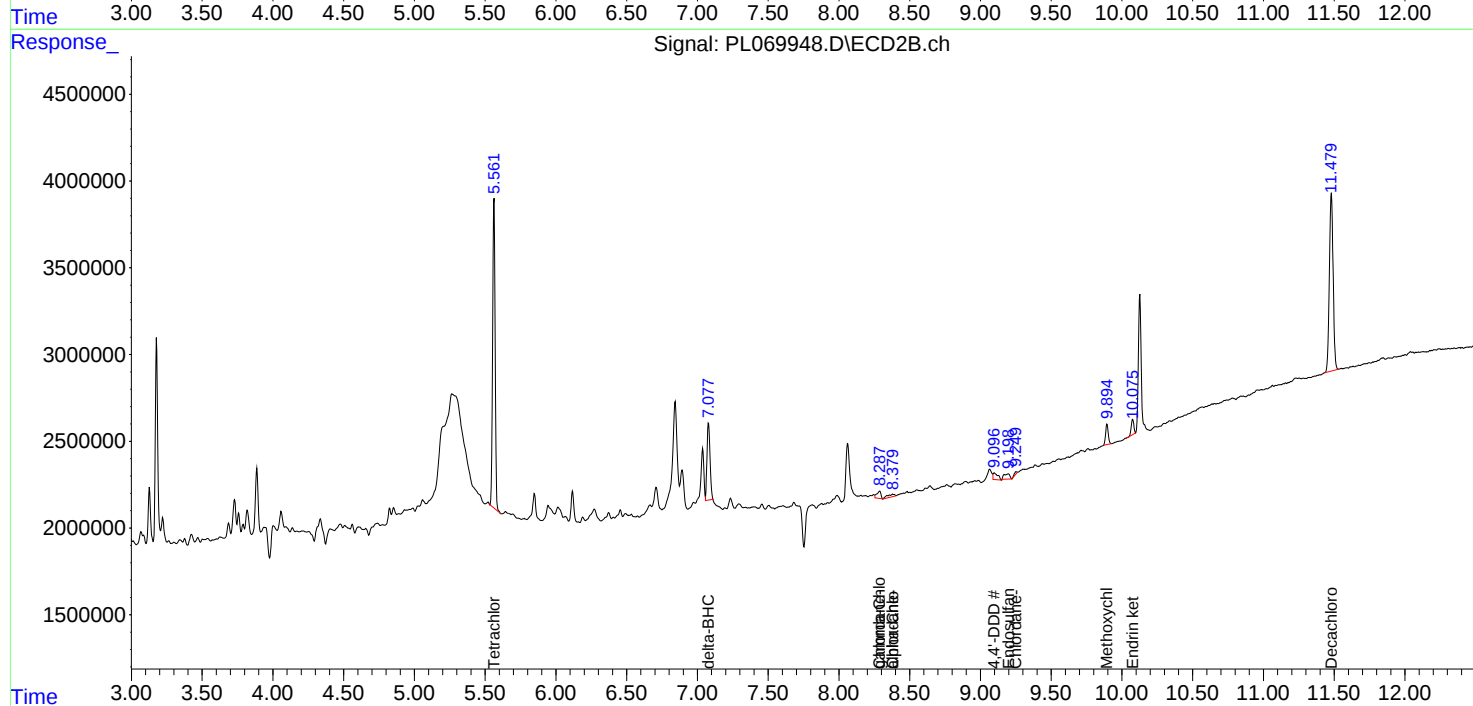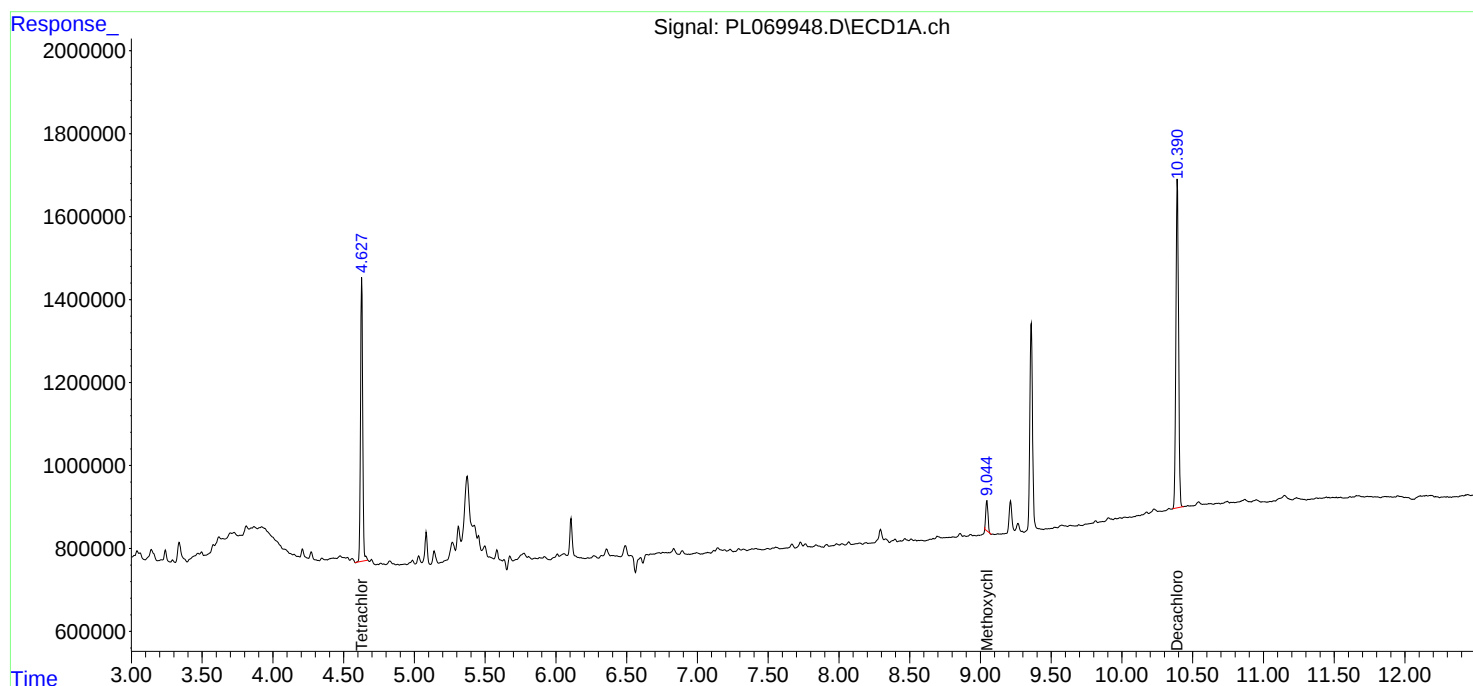


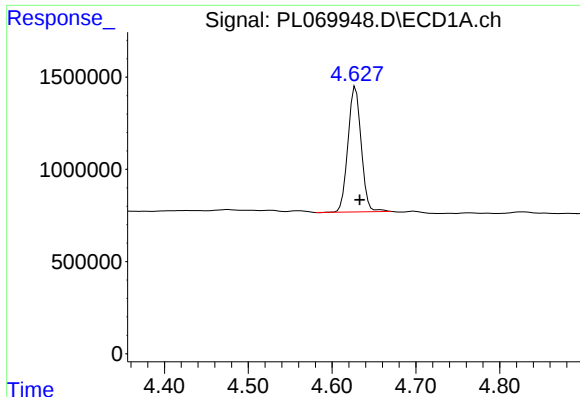

#1 Tetrachloro-m-xylene


R.T.: 4.628 min
Delta R.T.: -0.005 min
Response: 7488332
Conc: 18.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

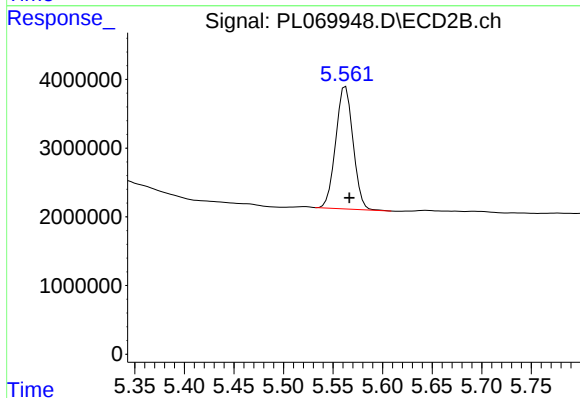


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 21645478
Conc: 17.78 ng/ml

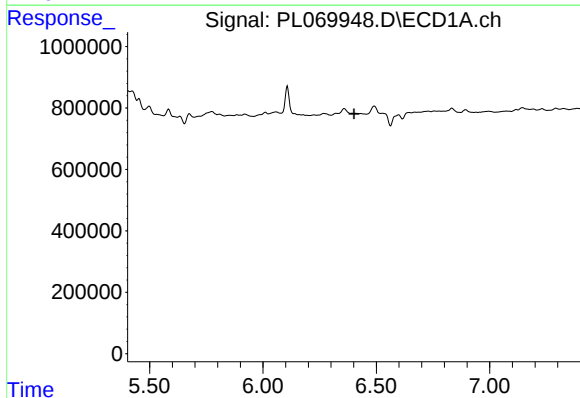


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

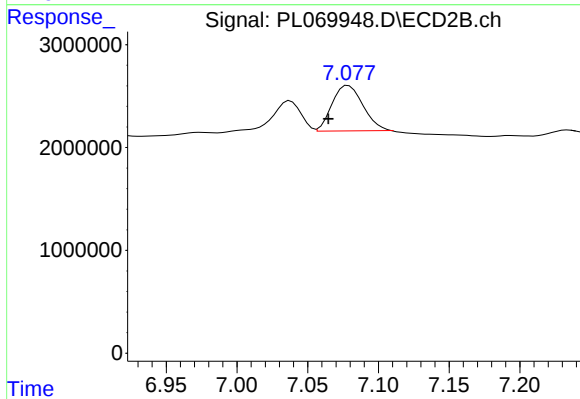

#7 delta-BHC


R.T.: 7.079 min
Delta R.T.: 0.014 min
Response: 6742614
Conc: 4.05 ng/ml

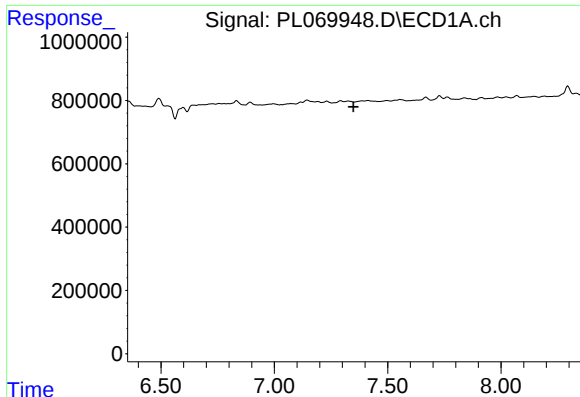

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

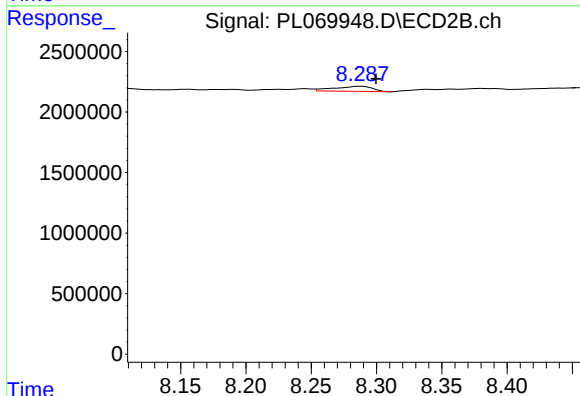


#10 gamma-Chlordane

R.T.: 8.288 min
Delta R.T.: -0.012 min
Response: 867856
Conc: 0.65 ng/ml

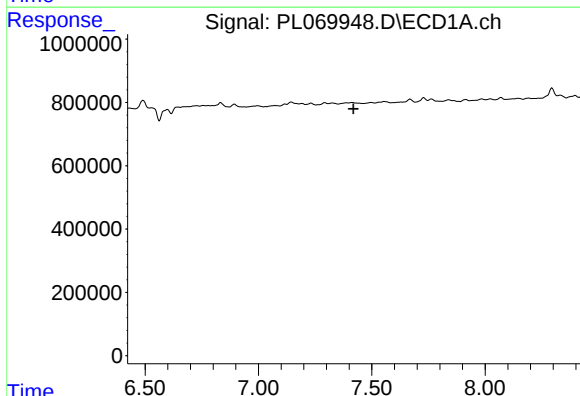


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

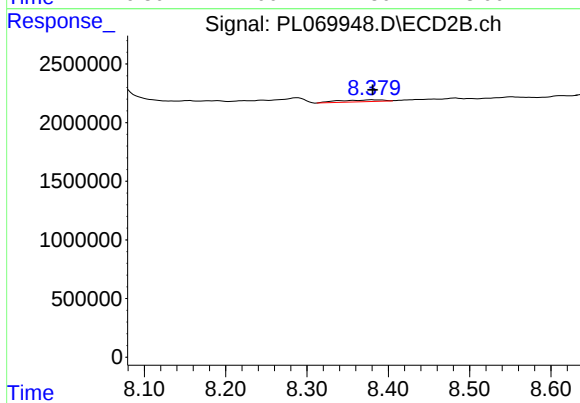

#11 alpha-Chlordane


R.T.: 8.380 min
Delta R.T.: 0.000 min
Response: 565747
Conc: 0.42 ng/ml

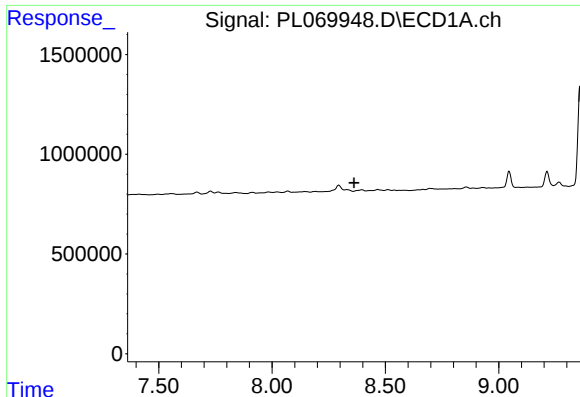

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

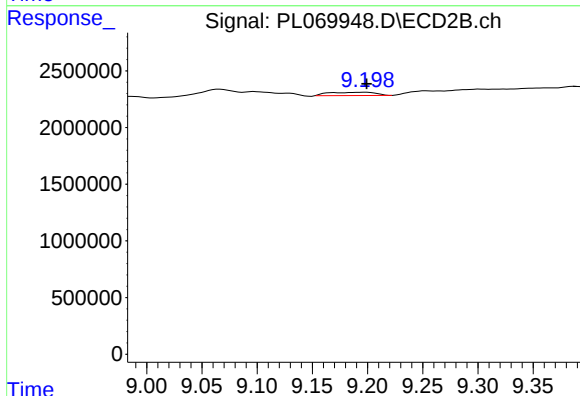


#15 Endosulfan II

R.T.: 9.198 min
Delta R.T.: -0.001 min
Response: 874739
Conc: 0.78 ng/ml

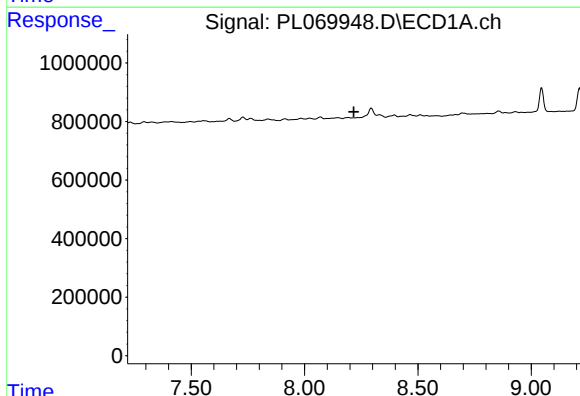


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.218 min
Response: 0
Conc: N.D.

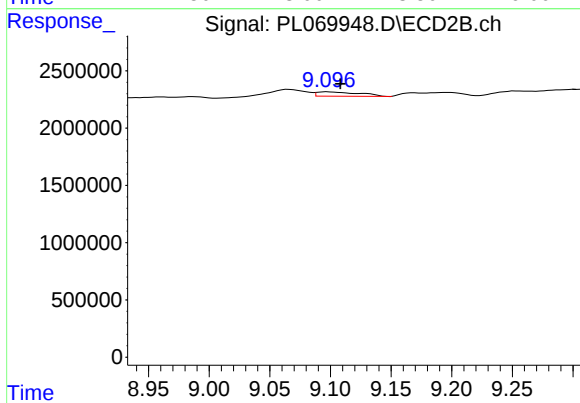

#16 4,4'-DDD


R.T.: 9.098 min
Delta R.T.: -0.010 min
Response: 914159
Conc: 0.86 ng/ml

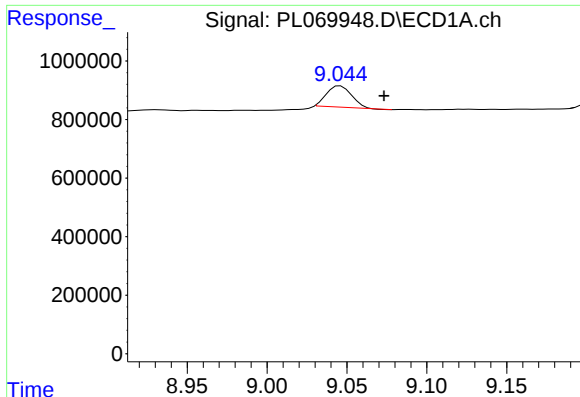

#20 Methoxychlor


R.T.: 9.046 min
Delta R.T.: -0.027 min
Response: 789655
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

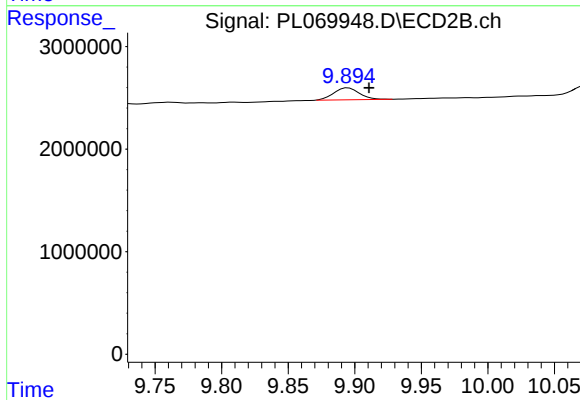


#20 Methoxychlor

R.T.: 9.895 min
Delta R.T.: -0.016 min
Response: 1554336
Conc: 2.58 ng/ml

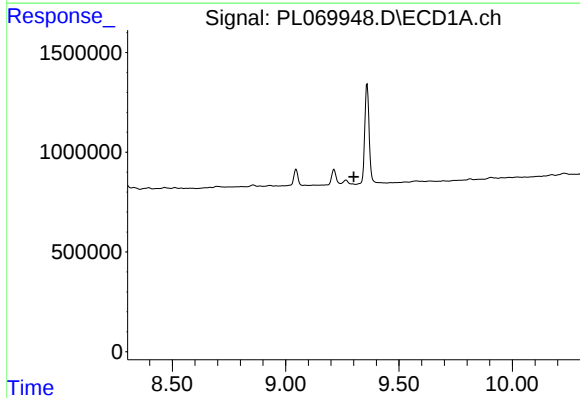


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.301 min
Response: 0
Conc: N.D.

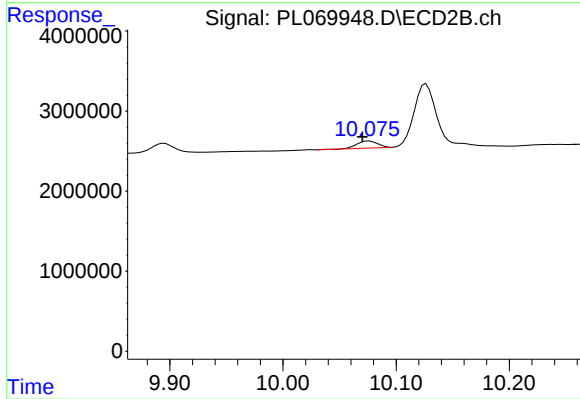

#21 Endrin ketone


R.T.: 10.076 min
Delta R.T.: 0.006 min
Response: 1119438
Conc: 0.91 ng/ml

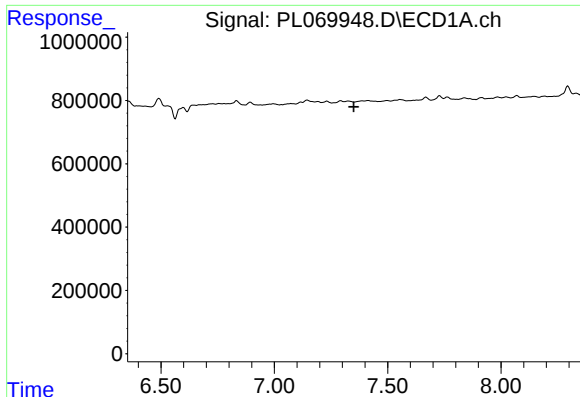

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

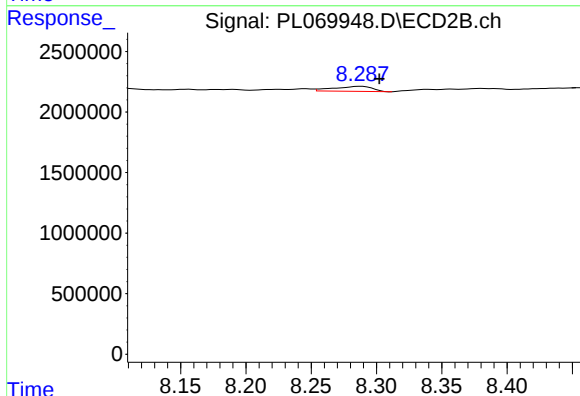


#25 Chlordane-3

R.T.: 8.288 min
Delta R.T.: -0.014 min
Response: 867856
Conc: 4.58 ng/ml

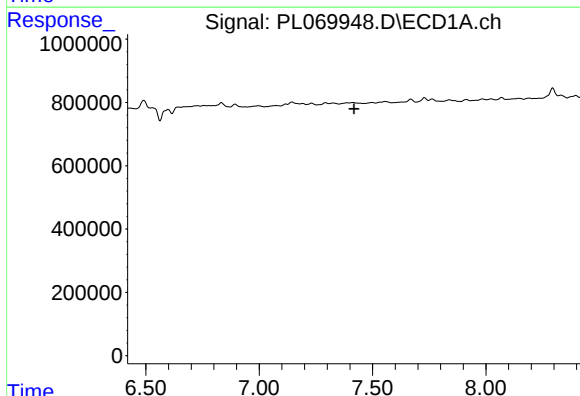


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.418 min
Response: 0
Conc: N.D.

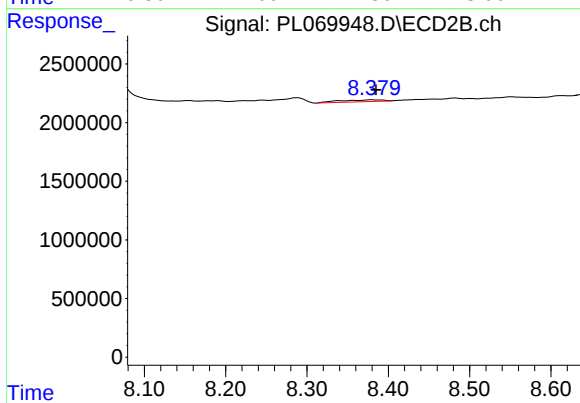

#26 Chlordane-4


R.T.: 8.380 min
Delta R.T.: -0.005 min
Response: 565747
Conc: 2.43 ng/ml

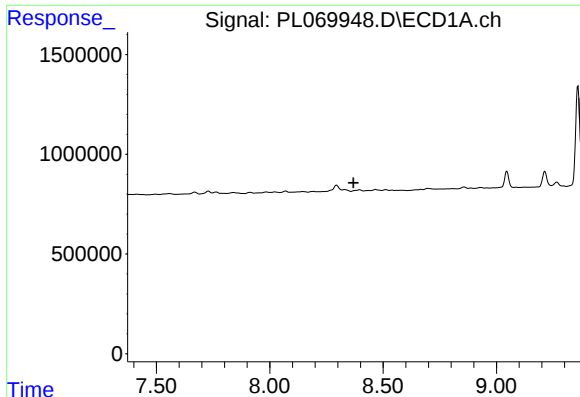

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

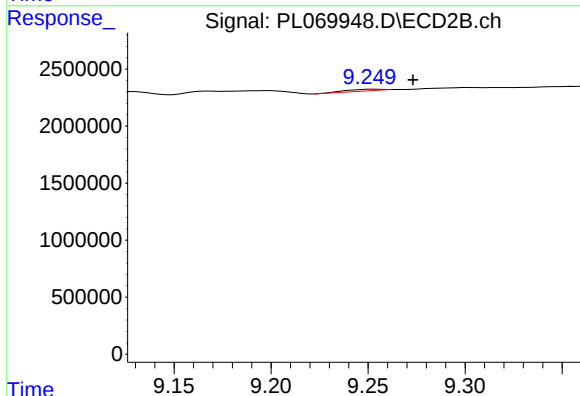


#27 Chlordane-5

R.T.: 9.254 min
Delta R.T.: -0.019 min
Response: 169479
Conc: 4.03 ng/ml

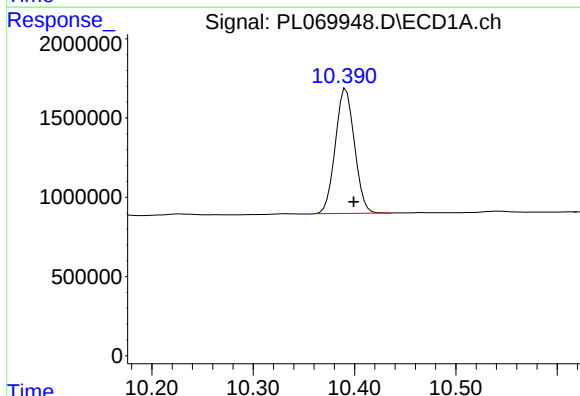

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.008 min
Response: 10338290
Conc: 14.04 ng/ml

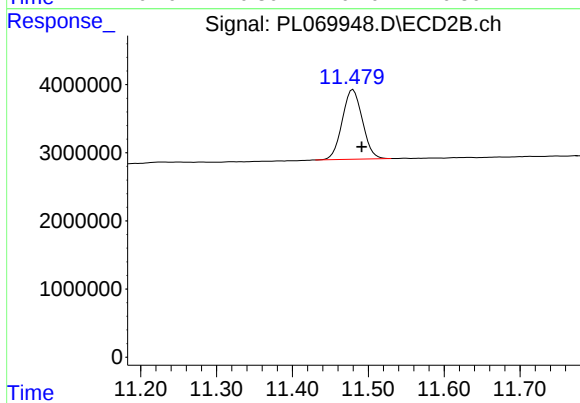

#28 Decachlorobiphenyl

R.T.: 11.480 min
Delta R.T.: -0.011 min
Response: 18871053
Conc: 16.52 ng/ml