

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
 Data File : PL069949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2021 18:49
 Operator : AR\AJ
 Sample : PB139246BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 04:18:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.627	5.563	8581229	25079860	21.063	20.604
28)	SA Decachlor...	10.392	11.480	12687962	23030675	17.229	20.156
Target Compounds							
7)	B delta-BHC	0.000	7.080f	0	1134093	N.D.	0.681 #
10)	B gamma-Chl...	0.000	8.292	0	153996	N.D.	0.115 #
17)	MA 4,4'-DDT	0.000	9.419	0	80565	N.D.	0.072 #
23)	Chlordane-1	0.000	6.971f	0	137497	N.D.	3.350 #
25)	Chlordane-3	0.000	8.292	0	153996	N.D.	0.812 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
Data File : PL069949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2021 18:49
Operator : AR\AJ
Sample : PB139246BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 04:18:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

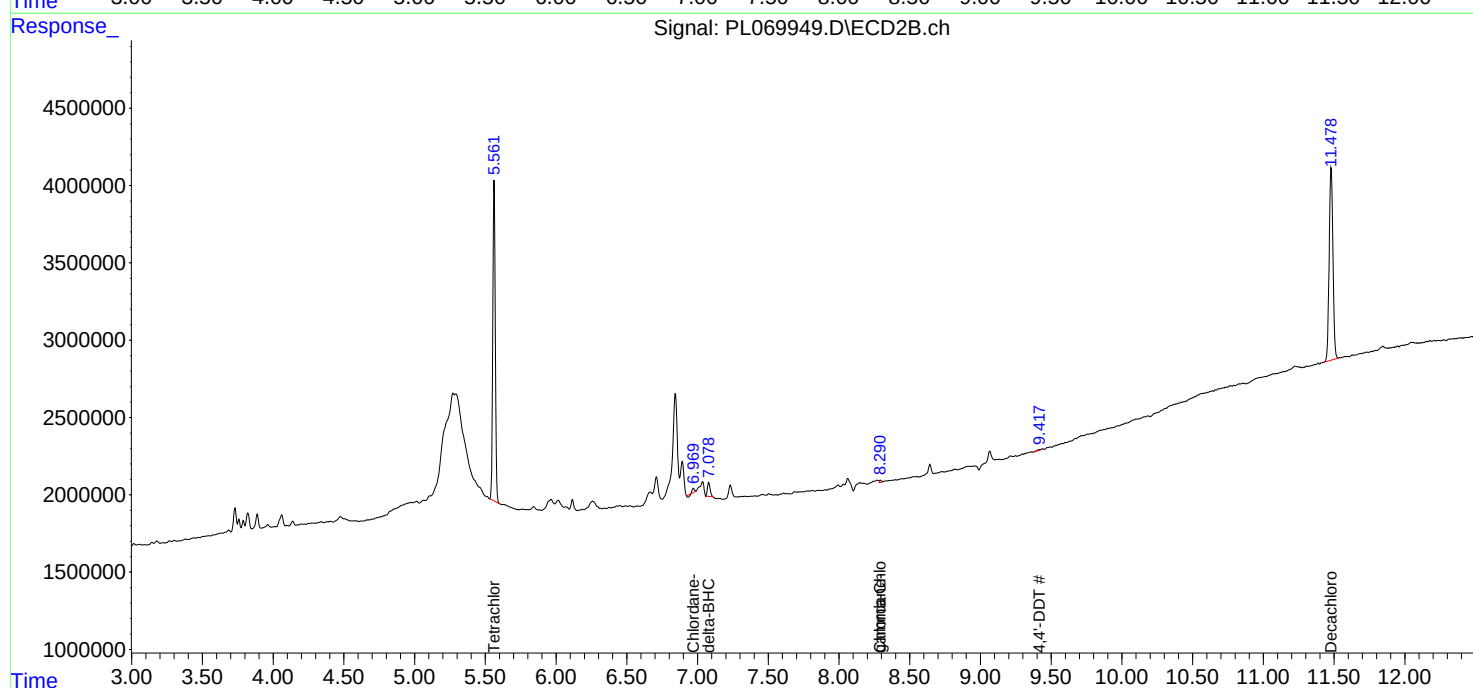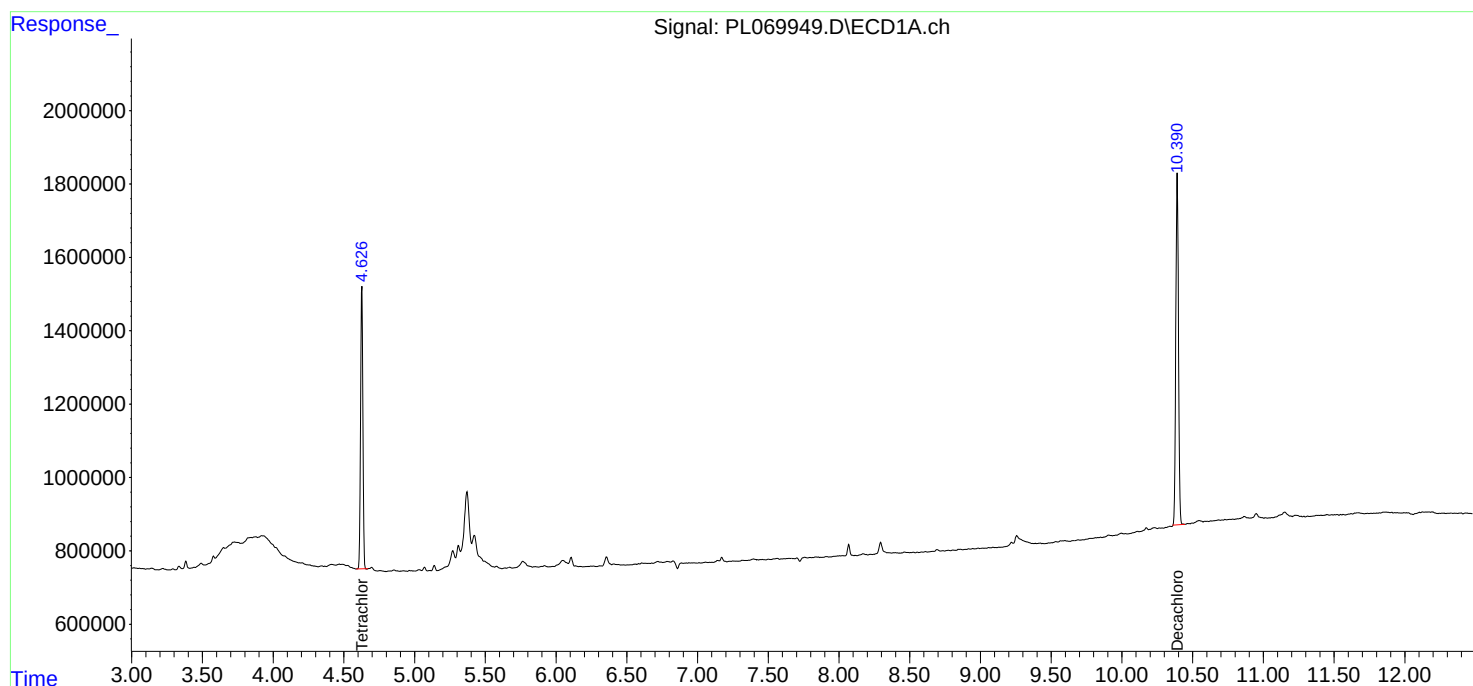


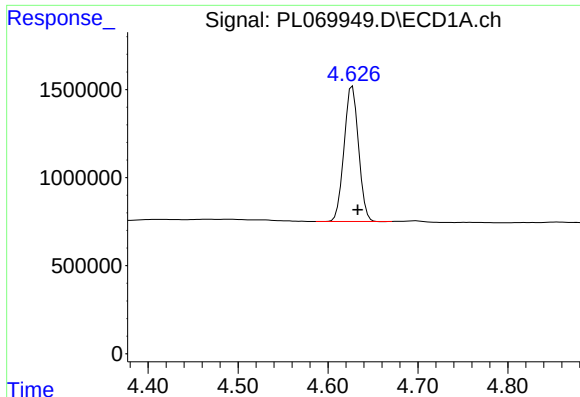

#1 Tetrachloro-m-xylene


R.T.: 4.627 min
Delta R.T.: -0.006 min
Response: 8581229
Conc: 21.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

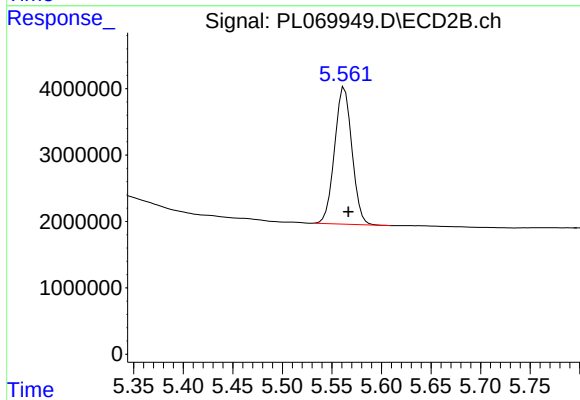


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 25079860
Conc: 20.60 ng/ml

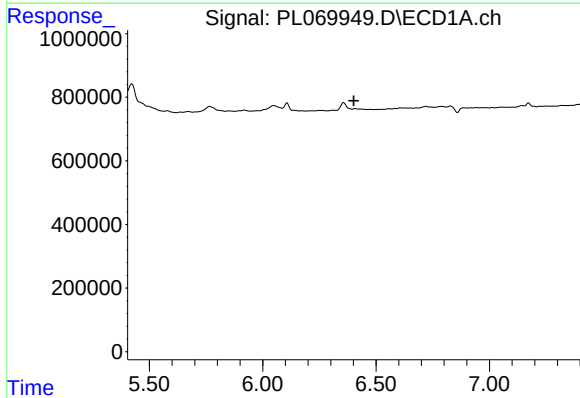


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

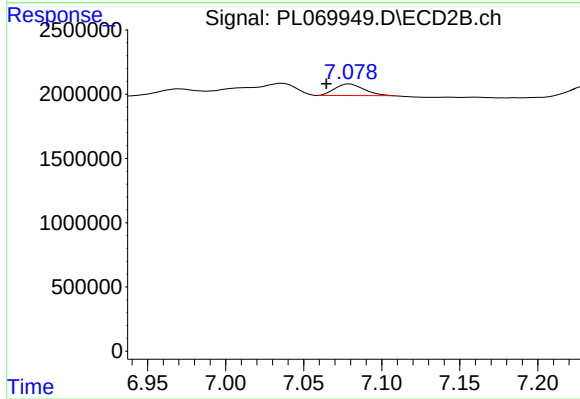

#7 delta-BHC


R.T.: 7.080 min
Delta R.T.: 0.015 min
Response: 1134093
Conc: 0.68 ng/ml

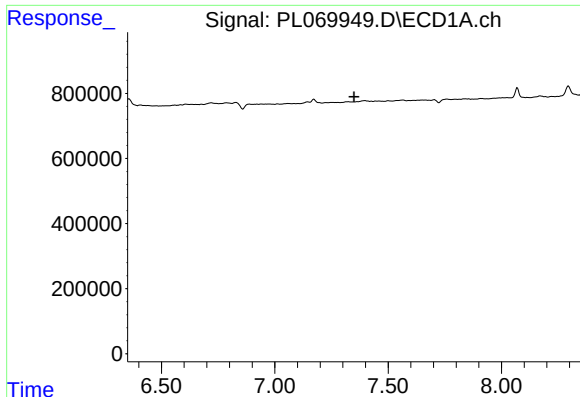

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

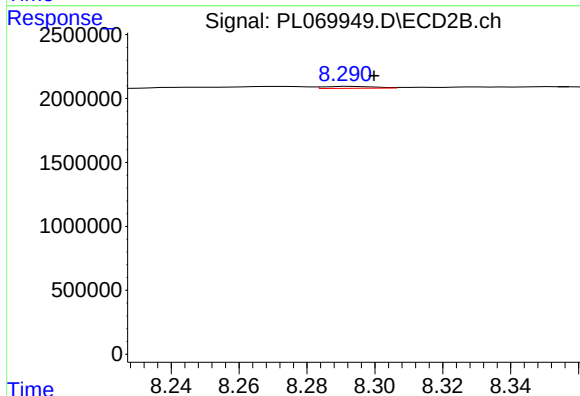


#10 gamma-Chlordane

R.T.: 8.292 min
Delta R.T.: -0.007 min
Response: 153996
Conc: 0.12 ng/ml

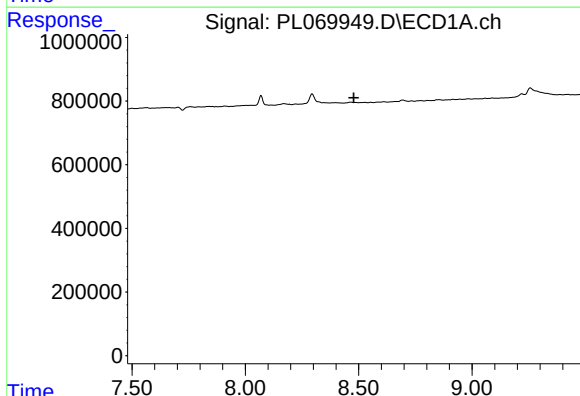


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

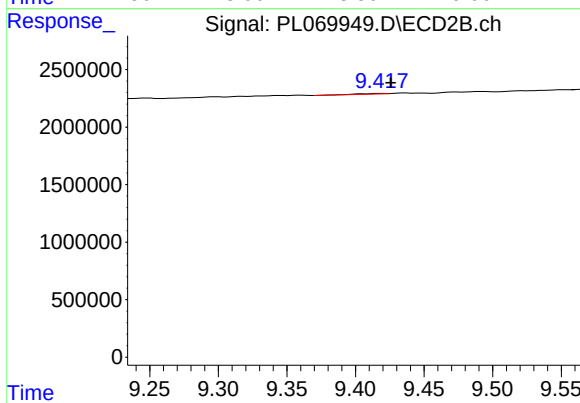

#17 4,4'-DDT


R.T.: 9.419 min
Delta R.T.: -0.007 min
Response: 80565
Conc: 0.07 ng/ml

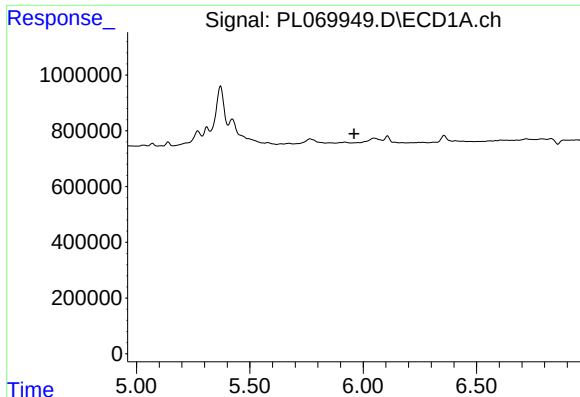

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

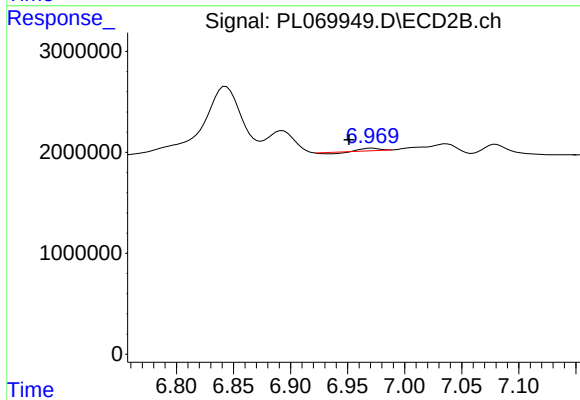


#23 Chlordane-1

R.T.: 6.971 min
Delta R.T.: 0.020 min
Response: 137497
Conc: 3.35 ng/ml

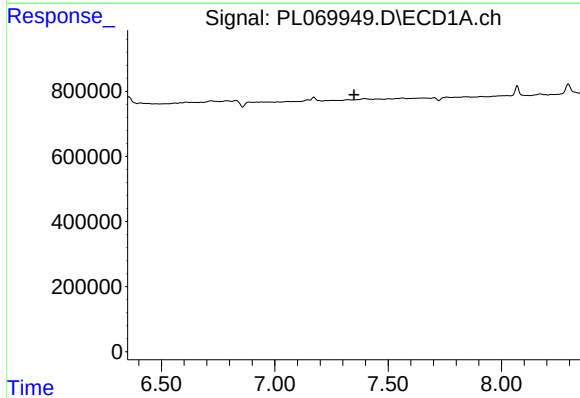


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

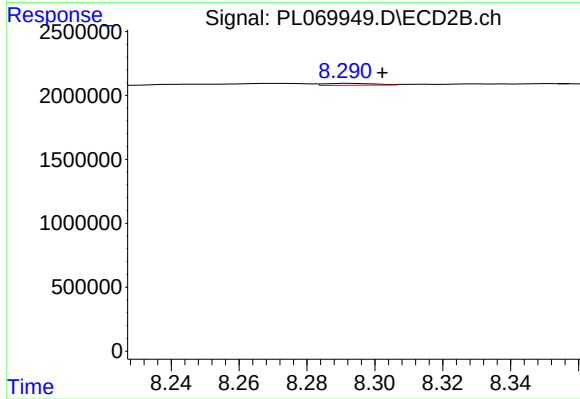

#25 Chlordane-3


R.T.: 8.292 min
Delta R.T.: -0.010 min
Response: 153996
Conc: 0.81 ng/ml

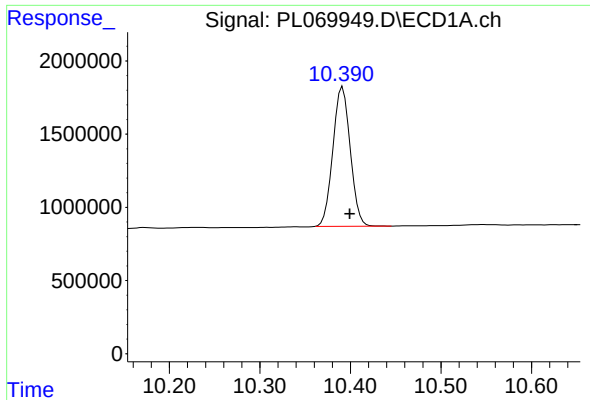

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.008 min
Response: 12687962
Conc: 17.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

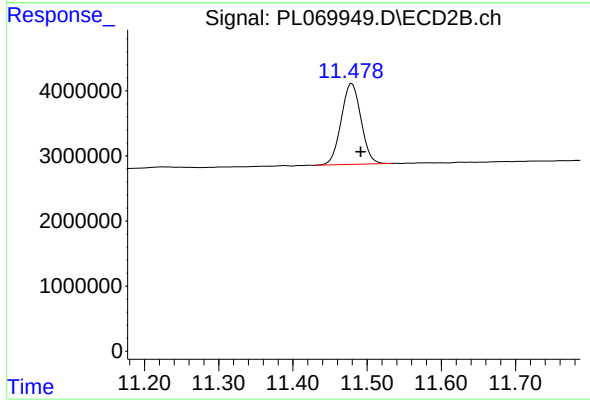

#28 Decachlorobiphenyl

R.T.: 11.480 min
Delta R.T.: -0.012 min
Response: 23030675
Conc: 20.16 ng/ml