

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
 Data File : PL069951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2021 19:23
 Operator : AR\AJ
 Sample : PB139246TB
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 04:18:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.628	5.562	8275361	24304727	20.312	19.967
28)	SA Decachlor...	10.391	11.480	12438799	22241976	16.891	19.465
Target Compounds							
7)	B delta-BHC	0.000	7.080f	0	1247540	N.D.	0.749 #
9)	A Endosulfan I	0.000	8.464f	0	28335	N.D.	0.022 #
10)	B gamma-Chl...	0.000	8.287	0	410698	N.D.	0.307 #
22)	Mirex	0.000	10.554f	0	255879	N.D.	0.273 #
23)	Chlordane-1	0.000	6.974f	0	19080	N.D.	0.465 #
25)	Chlordane-3	0.000	8.287f	0	410698	N.D.	2.165 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092121\
Data File : PL069951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2021 19:23
Operator : AR\AJ
Sample : PB139246TB
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 04:18:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

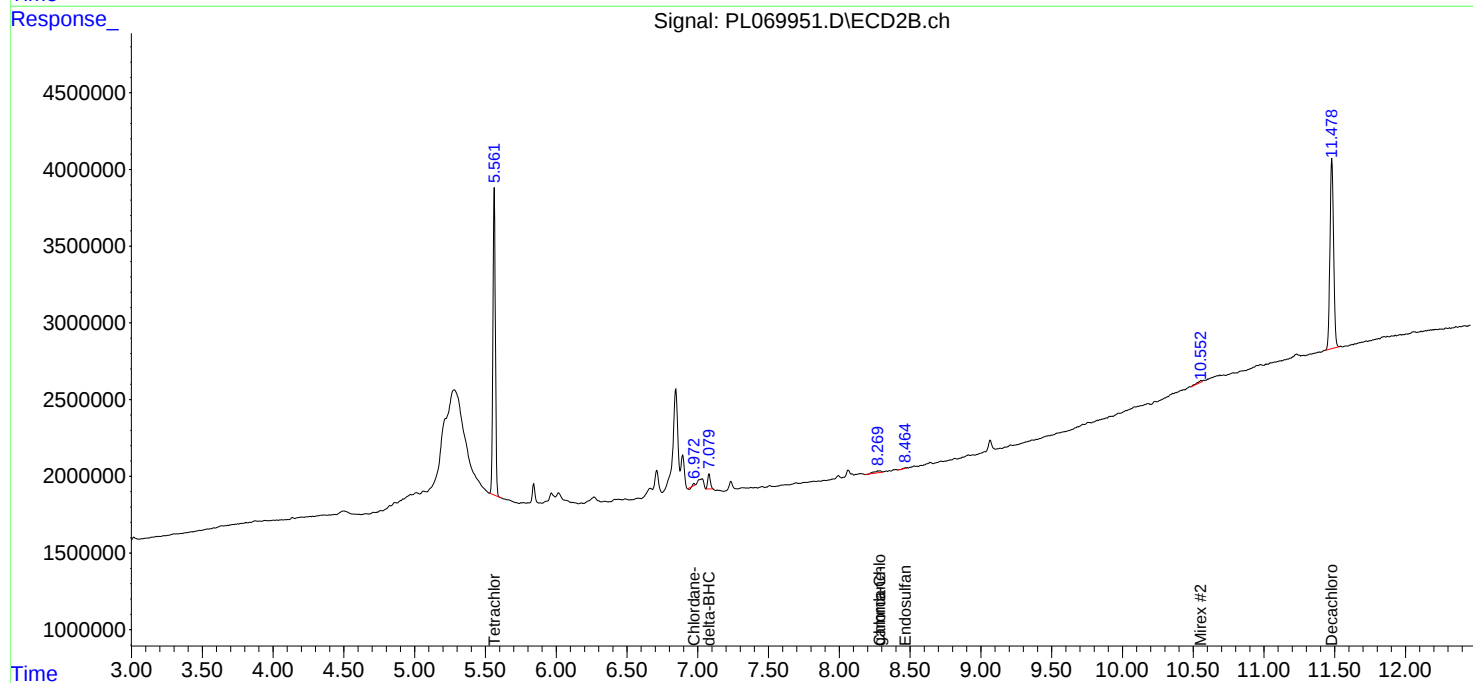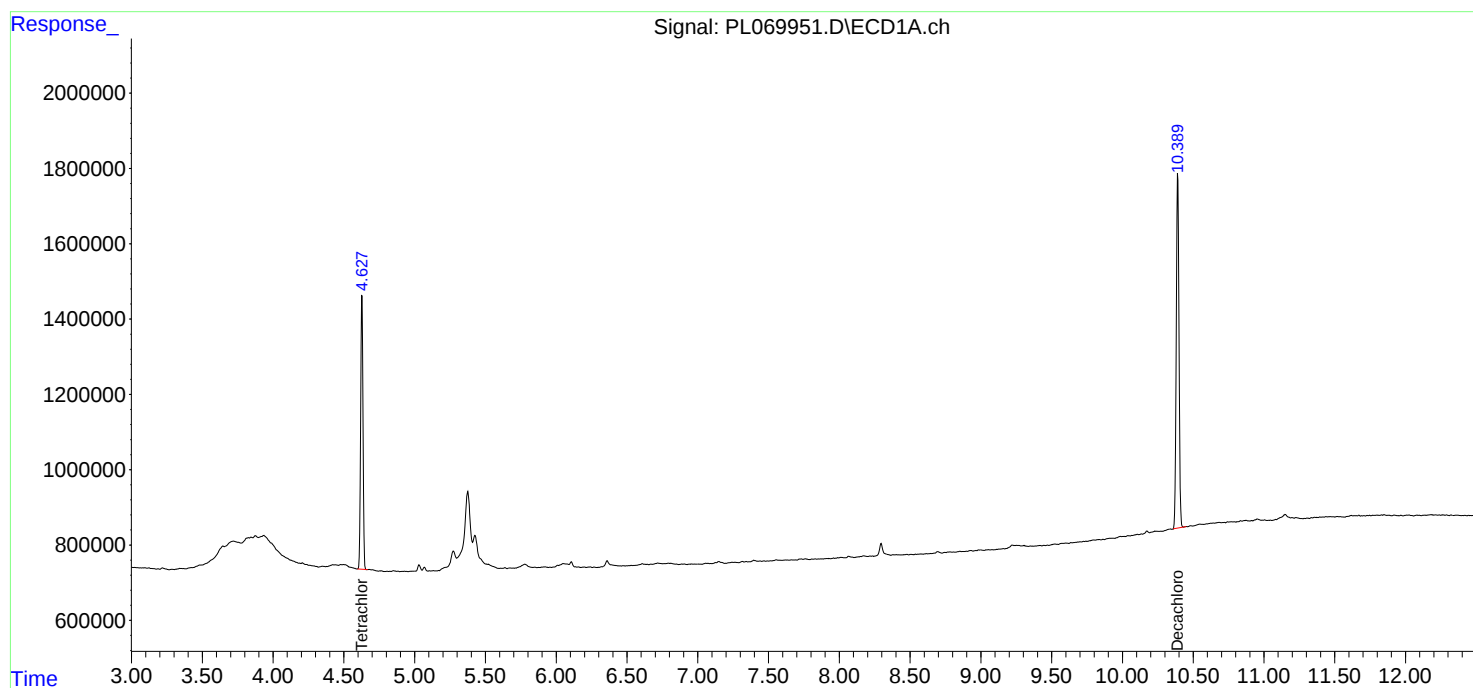


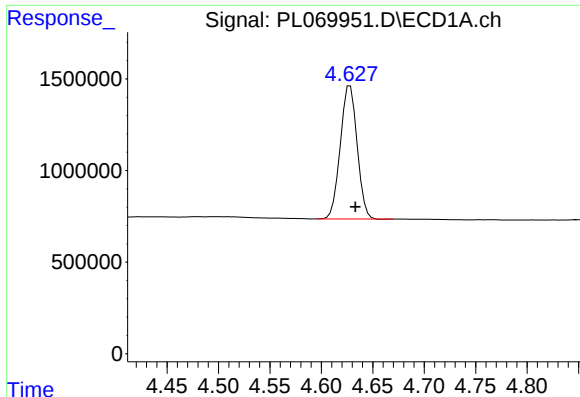

#1 Tetrachloro-m-xylene


R.T.: 4.628 min
Delta R.T.: -0.005 min
Response: 8275361
Conc: 20.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

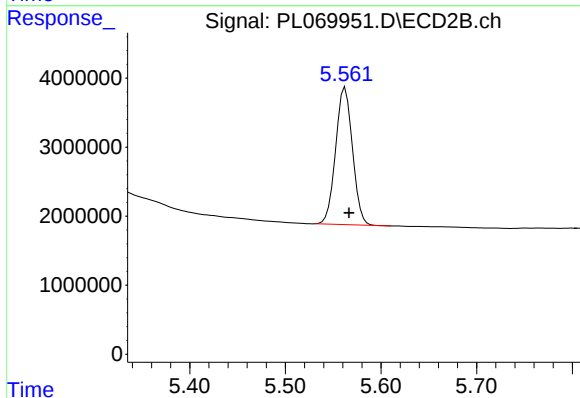


#1 Tetrachloro-m-xylene

R.T.: 5.562 min
Delta R.T.: -0.004 min
Response: 24304727
Conc: 19.97 ng/ml

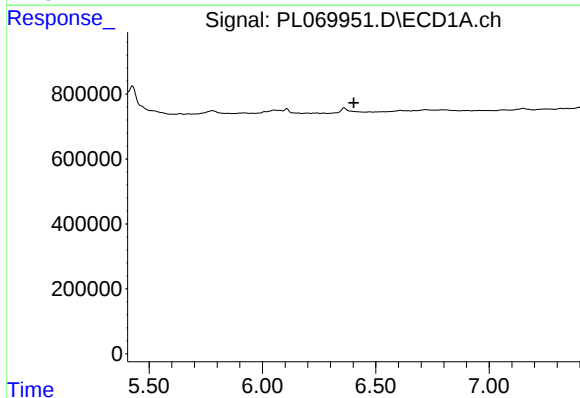


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

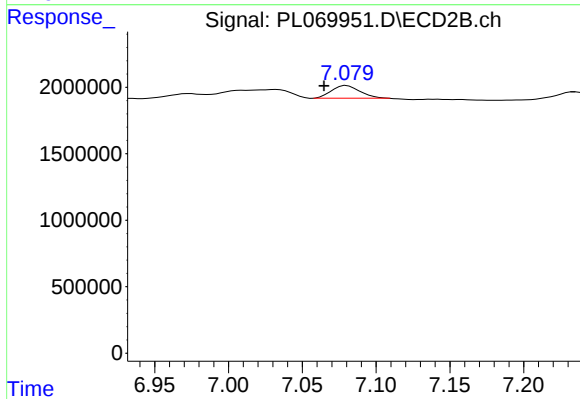

#7 delta-BHC


R.T.: 7.080 min
Delta R.T.: 0.015 min
Response: 1247540
Conc: 0.75 ng/ml

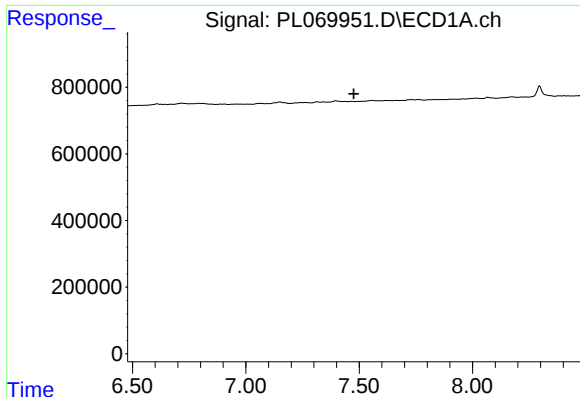

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

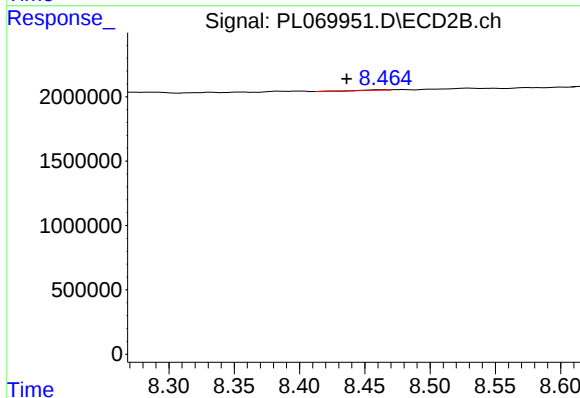


#9 Endosulfan I

R.T.: 8.464 min
Delta R.T.: 0.027 min
Response: 28335
Conc: 0.02 ng/ml

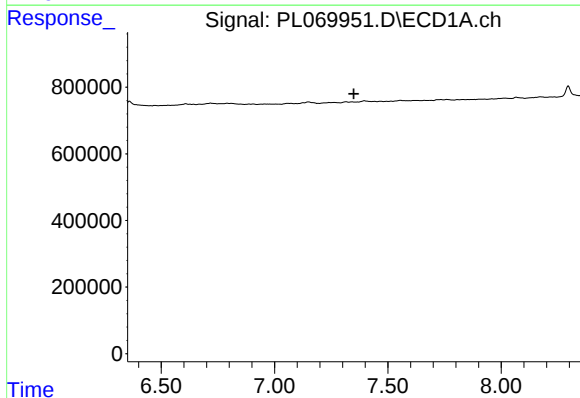


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

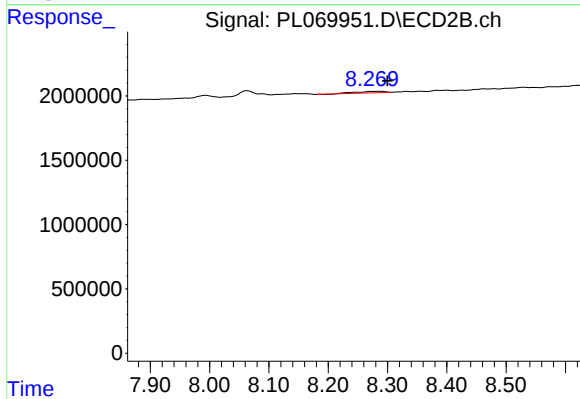

#10 gamma-Chlordane


R.T.: 8.287 min
Delta R.T.: -0.013 min
Response: 410698
Conc: 0.31 ng/ml

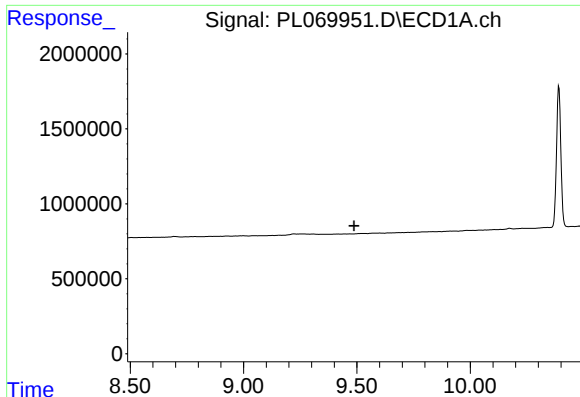

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

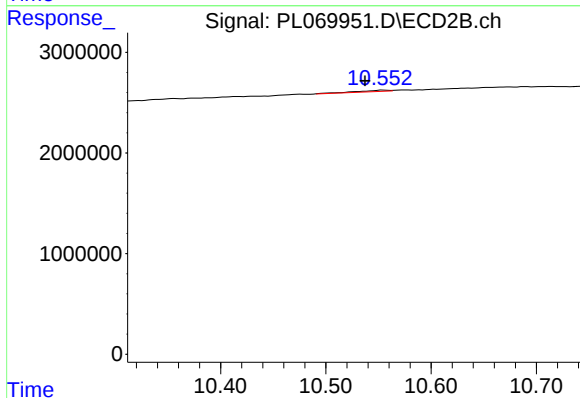


#22 Mirex

R.T.: 10.554 min
Delta R.T.: 0.017 min
Response: 255879
Conc: 0.27 ng/ml

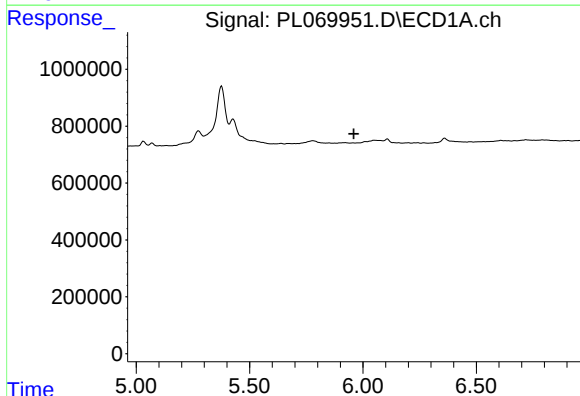


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

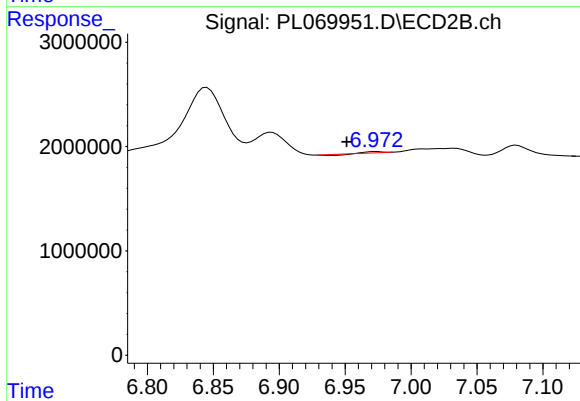

#23 Chlordane-1


R.T.: 6.974 min
Delta R.T.: 0.023 min
Response: 19080
Conc: 0.46 ng/ml

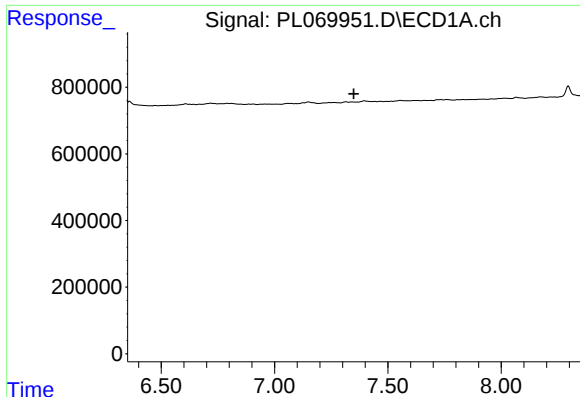

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

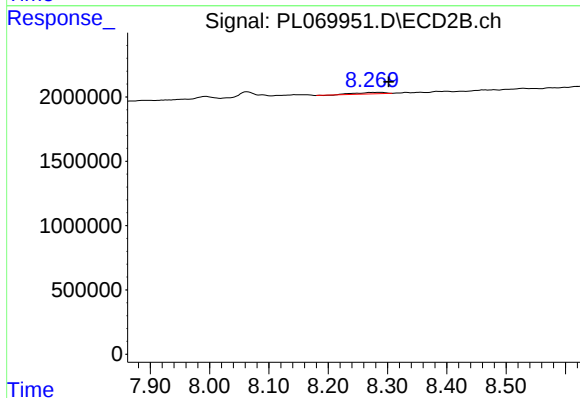


#25 Chlordane-3

R.T.: 8.287 min
Delta R.T.: -0.015 min
Response: 410698
Conc: 2.17 ng/ml

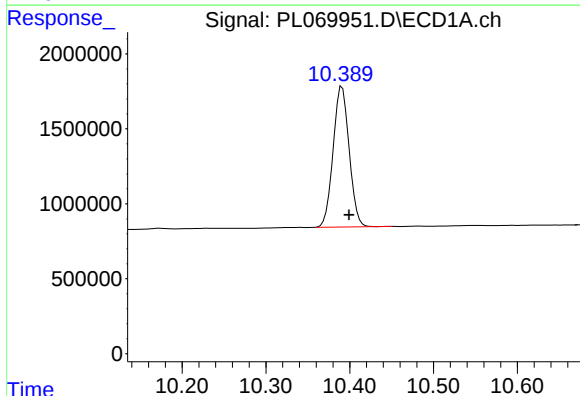

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.008 min
Response: 12438799
Conc: 16.89 ng/ml

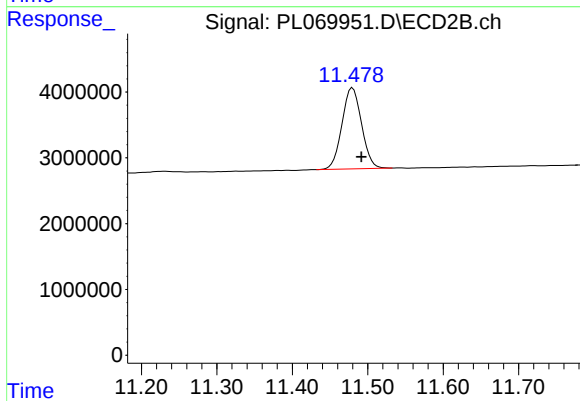

#28 Decachlorobiphenyl

R.T.: 11.480 min
Delta R.T.: -0.011 min
Response: 22241976
Conc: 19.47 ng/ml