

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092124\
 Data File : PL091910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 13:45
 Operator : AR\AJ
 Sample : P4126-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-08-09192024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/23/2024
 Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 00:01:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.782	3873519	4744466	2.485m	2.537
28) SA Decachlor...	9.056	7.922	2585671	4538236	2.128m	2.458m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092124\
Data File : PL091910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 13:45
Operator : AR\AJ
Sample : P4126-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-08-09192024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/23/2024
Supervised By : Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 00:01:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

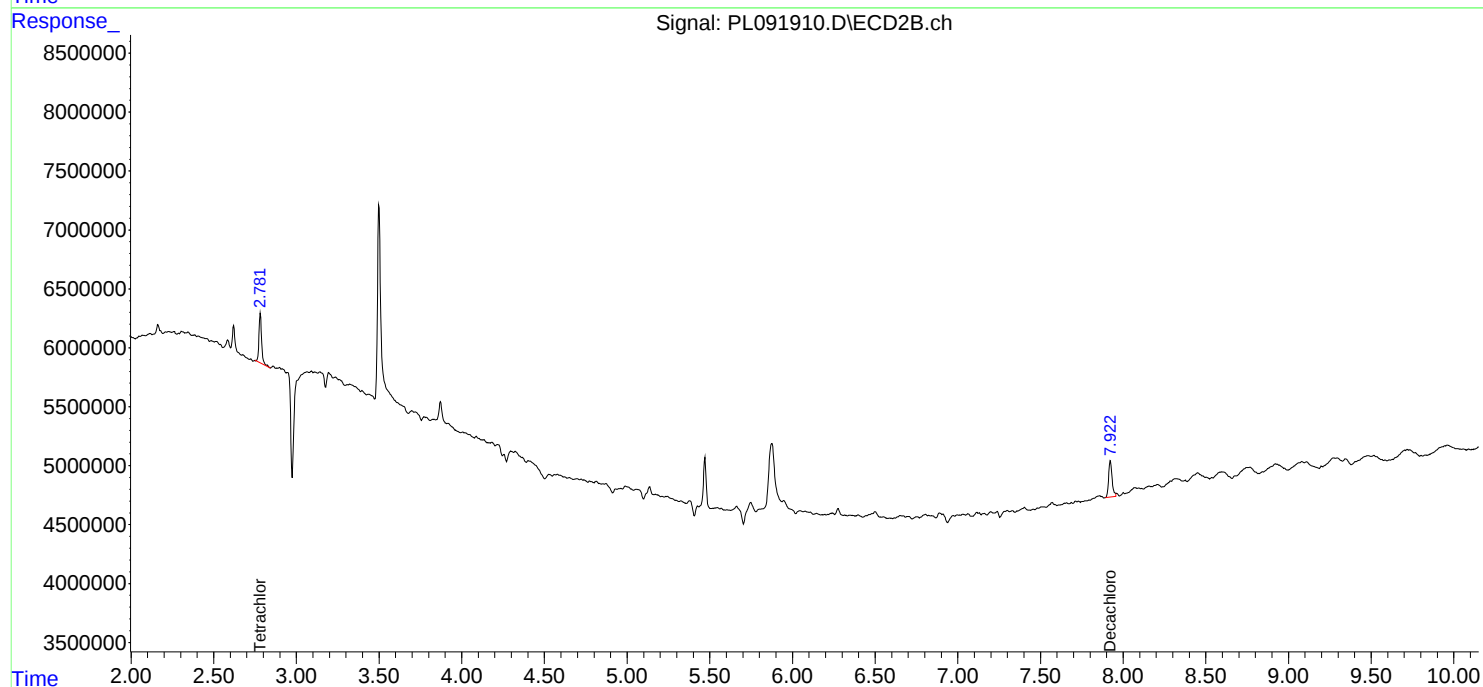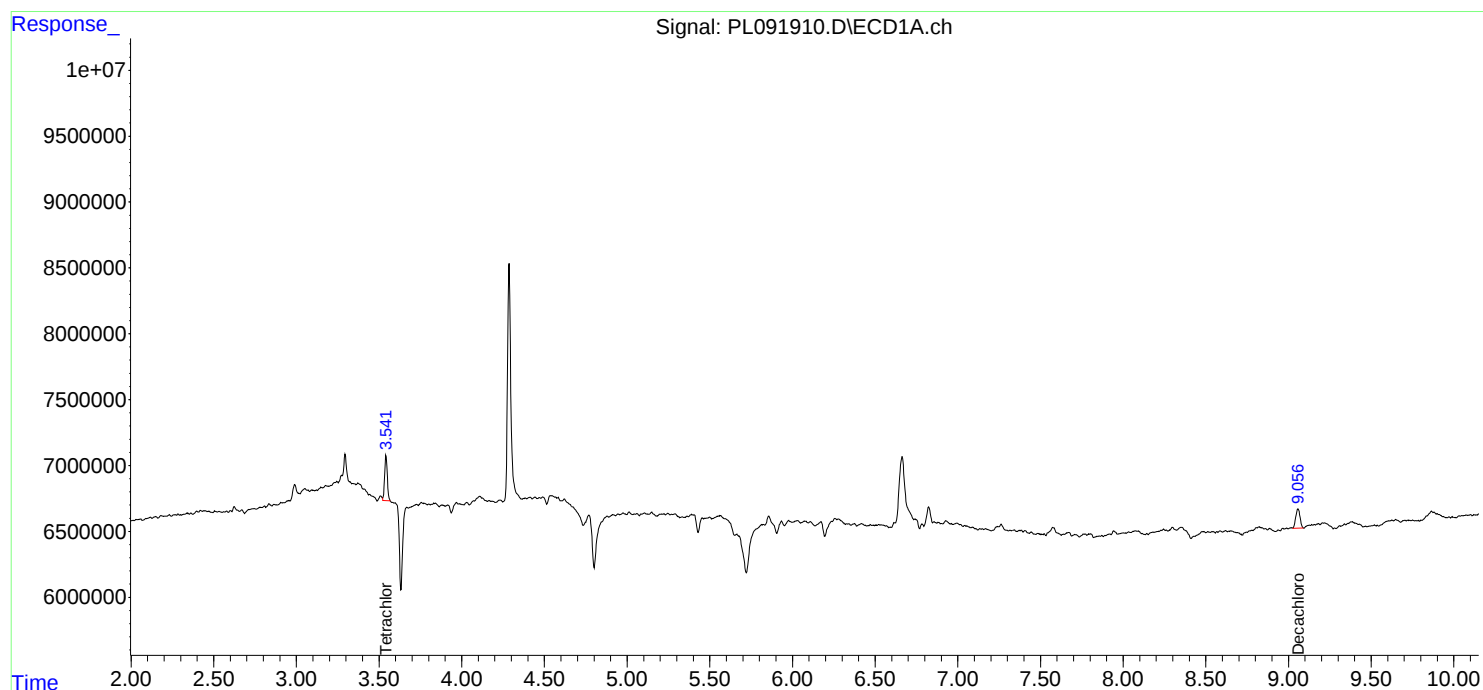

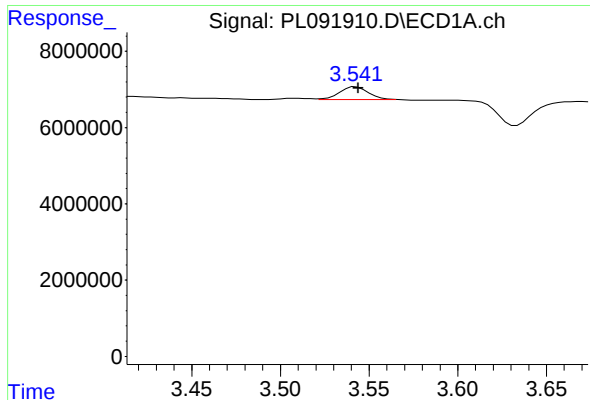


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: -0.003 min
Response: 3873519
Conc: 2.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-08-09192024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

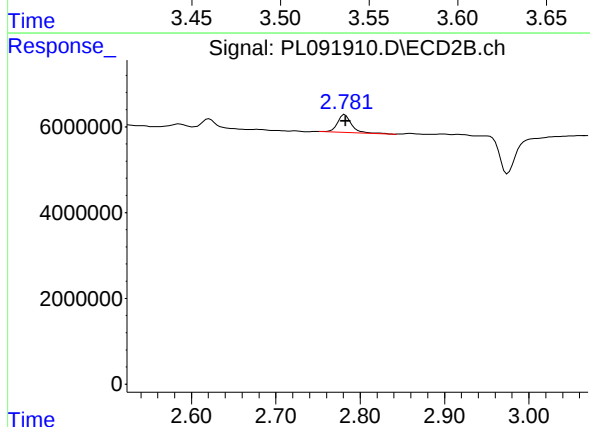


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 4744466
Conc: 2.54 ng/ml

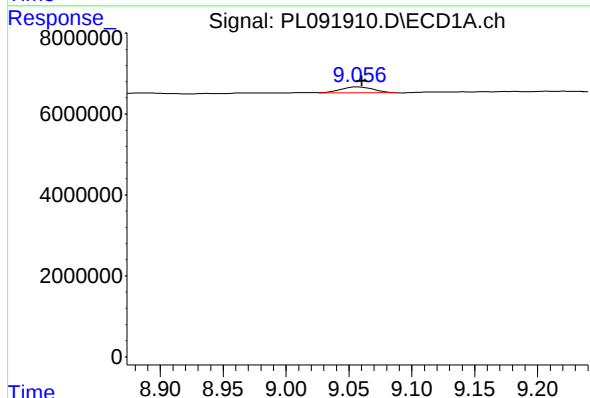

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: -0.004 min
Response: 2585671
Conc: 2.13 ng/ml m

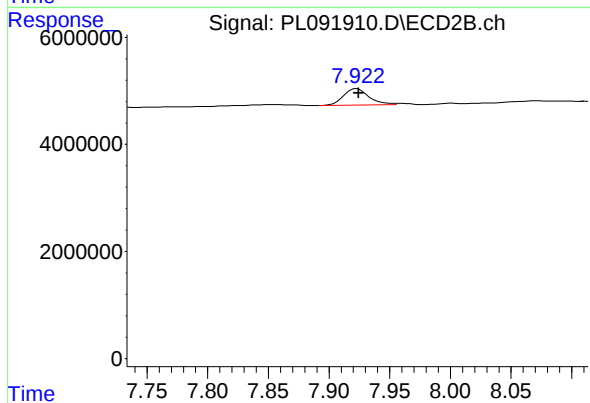

#28 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: -0.003 min
Response: 4538236
Conc: 2.46 ng/ml m