

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092125\
 Data File : PL097292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2025 10:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:17:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	2.823	72503943	109.5E6	16.015	16.653
28)	SA Decachlor...	9.002	7.982	58320157	101.6E6	17.823	17.855
Target Compounds							
8)	B Heptachlo...	5.644	0.000	25578378	0	4.451	N.D. #
13)	MA Dieldrin	0.000	5.416	0	13790492	N.D.	1.687 #
14)	MA Endrin	0.000	5.710	0	14945129	N.D.	1.990 #
18)	B Endrin al...	0.000	6.168	0	11486305	N.D.	2.152 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092125\
Data File : PL097292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2025 10:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:17:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

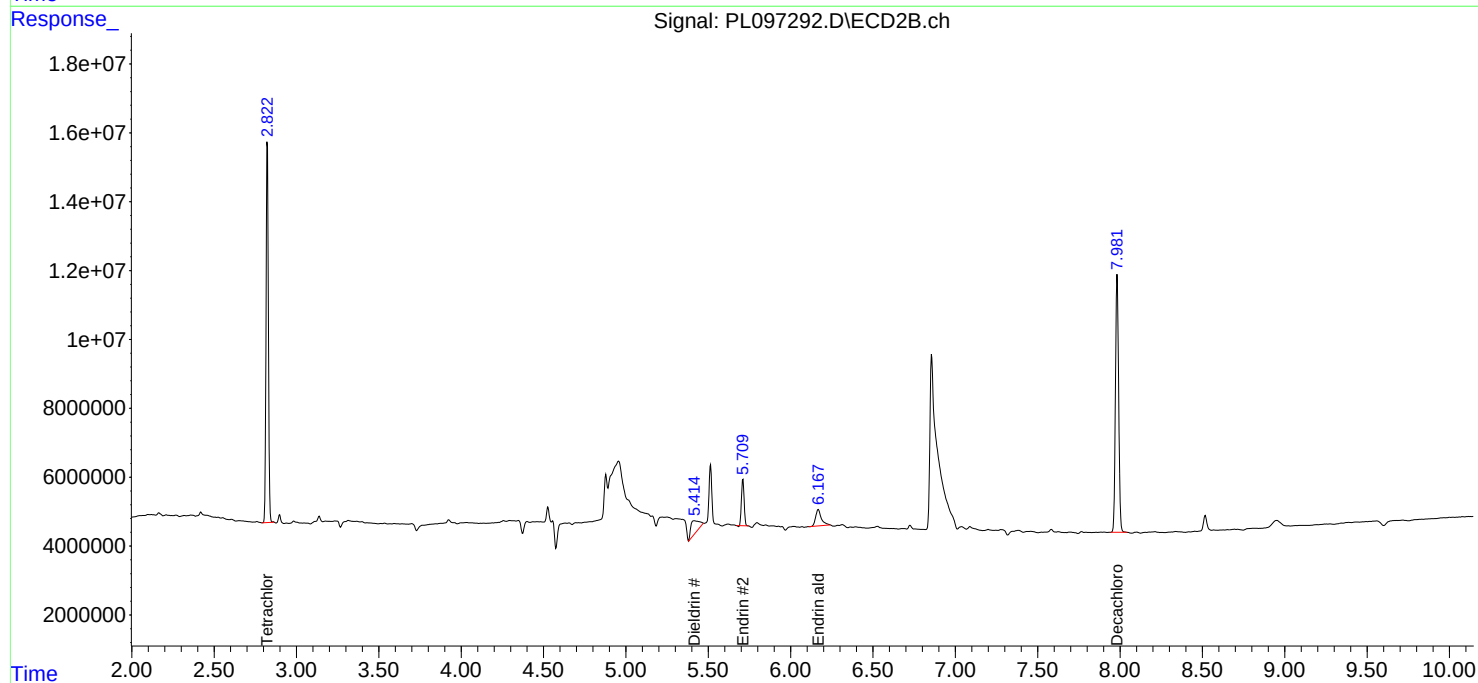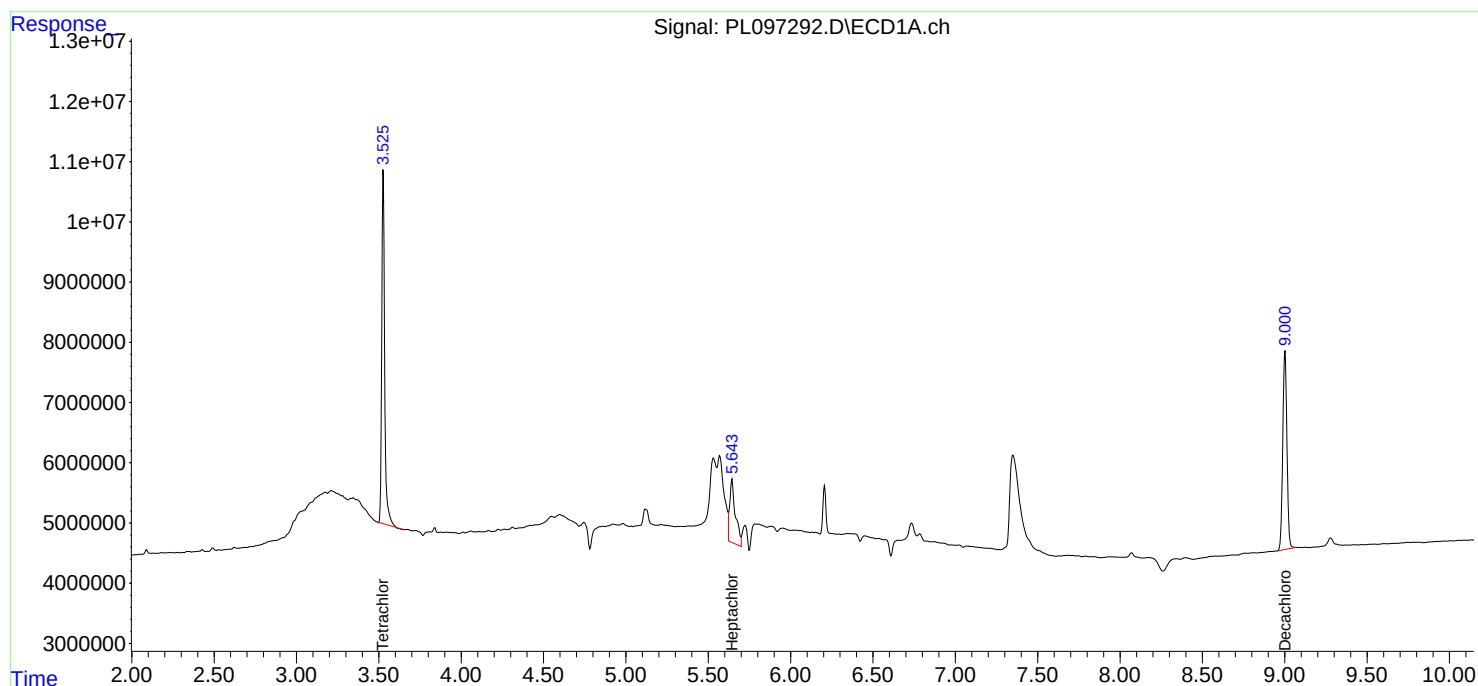


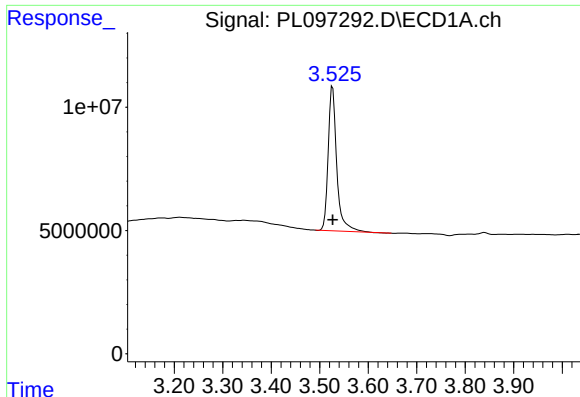

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 72503943
Conc: 16.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

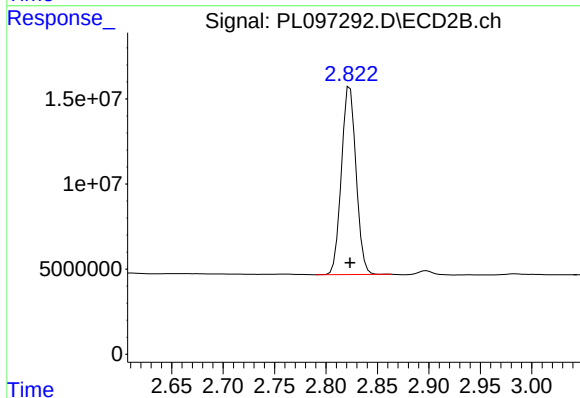


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 109504633
Conc: 16.65 ng/ml

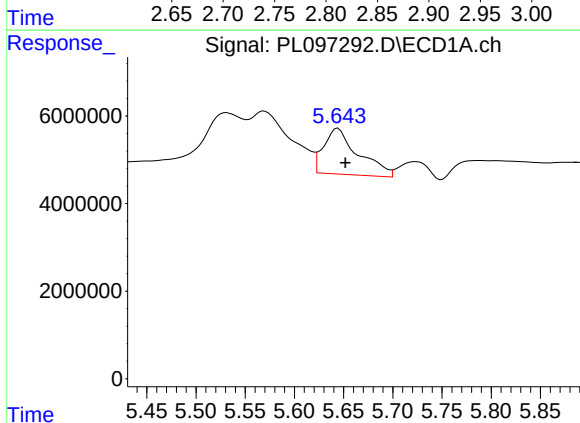


#8 Heptachlor epoxide

R.T.: 5.644 min
Delta R.T.: -0.008 min
Response: 25578378
Conc: 4.45 ng/ml

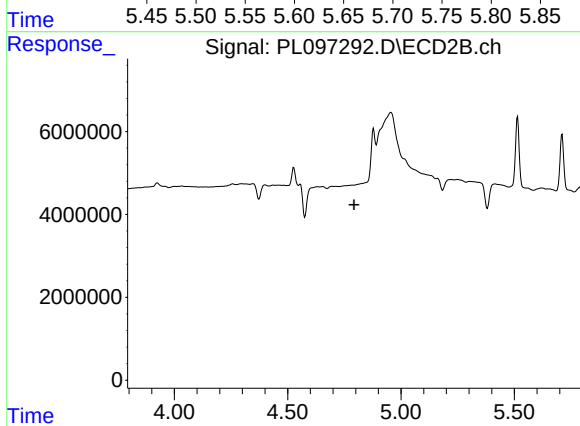

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.793 min
Response: 0
Conc: N.D.

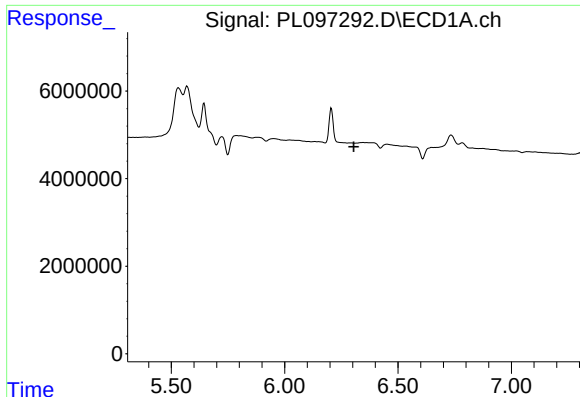

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

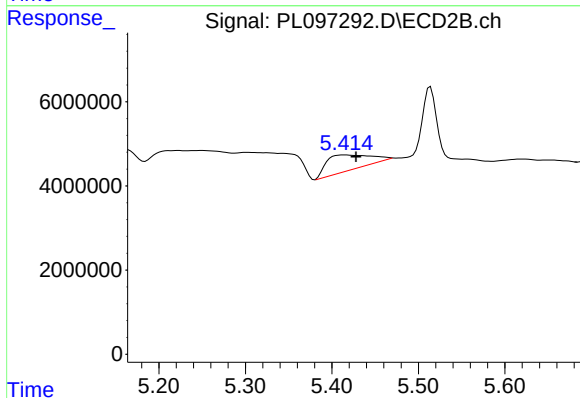


#13 Dieldrin

R.T.: 5.416 min
Delta R.T.: -0.012 min
Response: 13790492
Conc: 1.69 ng/ml

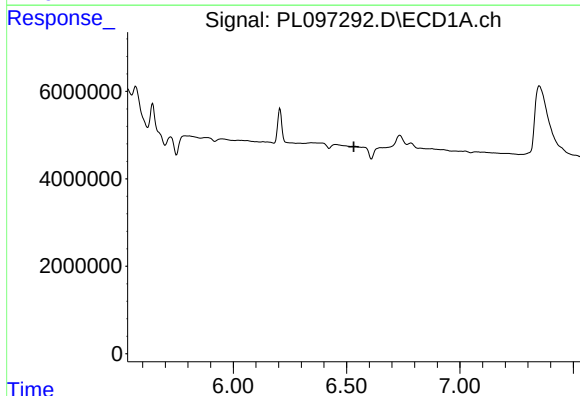


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

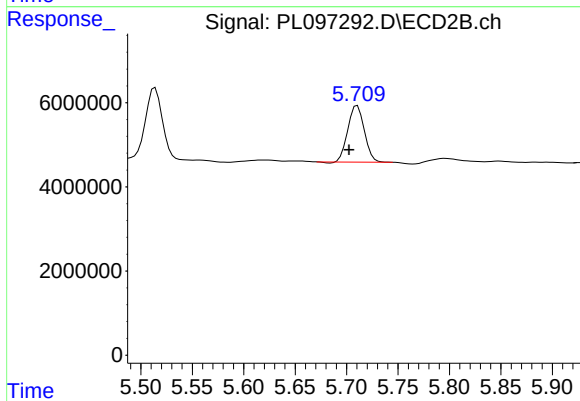

#14 Endrin


R.T.: 5.710 min
Delta R.T.: 0.008 min
Response: 14945129
Conc: 1.99 ng/ml

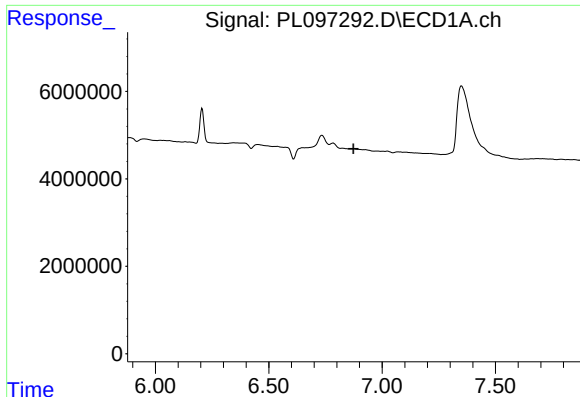

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

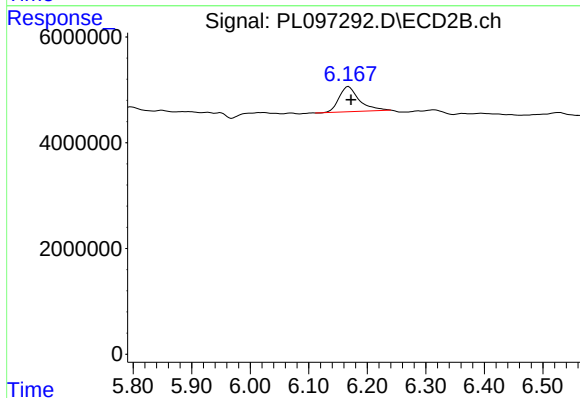


#18 Endrin aldehyde

R.T.: 6.168 min
Delta R.T.: -0.004 min
Response: 11486305
Conc: 2.15 ng/ml

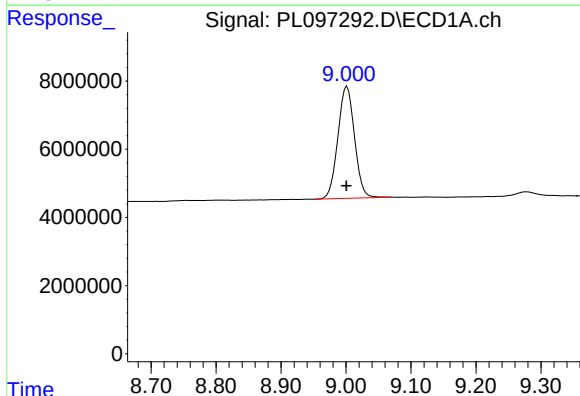

#28 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.000 min
Response: 58320157
Conc: 17.82 ng/ml

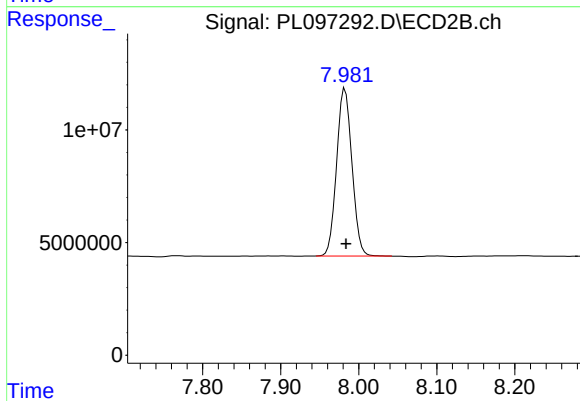

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.002 min
Response: 101623401
Conc: 17.86 ng/ml