

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092218\
 Data File : PL040194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2018 20:39
 Operator : AJ\SJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 05:35:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.249	3.843	156.9E6	67172739	20.628	20.570
28)	SA Decachlor...	7.876	8.796	184.9E6	68349850	20.883	21.362
Target Compounds							
2)	A alpha-BHC	3.672	4.217	116.8E6	44711117	9.718	9.378
3)	MA gamma-BHC...	3.945	4.493	110.2E6	43328907	9.982	9.813
4)	MA Heptachlor	4.200	0.000	49697995	0	4.325	N.D. #
6)	B beta-BHC	4.200	4.656	49697995	20466996	11.309	10.368
7)	B delta-BHC	0.000	4.885	0	16450872	N.D.	3.637 #
14)	MA Endrin	5.705	6.486	508.4E6	164.6E6	51.644	51.572
15)	B Endosulfa...	5.923f	0.000	287.2E6	0	27.641	N.D. #
16)	A 4,4'-DDD	0.000	6.566f	0	106.9E6	N.D.	33.386 #
17)	MA 4,4'-DDT	6.075	6.910	915.0E6	311.5E6	108.233	109.071
20)	A Methoxychlor	6.622	7.367	1145.3E6	393.8E6	244.357	258.540
27)	Chlordane-5	5.923	0.000	287.2E6	0	692.356	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092218\
Data File : PL040194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2018 20:39
Operator : AJ\SJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 05:35:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

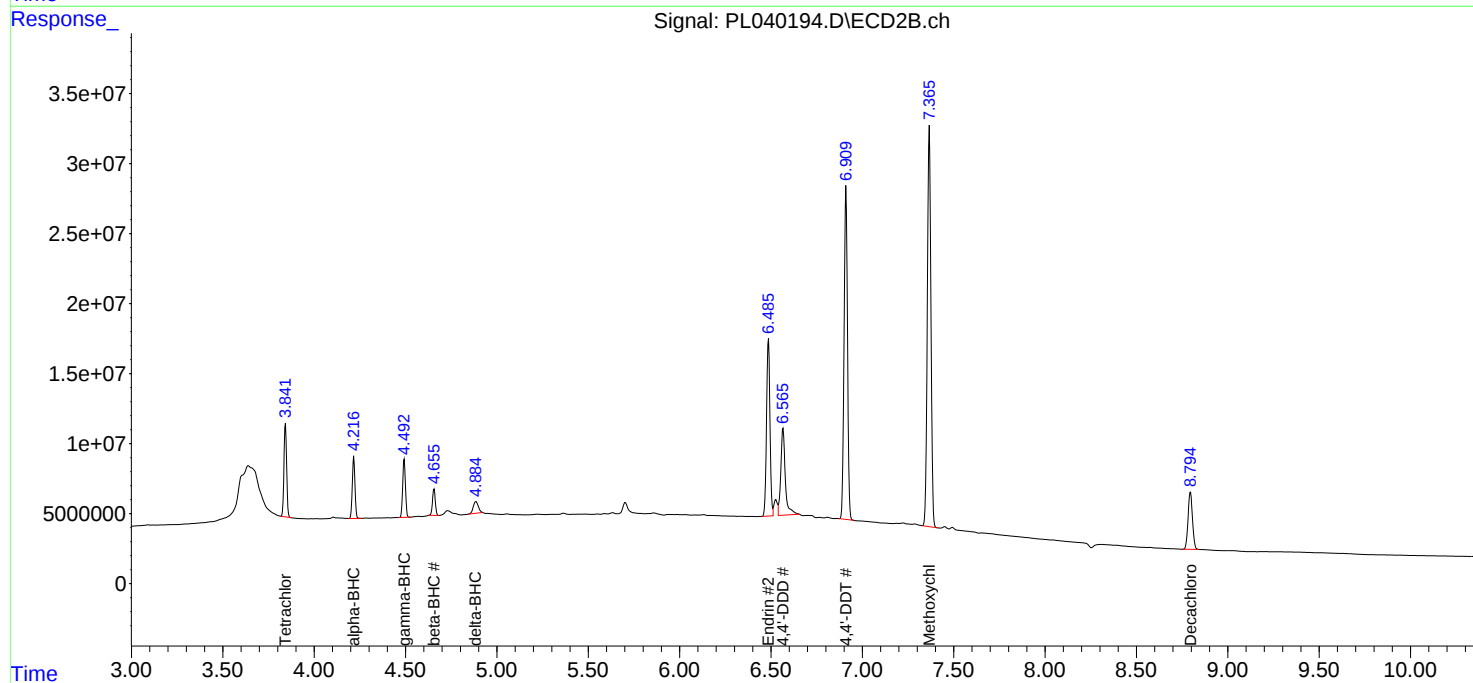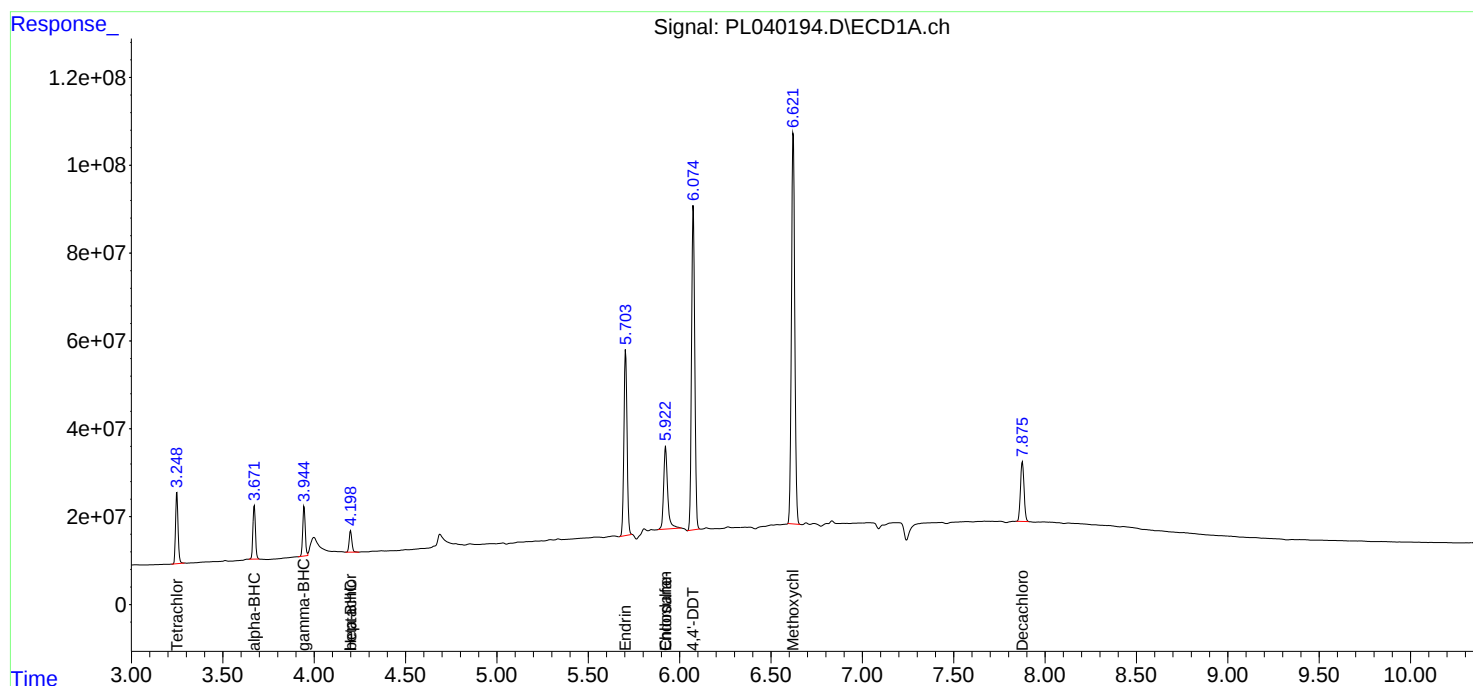


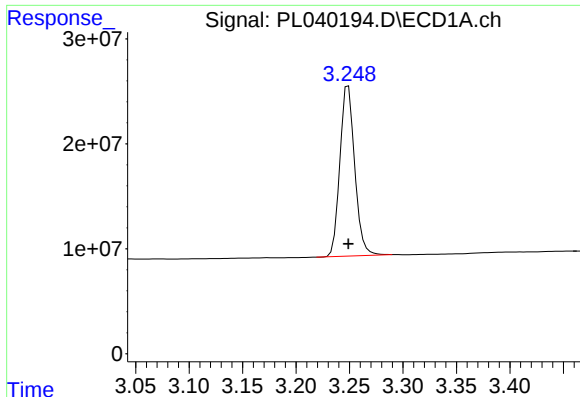

#1 Tetrachloro-m-xylene


R.T.: 3.249 min
Delta R.T.: 0.000 min
Response: 156941122
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

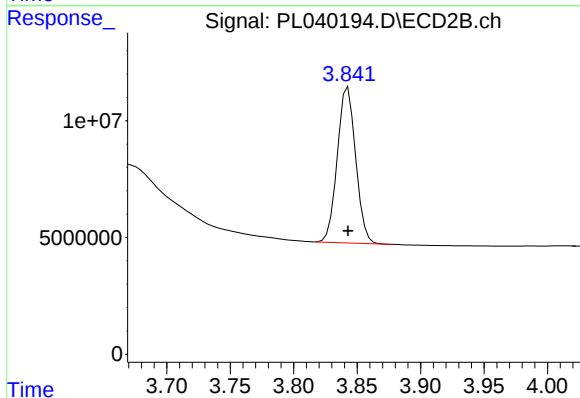


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 67172739
Conc: 20.57 ng/ml

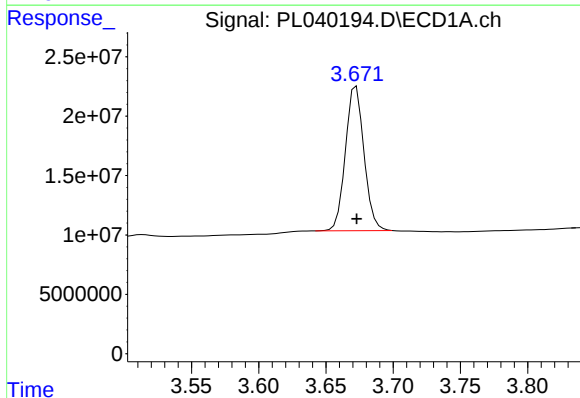


#2 alpha-BHC

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 116754457
Conc: 9.72 ng/ml

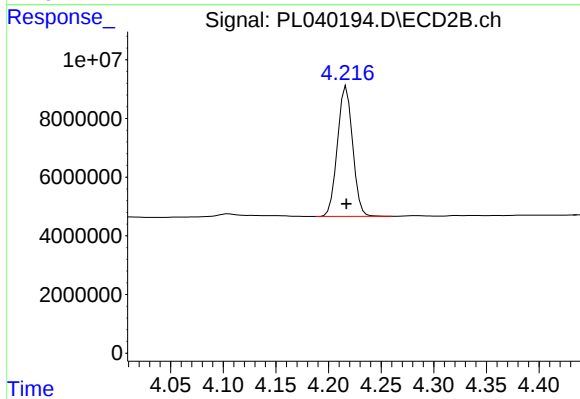

#2 alpha-BHC


R.T.: 4.217 min
Delta R.T.: 0.000 min
Response: 44711117
Conc: 9.38 ng/ml

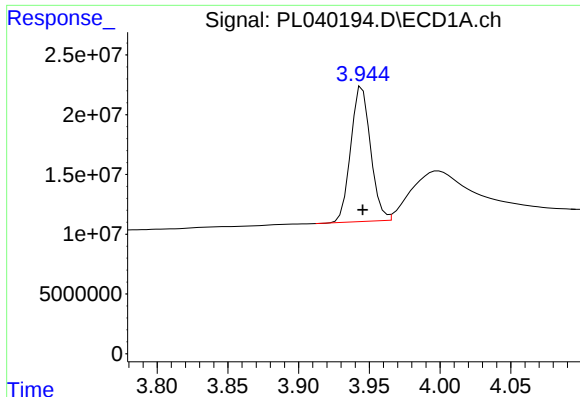

#3 gamma-BHC (Lindane)


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 110168852
Conc: 9.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

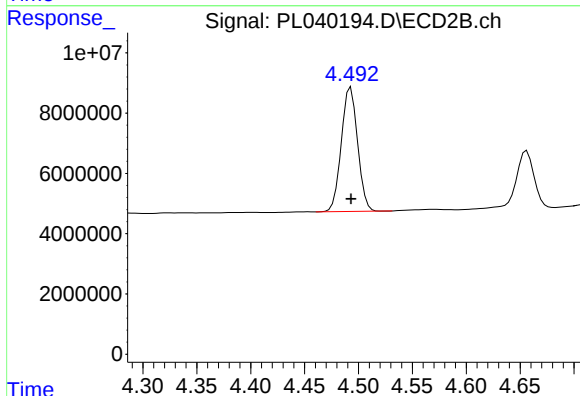


#3 gamma-BHC (Lindane)

R.T.: 4.493 min
Delta R.T.: 0.000 min
Response: 43328907
Conc: 9.81 ng/ml

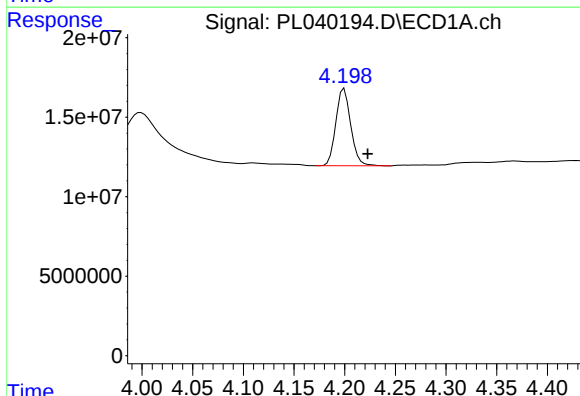


#4 Heptachlor

R.T.: 4.200 min
Delta R.T.: -0.023 min
Response: 49697995
Conc: 4.33 ng/ml

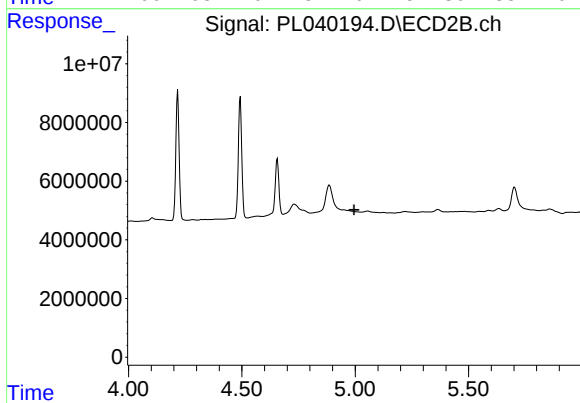

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.995 min
Response: 0
Conc: N.D.

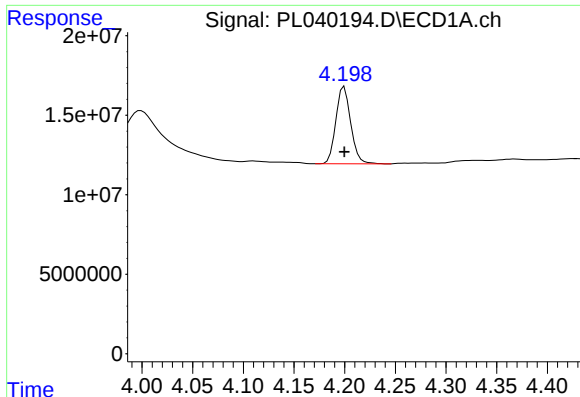

#6 beta-BHC


R.T.: 4.200 min
Delta R.T.: 0.000 min
Response: 49697995
Conc: 11.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

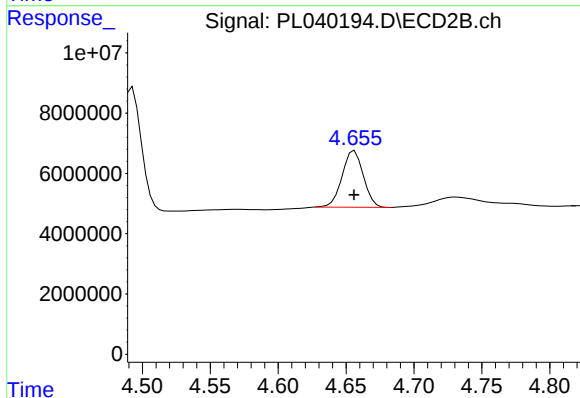


#6 beta-BHC

R.T.: 4.656 min
Delta R.T.: 0.000 min
Response: 20466996
Conc: 10.37 ng/ml

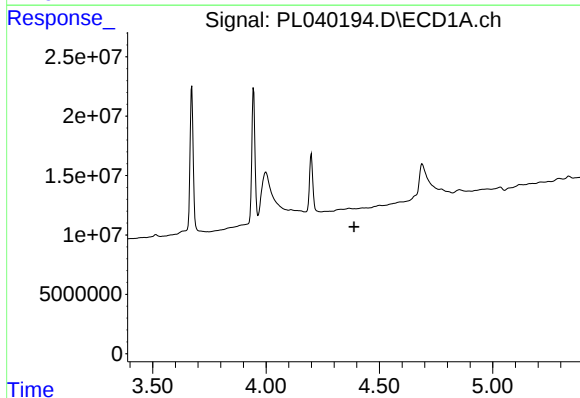


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.389 min
Response: 0
Conc: N.D.

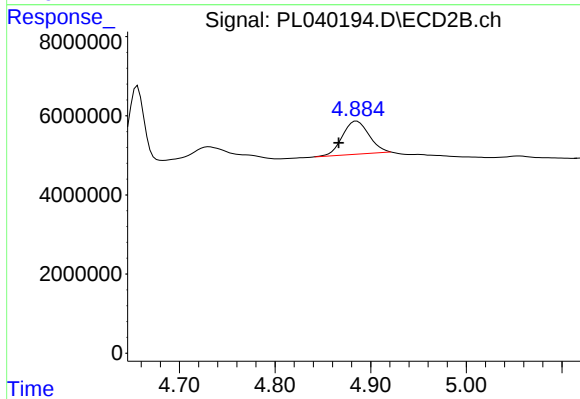

#7 delta-BHC


R.T.: 4.885 min
Delta R.T.: 0.019 min
Response: 16450872
Conc: 3.64 ng/ml

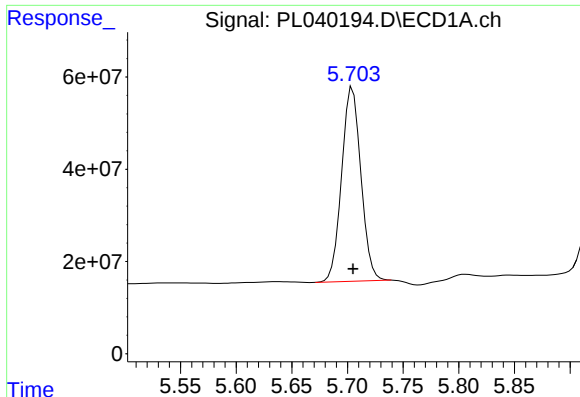

#14 Endrin


R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 508442588
Conc: 51.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

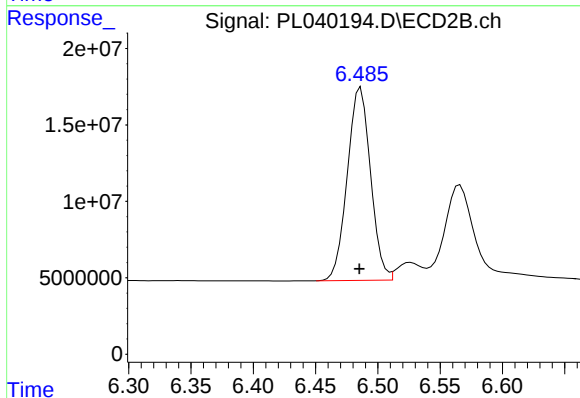


#14 Endrin

R.T.: 6.486 min
Delta R.T.: 0.001 min
Response: 164619286
Conc: 51.57 ng/ml

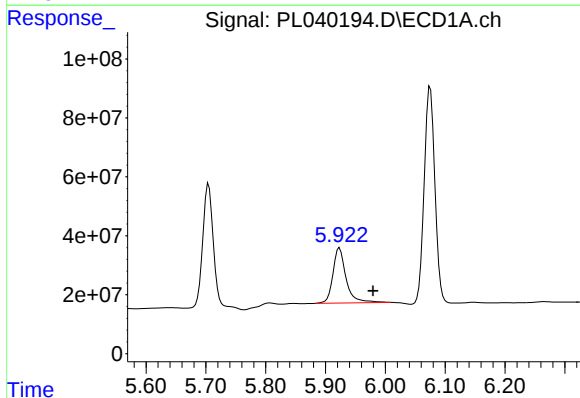


#15 Endosulfan II

R.T.: 5.923 min
Delta R.T.: -0.056 min
Response: 287151617
Conc: 27.64 ng/ml

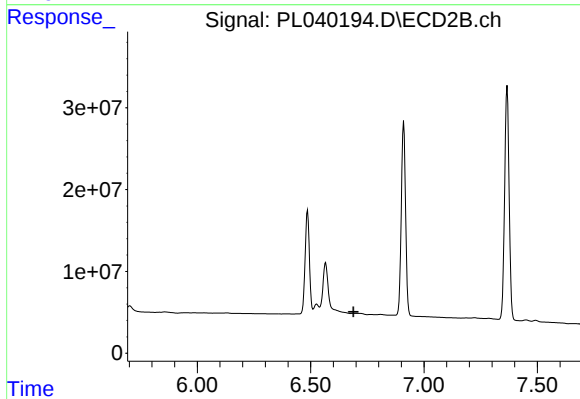

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.690 min
Response: 0
Conc: N.D.

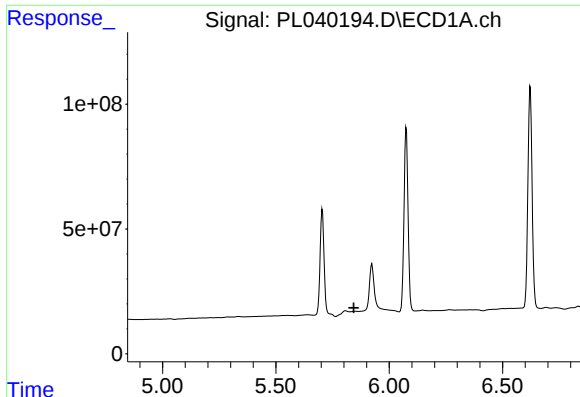

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

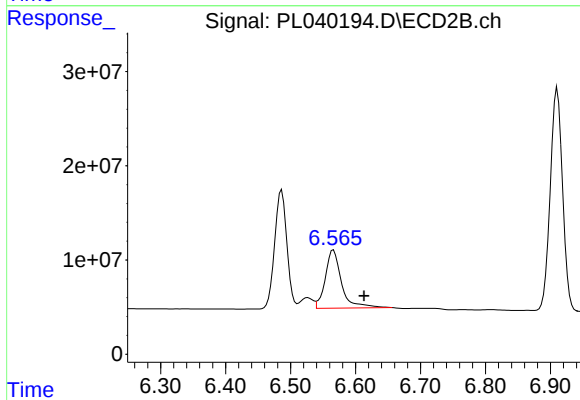


#16 4,4'-DDD

R.T.: 6.566 min
Delta R.T.: -0.047 min
Response: 106921600
Conc: 33.39 ng/ml

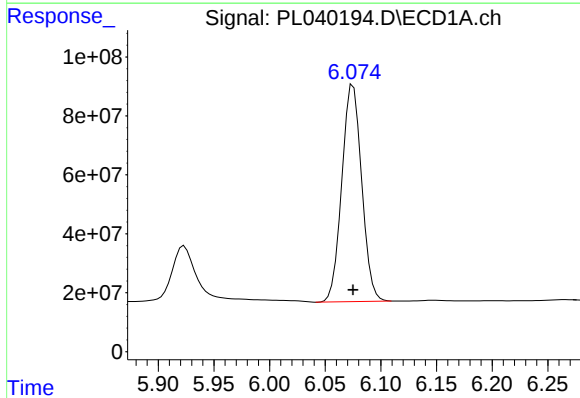


#17 4,4'-DDT

R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 914985957
Conc: 108.23 ng/ml

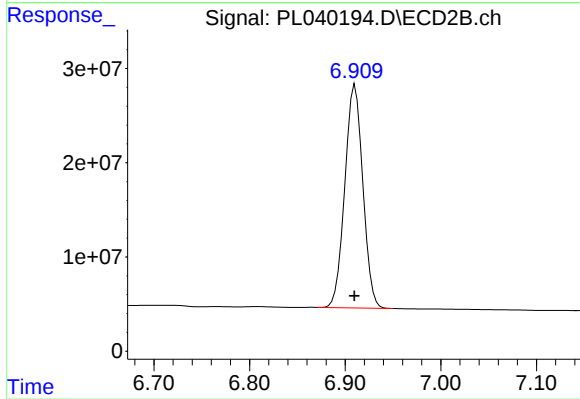

#17 4,4'-DDT


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 311543412
Conc: 109.07 ng/ml

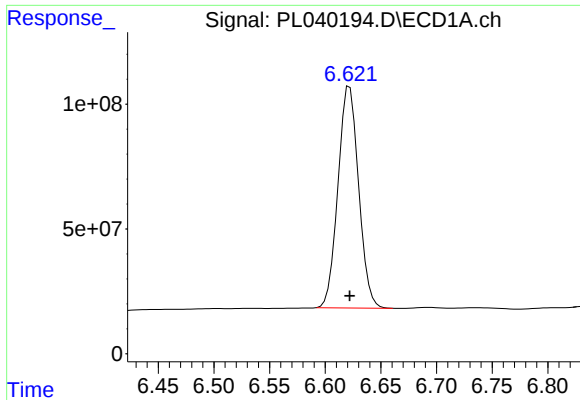

#20 Methoxychlor


R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 1145274529
Conc: 244.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

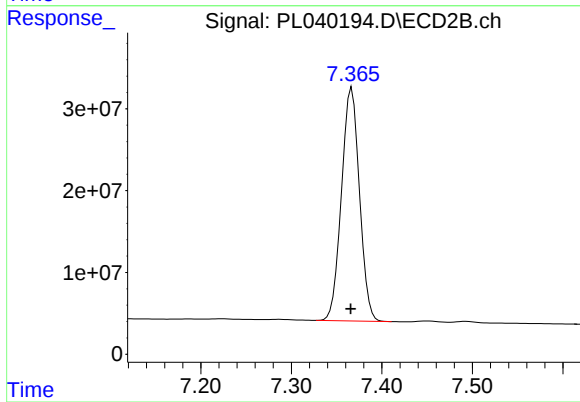


#20 Methoxychlor

R.T.: 7.367 min
Delta R.T.: 0.001 min
Response: 393819681
Conc: 258.54 ng/ml

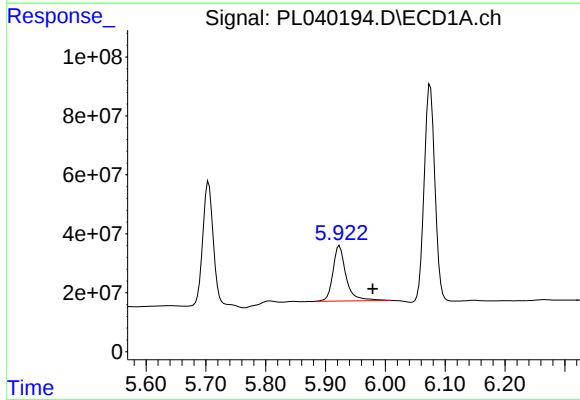


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: -0.056 min
Response: 287151617
Conc: 692.36 ng/ml

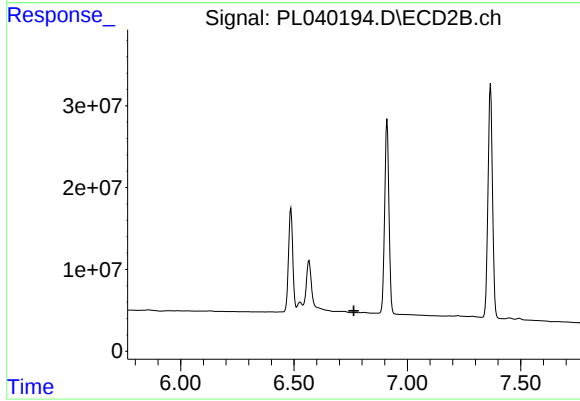

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

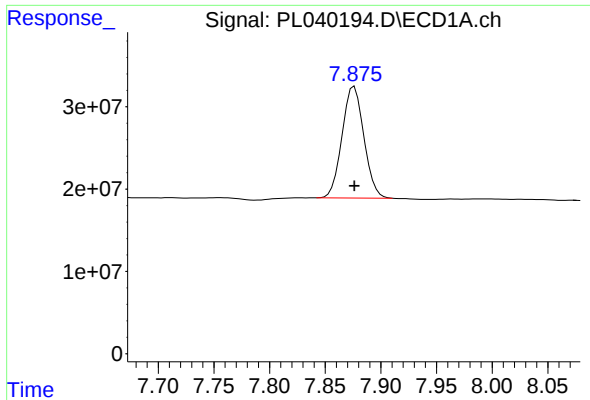

#28 Decachlorobiphenyl


R.T.: 7.876 min

Delta R.T.: 0.000 min

Response: 184935198

Conc: 20.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

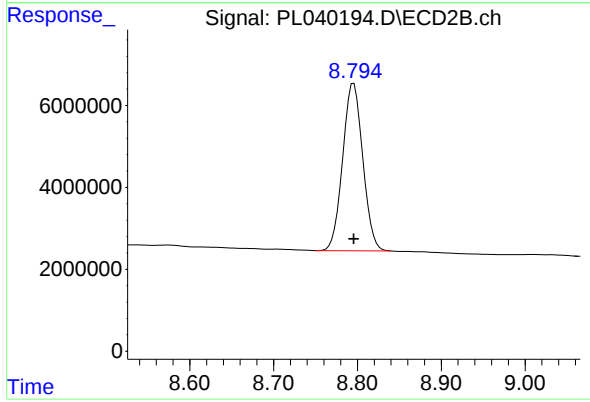

#28 Decachlorobiphenyl

R.T.: 8.796 min

Delta R.T.: 0.000 min

Response: 68349850

Conc: 21.36 ng/ml