

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092218\
 Data File : PL040201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2018 22:18
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Manual Integrations
 APPROVED

Sohil
 9/24/2018 12:00:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 05:22:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.249	3.843	795.7E6	326.8E6	99.495	99.489
28)	SA Decachlor...	7.877	8.796	844.1E6	295.3E6	98.105	97.092
Target Compounds							
23)	Chlordane-1	4.078	4.812	370.7E6	158.4E6	1009.565	1004.261
24)	Chlordane-2	4.563	5.270	384.1E6	159.0E6	984.377	983.344
25)	Chlordane-3	5.110	5.904	1214.1E6	544.2E6	949.575m	1002.766
26)	Chlordane-4	5.166	5.978	1151.1E6	638.9E6	986.603	995.302
27)	Chlordane-5	5.981	6.764	399.0E6	120.2E6	984.875	1003.123

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092218\
Data File : PL040201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2018 22:18
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000


Manual Integrations
APPROVED

Sohil
9/24/2018 12:00:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 05:22:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

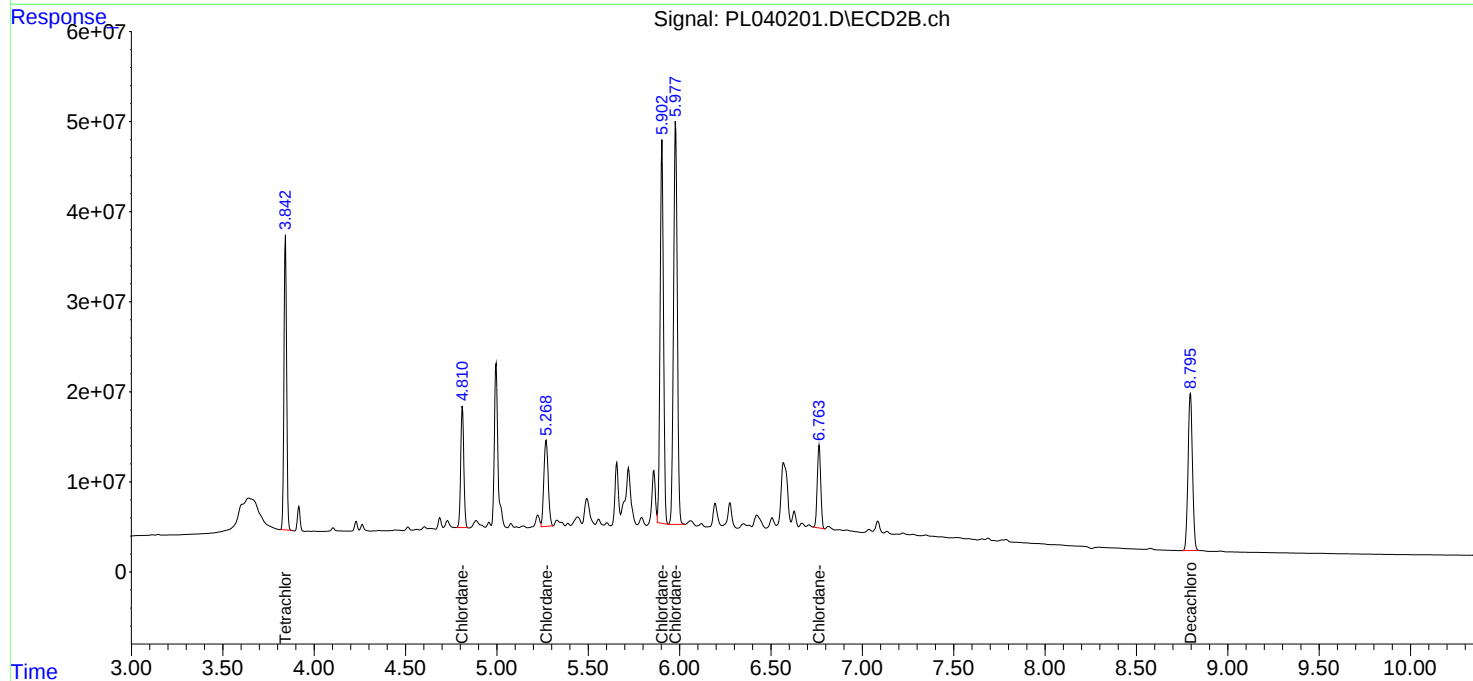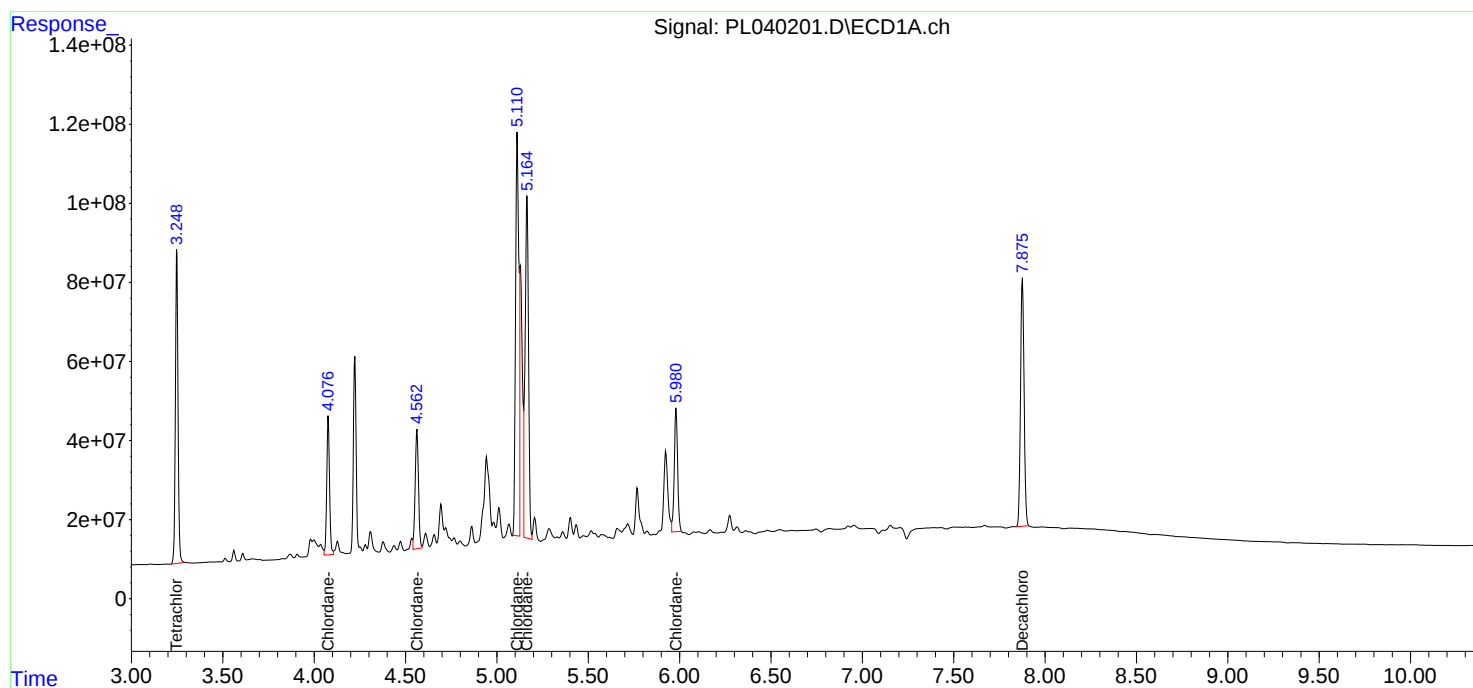

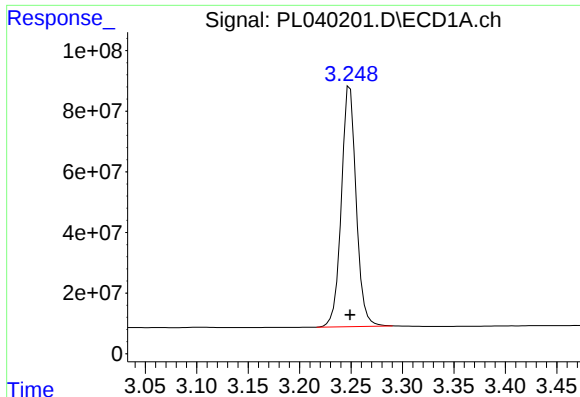


#1 Tetrachloro-m-xylene

R.T.: 3.249 min
Delta R.T.: 0.000 min
Response: 795682121
Conc: 99.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000


Manual Integrations
APPROVED

Sohil
9/24/2018 12:00:27 PM

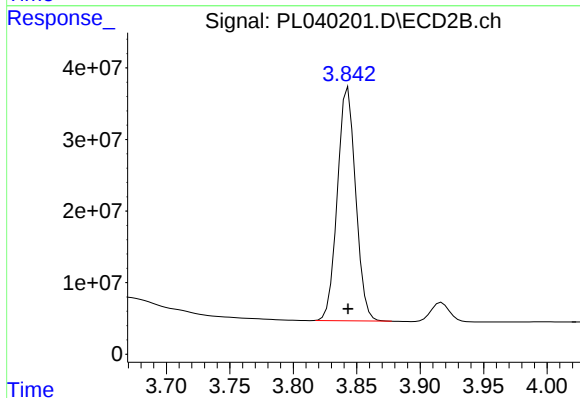


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 326794184
Conc: 99.49 ng/ml

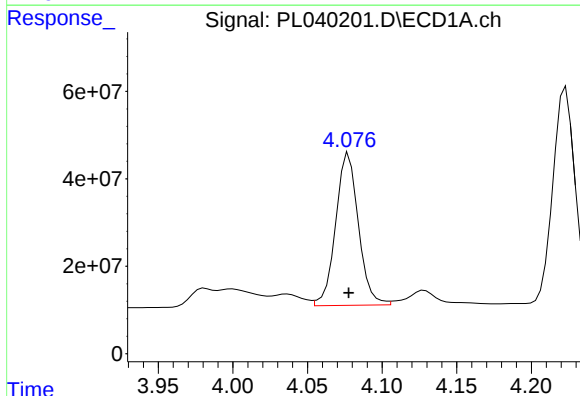


#23 Chlordane-1

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 370739194
Conc: 1009.56 ng/ml

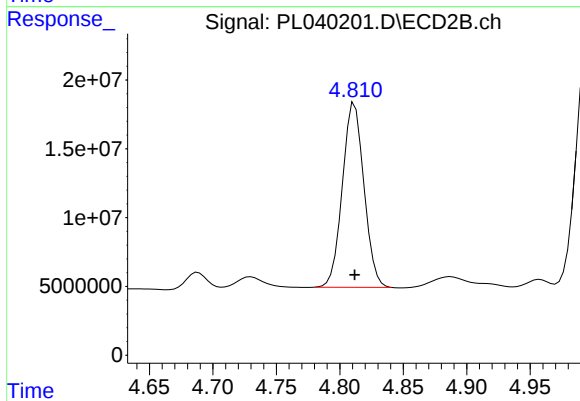

#23 Chlordane-1

R.T.: 4.812 min
Delta R.T.: 0.000 min
Response: 158396425
Conc: 1004.26 ng/ml

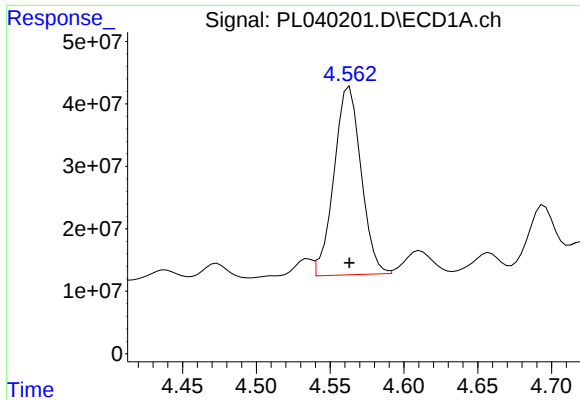


#24 Chlordane-2

R.T.: 4.563 min
Delta R.T.: 0.000 min
Response: 384134515
Conc: 984.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000


Manual Integrations
APPROVED

Sohil
9/24/2018 12:00:27 PM

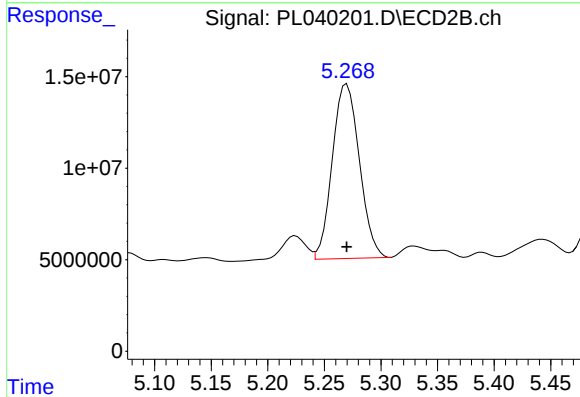


#24 Chlordane-2

R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 158952514
Conc: 983.34 ng/ml

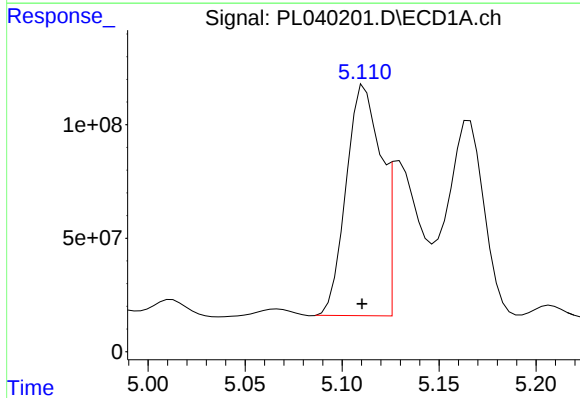


#25 Chlordane-3

R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 1214064255
Conc: 949.57 ng/ml m

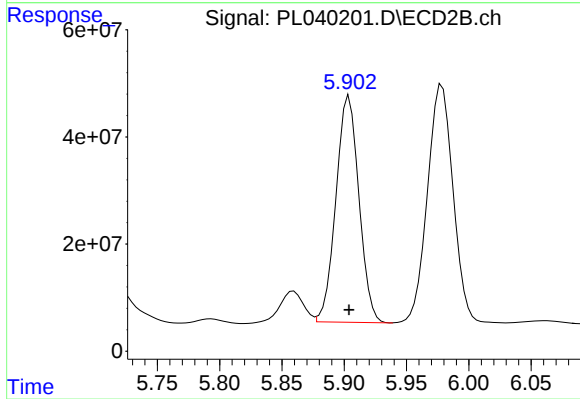

#25 Chlordane-3

R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 544155815
Conc: 1002.77 ng/ml

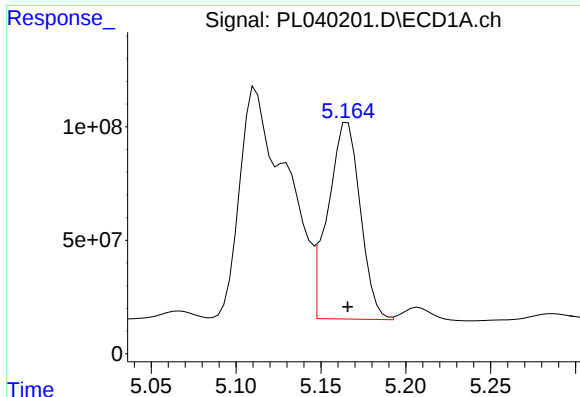


#26 Chlordane-4

R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 1151073877
Conc: 986.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000


Manual Integrations
APPROVED

Sohil
9/24/2018 12:00:27 PM

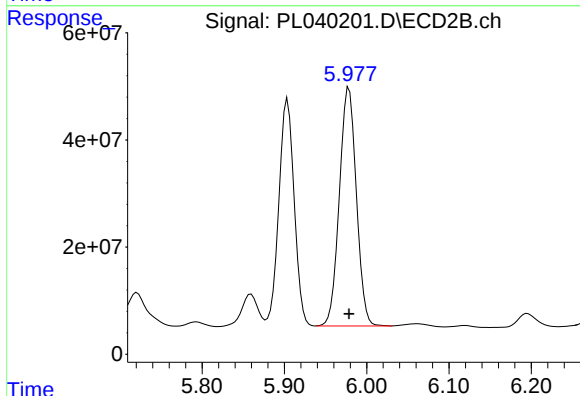


#26 Chlordane-4

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 638910110
Conc: 995.30 ng/ml

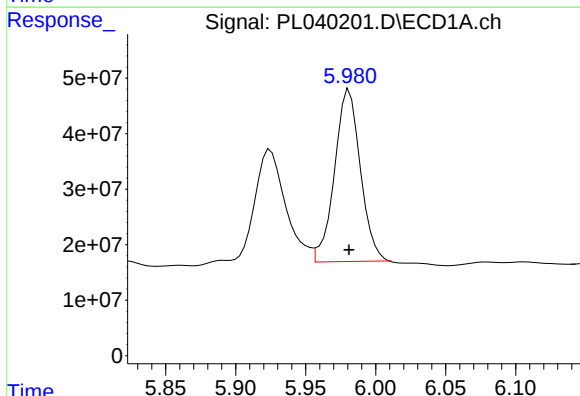


#27 Chlordane-5

R.T.: 5.981 min
Delta R.T.: 0.000 min
Response: 399031343
Conc: 984.87 ng/ml

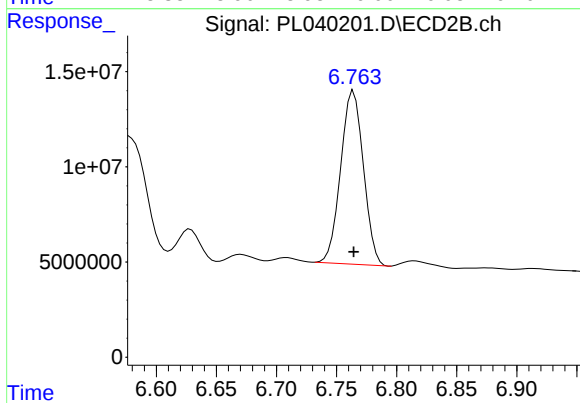

#27 Chlordane-5

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 120248570
Conc: 1003.12 ng/ml

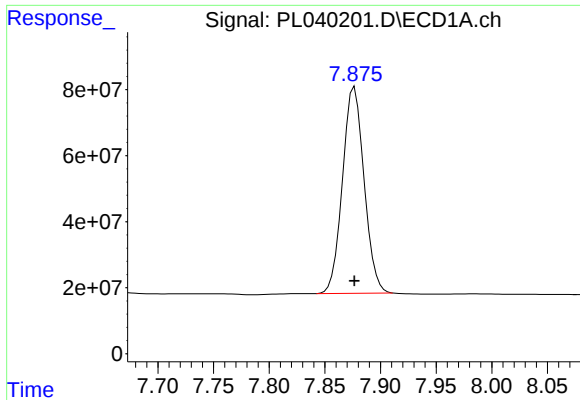

#28 Decachlorobiphenyl

R.T.: 7.877 min

Delta R.T.: 0.000 min


Response: 844059462

Conc: 98.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Manual Integrations
APPROVED

Sohil
9/24/2018 12:00:27 PM

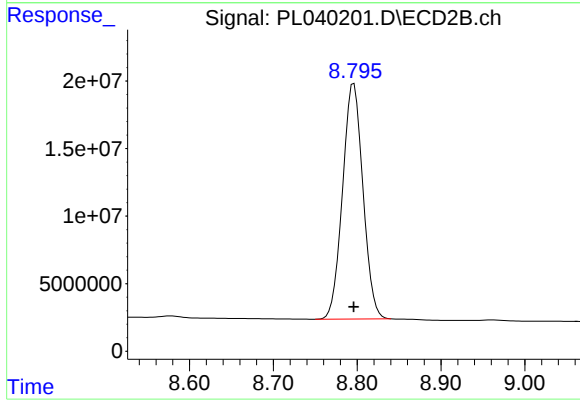

#28 Decachlorobiphenyl

R.T.: 8.796 min

Delta R.T.: 0.000 min

Response: 295332461

Conc: 97.09 ng/ml