

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092218\
 Data File : PL040202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2018 22:33
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 05:24:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.249	3.844	602.7E6	246.8E6	75.241	75.100
28)	SA Decachlor...	7.877	8.796	645.5E6	226.4E6	75.020	74.627
Target Compounds							
23)	Chlordane-1	4.078	4.812	286.8E6	118.3E6	770.334	750.198
24)	Chlordane-2	4.564	5.269	291.1E6	121.0E6	747.313	748.839
25)	Chlordane-3	5.111	5.904	937.6E6	407.5E6	760.904	750.682
26)	Chlordane-4	5.166	5.979	876.6E6	483.0E6	750.892	751.603
27)	Chlordane-5	5.981	6.765	304.0E6	89463150	750.189	747.535



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092218\
Data File : PL040202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2018 22:33
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 05:24:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

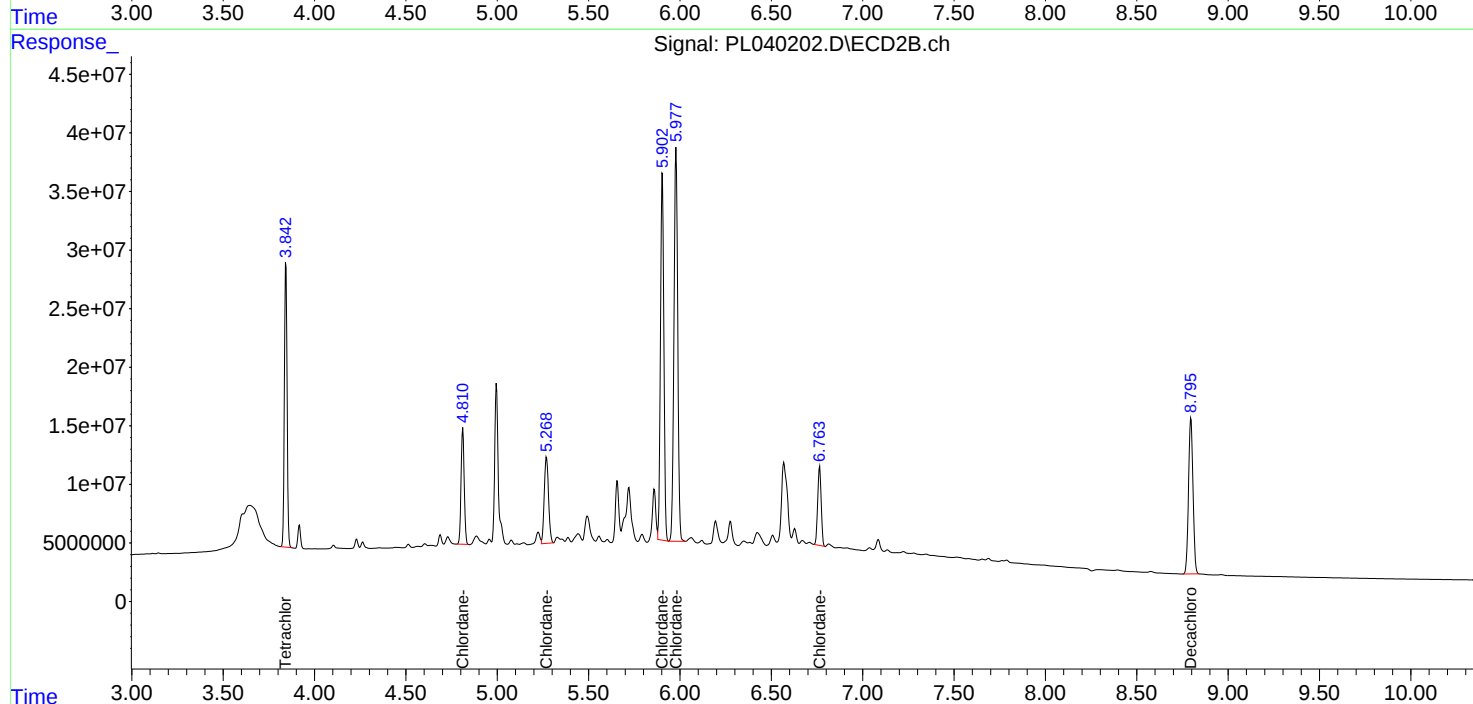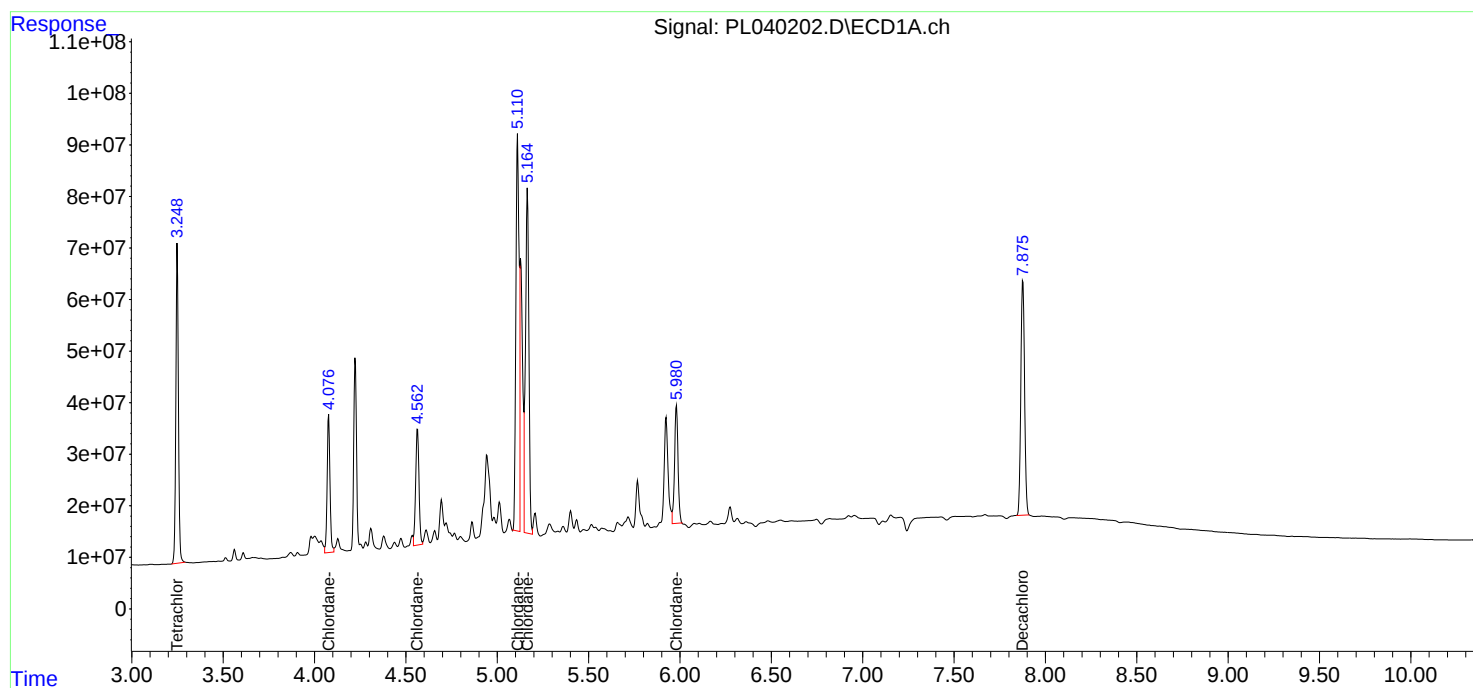


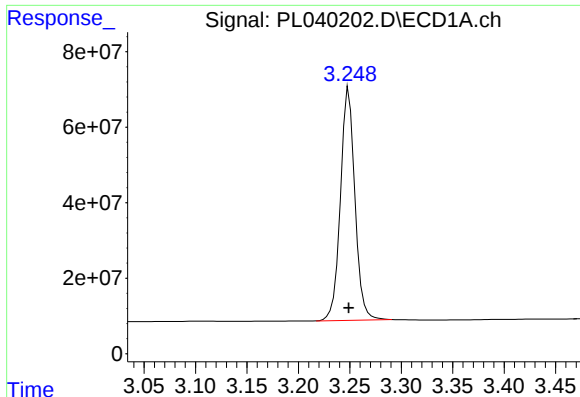

#1 Tetrachloro-m-xylene


R.T.: 3.249 min
Delta R.T.: 0.000 min
Response: 602690068
Conc: 75.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

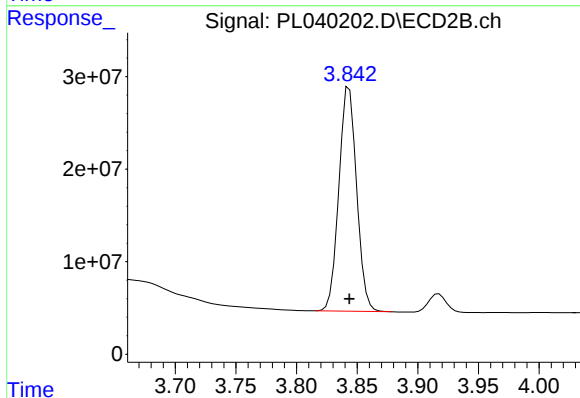


#1 Tetrachloro-m-xylene

R.T.: 3.844 min
Delta R.T.: 0.000 min
Response: 246844873
Conc: 75.10 ng/ml

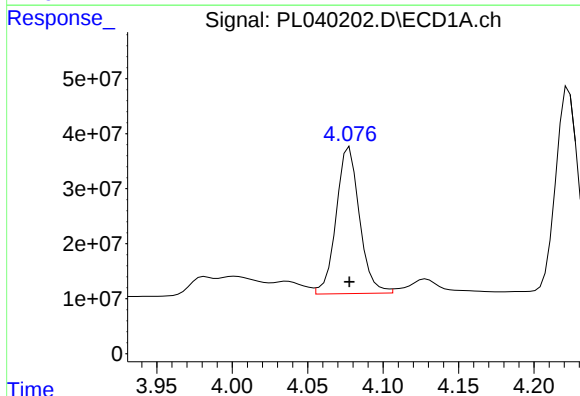


#23 Chlordane-1

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 286774813
Conc: 770.33 ng/ml

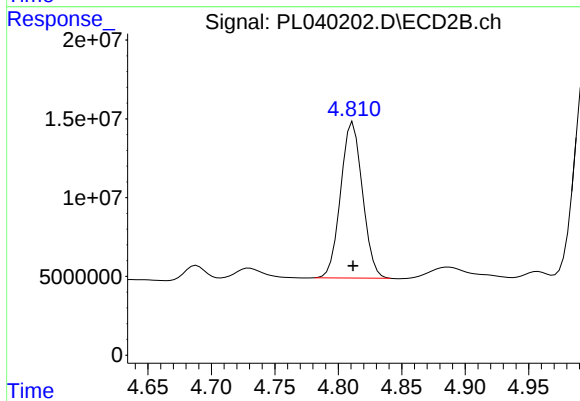

#23 Chlordane-1


R.T.: 4.812 min
Delta R.T.: 0.000 min
Response: 118340180
Conc: 750.20 ng/ml

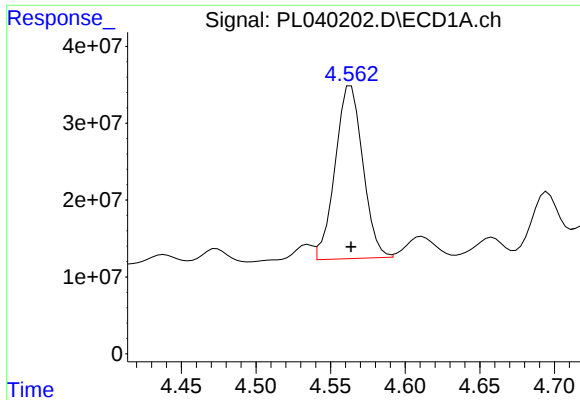

#24 Chlordane-2


R.T.: 4.564 min
Delta R.T.: 0.000 min
Response: 291103302
Conc: 747.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

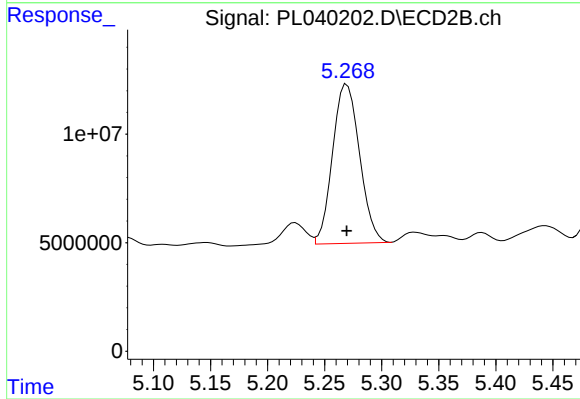


#24 Chlordane-2

R.T.: 5.269 min
Delta R.T.: 0.000 min
Response: 120952530
Conc: 748.84 ng/ml

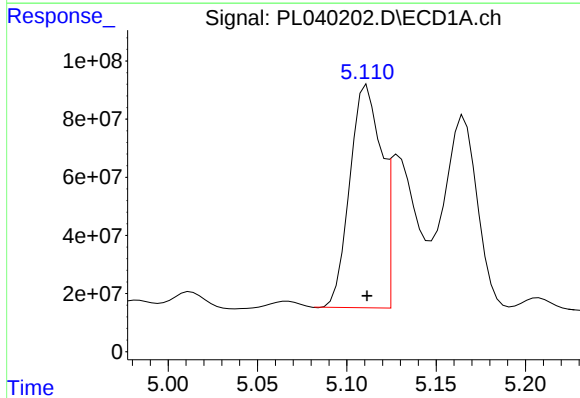


#25 Chlordane-3

R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 937554776
Conc: 760.90 ng/ml

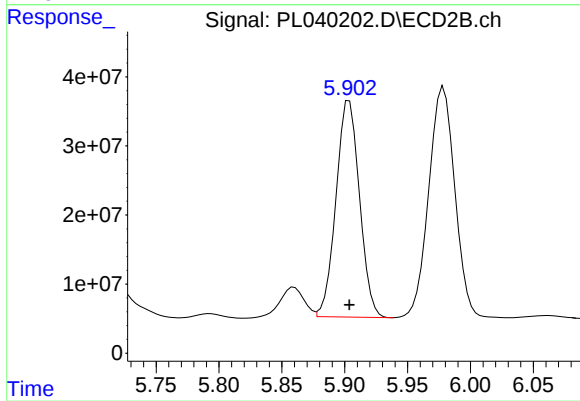

#25 Chlordane-3


R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 407546775
Conc: 750.68 ng/ml

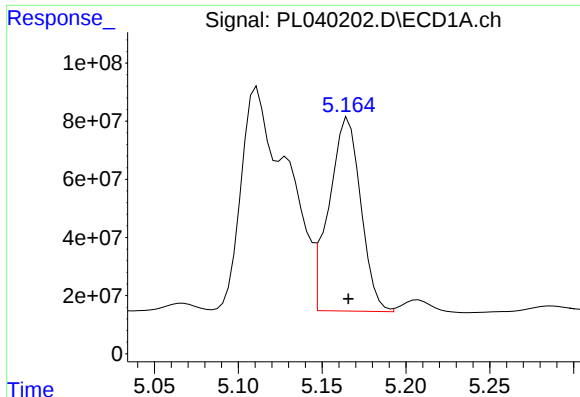

#26 Chlordane-4


R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 876590475
Conc: 750.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

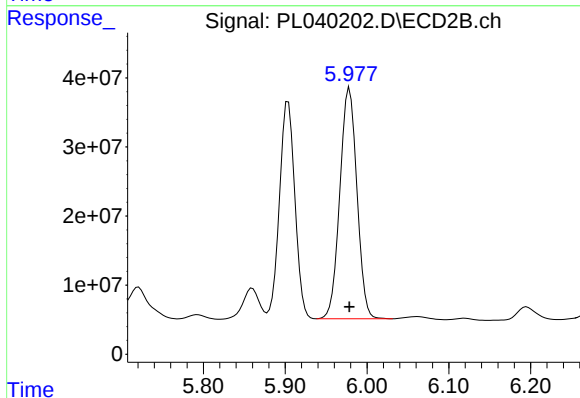


#26 Chlordane-4

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 482989678
Conc: 751.60 ng/ml

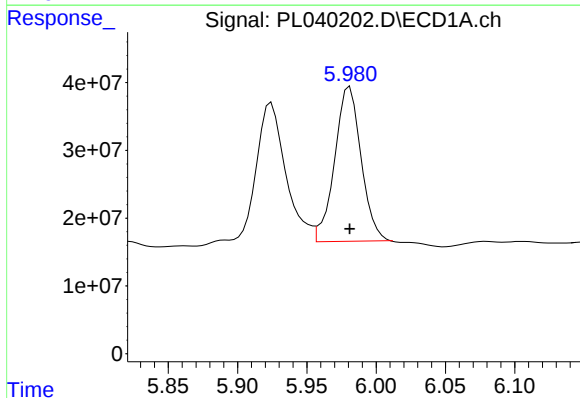


#27 Chlordane-5

R.T.: 5.981 min
Delta R.T.: 0.000 min
Response: 303984220
Conc: 750.19 ng/ml

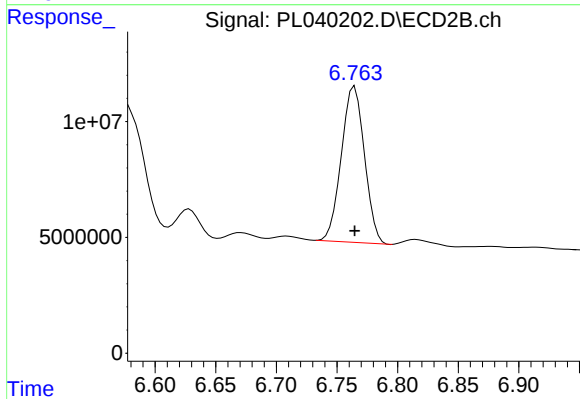

#27 Chlordane-5

R.T.: 6.765 min
Delta R.T.: 0.000 min
Response: 89463150
Conc: 747.54 ng/ml

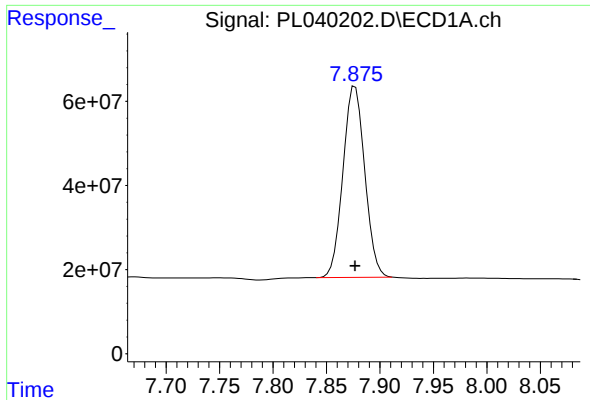

#28 Decachlorobiphenyl


R.T.: 7.877 min

Delta R.T.: 0.000 min

Response: 645526346

Conc: 75.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

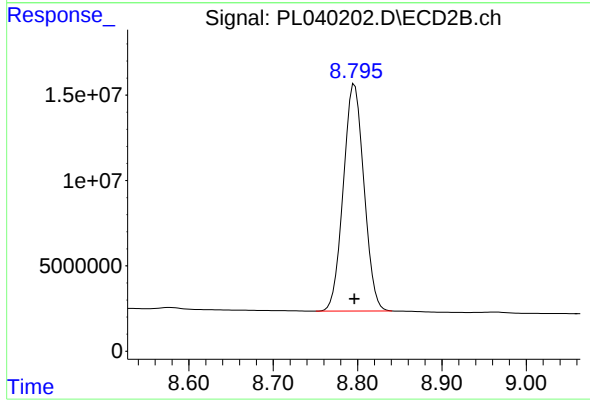

#28 Decachlorobiphenyl

R.T.: 8.796 min

Delta R.T.: 0.000 min

Response: 226433804

Conc: 74.63 ng/ml