

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092220\
 Data File : PL061649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2020 13:55
 Operator : DD\AJ
 Sample : L4099-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 17:29:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	31166414	50847764	18.071	16.531
28)	SA Decachlor...	8.208	9.094	14460450	20476690	8.668	8.660
Target Compounds							
2)	A alpha-BHC	0.000	4.422f	0	13871300	N.D.	3.004 #
3)	MA gamma-BHC...	4.183	0.000	2346937	0	1.028	N.D. #
9)	A Endosulfan I	5.528f	0.000	25609630	0	14.886	N.D. #
10)	B gamma-Chl...	0.000	6.117	0	7485555	N.D.	2.171 #
11)	B alpha-Chl...	0.000	6.194	0	9232884	N.D.	2.653 #
13)	MA Dieldrin	5.751	0.000	5958617	0	3.320	N.D. #
17)	MA 4,4'-DDT	0.000	7.143	0	3371758	N.D.	1.347 #
23)	Chlordane-1	4.329	0.000	2612557	0	49.804	N.D. #
25)	Chlordane-3	0.000	6.117	0	7485555	N.D.	17.329 #
26)	Chlordane-4	0.000	6.194	0	9232884	N.D.	17.638 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092220\
Data File : PL061649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2020 13:55
Operator : DD\AJ
Sample : L4099-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 17:29:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

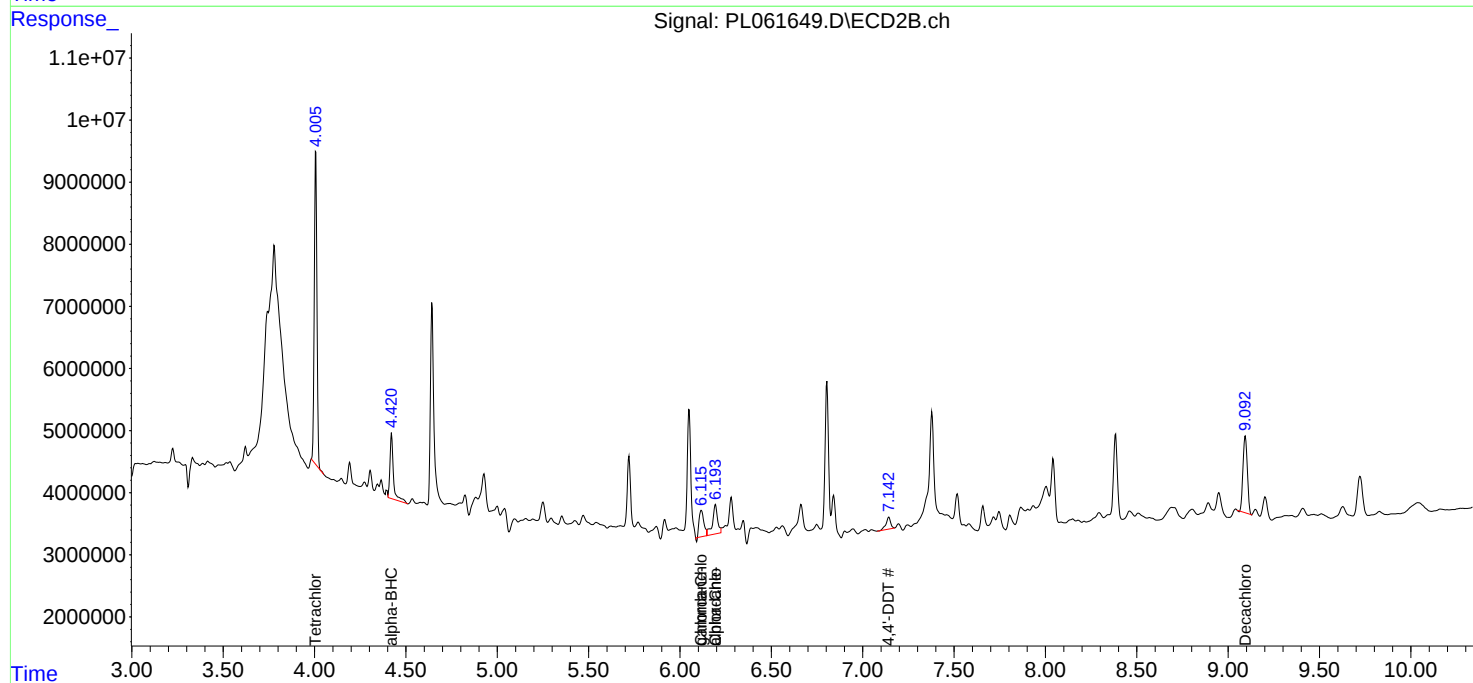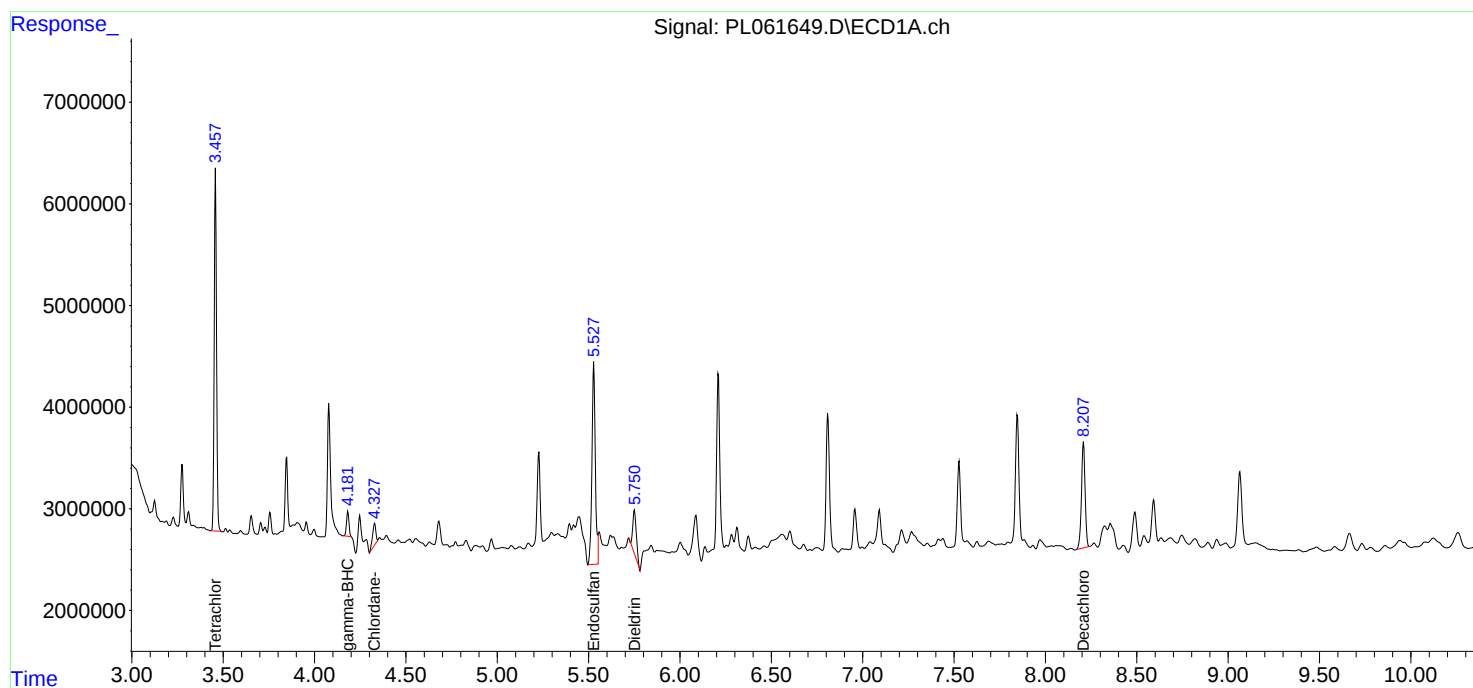


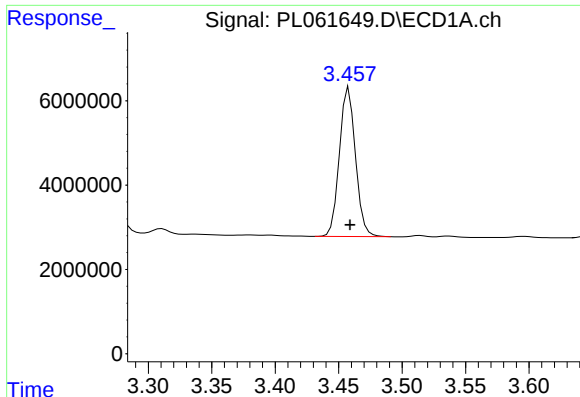

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 31166414
Conc: 18.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

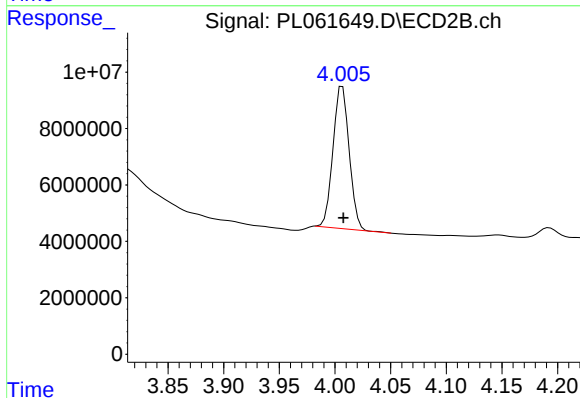


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 50847764
Conc: 16.53 ng/ml

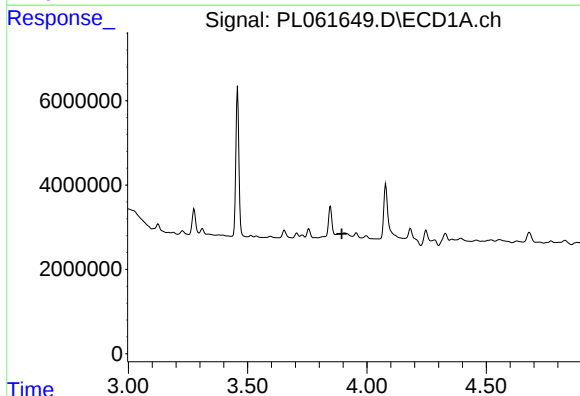


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.895 min
Response: 0
Conc: N.D.

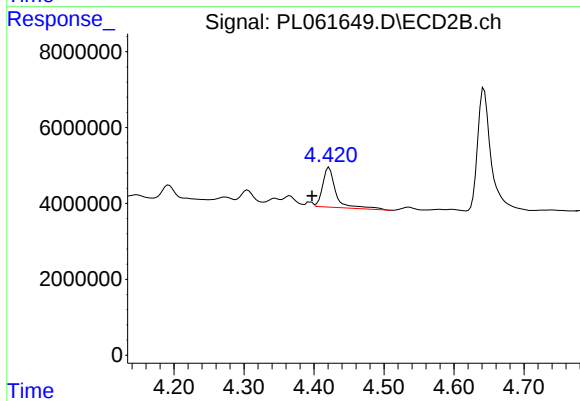

#2 alpha-BHC


R.T.: 4.422 min
Delta R.T.: 0.025 min
Response: 13871300
Conc: 3.00 ng/ml

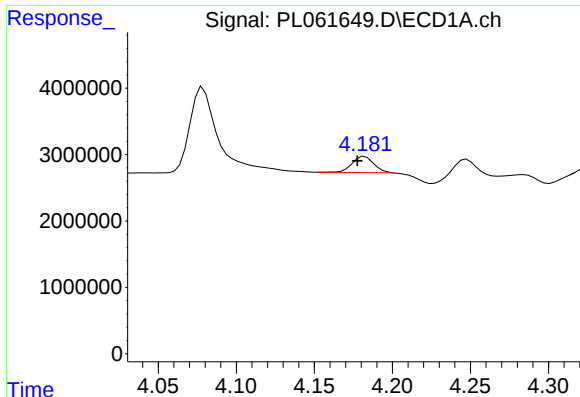

#3 gamma-BHC (Lindane)


R.T.: 4.183 min
Delta R.T.: 0.005 min
Response: 2346937
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

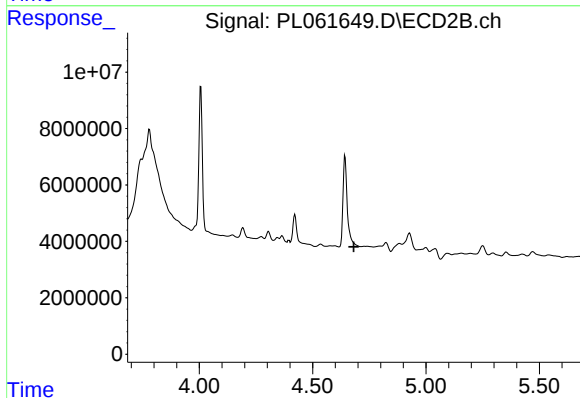


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.682 min
Response: 0
Conc: N.D.

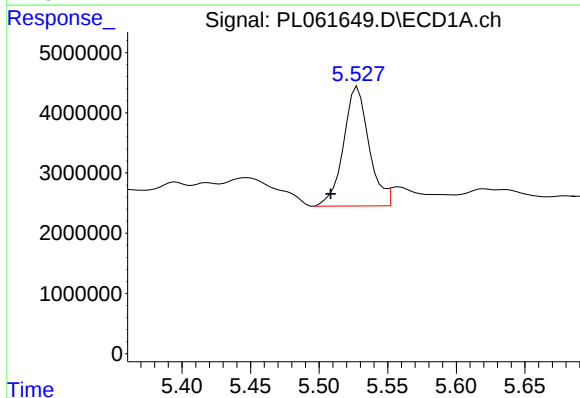


#9 Endosulfan I

R.T.: 5.528 min
Delta R.T.: 0.020 min
Response: 25609630
Conc: 14.89 ng/ml

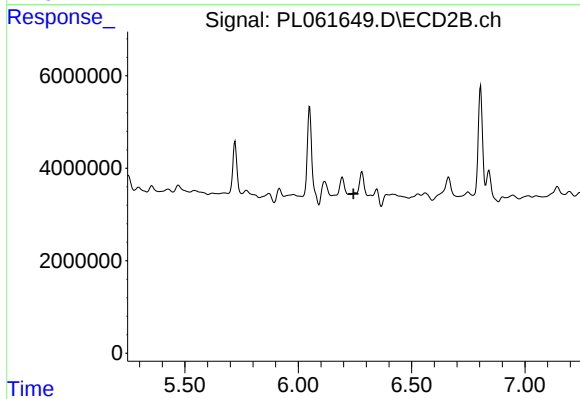

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

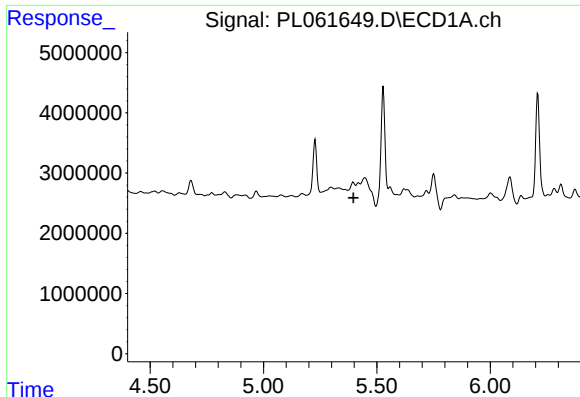

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

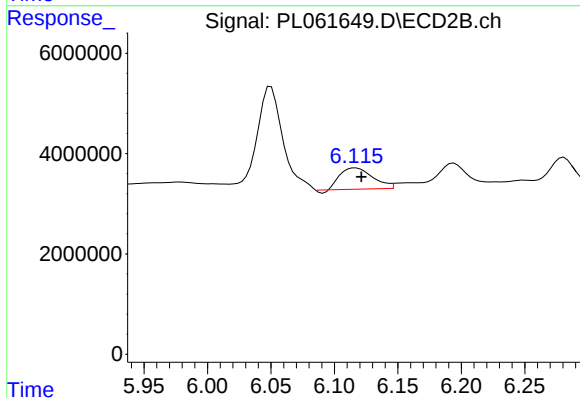


#10 gamma-Chlordane

R.T.: 6.117 min
Delta R.T.: -0.004 min
Response: 748555
Conc: 2.17 ng/ml

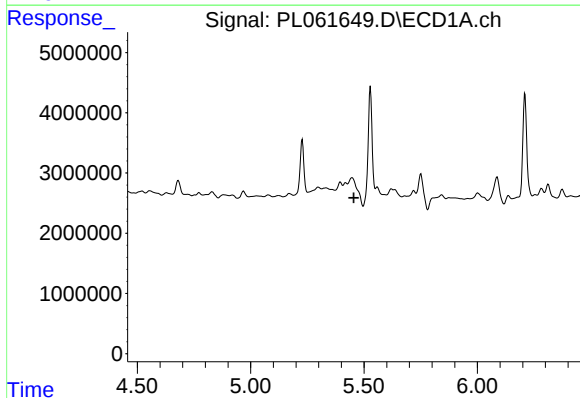


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

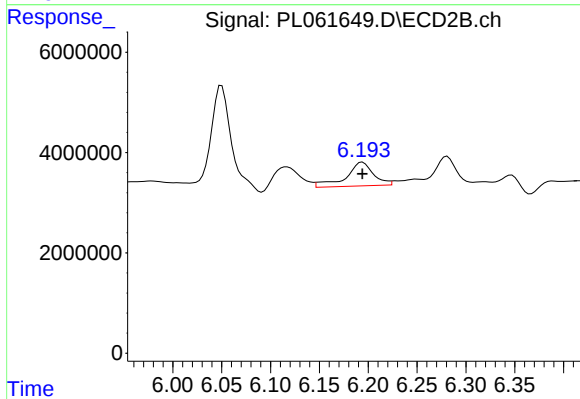

#11 alpha-Chlordane


R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 9232884
Conc: 2.65 ng/ml

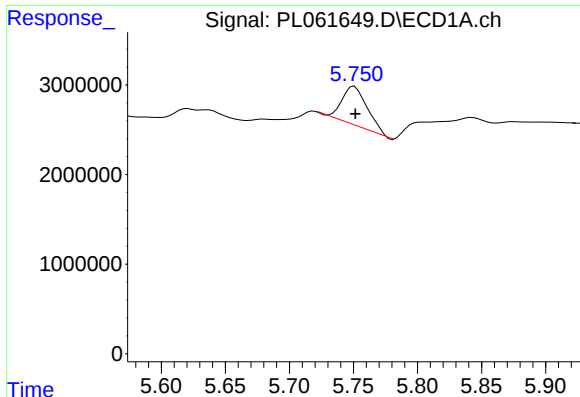

#13 Dieldrin


R.T.: 5.751 min
Delta R.T.: 0.000 min
Response: 5958617
Conc: 3.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

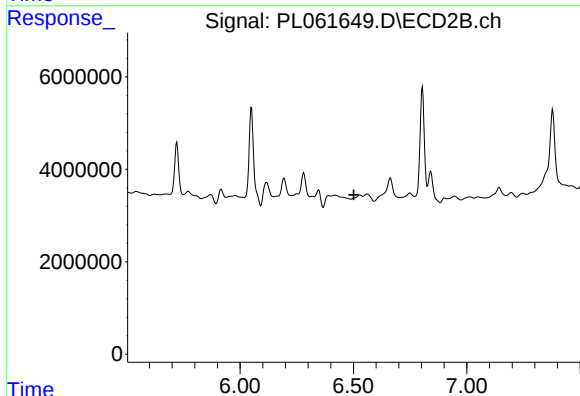


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.502 min
Response: 0
Conc: N.D.

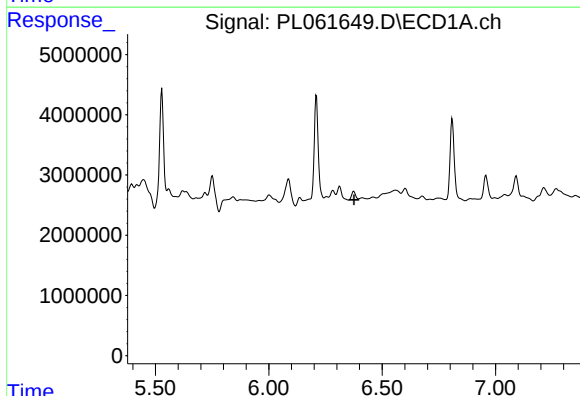


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.376 min
Response: 0
Conc: N.D.

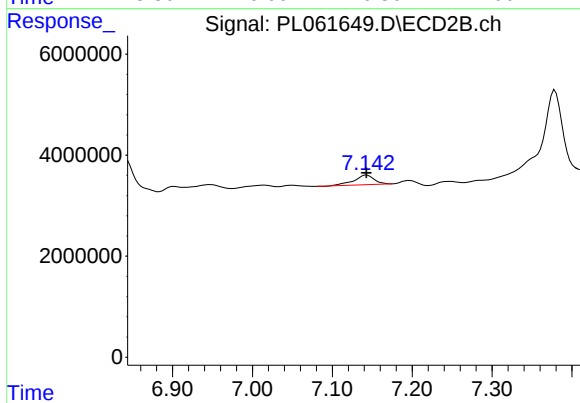

#17 4,4'-DDT


R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 3371758
Conc: 1.35 ng/ml

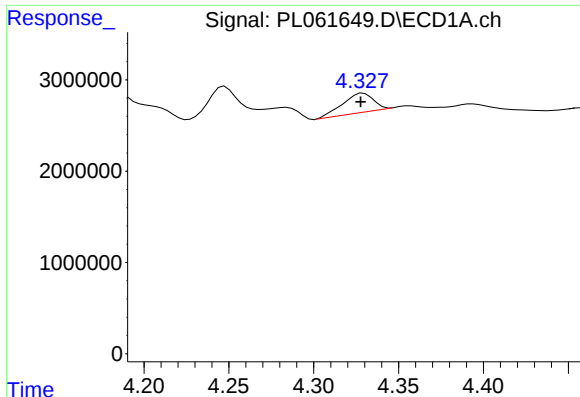

#23 Chlordane-1


R.T.: 4.329 min
Delta R.T.: 0.002 min
Response: 2612557
Conc: 49.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

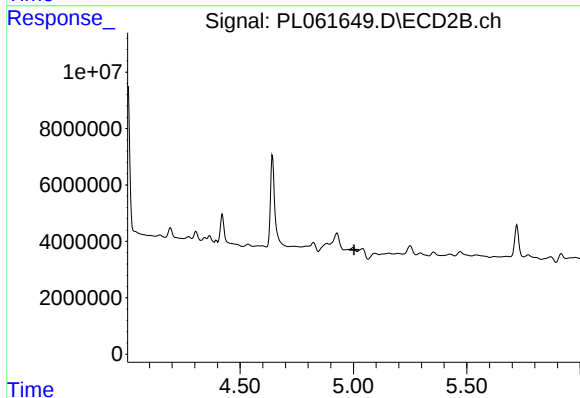


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

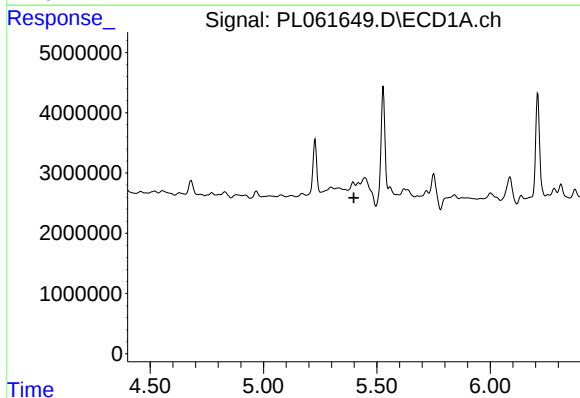


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

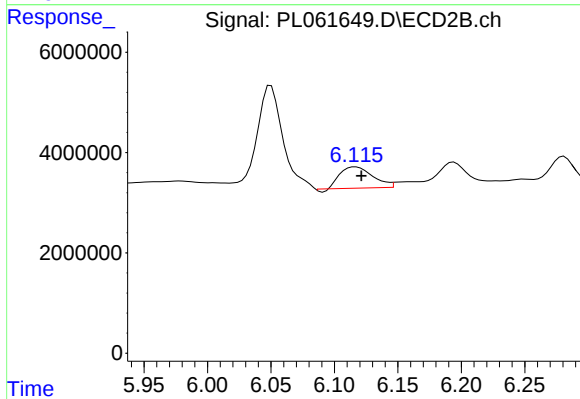

#25 Chlordane-3


R.T.: 6.117 min
Delta R.T.: -0.004 min
Response: 7485555
Conc: 17.33 ng/ml

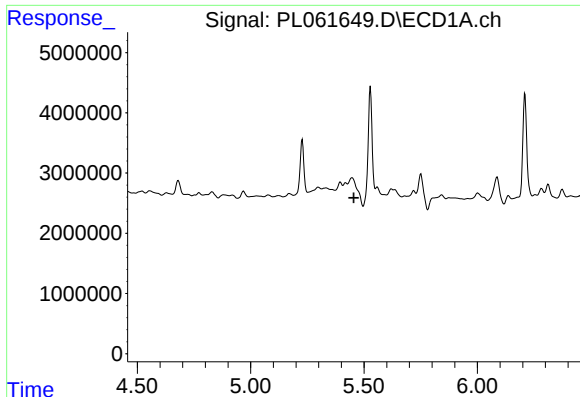

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

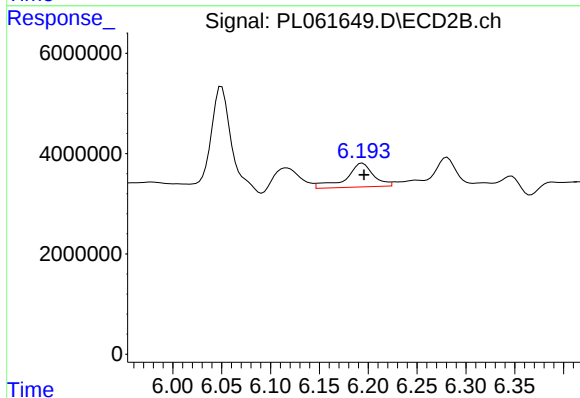


#26 Chlordane-4

R.T.: 6.194 min
Delta R.T.: -0.002 min
Response: 9232884
Conc: 17.64 ng/ml

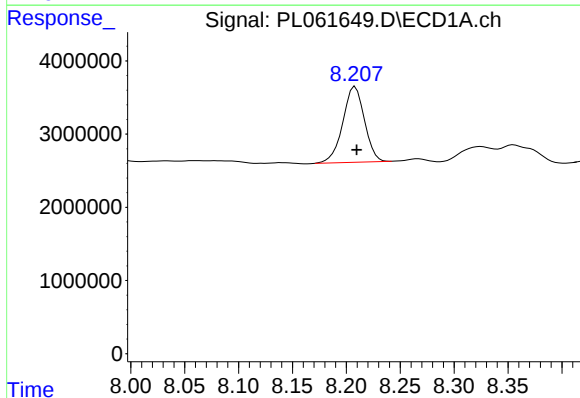

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.001 min
Response: 14460450
Conc: 8.67 ng/ml

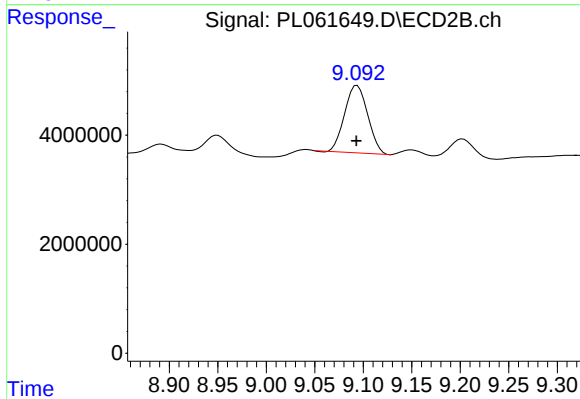

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 20476690
Conc: 8.66 ng/ml