

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092220\
 Data File : PL061650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2020 14:09
 Operator : DD\AJ
 Sample : L4100-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 17:29:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	27820950	50081409	16.131	16.282
28)	SA Decachlor...	8.210	9.094	22443285	31312939	13.453	13.243
Target Compounds							
10)	B gamma-Chl...	0.000	6.120	0	2599223	N.D.	0.754 #
11)	B alpha-Chl...	0.000	6.195	0	7160476	N.D.	2.058 #
12)	B 4,4'-DDE	0.000	6.349	0	3115759	N.D.	0.972 #
25)	Chlordane-3	0.000	6.120	0	2599223	N.D.	6.017 #
26)	Chlordane-4	0.000	6.195	0	7160476	N.D.	13.679 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092220\
Data File : PL061650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2020 14:09
Operator : DD\AJ
Sample : L4100-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 17:29:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

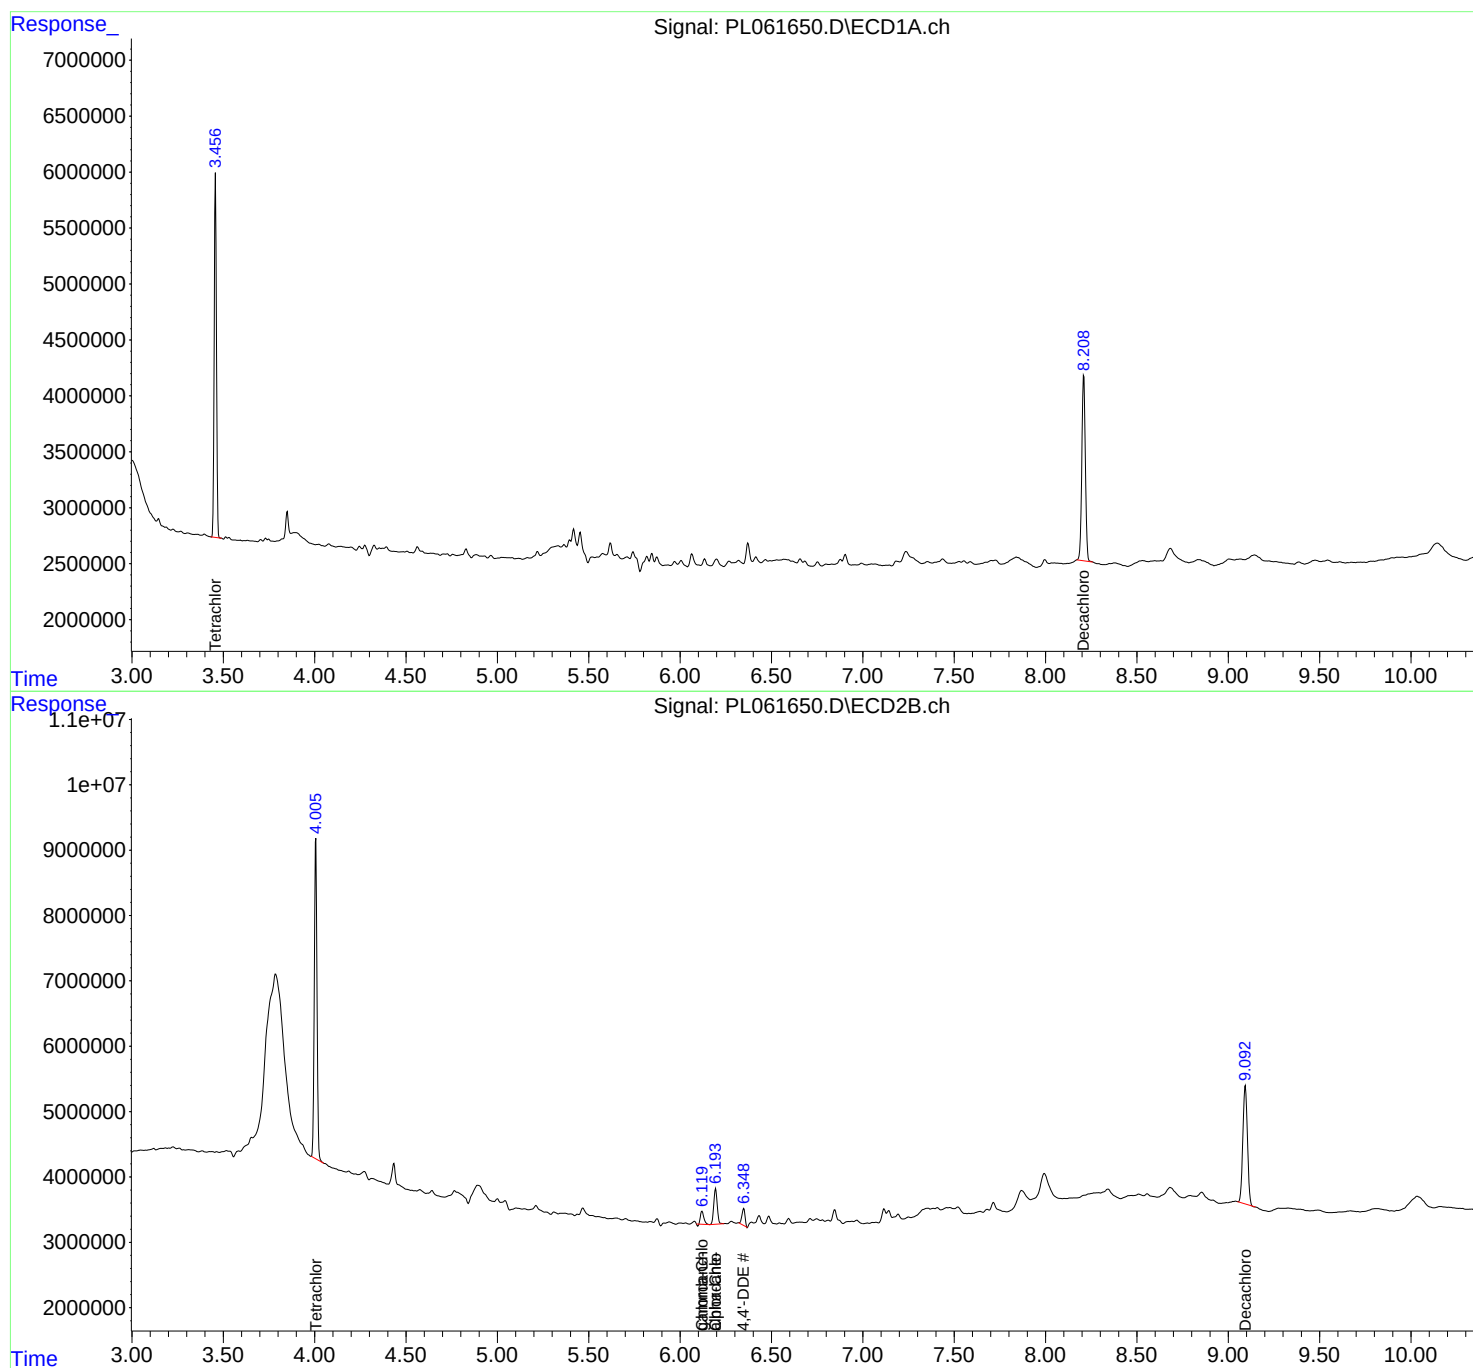


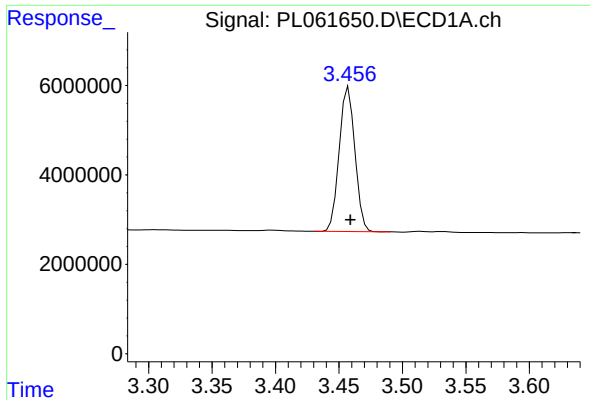

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: -0.001 min
Response: 27820950
Conc: 16.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

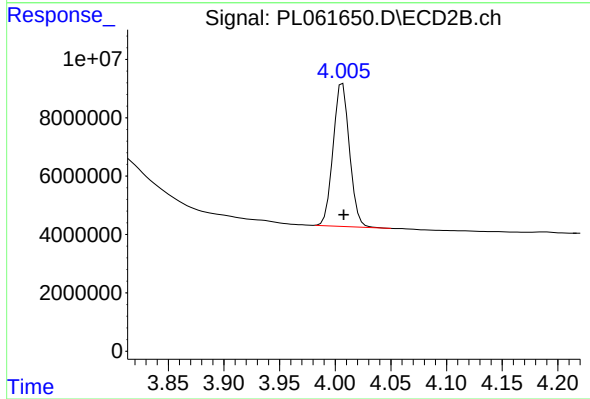


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 50081409
Conc: 16.28 ng/ml

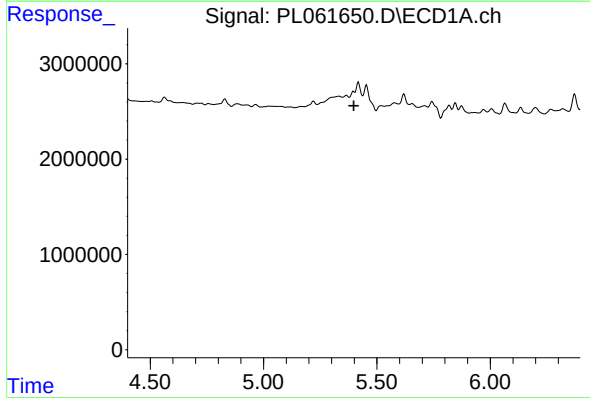


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

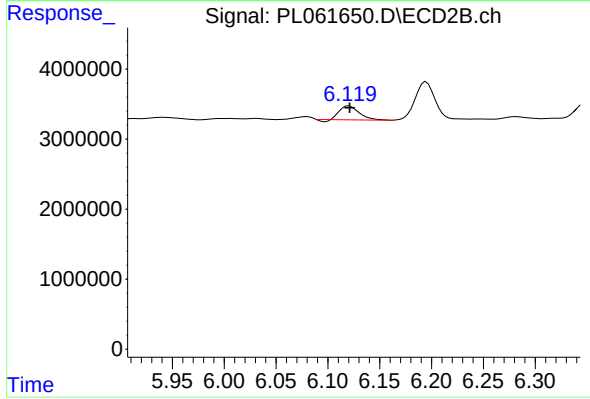

#10 gamma-Chlordane


R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 2599223
Conc: 0.75 ng/ml

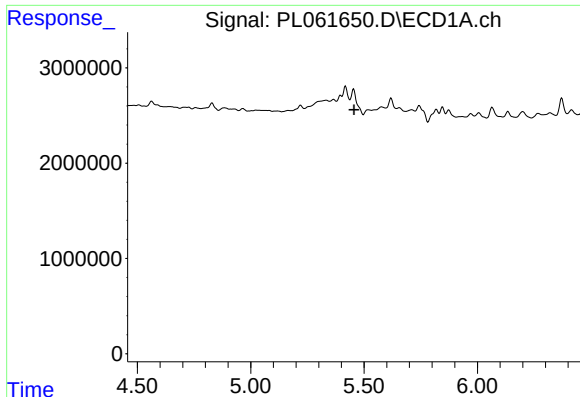

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

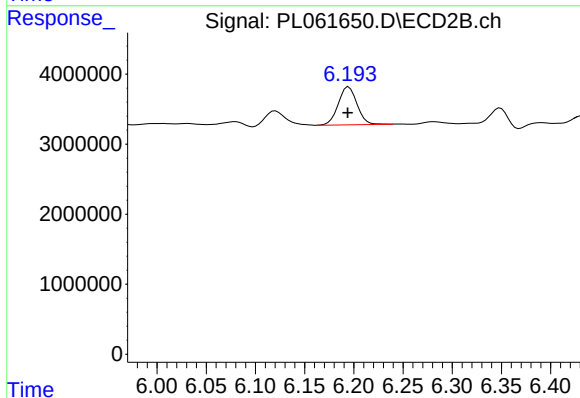


#11 alpha-Chlordane

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 7160476
Conc: 2.06 ng/ml

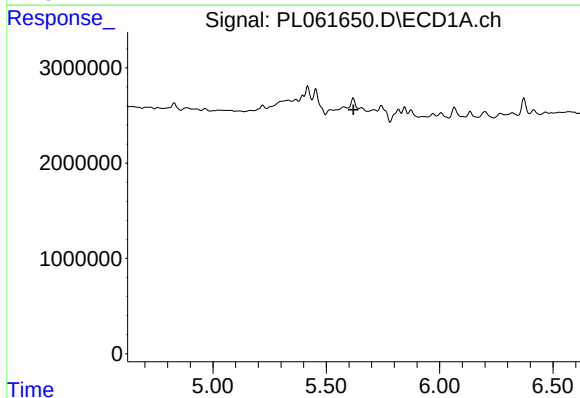


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.621 min
Response: 0
Conc: N.D.

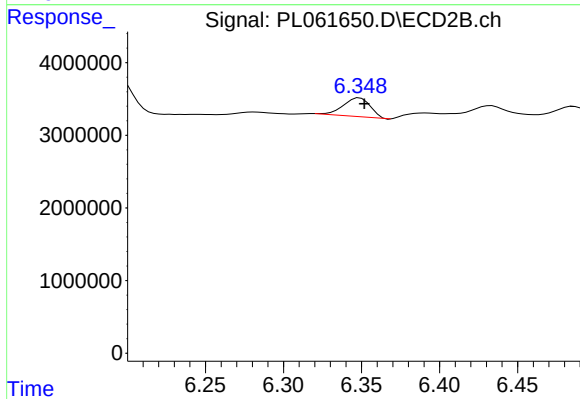

#12 4,4'-DDE


R.T.: 6.349 min
Delta R.T.: -0.003 min
Response: 3115759
Conc: 0.97 ng/ml

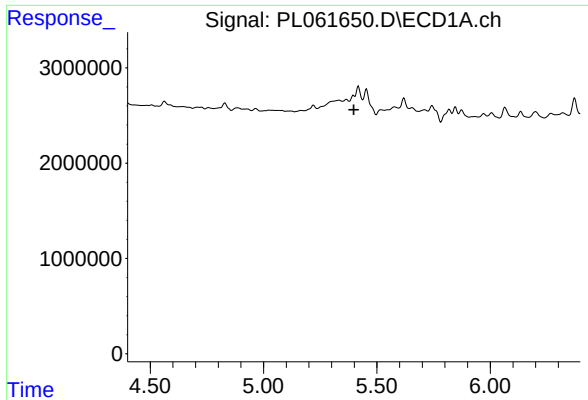

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

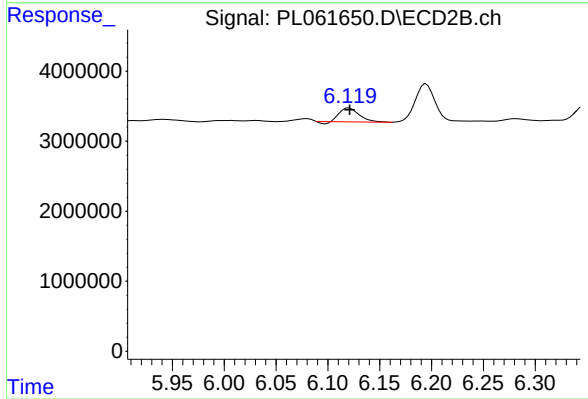


#25 Chlordane-3

R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 2599223
Conc: 6.02 ng/ml

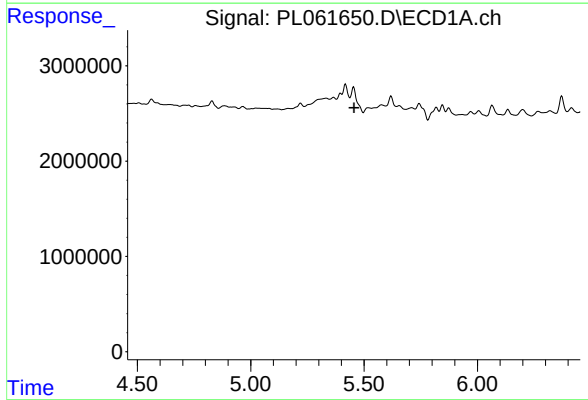


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

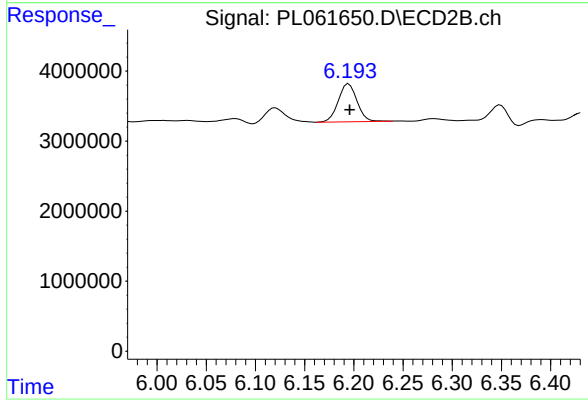

#26 Chlordane-4


R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 7160476
Conc: 13.68 ng/ml

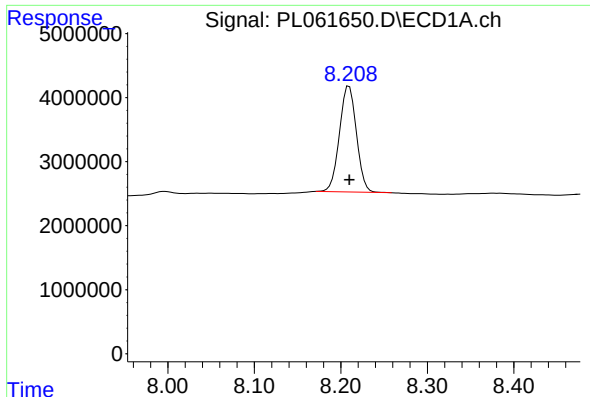

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 22443285
Conc: 13.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

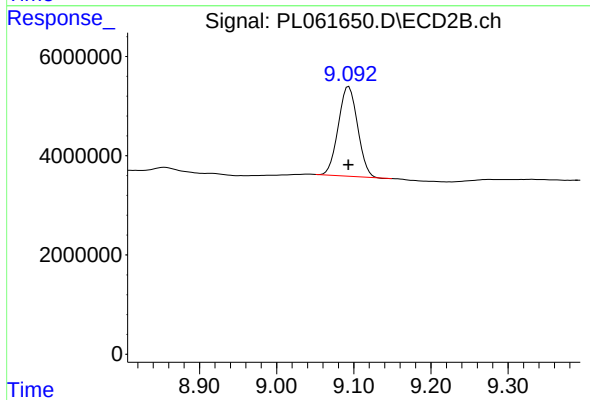

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 31312939
Conc: 13.24 ng/ml