

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092220\
 Data File : PL061652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2020 14:37
 Operator : DD\AJ
 Sample : L4100-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 17:29:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	38183907	67956194	22.140	22.093
28)	SA Decachlor...	8.210	9.094	20336250	28592452	12.190	12.092
Target Compounds							
2)	A alpha-BHC	0.000	4.422f	0	3607644	N.D.	0.781 #
6)	B beta-BHC	4.432	0.000	9262847	0	9.643	N.D. #
7)	B delta-BHC	0.000	5.095f	0	6675298	N.D.	2.093 #
9)	A Endosulfan I	5.528f	0.000	1563582	0	0.909	N.D. #
10)	B gamma-Chl...	0.000	6.105f	0	7530412	N.D.	2.184 #
12)	B 4,4'-DDE	5.619	6.351	24382455	41713329	14.339	13.013
17)	MA 4,4'-DDT	6.375	7.143	11040866	19942641	8.041	7.967
25)	Chlordane-3	0.000	6.105f	0	7530412	N.D.	17.432 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092220\
Data File : PL061652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2020 14:37
Operator : DD\AJ
Sample : L4100-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 17:29:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

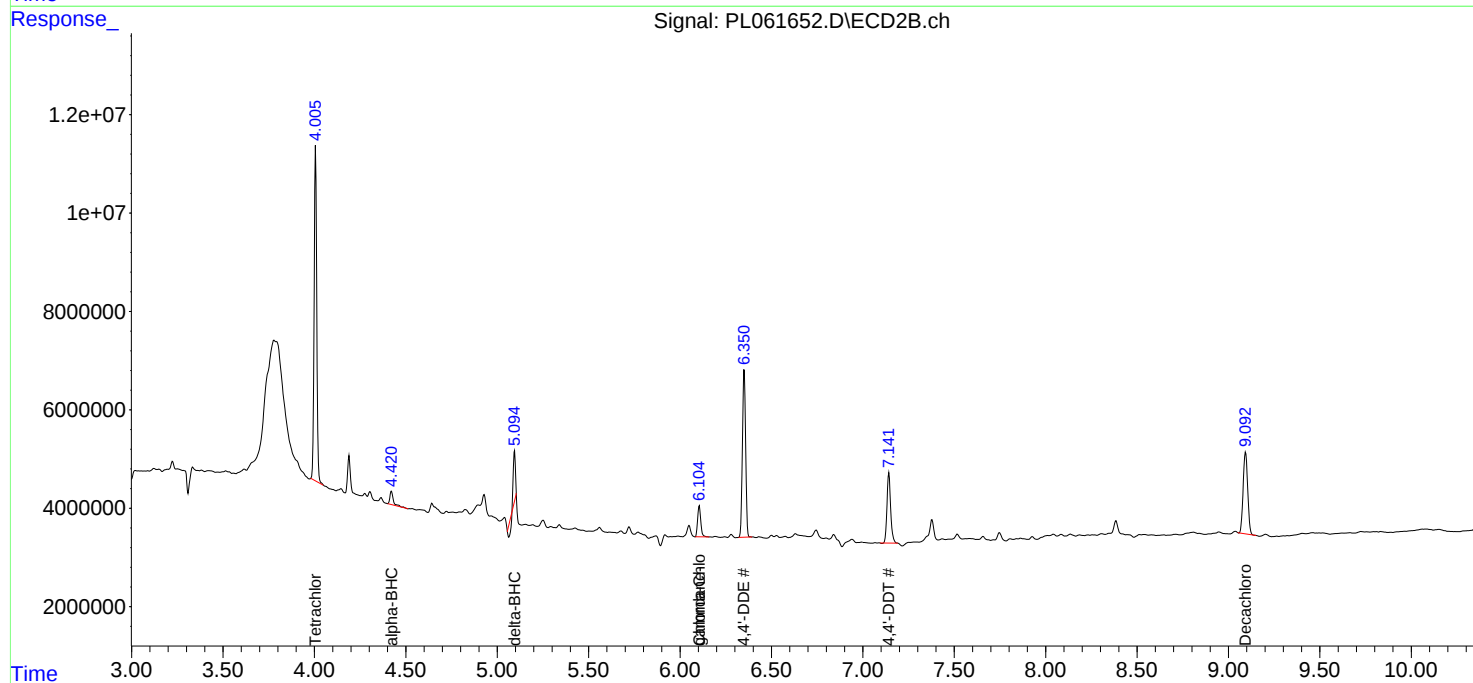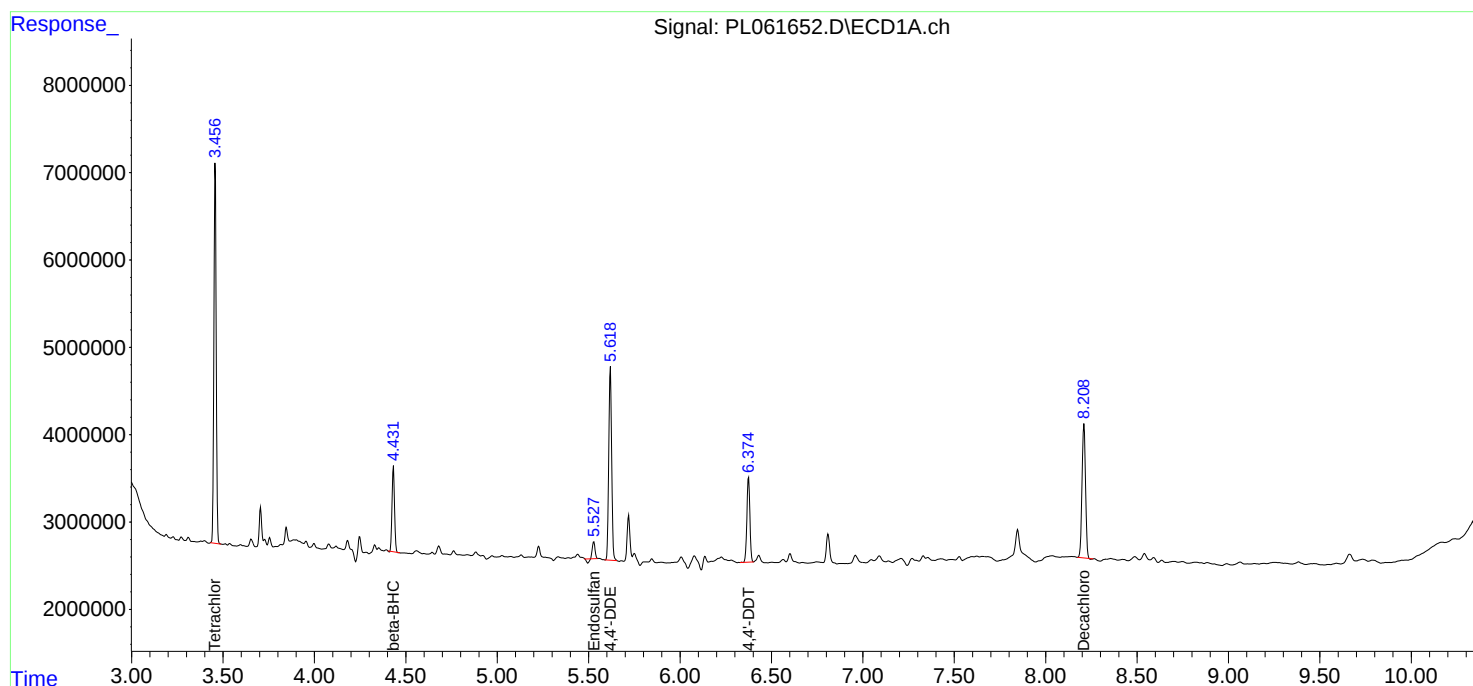


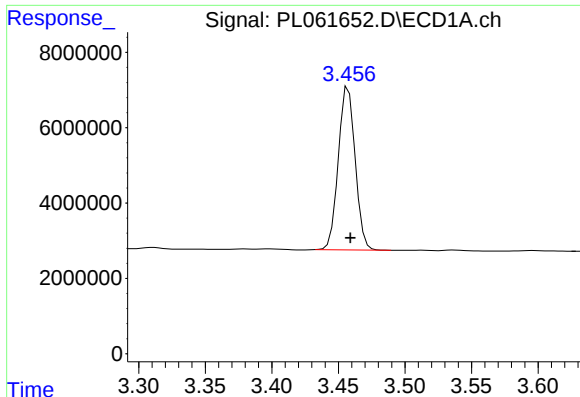

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: -0.001 min
Response: 38183907
Conc: 22.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

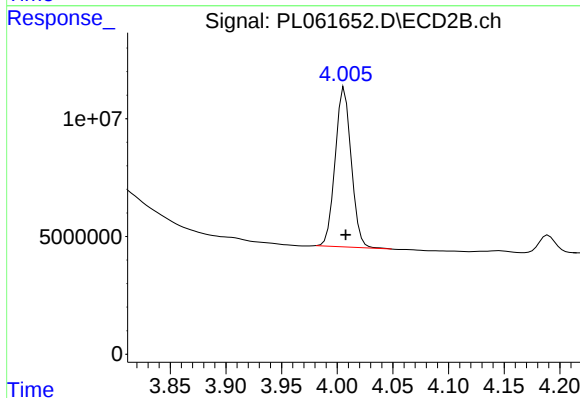


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.001 min
Response: 67956194
Conc: 22.09 ng/ml

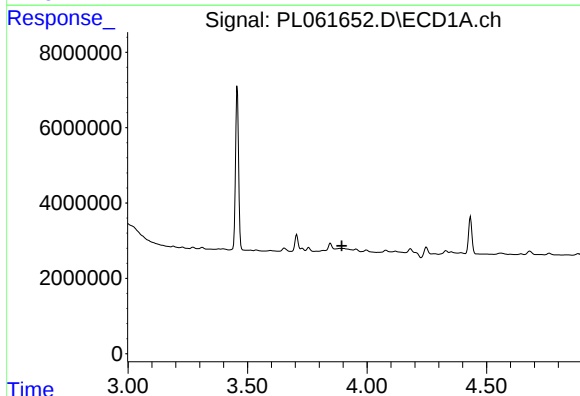


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.895 min
Response: 0
Conc: N.D.

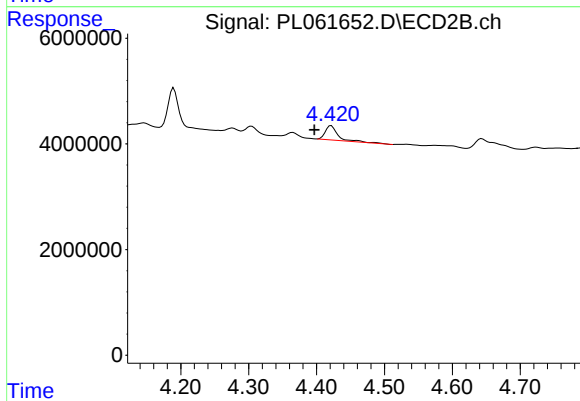

#2 alpha-BHC


R.T.: 4.422 min
Delta R.T.: 0.025 min
Response: 3607644
Conc: 0.78 ng/ml

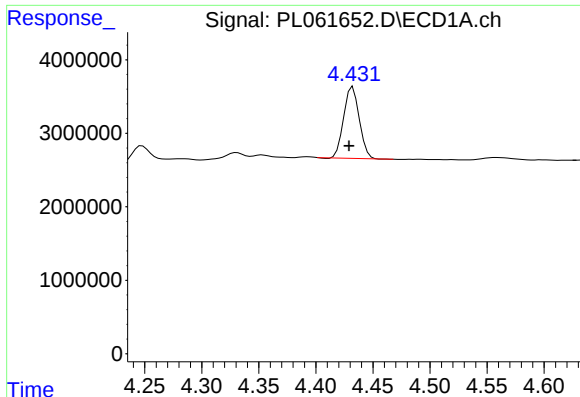

#6 beta-BHC


R.T.: 4.432 min
Delta R.T.: 0.003 min
Response: 9262847
Conc: 9.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

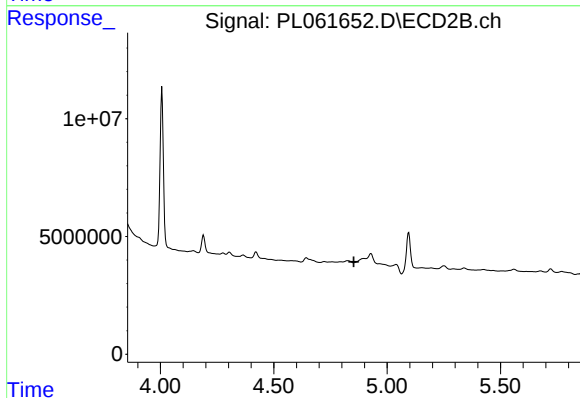


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.853 min
Response: 0
Conc: N.D.

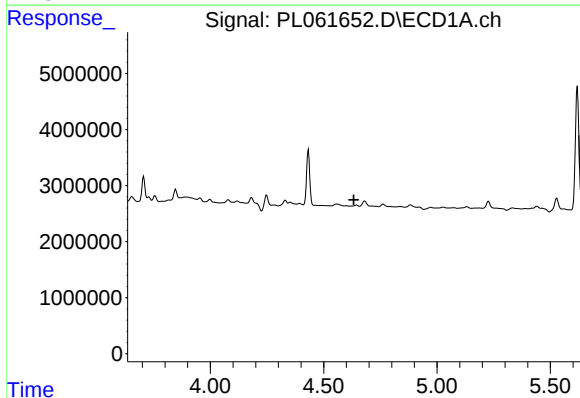


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.633 min
Response: 0
Conc: N.D.

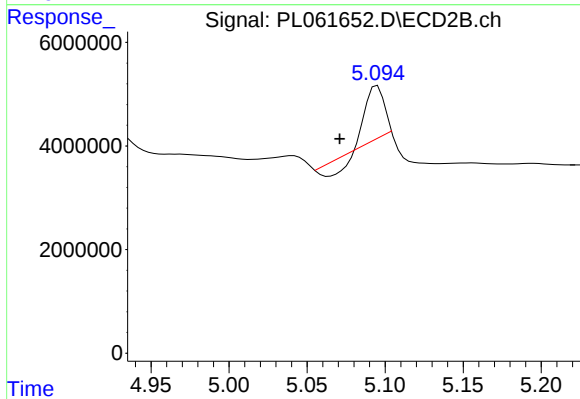

#7 delta-BHC


R.T.: 5.095 min
Delta R.T.: 0.024 min
Response: 6675298
Conc: 2.09 ng/ml

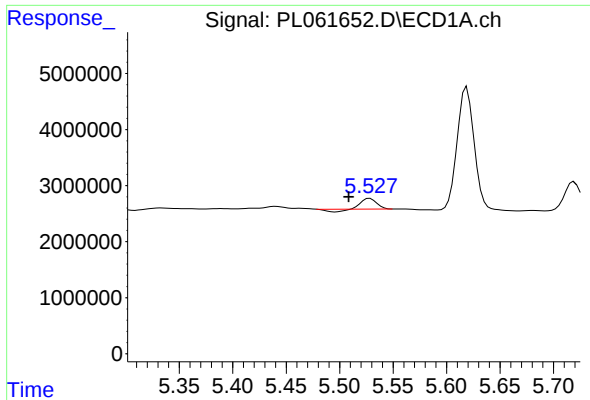

#9 Endosulfan I


R.T.: 5.528 min
Delta R.T.: 0.020 min
Response: 1563582
Conc: 0.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

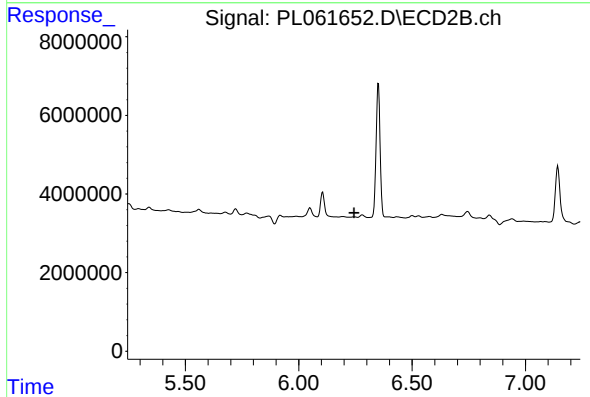


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

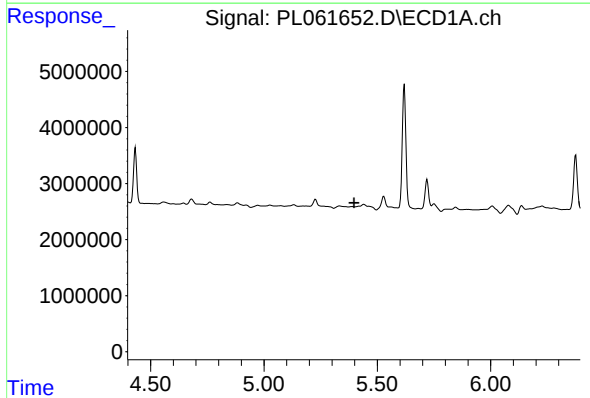


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

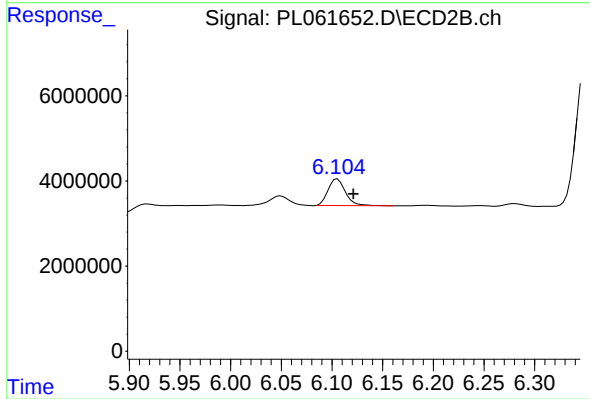

#10 gamma-Chlordane


R.T.: 6.105 min
Delta R.T.: -0.016 min
Response: 7530412
Conc: 2.18 ng/ml

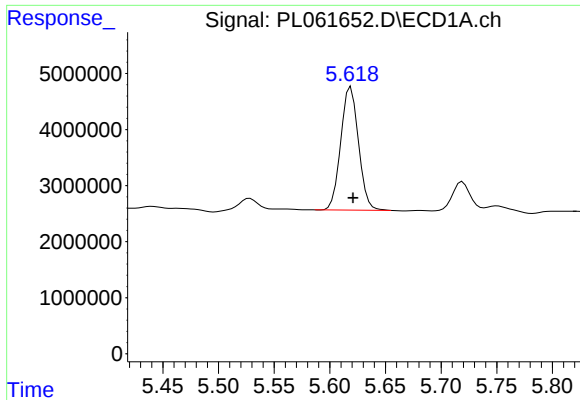

#12 4,4'-DDE


R.T.: 5.619 min
Delta R.T.: -0.002 min
Response: 24382455
Conc: 14.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

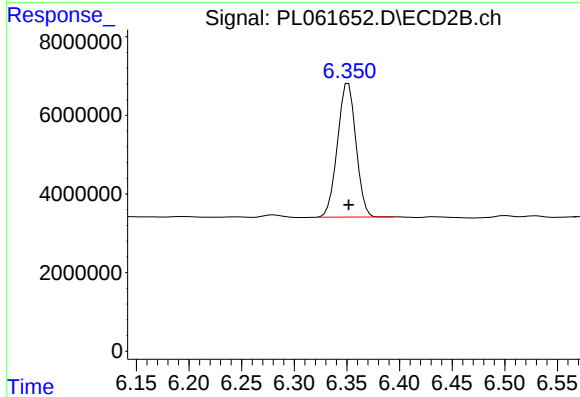


#12 4,4'-DDE

R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 41713329
Conc: 13.01 ng/ml

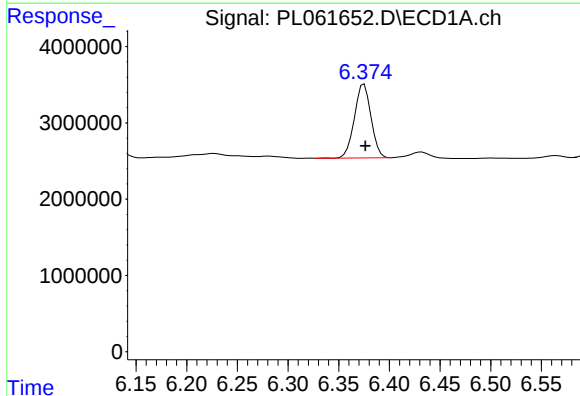


#17 4,4'-DDT

R.T.: 6.375 min
Delta R.T.: -0.001 min
Response: 11040866
Conc: 8.04 ng/ml

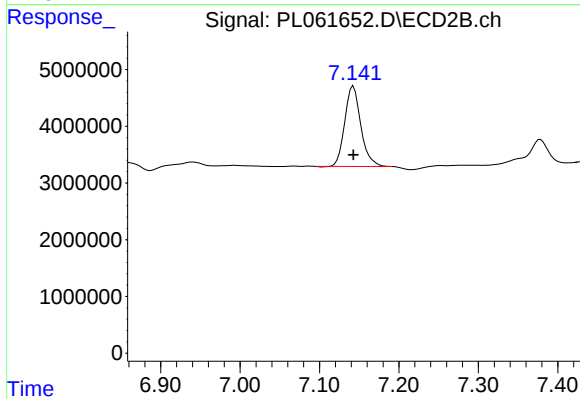

#17 4,4'-DDT


R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 19942641
Conc: 7.97 ng/ml

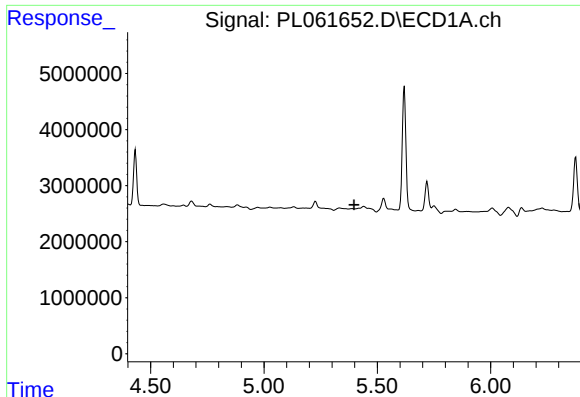

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

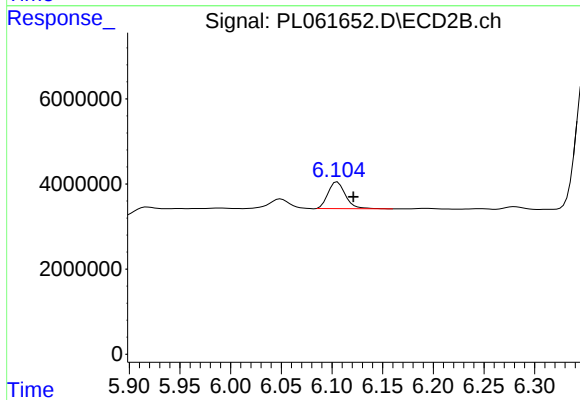


#25 Chlordane-3

R.T.: 6.105 min
Delta R.T.: -0.016 min
Response: 7530412
Conc: 17.43 ng/ml

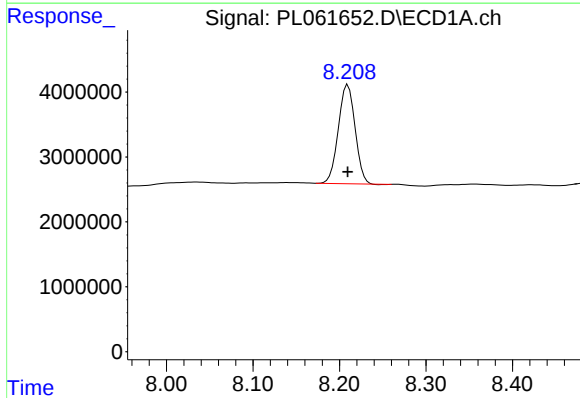

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.000 min
Response: 20336250
Conc: 12.19 ng/ml

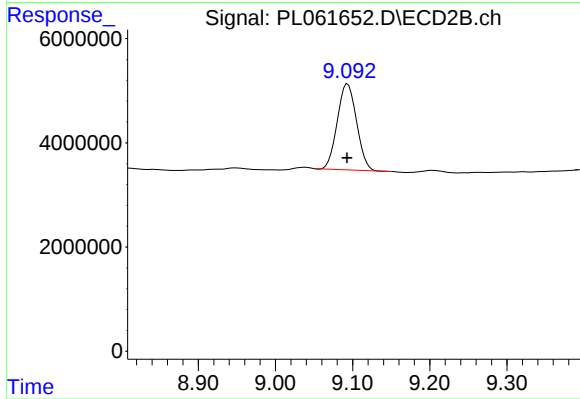

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 28592452
Conc: 12.09 ng/ml