

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092220\
 Data File : PL061644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2020 12:45
 Operator : DD\AJ
 Sample : L3866-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-092120

Manual Integrations
 APPROVED

Ankita
 9/23/2020 11:27:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 17:28:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 01:27:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	4.007	28667357	40917876	16.622m	13.302
28)	SA Decachlor...	8.208	9.093	26984791	35657353	16.175	15.080m
Target Compounds							
10)	B gamma-Chl...	5.397	6.121	16474703	36802165	8.893	10.675
11)	B alpha-Chl...	5.454	6.195	39206885	88019058	21.164	25.292
12)	B 4,4'-DDE	5.620	6.350	41434005	62380322	24.367	19.461
16)	A 4,4'-DDD	6.135	6.843	2378069	5662211	1.646m	2.205 #
17)	MA 4,4'-DDT	6.373	7.142	12447281	20577590	9.065m	8.221

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092220\
Data File : PL061644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2020 12:45
Operator : DD\AJ
Sample : L3866-06
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
OK-01-092120


Manual Integrations
APPROVED

Ankita
9/23/2020 11:27:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 17:28:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 01:27:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

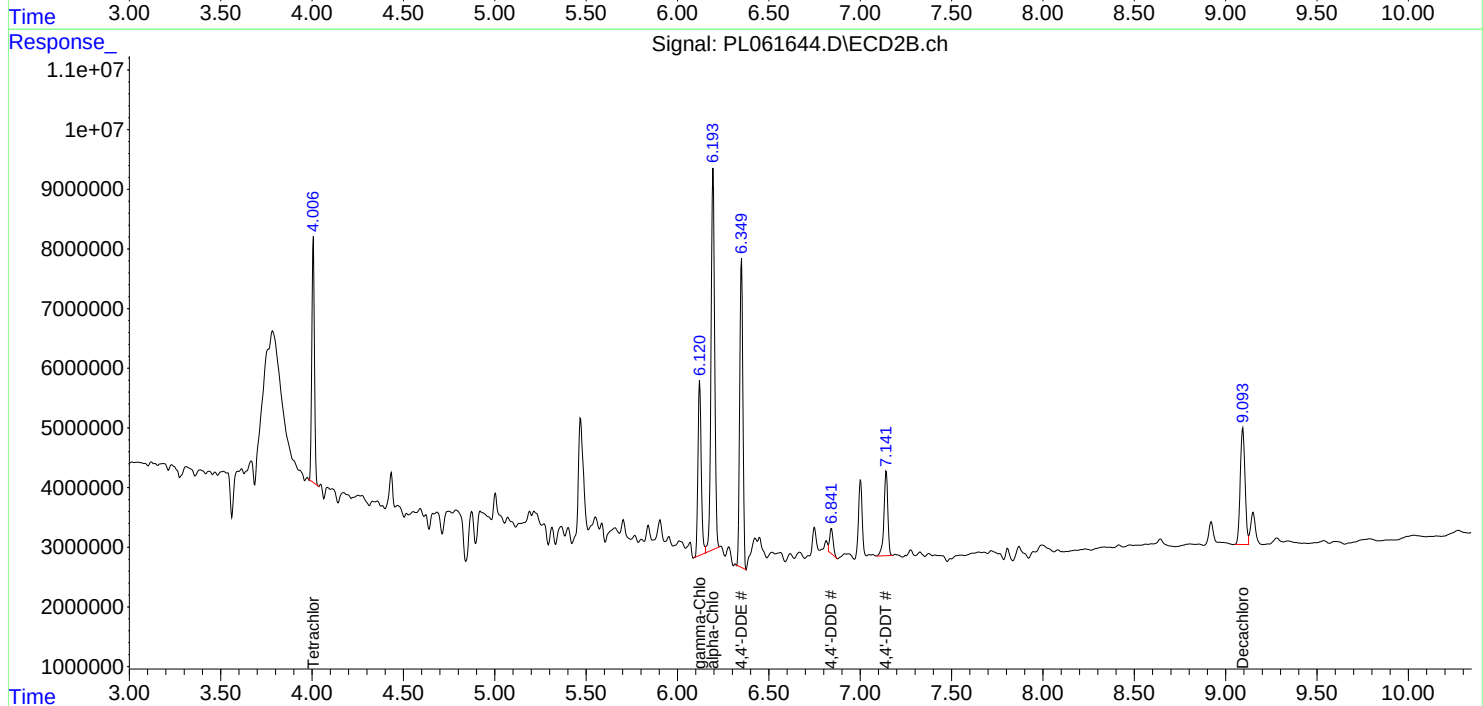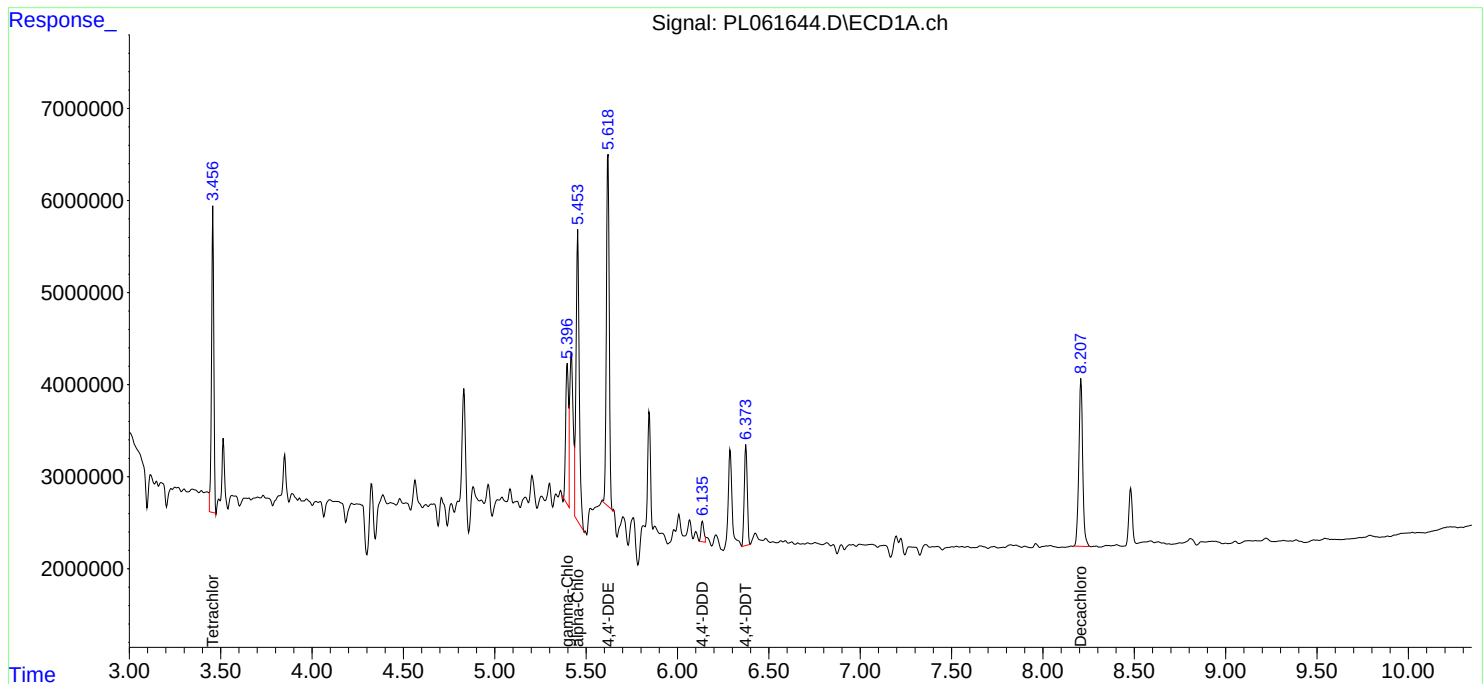

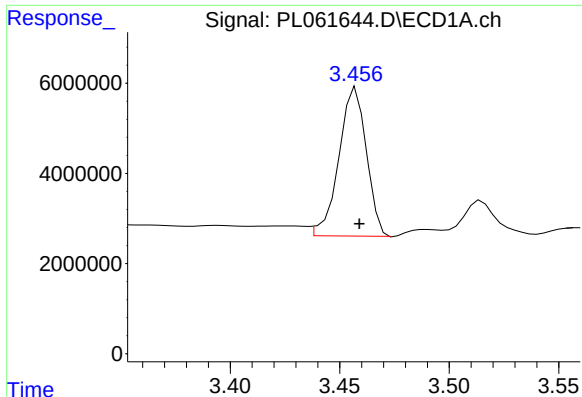


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: -0.003 min
Response: 28667357
Conc: 16.62 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-01-092120


Manual Integrations
APPROVED

Ankita
9/23/2020 11:27:33 AM

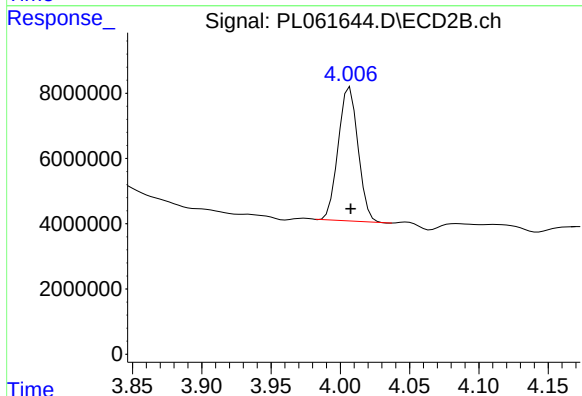


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 40917876
Conc: 13.30 ng/ml

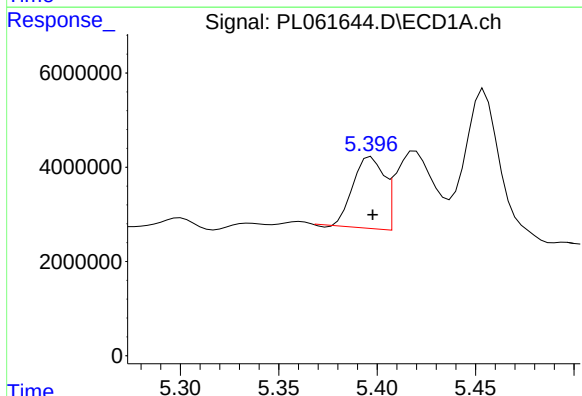


#10 gamma-Chlordane

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 16474703
Conc: 8.89 ng/ml

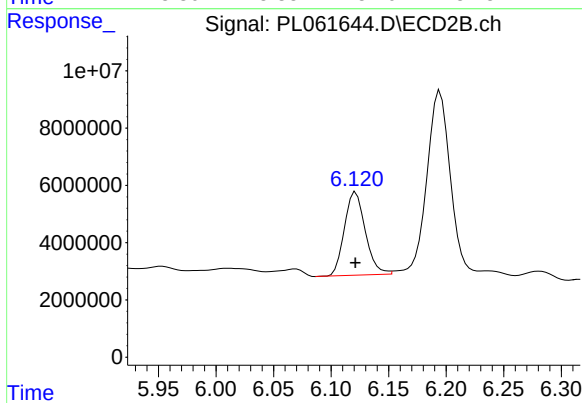

#10 gamma-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 36802165
Conc: 10.68 ng/ml

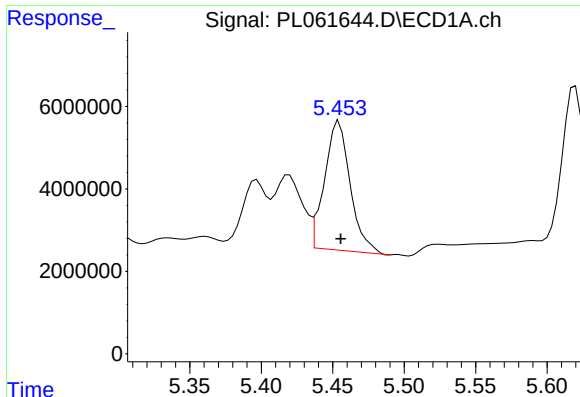


#11 alpha-Chlordane

R.T.: 5.454 min
Delta R.T.: -0.001 min
Response: 39206885
Conc: 21.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-092120


Manual Integrations
APPROVED

Ankita
9/23/2020 11:27:33 AM

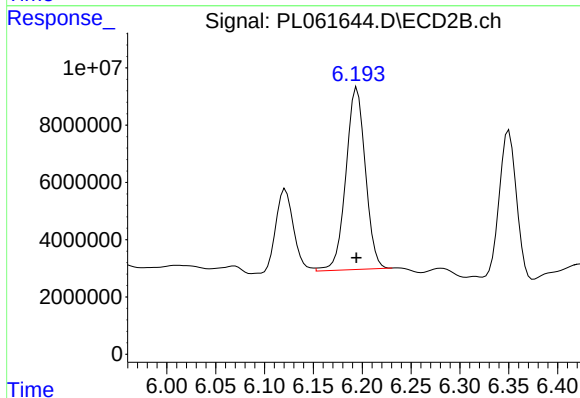


#11 alpha-Chlordane

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 88019058
Conc: 25.29 ng/ml

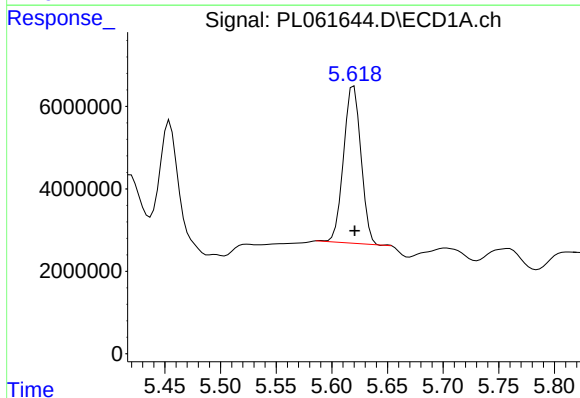


#12 4,4'-DDE

R.T.: 5.620 min
Delta R.T.: 0.000 min
Response: 41434005
Conc: 24.37 ng/ml

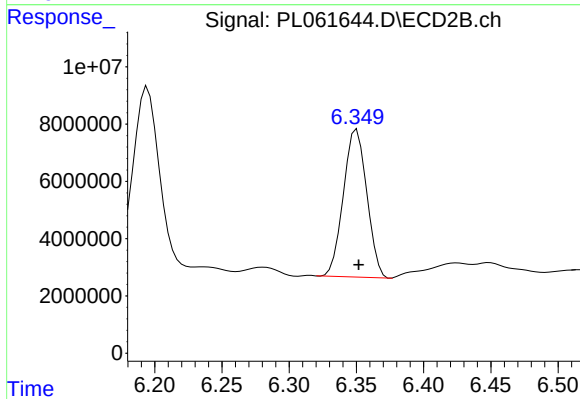

#12 4,4'-DDE

R.T.: 6.350 min
Delta R.T.: -0.002 min
Response: 62380322
Conc: 19.46 ng/ml

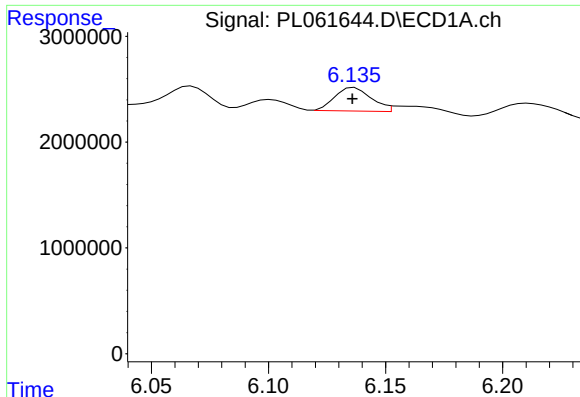


#16 4,4'-DDD

R.T.: 6.135 min
Delta R.T.: 0.000 min
Response: 2378069
Conc: 1.65 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-01-092120


Manual Integrations
APPROVED

Ankita
9/23/2020 11:27:33 AM

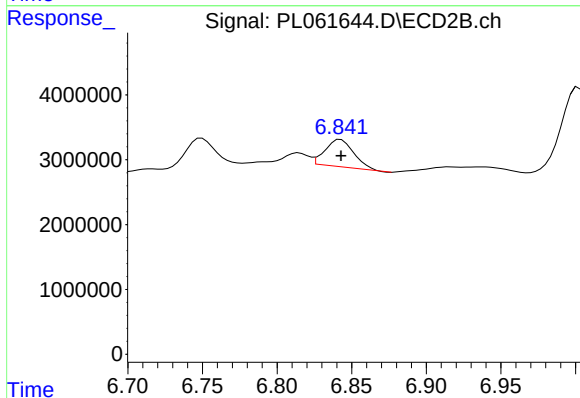


#16 4,4'-DDD

R.T.: 6.843 min
Delta R.T.: 0.000 min
Response: 5662211
Conc: 2.20 ng/ml

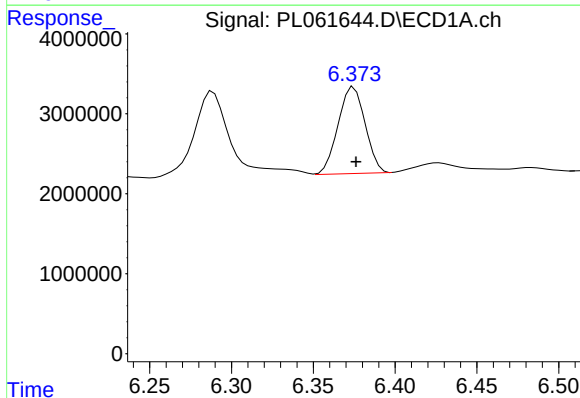


#17 4,4'-DDT

R.T.: 6.373 min
Delta R.T.: -0.003 min
Response: 12447281
Conc: 9.07 ng/ml m

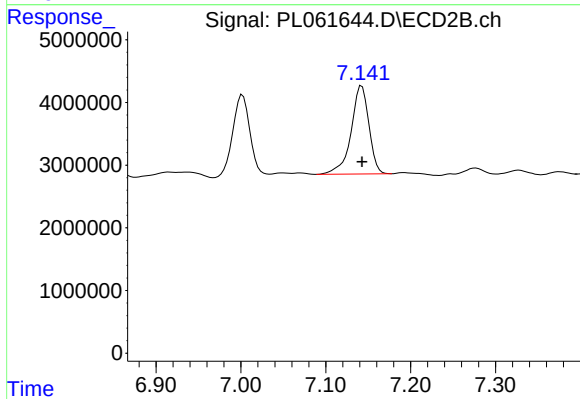

#17 4,4'-DDT

R.T.: 7.142 min
Delta R.T.: 0.000 min
Response: 20577590
Conc: 8.22 ng/ml

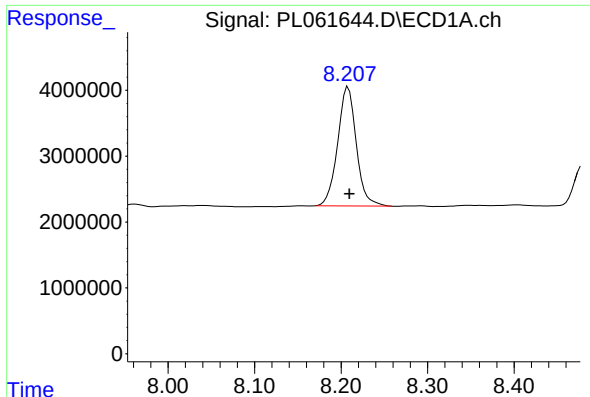


#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.001 min
Response: 26984791
Conc: 16.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-092120

Manual Integrations
APPROVED

Ankita
9/23/2020 11:27:33 AM

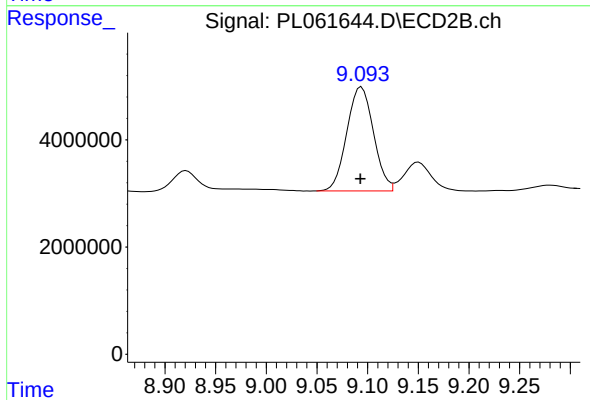

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 35657353
Conc: 15.08 ng/ml m