

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092221\
 Data File : PL069961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 08:57
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 02:09:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	5.354	0.000	1216927	0	2.220	N.D.	#
8) B	Heptachlo...	0.000	8.035	0	609763	N.D.	0.475	#
10) B	gamma-Chl...	0.000	8.284f	0	2675622	N.D.	2.003	#
11) B	alpha-Chl...	0.000	8.384	0	380355	N.D.	0.279	#
17) MA	4,4'-DDT	0.000	9.431	0	140047	N.D.	0.125	#
23)	Chlordane-1	0.000	6.969f	0	2557310	N.D.	62.302	#
25)	Chlordane-3	0.000	8.284f	0	2675622	N.D.	14.105	#
26)	Chlordane-4	0.000	8.384	0	380355	N.D.	1.633	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092221\
Data File : PL069961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 08:57
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 02:09:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

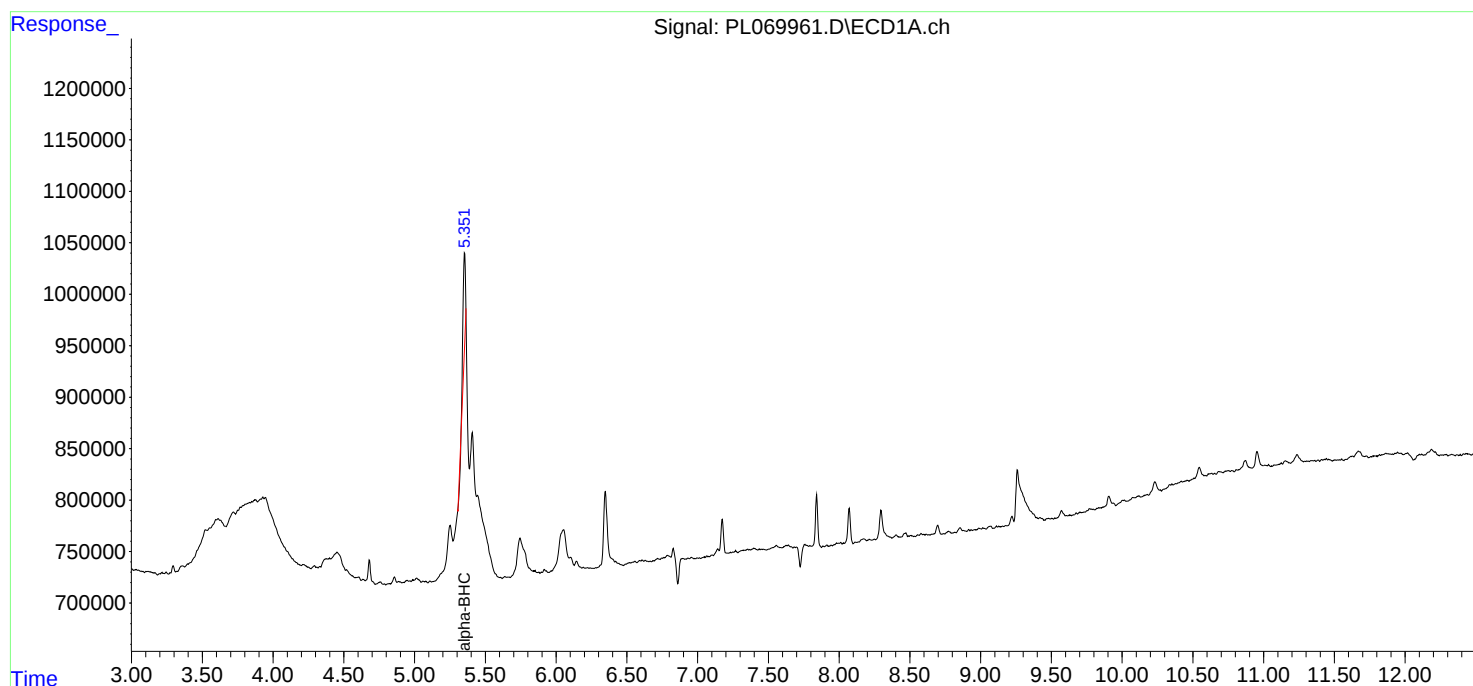


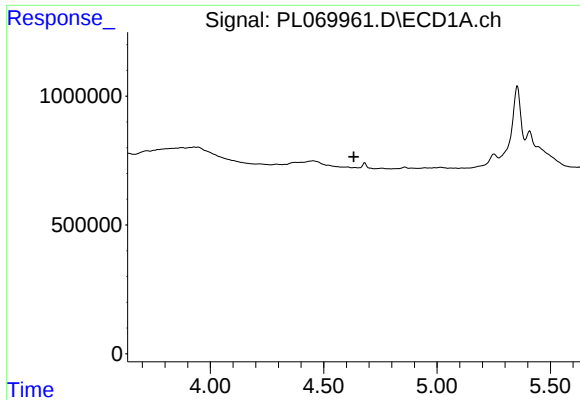

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.633 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

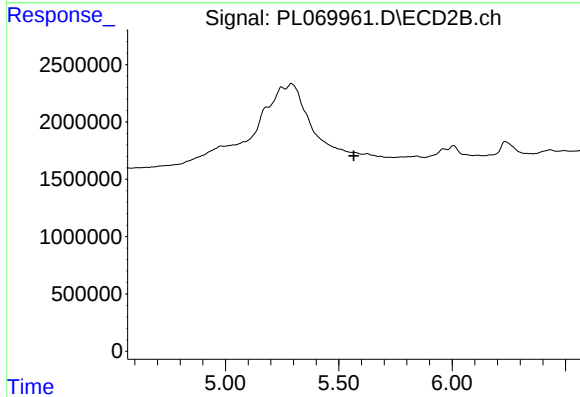


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.567 min
Response: 0
Conc: N.D.

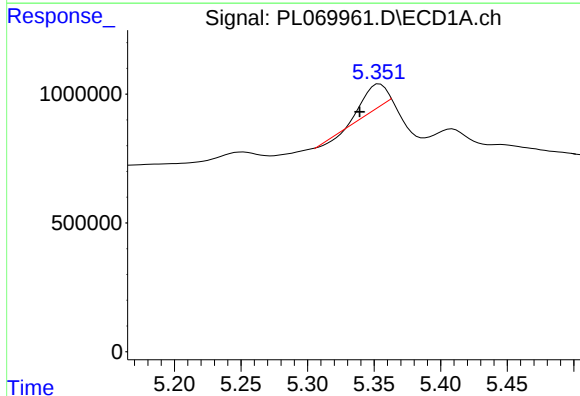


#2 alpha-BHC

R.T.: 5.354 min
Delta R.T.: 0.015 min
Response: 1216927
Conc: 2.22 ng/ml

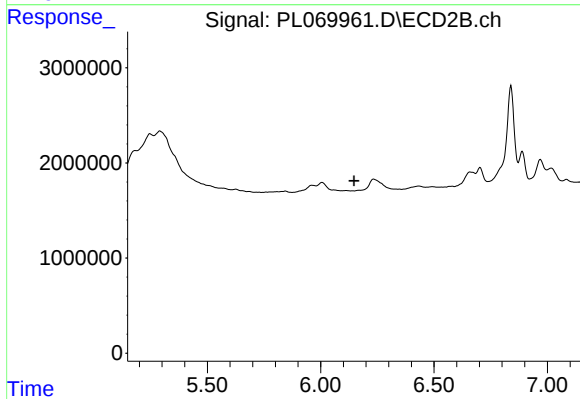

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.147 min
Response: 0
Conc: N.D.

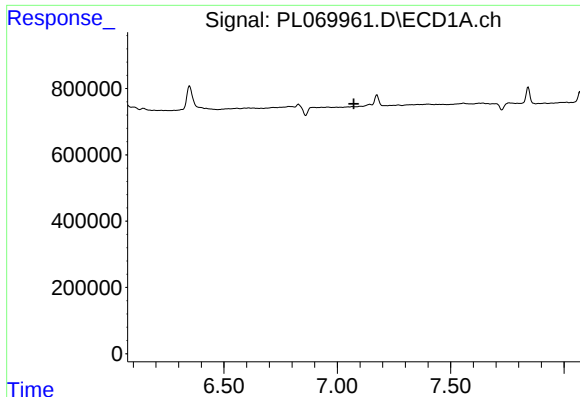

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

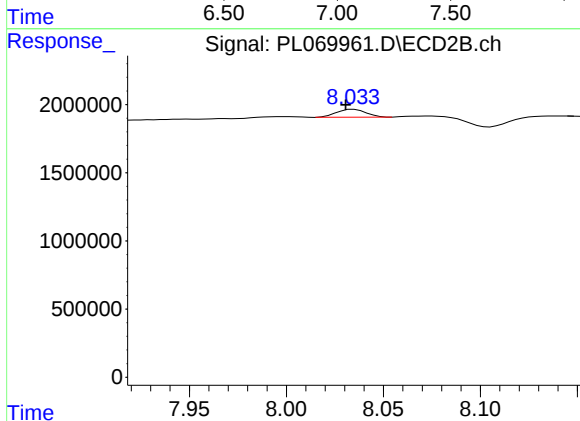


#8 Heptachlor epoxide

R.T.: 8.035 min
Delta R.T.: 0.004 min
Response: 609763
Conc: 0.48 ng/ml

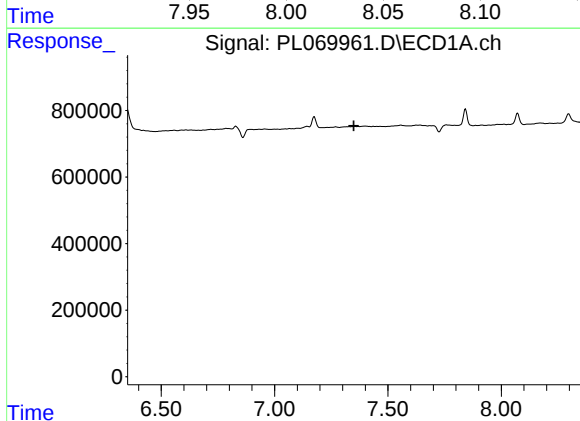


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

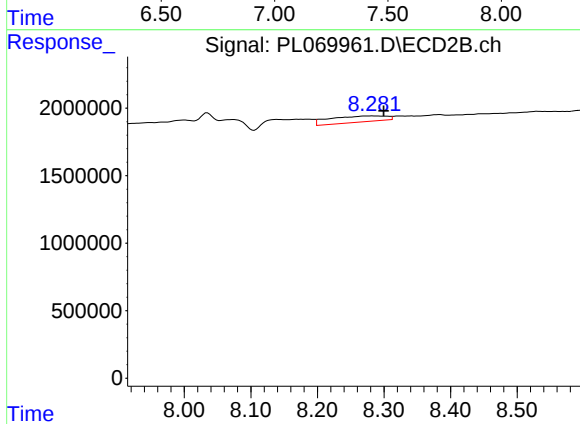

#10 gamma-Chlordane


R.T.: 8.284 min
Delta R.T.: -0.016 min
Response: 2675622
Conc: 2.00 ng/ml

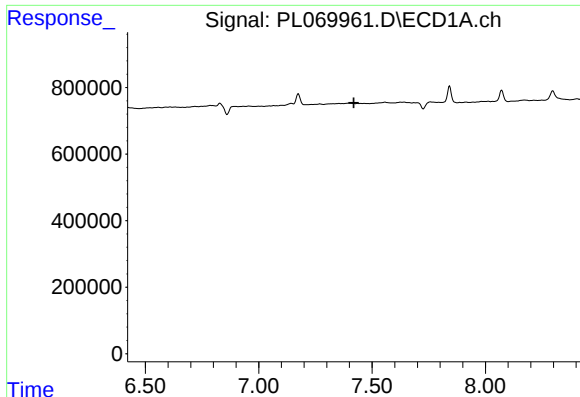

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

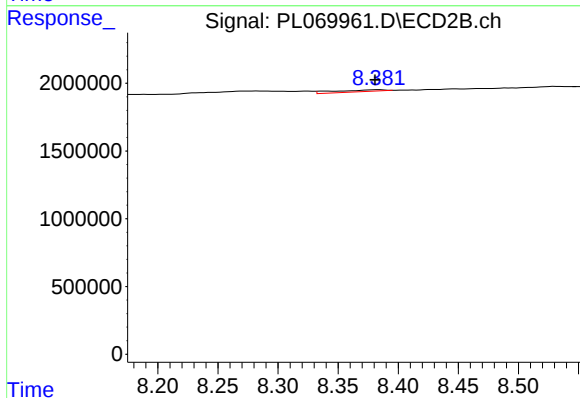


#11 alpha-Chlordane

R.T.: 8.384 min
Delta R.T.: 0.003 min
Response: 380355
Conc: 0.28 ng/ml

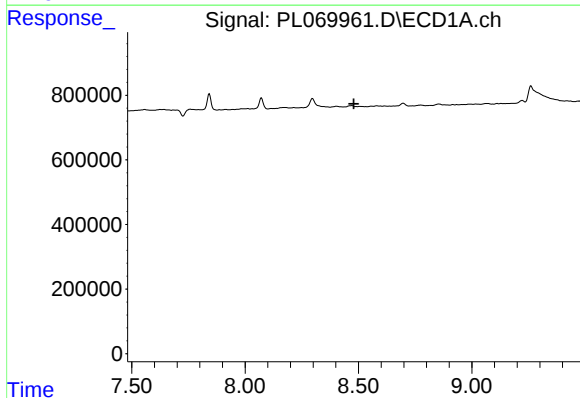


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

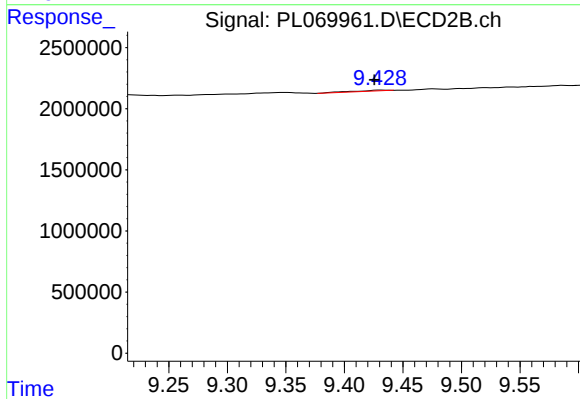

#17 4,4'-DDT


R.T.: 9.431 min
Delta R.T.: 0.005 min
Response: 140047
Conc: 0.13 ng/ml

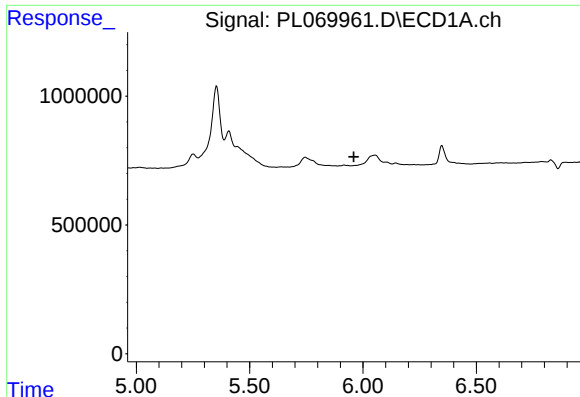

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

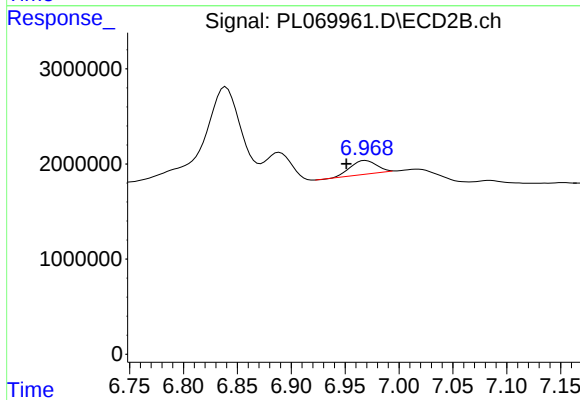


#23 Chlordane-1

R.T.: 6.969 min
Delta R.T.: 0.018 min
Response: 2557310
Conc: 62.30 ng/ml

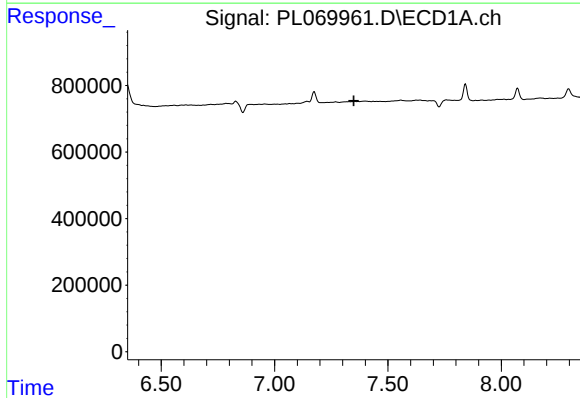


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

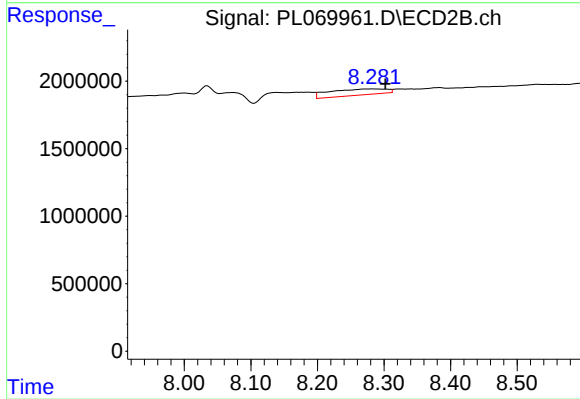

#25 Chlordane-3


R.T.: 8.284 min
Delta R.T.: -0.018 min
Response: 2675622
Conc: 14.11 ng/ml

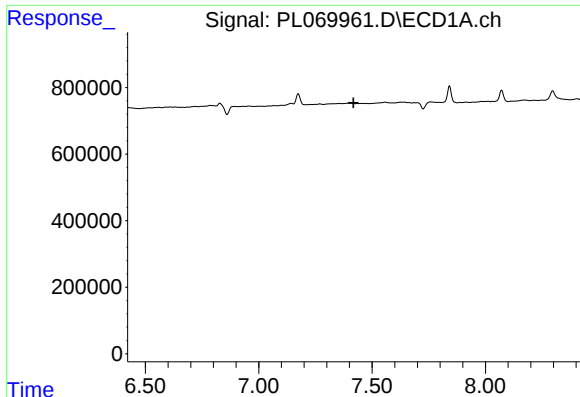

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 7.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

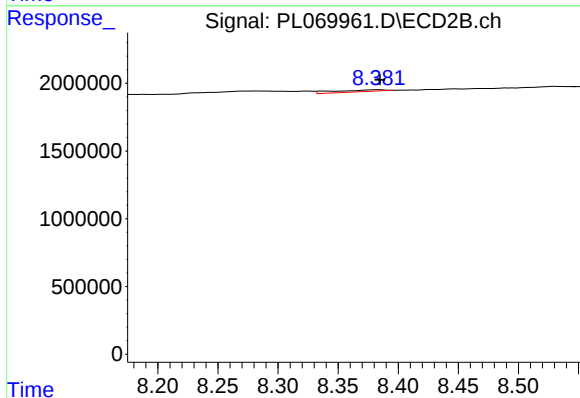


#26 Chlordane-4

R.T.: 8.384 min
Delta R.T.: -0.001 min
Response: 380355
Conc: 1.63 ng/ml

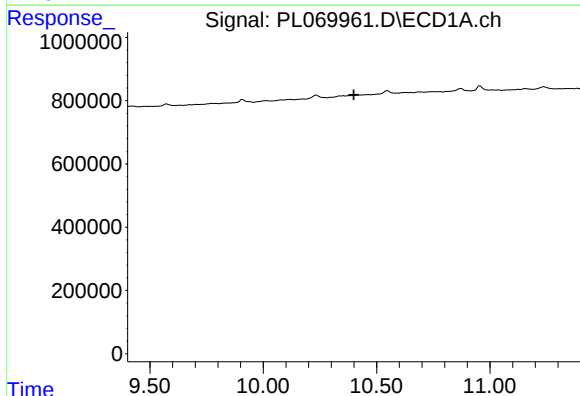

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.399 min
Response: 0
Conc: N.D.

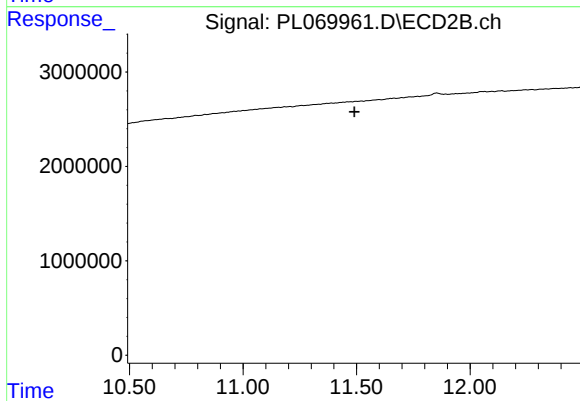

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.491 min
Response: 0
Conc: N.D.