

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092221\
 Data File : PL069974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 20:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 02:16:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 13 17:55:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.628	5.563	9917872	29189096	24.343	23.980
28)	SA Decachlor...	10.393	11.483	13048063	25657985	17.718	22.455 #
Target Compounds							
7)	B delta-BHC	0.000	7.081f	0	1264815	N.D.	0.759 #
10)	B gamma-Chl...	0.000	8.286	0	510910	N.D.	0.382 #
16)	A 4,4'-DDD	0.000	9.120	0	568035	N.D.	0.534 #
22)	Mirex	0.000	10.558f	0	266763	N.D.	0.285 #
23)	Chlordane-1	0.000	6.971f	0	229958	N.D.	5.602 #
25)	Chlordane-3	0.000	8.286f	0	510910	N.D.	2.693 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092221\
Data File : PL069974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 20:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 02:16:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091021.M
Quant Title : GC Extractables
QLast Update : Mon Sep 13 17:55:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

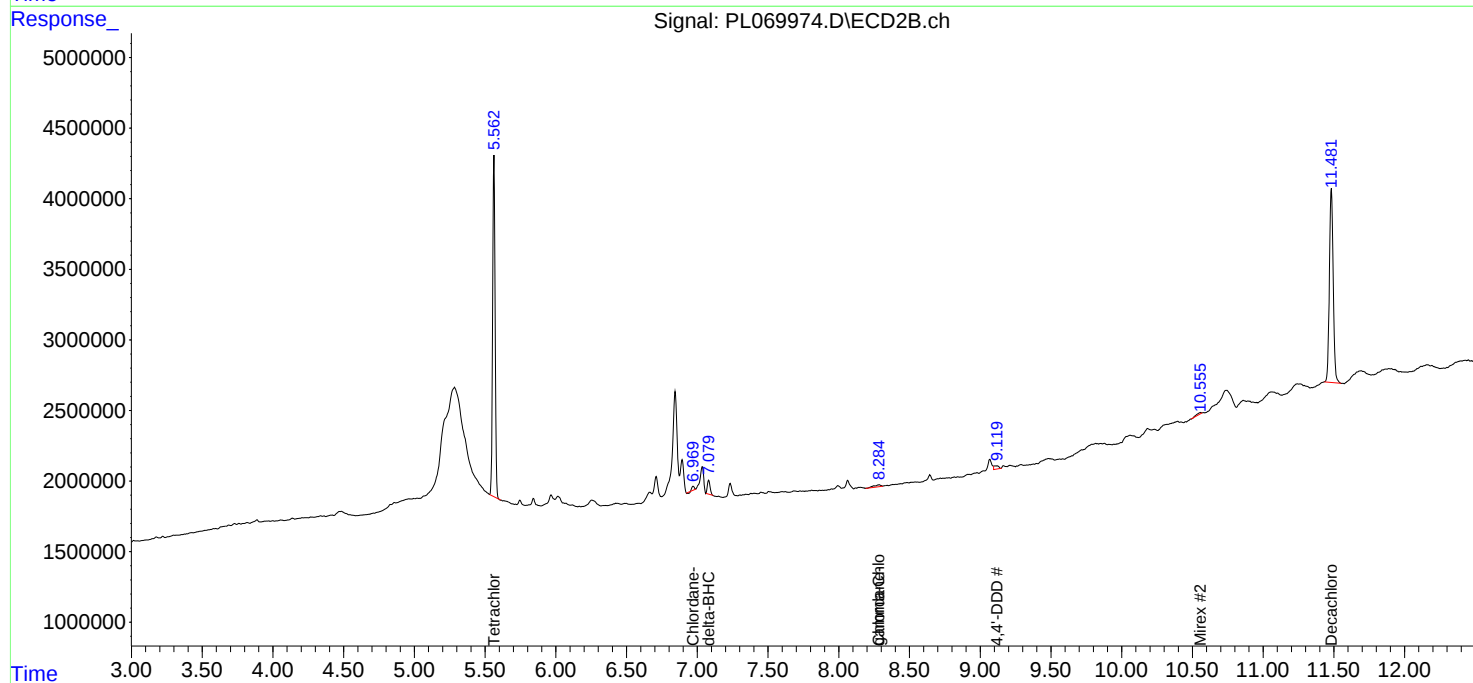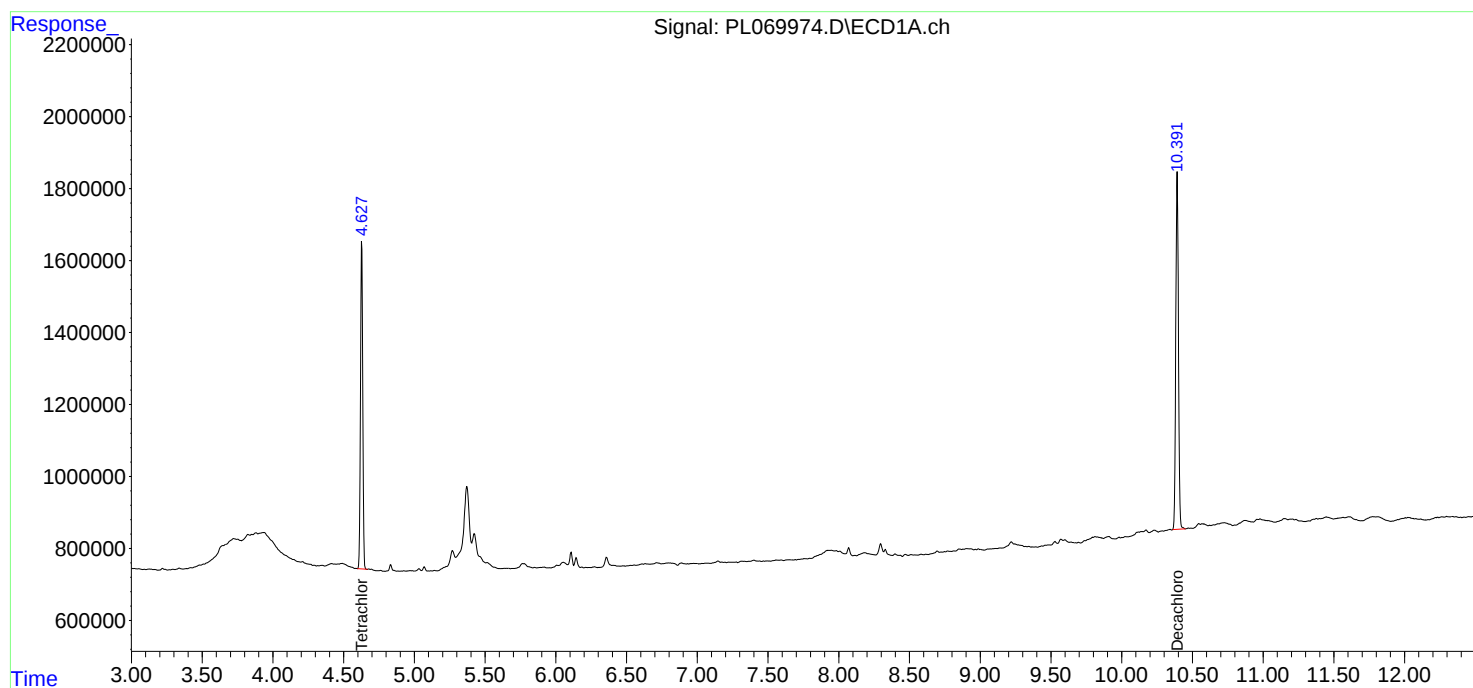


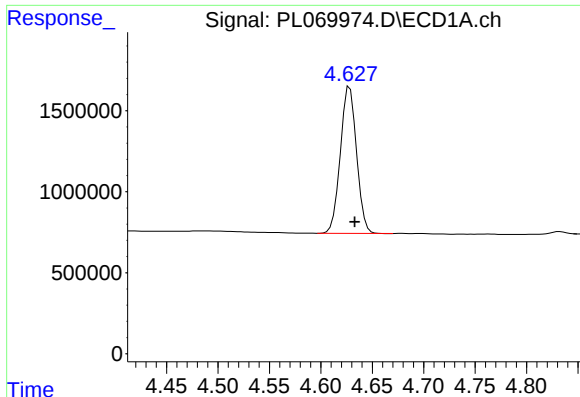

#1 Tetrachloro-m-xylene


R.T.: 4.628 min
Delta R.T.: -0.005 min
Response: 9917872
Conc: 24.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

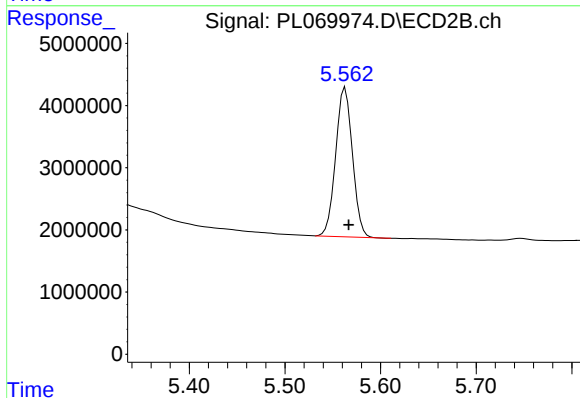


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 29189096
Conc: 23.98 ng/ml

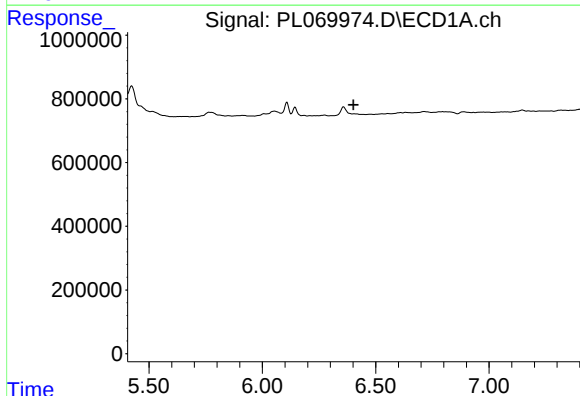


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

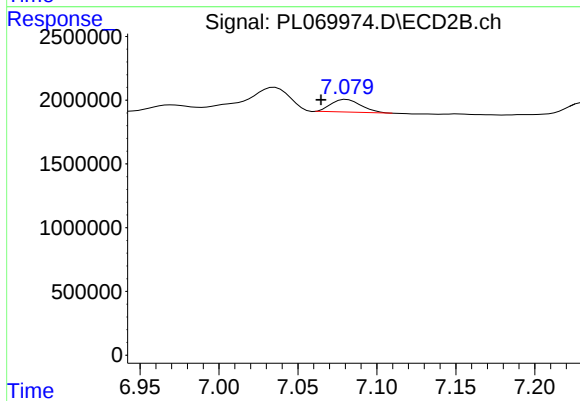

#7 delta-BHC


R.T.: 7.081 min
Delta R.T.: 0.016 min
Response: 1264815
Conc: 0.76 ng/ml

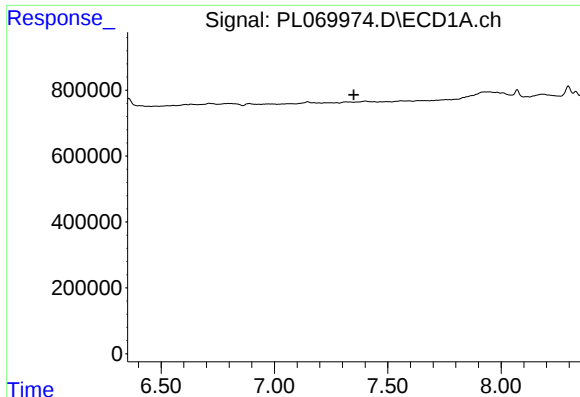

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

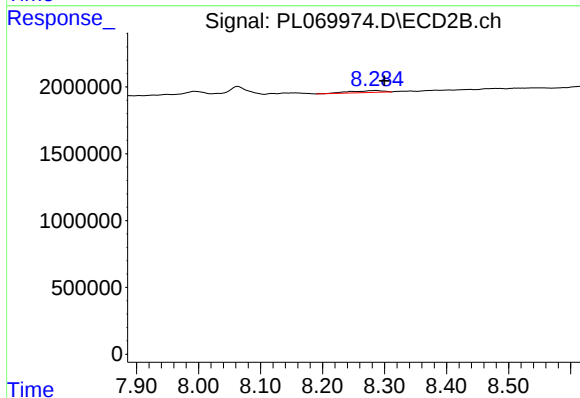


#10 gamma-Chlordane

R.T.: 8.286 min
Delta R.T.: -0.014 min
Response: 510910
Conc: 0.38 ng/ml

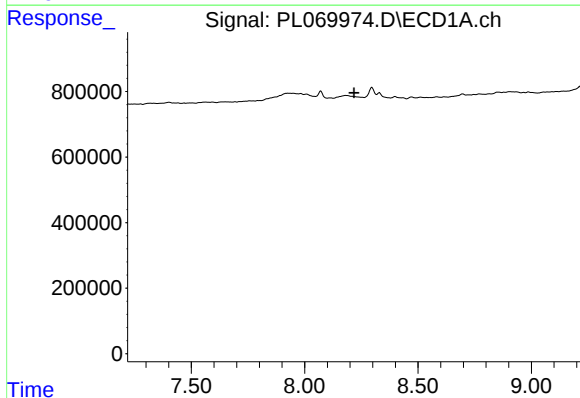


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.218 min
Response: 0
Conc: N.D.

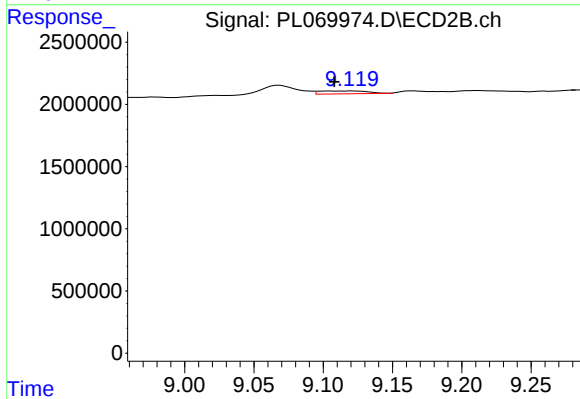

#16 4,4'-DDD


R.T.: 9.120 min
Delta R.T.: 0.012 min
Response: 568035
Conc: 0.53 ng/ml

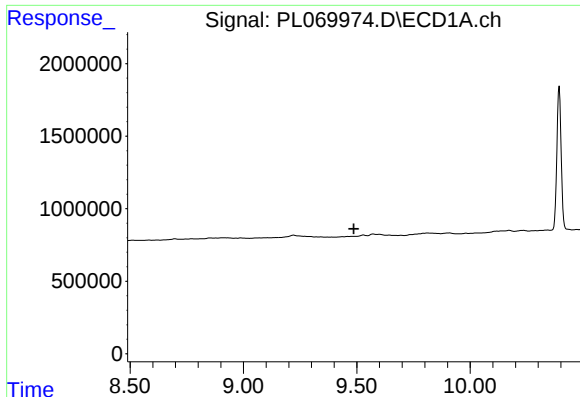

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

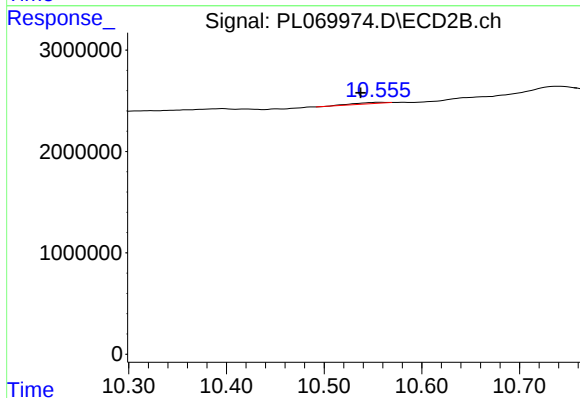


#22 Mirex

R.T.: 10.558 min
Delta R.T.: 0.020 min
Response: 266763
Conc: 0.29 ng/ml

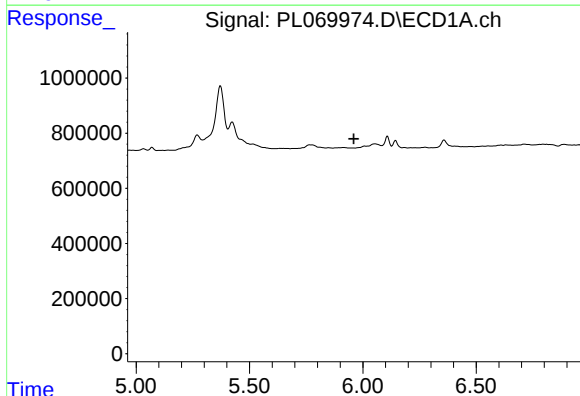


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

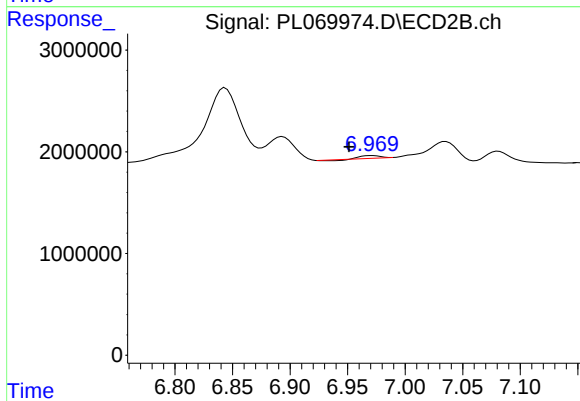

#23 Chlordane-1


R.T.: 6.971 min
Delta R.T.: 0.019 min
Response: 229958
Conc: 5.60 ng/ml

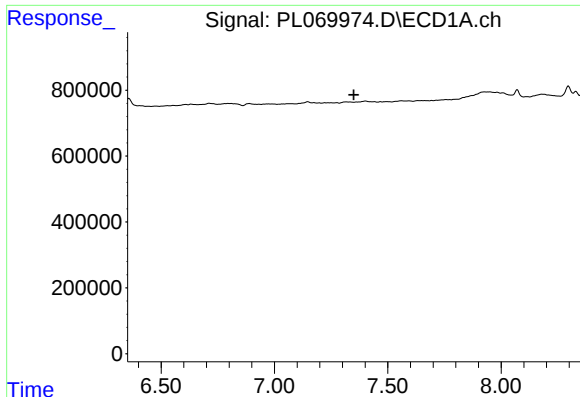

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

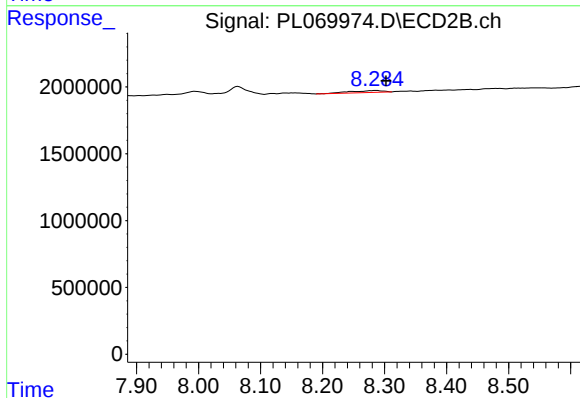


#25 Chlordane-3

R.T.: 8.286 min
Delta R.T.: -0.016 min
Response: 510910
Conc: 2.69 ng/ml

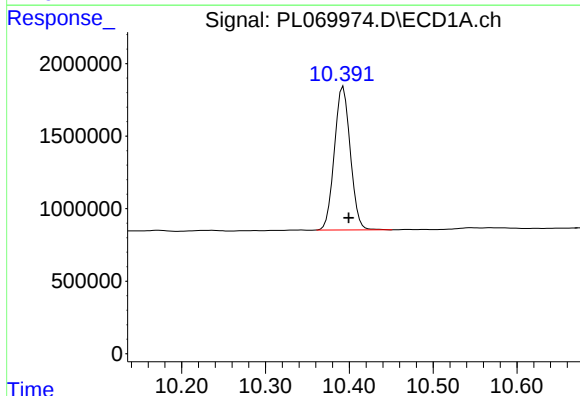

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: -0.006 min
Response: 13048063
Conc: 17.72 ng/ml

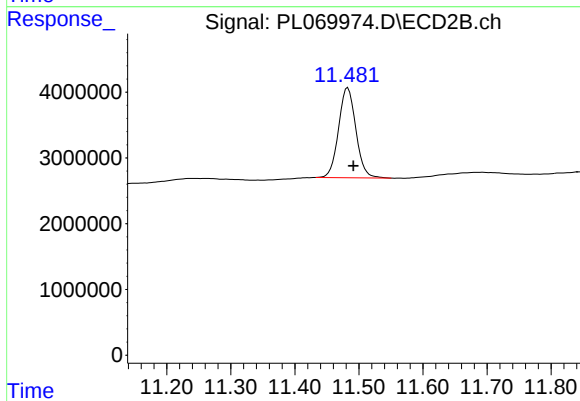

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.009 min
Response: 25657985
Conc: 22.45 ng/ml