

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092222\
 Data File : PL077877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2022 13:01
 Operator : AR\AJ
 Sample : PB147824BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB147824BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 18:17:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.624	31392561	54369061	19.584	18.314
28)	SA Decachlor...	8.916	7.727	27654837	46392708	21.398	18.481
Target Compounds							
7)	B delta-BHC	4.678	0.000	1180896	0	0.575	N.D. #
8)	B Heptachlo...	0.000	4.533f	0	156296	N.D.	0.046 #
10)	B gamma-Chl...	0.000	4.806	0	409576	N.D.	0.120 #
12)	B 4,4'-DDE	0.000	5.043	0	1975044	N.D.	0.607 #
14)	MA Endrin	0.000	5.474f	0	250831	N.D.	0.088 #
19)	B Endosulfa...	7.037f	0.000	732573	0	0.572	N.D. #
20)	A Methoxychlor	7.393	0.000	728746	0	1.103	N.D. #
25)	Chlordane-3	0.000	4.806	0	409576	N.D.	1.191 #
27)	Chlordane-5	0.000	5.545f	0	234496	N.D.	2.492 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092222\
Data File : PL077877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2022 13:01
Operator : AR\AJ
Sample : PB147824BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB147824BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 18:17:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

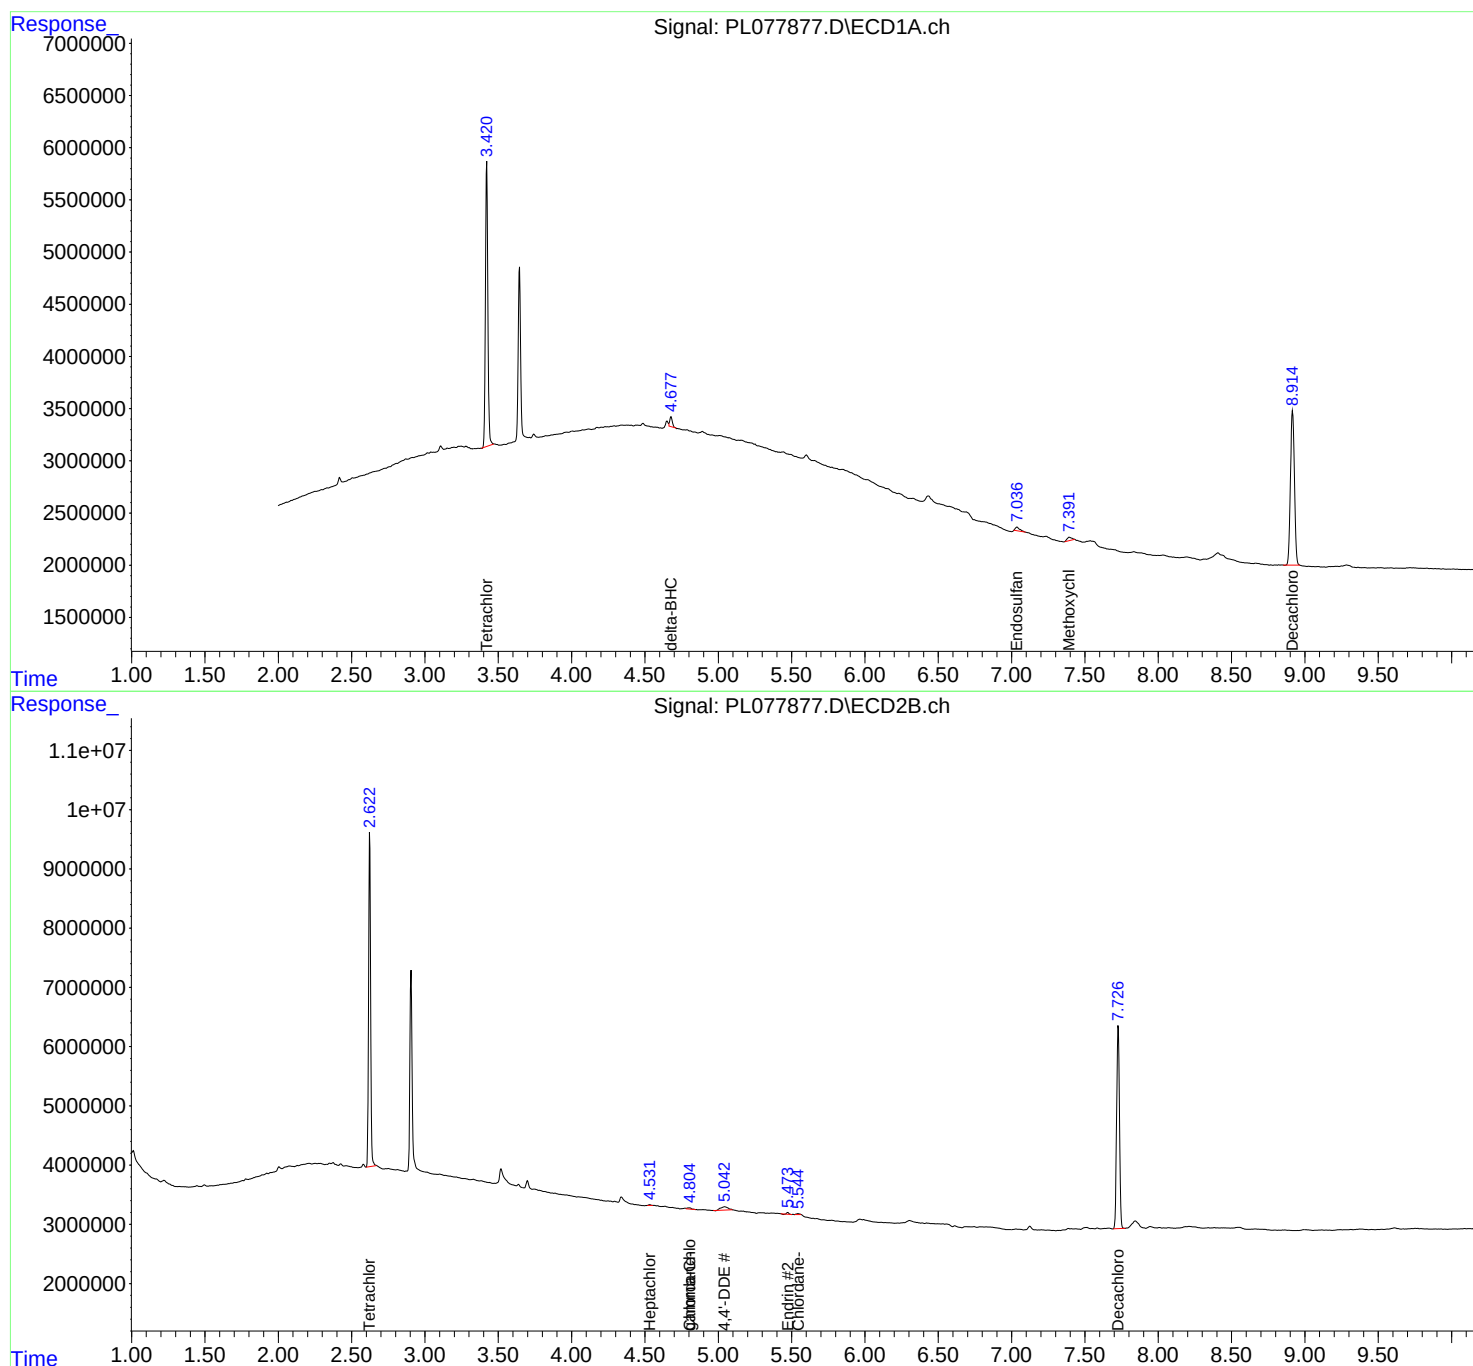


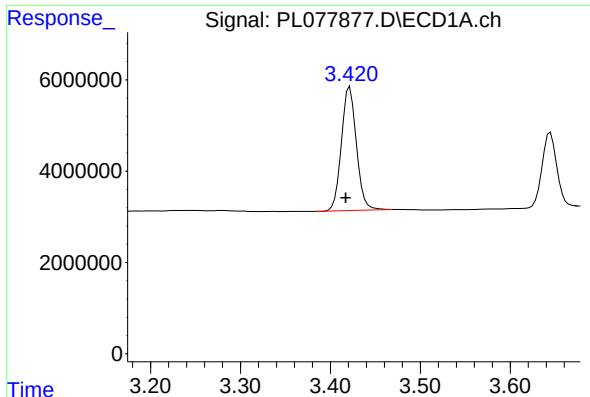

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.005 min
Response: 31392561
Conc: 19.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB147824BL

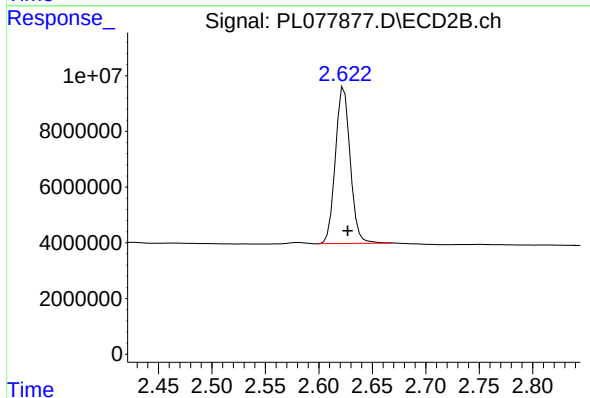


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: -0.003 min
Response: 54369061
Conc: 18.31 ng/ml

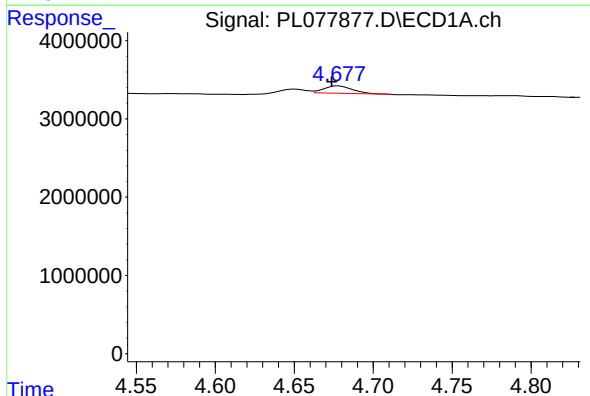


#7 delta-BHC

R.T.: 4.678 min
Delta R.T.: 0.004 min
Response: 1180896
Conc: 0.58 ng/ml

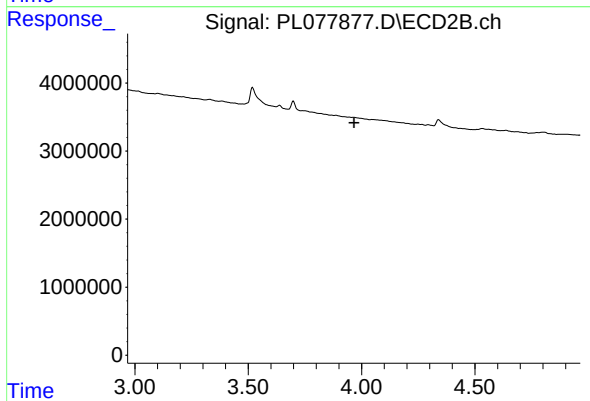

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

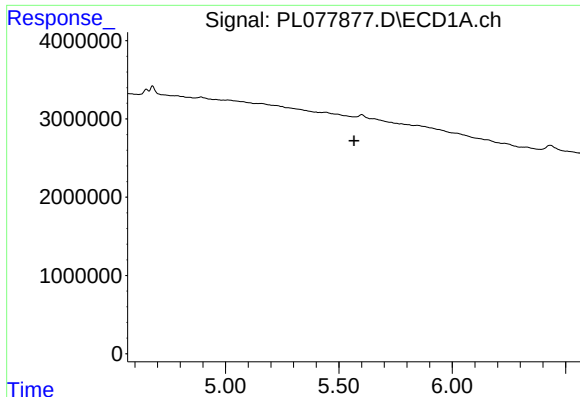

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.567 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB147824BL

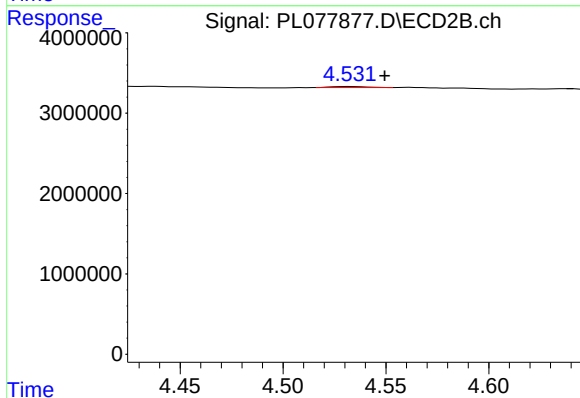


#8 Heptachlor epoxide

R.T.: 4.533 min
Delta R.T.: -0.017 min
Response: 156296
Conc: 0.05 ng/ml

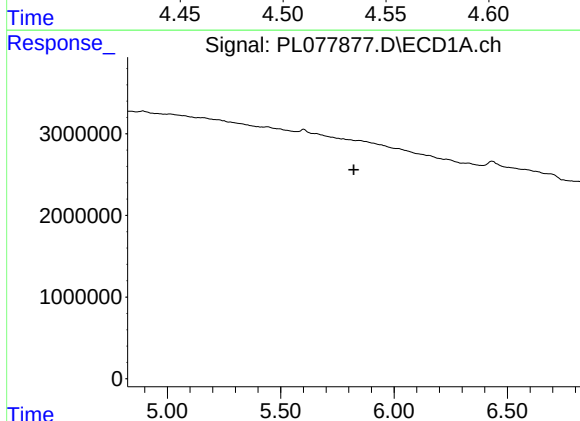


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

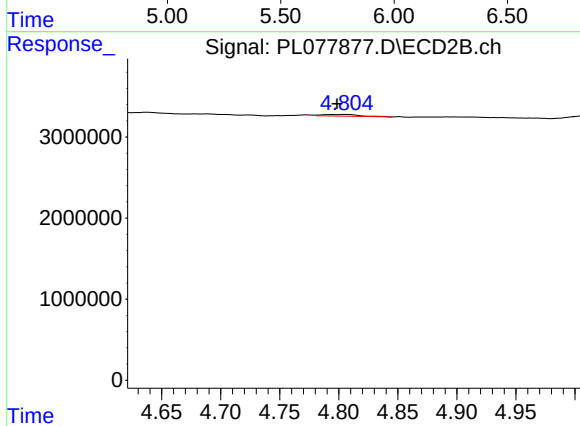

#10 gamma-Chlordane


R.T.: 4.806 min
Delta R.T.: 0.007 min
Response: 409576
Conc: 0.12 ng/ml

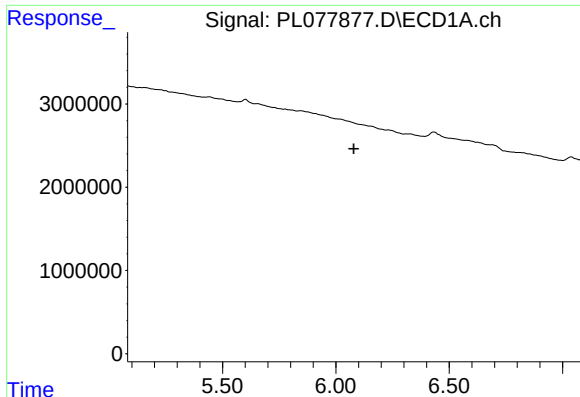

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.080 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB147824BL

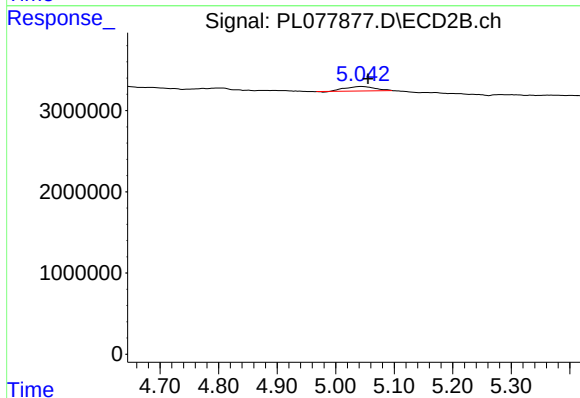


#12 4,4'-DDE

R.T.: 5.043 min
Delta R.T.: -0.012 min
Response: 1975044
Conc: 0.61 ng/ml

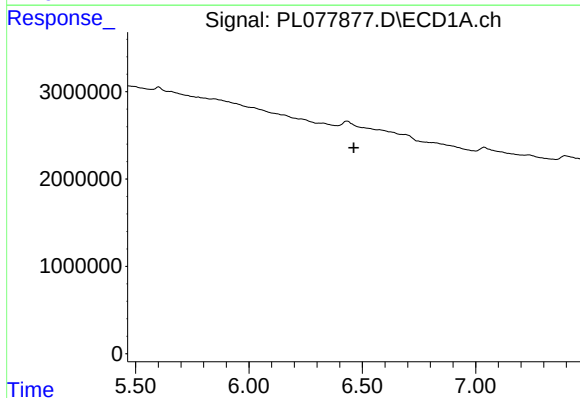


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

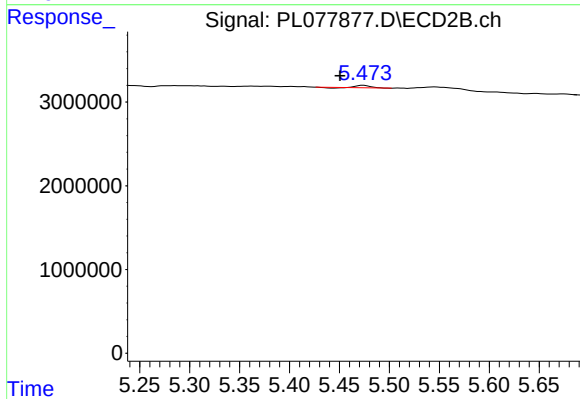

#14 Endrin

R.T.: 5.474 min
Delta R.T.: 0.024 min
Response: 250831
Conc: 0.09 ng/ml

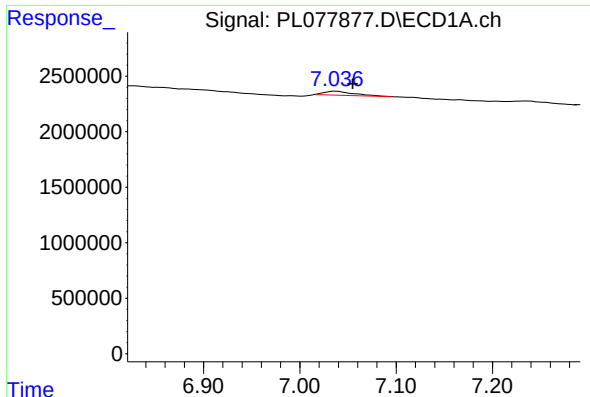

#19 Endosulfan Sulfate

R.T.: 7.037 min
Delta R.T.: -0.018 min
Response: 732573
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB147824BL

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.149 min
Response: 0
Conc: N.D.

#20 Methoxychlor

R.T.: 7.393 min
Delta R.T.: -0.004 min
Response: 728746
Conc: 1.10 ng/ml

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.435 min
Response: 0
Conc: N.D.

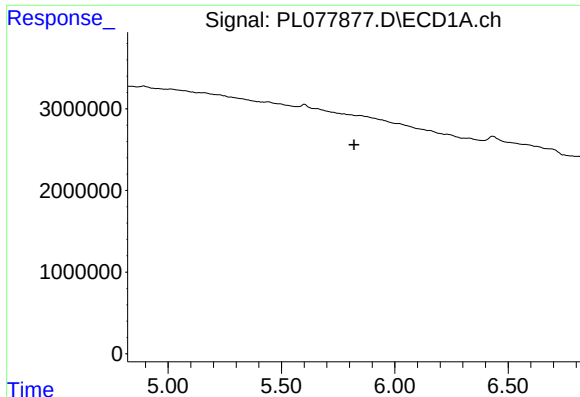

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.820 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB147824BL

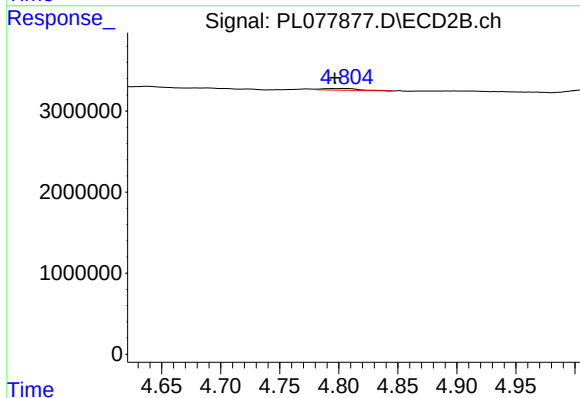


#25 Chlordane-3

R.T.: 4.806 min
Delta R.T.: 0.009 min
Response: 409576
Conc: 1.19 ng/ml

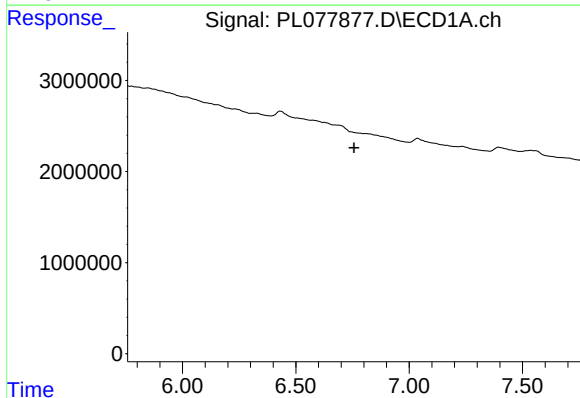


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.757 min
Response: 0
Conc: N.D.

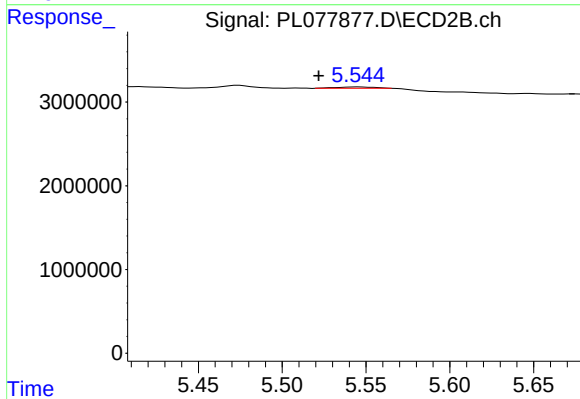

#27 Chlordane-5


R.T.: 5.545 min
Delta R.T.: 0.023 min
Response: 234496
Conc: 2.49 ng/ml

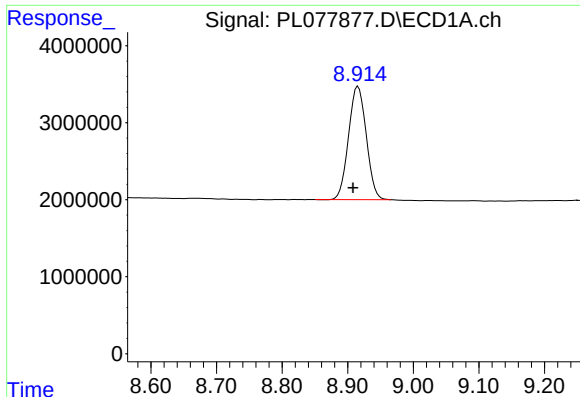

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: 0.007 min
Response: 27654837
Conc: 21.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB147824BL

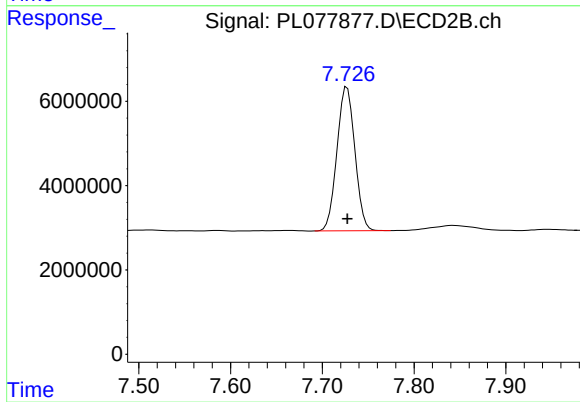

#28 Decachlorobiphenyl

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 46392708
Conc: 18.48 ng/ml