

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092222\
 Data File : PL077882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2022 15:52
 Operator : AR\AJ
 Sample : N4732-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 18:17:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 13 13:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.626	36292753	66247298	22.641	22.315
28)	SA Decachlor...	8.910	7.726	27276193	42401924	21.105	16.892
Target Compounds							
10)	B gamma-Chl...	5.822	4.796	8826659	17600601	5.041	5.164
11)	B alpha-Chl...	5.901	4.856	8519443	13554949	4.932	4.093m
12)	B 4,4'-DDE	6.077	5.053	9917774	23748636	6.230	7.299
13)	MA Dieldrin	6.229	5.177	8515072	27846110	5.276m	8.398m#
15)	B Endosulfa...	6.691	5.743	3928637	9752250	2.844m	3.701m#
16)	A 4,4'-DDD	6.602	5.606	4499993	3084256	3.843m	1.191 #
17)	MA 4,4'-DDT	6.915	5.854	26807114	64464504	21.156	24.467
19)	B Endosulfa...	7.055	6.147	6698458	17532335	5.231	6.520


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092222\
Data File : PL077882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2022 15:52
Operator : AR\AJ
Sample : N4732-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 18:17:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091222.M
Quant Title : GC Extractables
QLast Update : Tue Sep 13 13:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

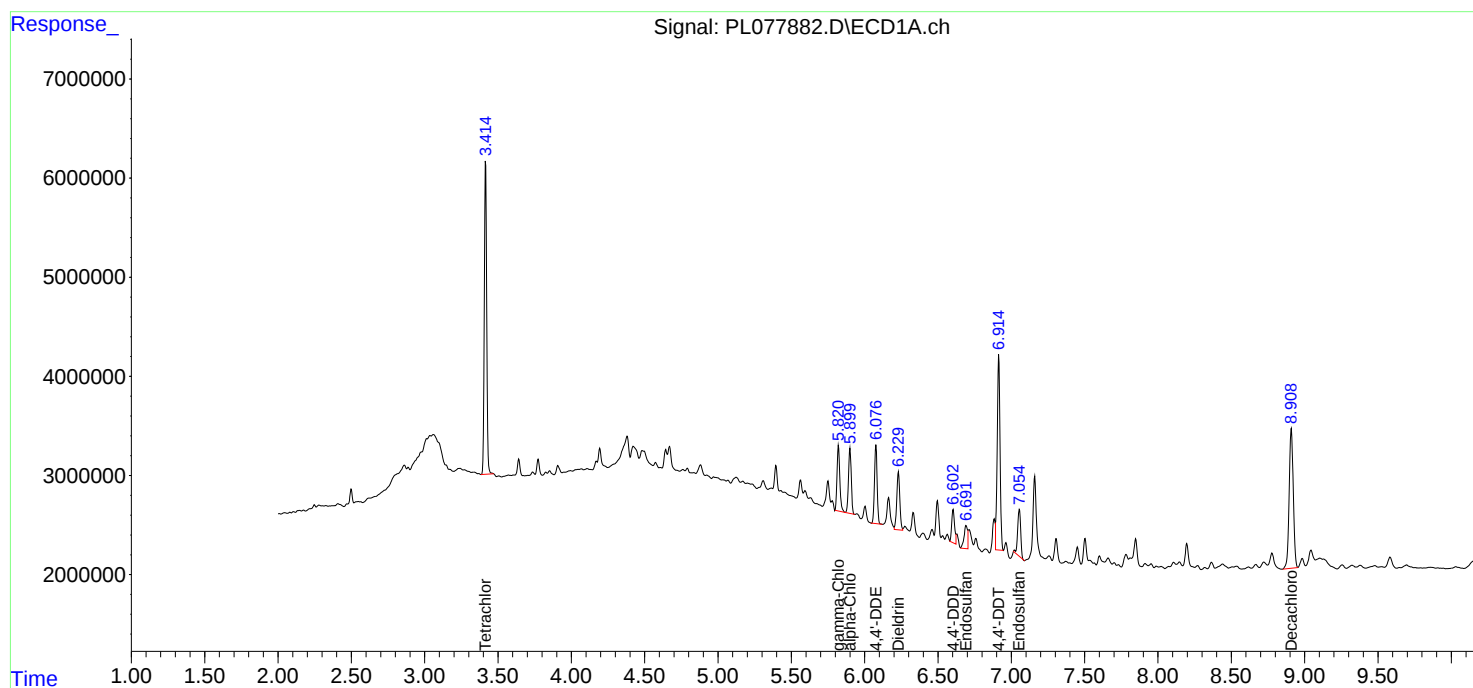


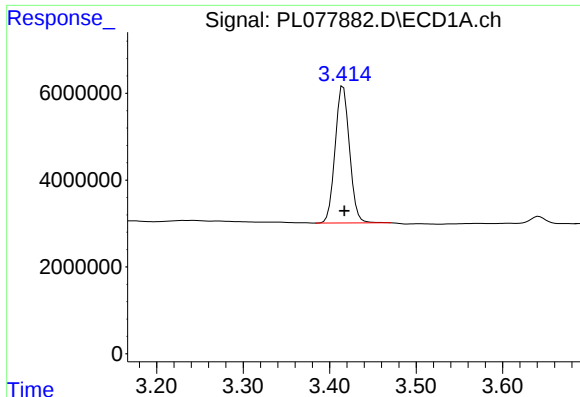

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: -0.001 min
Response: 36292753
Conc: 22.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-1

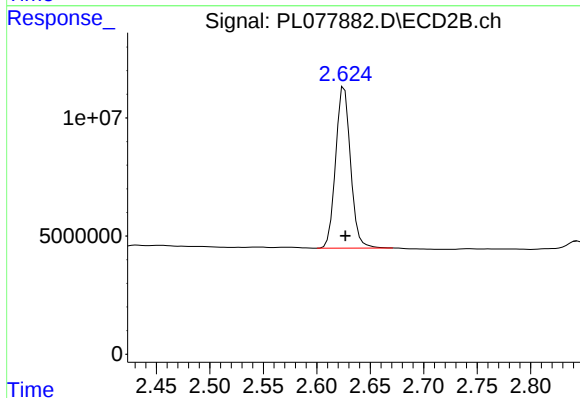


#1 Tetrachloro-m-xylene

R.T.: 2.626 min
Delta R.T.: -0.001 min
Response: 66247298
Conc: 22.31 ng/ml

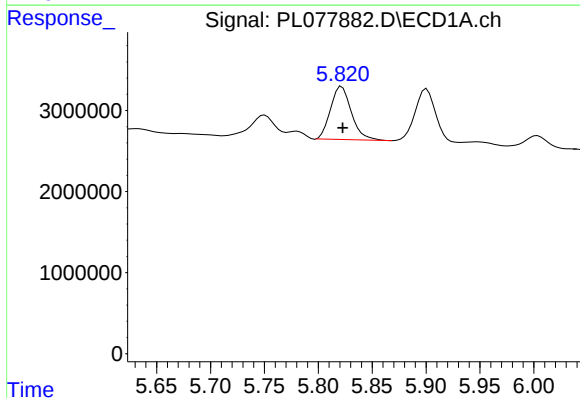


#10 gamma-Chlordane

R.T.: 5.822 min
Delta R.T.: 0.000 min
Response: 8826659
Conc: 5.04 ng/ml

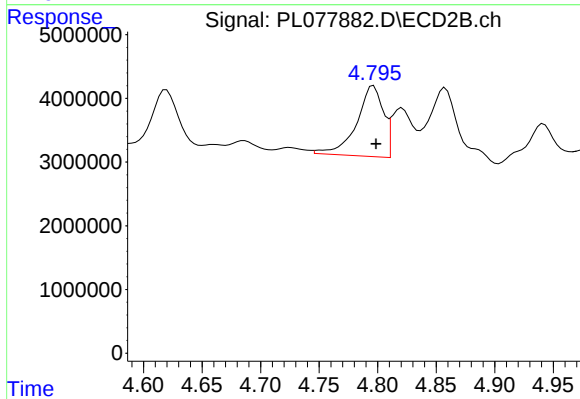

#10 gamma-Chlordane


R.T.: 4.796 min
Delta R.T.: -0.002 min
Response: 17600601
Conc: 5.16 ng/ml

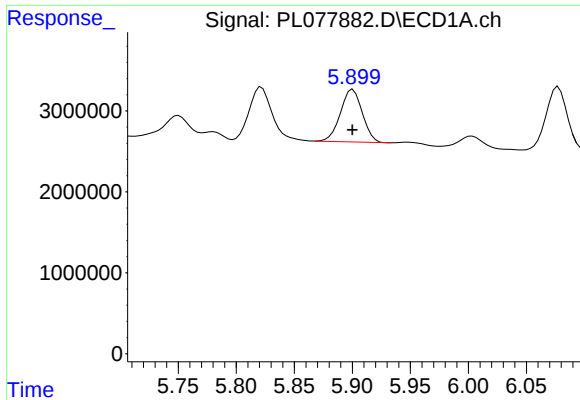

#11 alpha-Chlordane


R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 8519443
Conc: 4.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-1

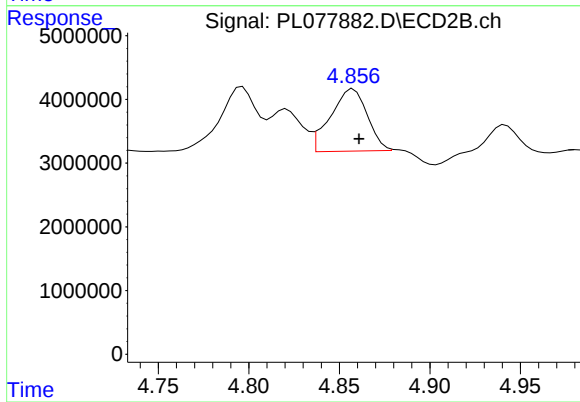


#11 alpha-Chlordane

R.T.: 4.856 min
Delta R.T.: -0.004 min
Response: 13554949
Conc: 4.09 ng/ml m

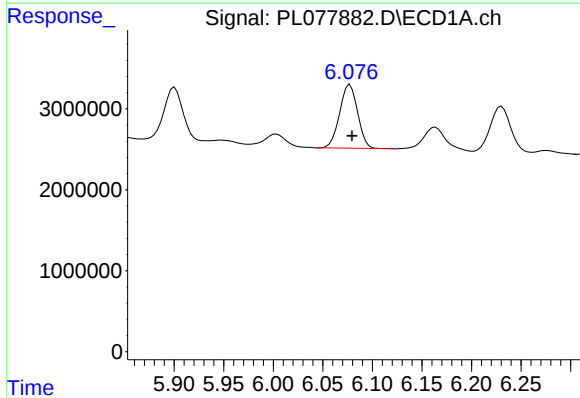


#12 4,4'-DDE

R.T.: 6.077 min
Delta R.T.: -0.002 min
Response: 9917774
Conc: 6.23 ng/ml

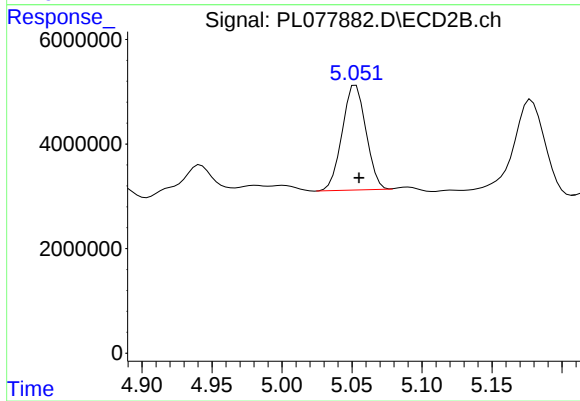

#12 4,4'-DDE


R.T.: 5.053 min
Delta R.T.: -0.002 min
Response: 23748636
Conc: 7.30 ng/ml

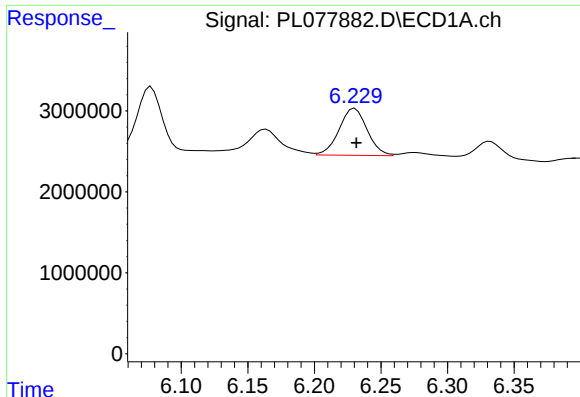

#13 Dieldrin


R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 8515072
Conc: 5.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-1

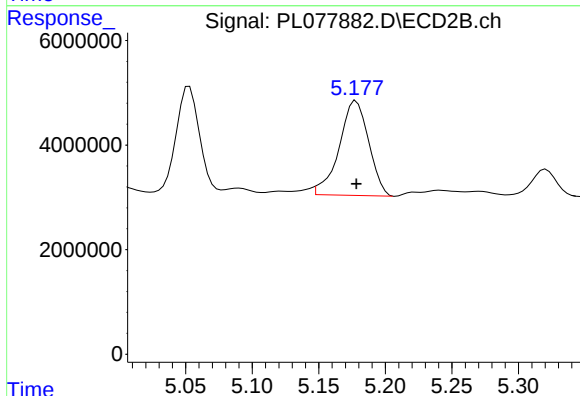


#13 Dieldrin

R.T.: 5.177 min
Delta R.T.: -0.002 min
Response: 27846110
Conc: 8.40 ng/ml m

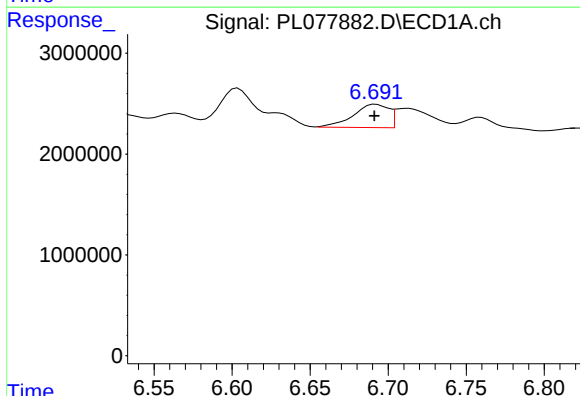


#15 Endosulfan II

R.T.: 6.691 min
Delta R.T.: 0.000 min
Response: 3928637
Conc: 2.84 ng/ml m

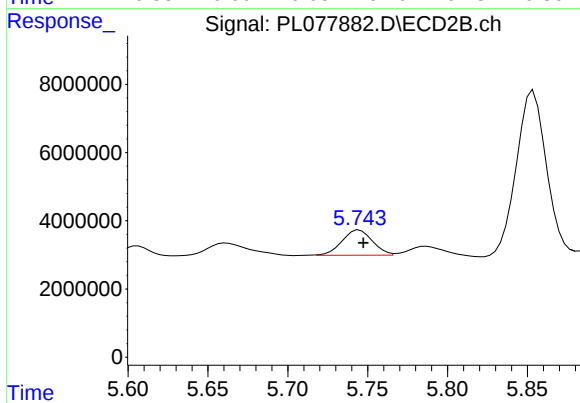

#15 Endosulfan II


R.T.: 5.743 min
Delta R.T.: -0.004 min
Response: 9752250
Conc: 3.70 ng/ml m

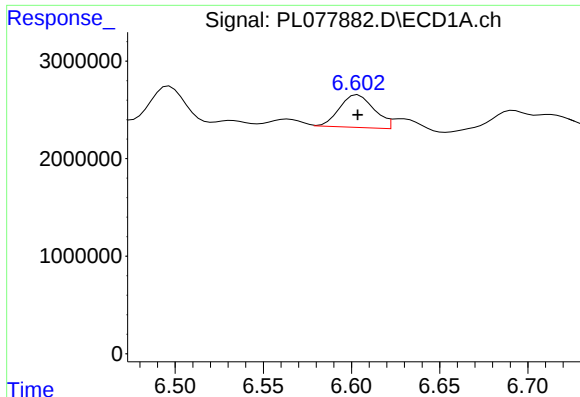

#16 4,4'-DDD


R.T.: 6.602 min
Delta R.T.: -0.001 min
Response: 4499993
Conc: 3.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-1

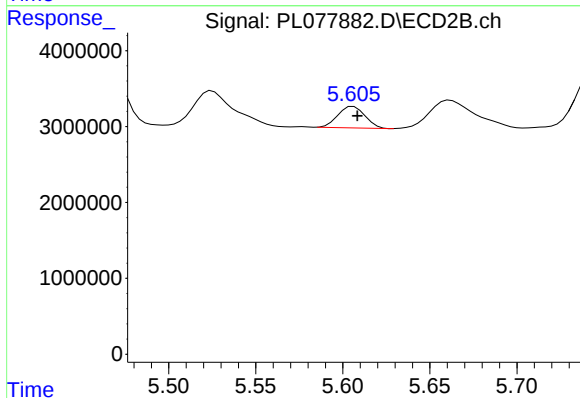


#16 4,4'-DDD

R.T.: 5.606 min
Delta R.T.: -0.002 min
Response: 3084256
Conc: 1.19 ng/ml

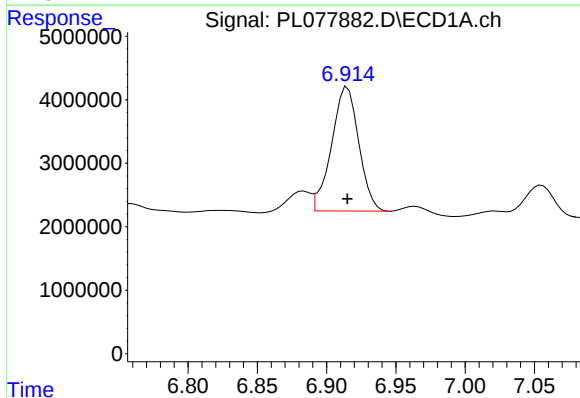


#17 4,4'-DDT

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 26807114
Conc: 21.16 ng/ml

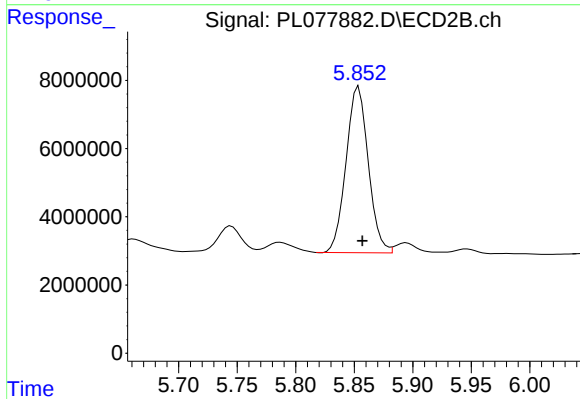

#17 4,4'-DDT


R.T.: 5.854 min
Delta R.T.: -0.003 min
Response: 64464504
Conc: 24.47 ng/ml

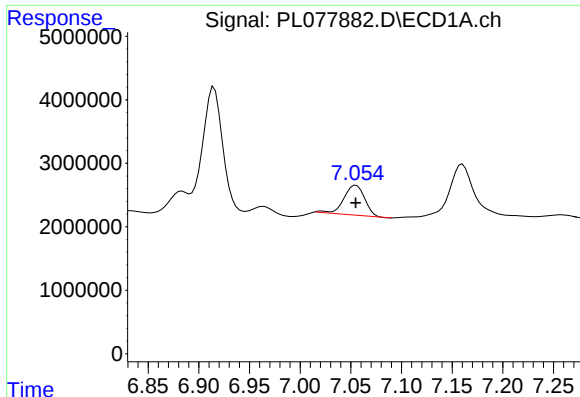

#19 Endosulfan Sulfate


R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 6698458
Conc: 5.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-1

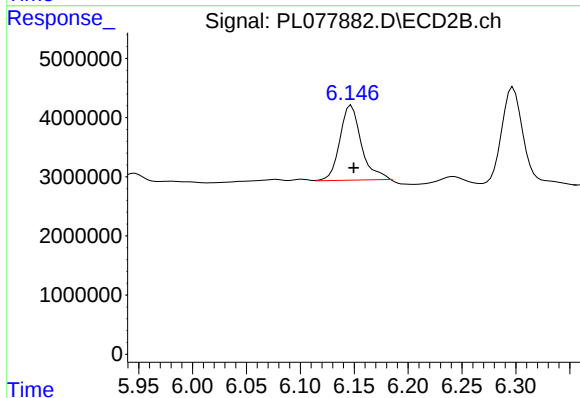


#19 Endosulfan Sulfate

R.T.: 6.147 min
Delta R.T.: -0.002 min
Response: 17532335
Conc: 6.52 ng/ml

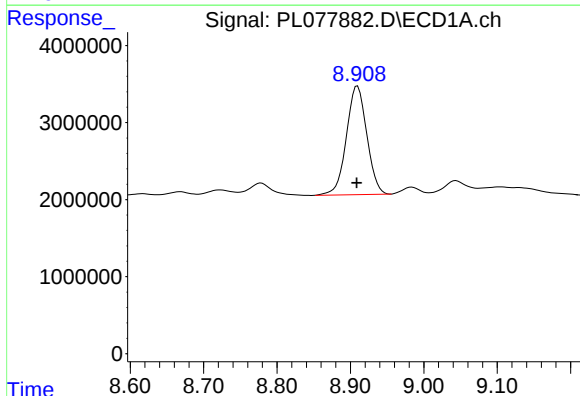

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: 0.001 min
Response: 27276193
Conc: 21.10 ng/ml

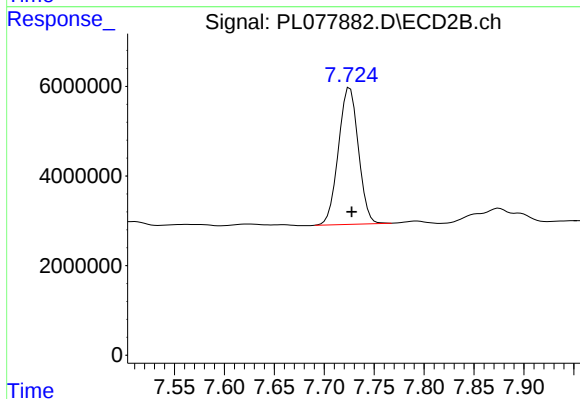

#28 Decachlorobiphenyl

R.T.: 7.726 min
Delta R.T.: -0.002 min
Response: 42401924
Conc: 16.89 ng/ml