

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092318\
 Data File : PL040214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2018 07:09
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:19:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
9) A	Endosulfan I	5.216	6.025	1116094	60957881	0.113	17.200 #
10) B	gamma-Chl...	0.000	5.929	0	181.5E6	N.D.	47.149 #
11) B	alpha-Chl...	5.216f	5.959	1116094	141.5E6	0.107	37.209 #
12) B	4,4'-DDE	5.319	6.127	13060521	13675916	1.239	3.609 #
13) MA	Dieldrin	5.392f	6.286	22403733	-1681237	2.102	N.D. #
14) MA	Endrin	5.698	6.494	24722276	48400043	2.511	15.163 #
16) A	4,4'-DDD	5.781f	0.000	4646131	0	0.538	N.D. #
21) B	Endrin ke...	6.841	0.000	42809682	0	4.380	N.D. #
25)	Chlordane-3	0.000	5.929	0	181.5E6	N.D.	339.476 #
26)	Chlordane-4	5.216	5.959	1116094	141.5E6	0.968	221.587 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092318\
Data File : PL040214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2018 07:09
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:19:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

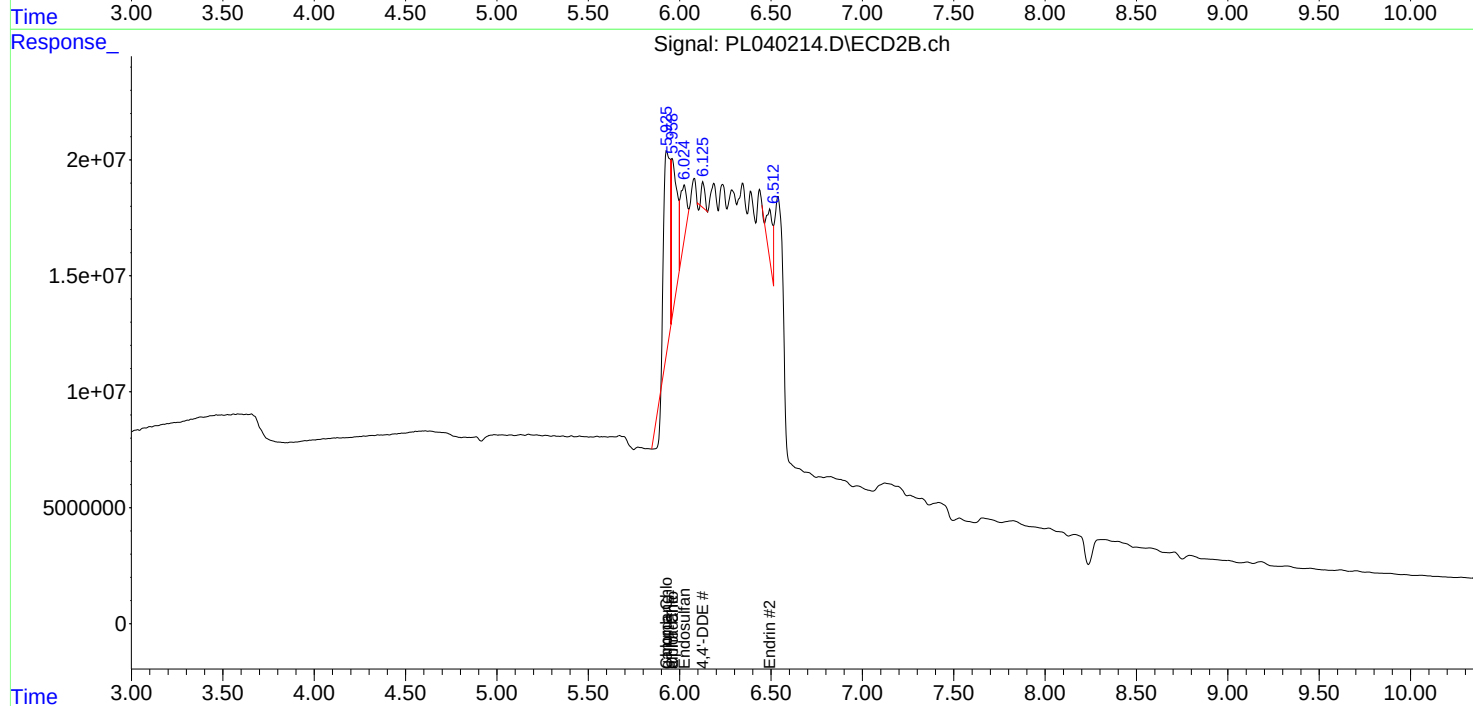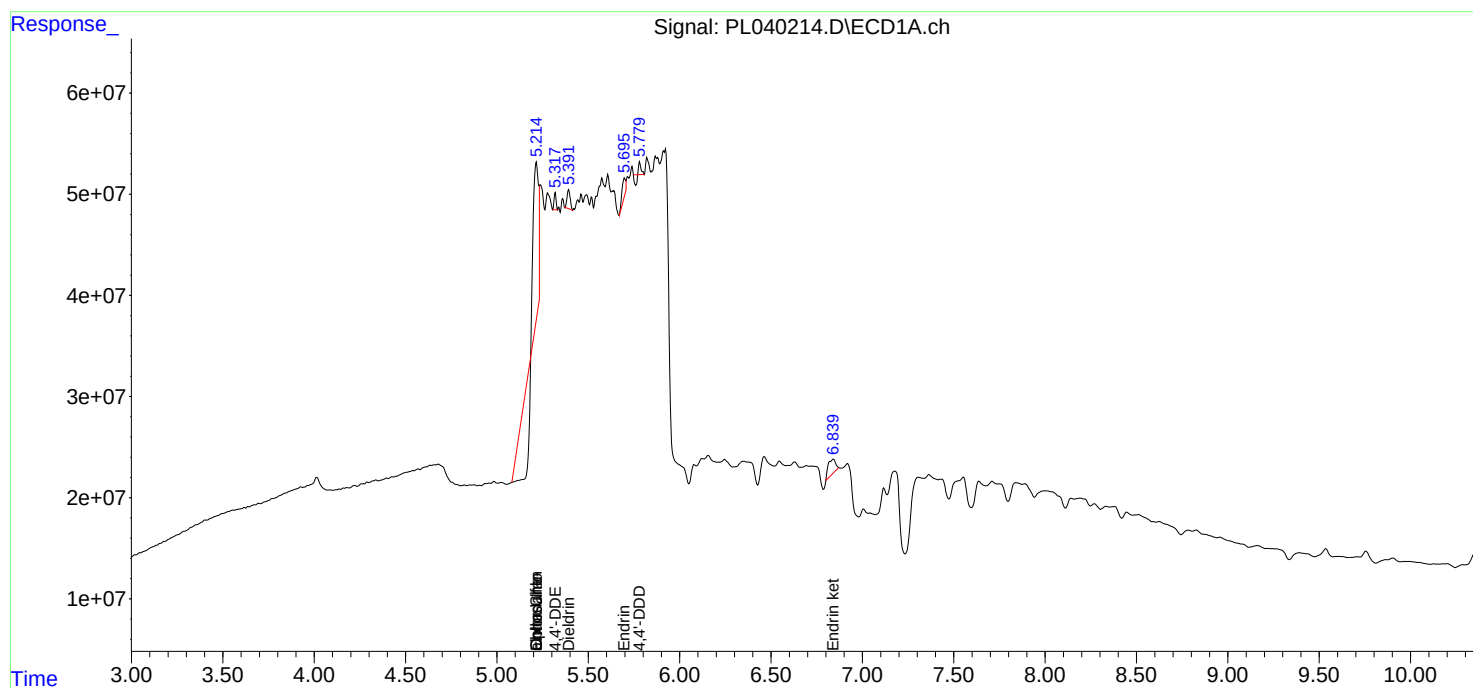


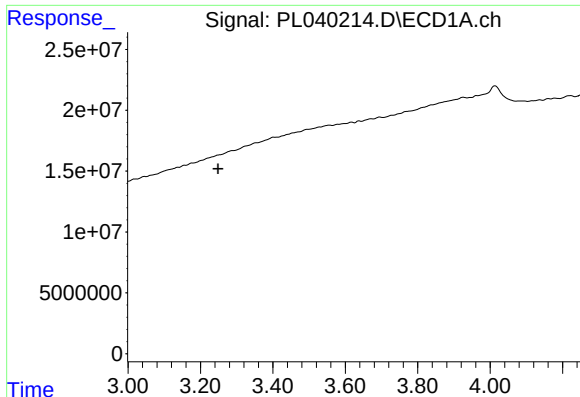

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.249 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

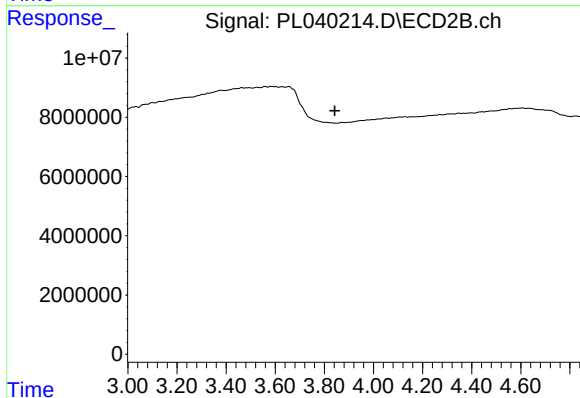


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.843 min
Response: 0
Conc: N.D.

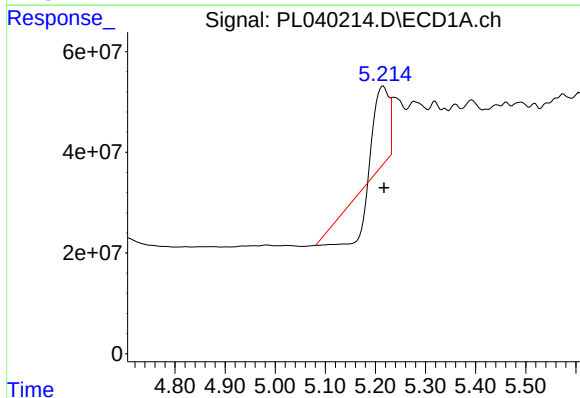


#9 Endosulfan I

R.T.: 5.216 min
Delta R.T.: -0.002 min
Response: 1116094
Conc: 0.11 ng/ml

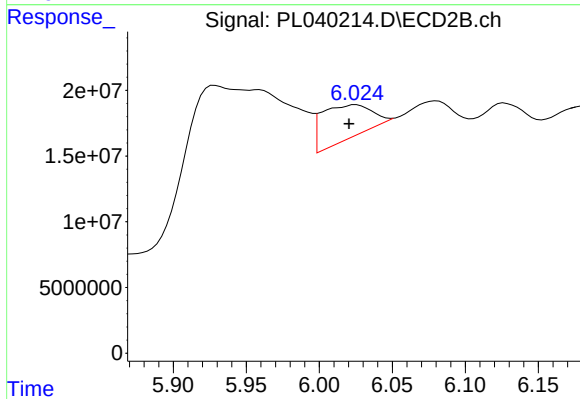

#9 Endosulfan I


R.T.: 6.025 min
Delta R.T.: 0.005 min
Response: 60957881
Conc: 17.20 ng/ml

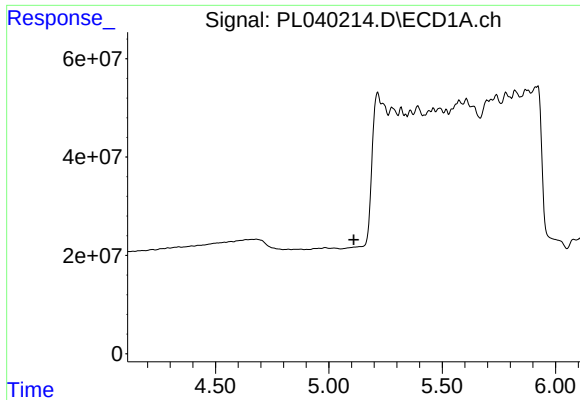

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.110 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

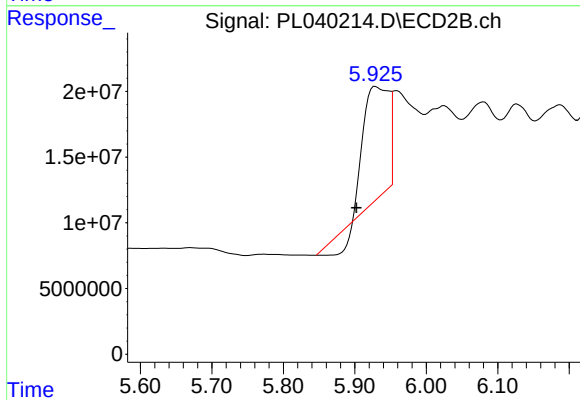


#10 gamma-Chlordane

R.T.: 5.929 min
Delta R.T.: 0.027 min
Response: 181539401
Conc: 47.15 ng/ml

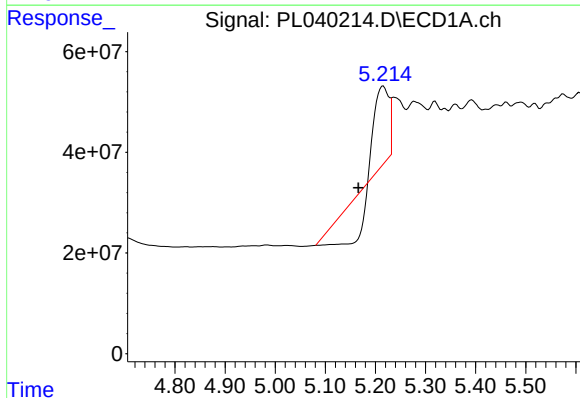


#11 alpha-Chlordane

R.T.: 5.216 min
Delta R.T.: 0.050 min
Response: 1116094
Conc: 0.11 ng/ml

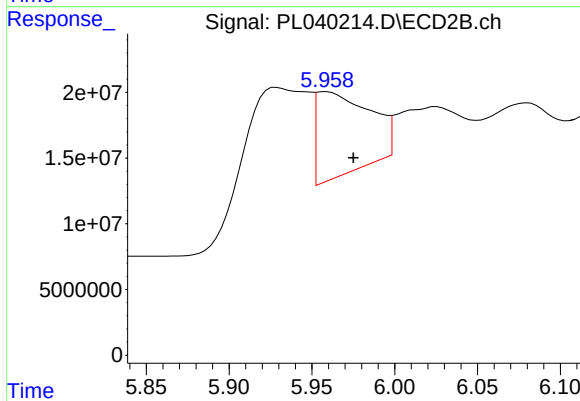

#11 alpha-Chlordane


R.T.: 5.959 min
Delta R.T.: -0.016 min
Response: 141505413
Conc: 37.21 ng/ml

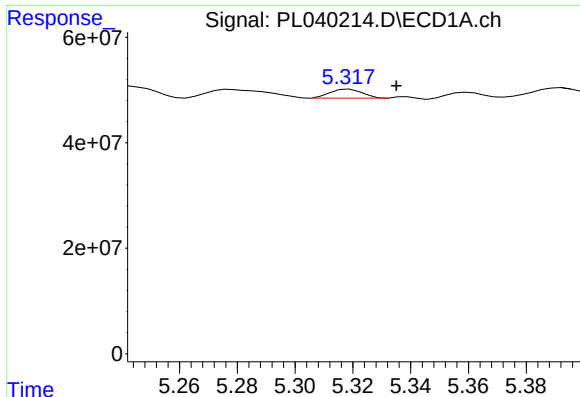

#12 4,4'-DDE


R.T.: 5.319 min
Delta R.T.: -0.016 min
Response: 13060521
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

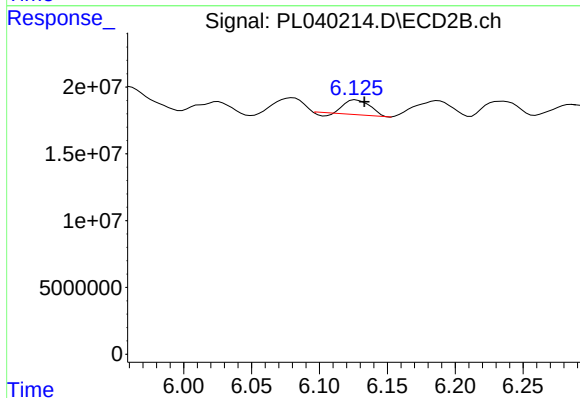


#12 4,4'-DDE

R.T.: 6.127 min
Delta R.T.: -0.006 min
Response: 13675916
Conc: 3.61 ng/ml

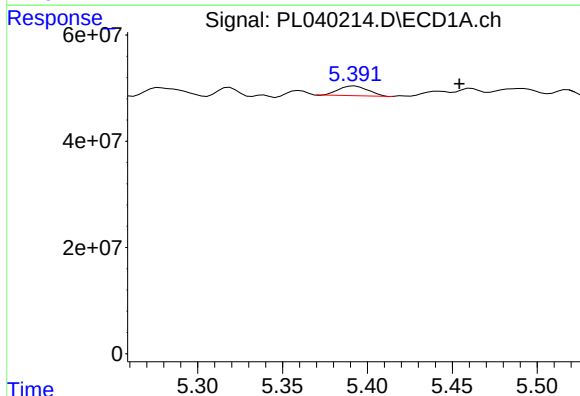


#13 Dieldrin

R.T.: 5.392 min
Delta R.T.: -0.062 min
Response: 22403733
Conc: 2.10 ng/ml

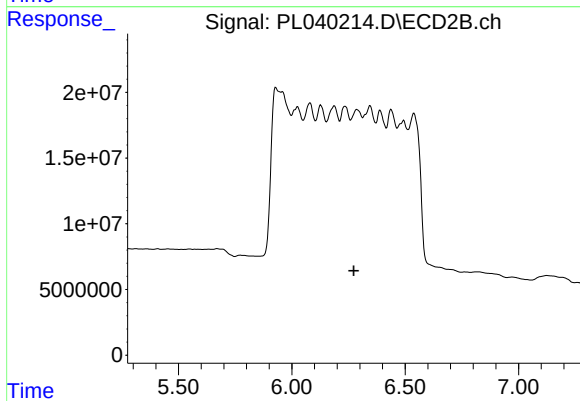

#13 Dieldrin


R.T.: 6.286 min
Delta R.T.: 0.014 min
Response: -1681237
Conc: N.D.

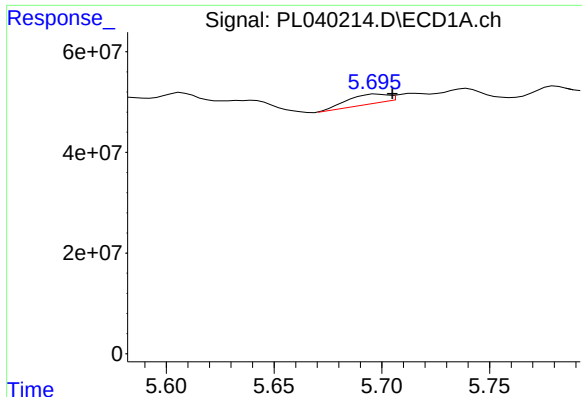

#14 Endrin


R.T.: 5.698 min
Delta R.T.: -0.007 min
Response: 24722276
Conc: 2.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

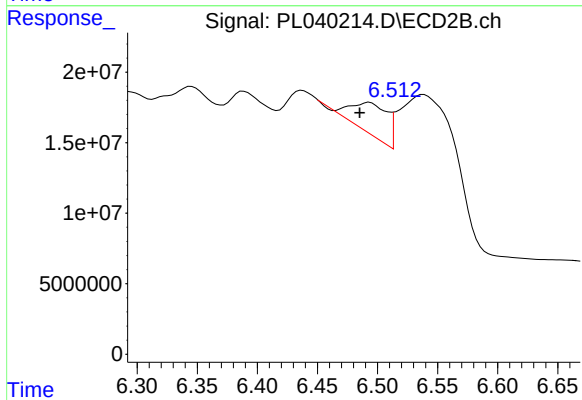


#14 Endrin

R.T.: 6.494 min
Delta R.T.: 0.009 min
Response: 48400043
Conc: 15.16 ng/ml

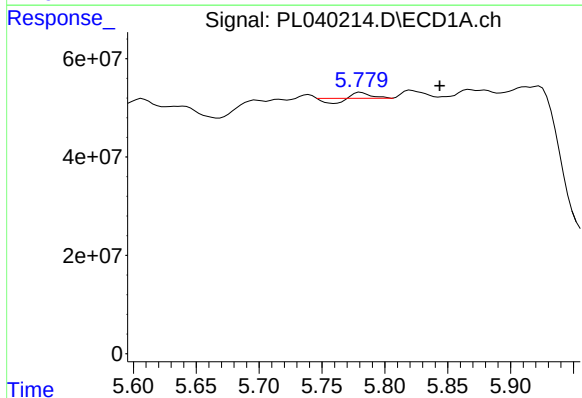


#16 4,4'-DDD

R.T.: 5.781 min
Delta R.T.: -0.063 min
Response: 4646131
Conc: 0.54 ng/ml

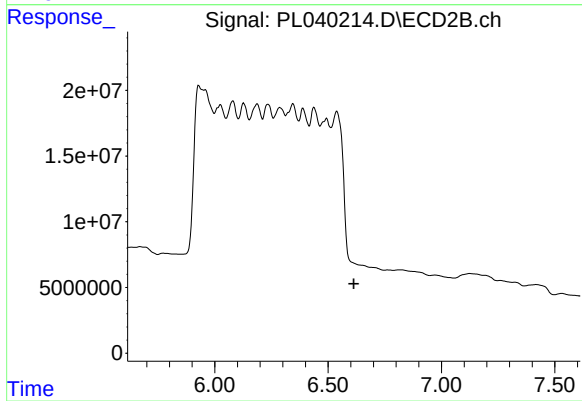

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.613 min
Response: 0
Conc: N.D.

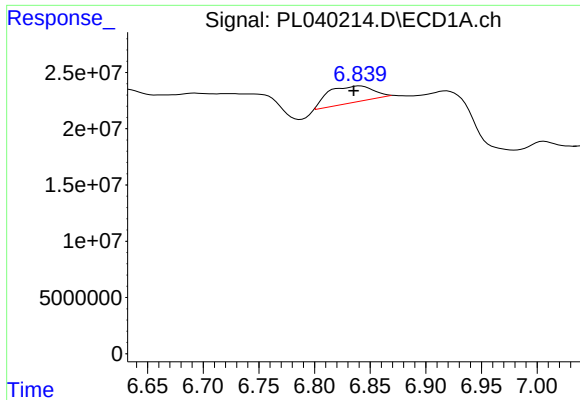

#21 Endrin ketone


R.T.: 6.841 min
Delta R.T.: 0.006 min
Response: 42809682
Conc: 4.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

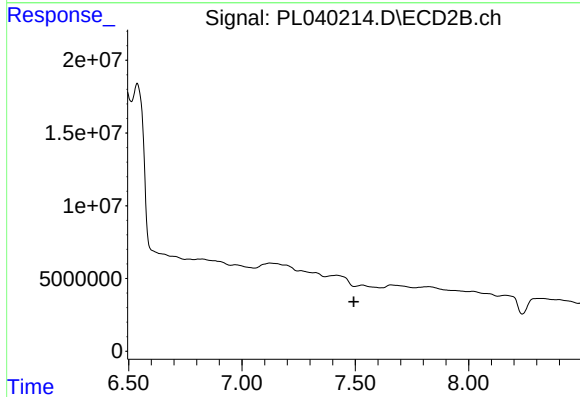


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.493 min
Response: 0
Conc: N.D.

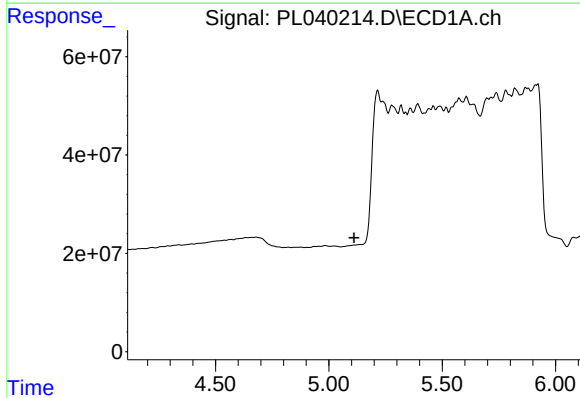


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

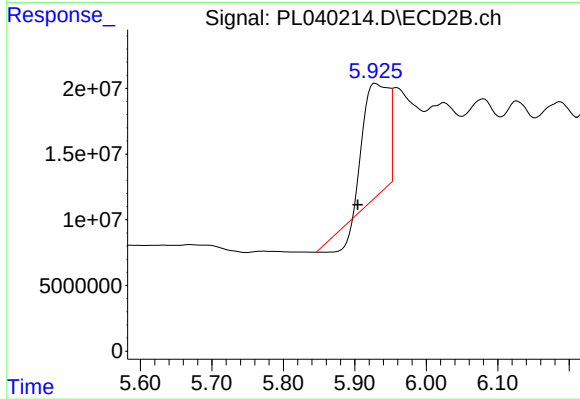

#25 Chlordane-3


R.T.: 5.929 min
Delta R.T.: 0.025 min
Response: 181539401
Conc: 339.48 ng/ml

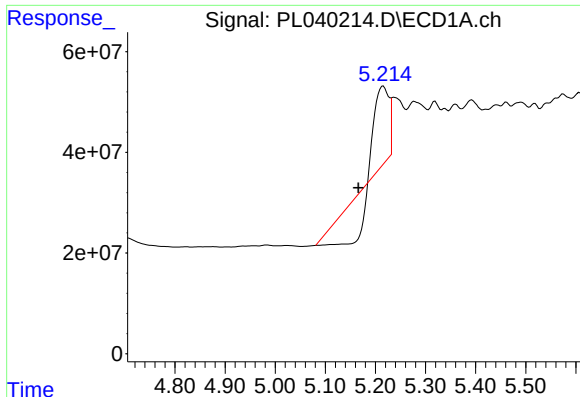

#26 Chlordane-4


R.T.: 5.216 min
Delta R.T.: 0.050 min
Response: 1116094
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

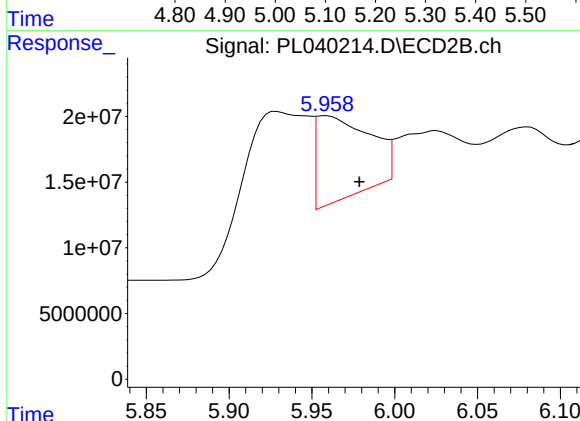


#26 Chlordane-4

R.T.: 5.959 min
Delta R.T.: -0.020 min
Response: 141505413
Conc: 221.59 ng/ml

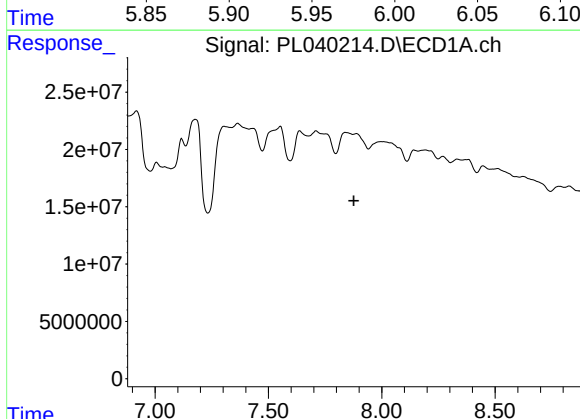

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.876 min
Response: 0
Conc: N.D.

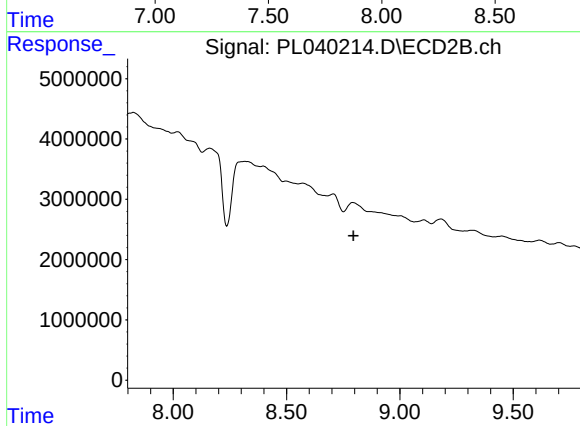

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.796 min
Response: 0
Conc: N.D.